

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032720\
 Data File : PD057639.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Mar 2020 12:37
 Operator : AJ\MA
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 14:00:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032720.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 27 13:59:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.226	3.896	38155649	38983501	50.000	50.000
28)	SA Decachlor...	7.866	8.898	37419843	42375162	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.056	4.874	12331341	15470642	500.000	500.000
24)	Chlordane-2	4.541	5.337	14089616	18723140	500.000	500.000
25)	Chlordane-3	5.089	5.978	42989462	71781813	500.000	500.000
26)	Chlordane-4	5.145	6.051	39516464	86547130	500.000	500.000
27)	Chlordane-5	5.961	6.849	13420244	17160054	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032720\
Data File : PD057639.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Mar 2020 12:37
Operator : AJ\MA
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 14:00:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032720.M
Quant Title : GC Extractables
QLast Update : Fri Mar 27 13:59:30 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

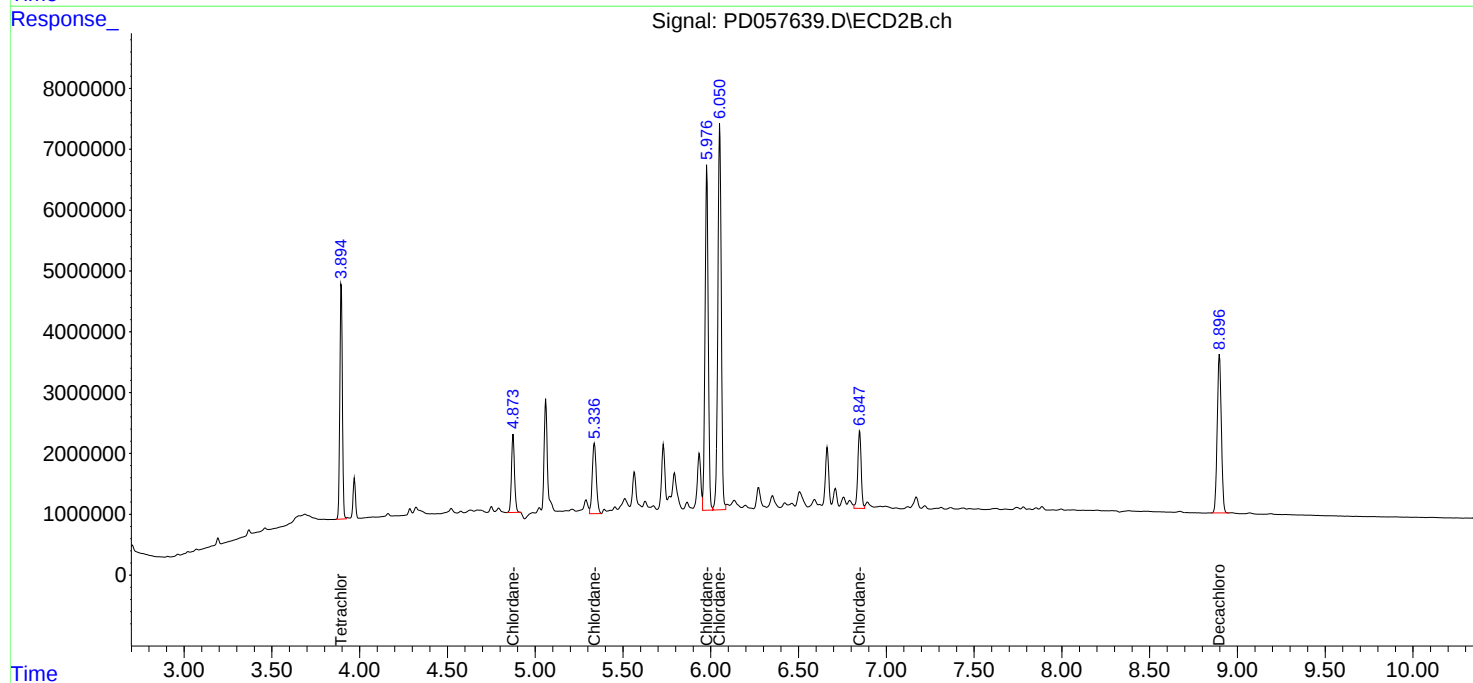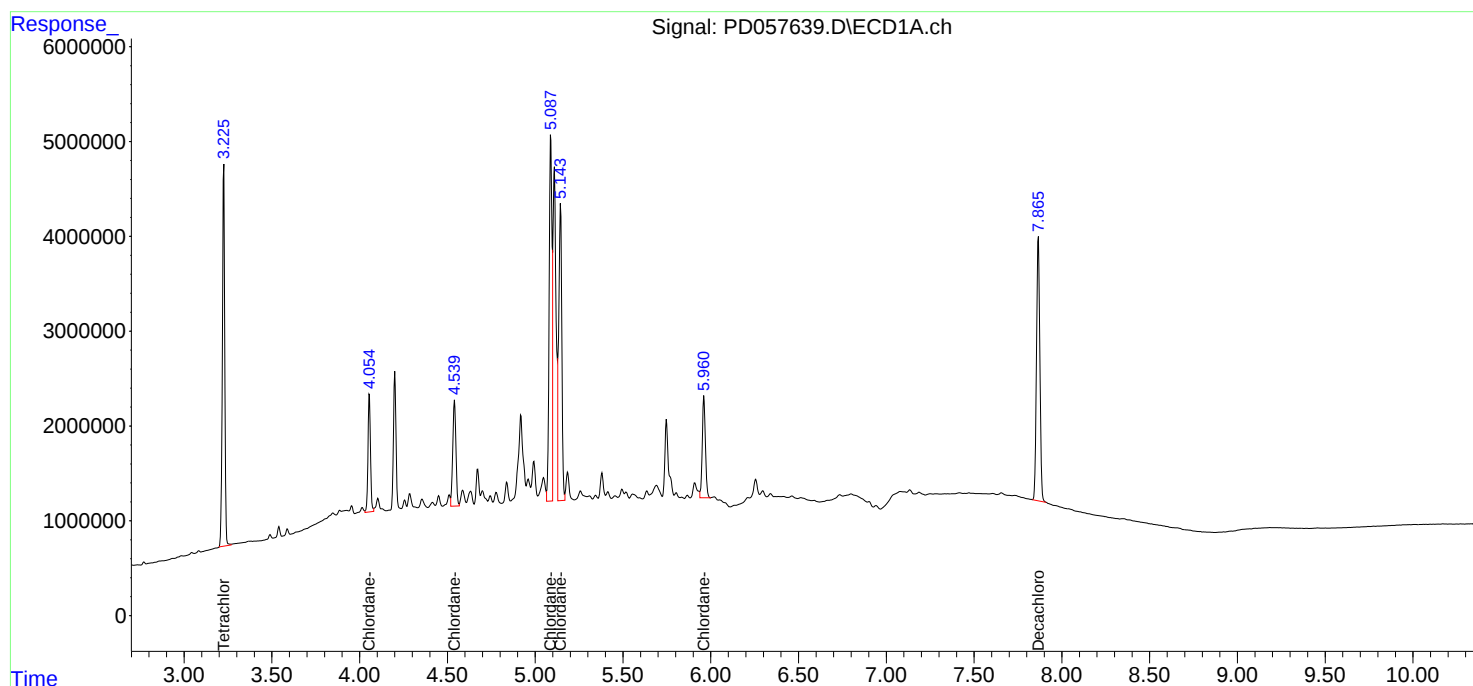


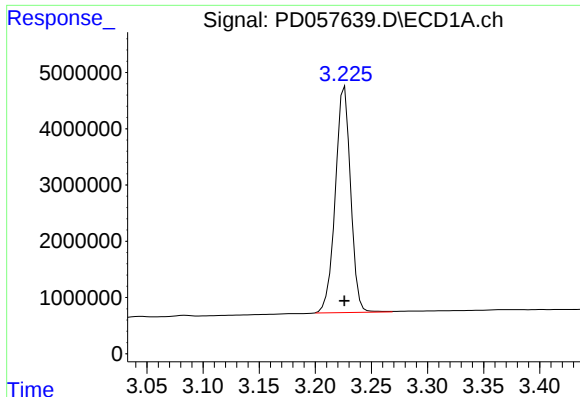

#1 Tetrachloro-m-xylene


R.T.: 3.226 min
Delta R.T.: 0.000 min
Response: 38155649
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

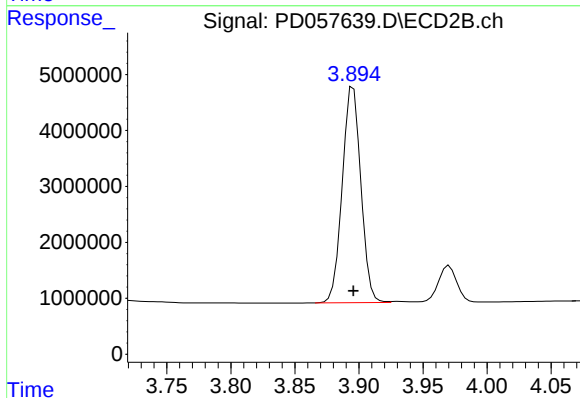


#1 Tetrachloro-m-xylene

R.T.: 3.896 min
Delta R.T.: 0.000 min
Response: 38983501
Conc: 50.00 ng/ml

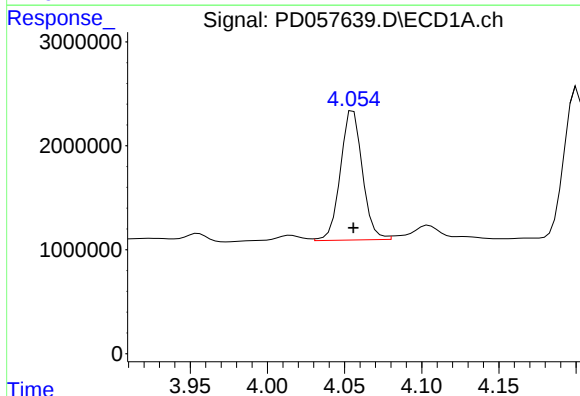


#23 Chlordane-1

R.T.: 4.056 min
Delta R.T.: 0.000 min
Response: 12331341
Conc: 500.00 ng/ml

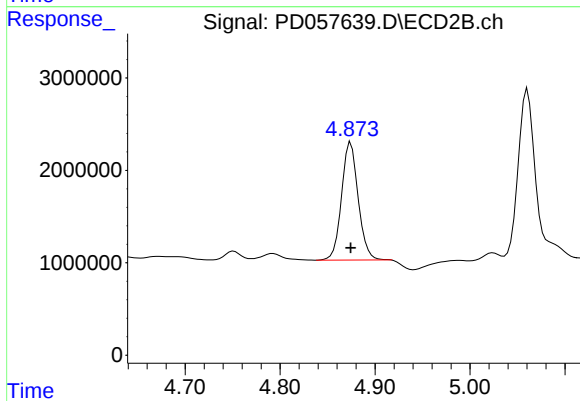

#23 Chlordane-1


R.T.: 4.874 min
Delta R.T.: 0.000 min
Response: 15470642
Conc: 500.00 ng/ml

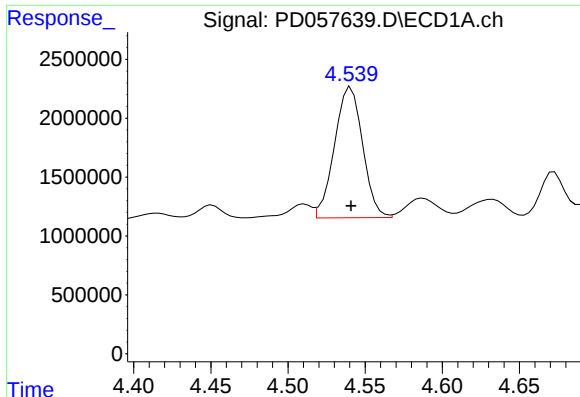

#24 Chlordane-2


R.T.: 4.541 min
Delta R.T.: 0.000 min
Response: 14089616
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

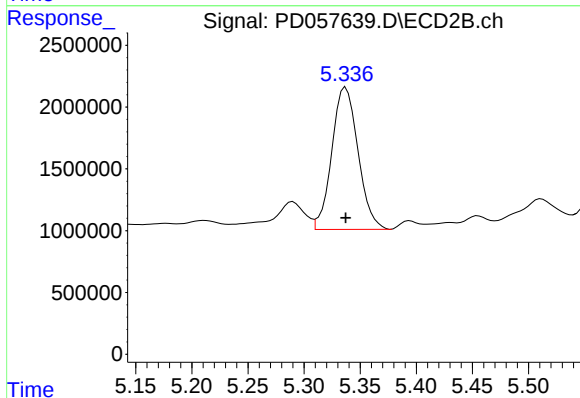


#24 Chlordane-2

R.T.: 5.337 min
Delta R.T.: 0.000 min
Response: 18723140
Conc: 500.00 ng/ml

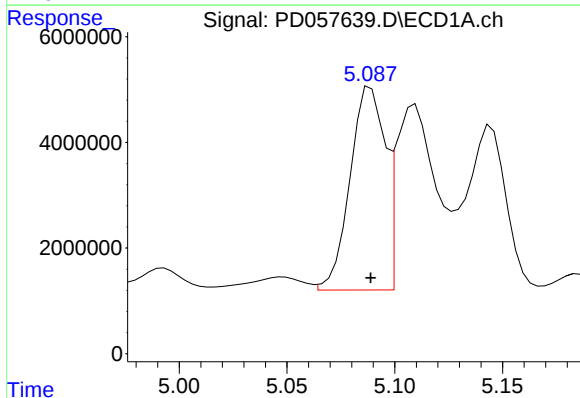


#25 Chlordane-3

R.T.: 5.089 min
Delta R.T.: 0.000 min
Response: 42989462
Conc: 500.00 ng/ml

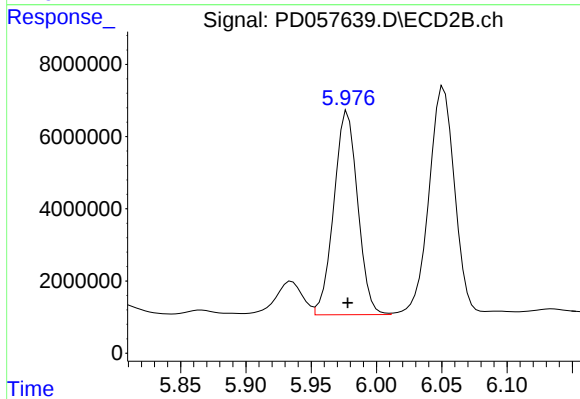

#25 Chlordane-3


R.T.: 5.978 min
Delta R.T.: 0.000 min
Response: 71781813
Conc: 500.00 ng/ml

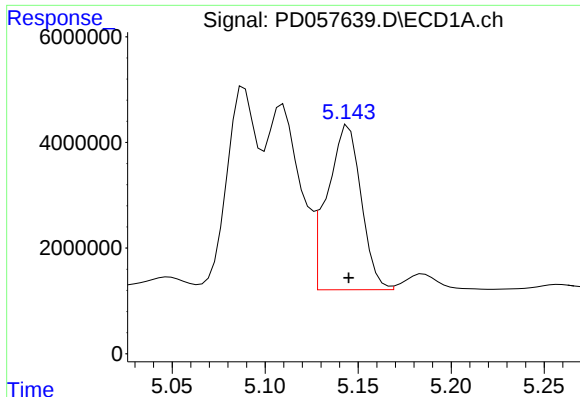

#26 Chlordane-4


R.T.: 5.145 min
Delta R.T.: 0.000 min
Response: 39516464
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

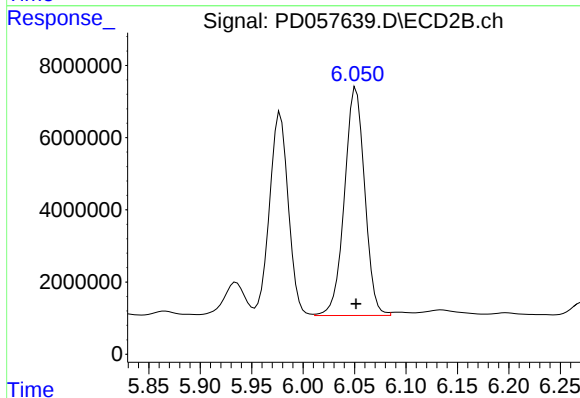


#26 Chlordane-4

R.T.: 6.051 min
Delta R.T.: 0.000 min
Response: 86547130
Conc: 500.00 ng/ml

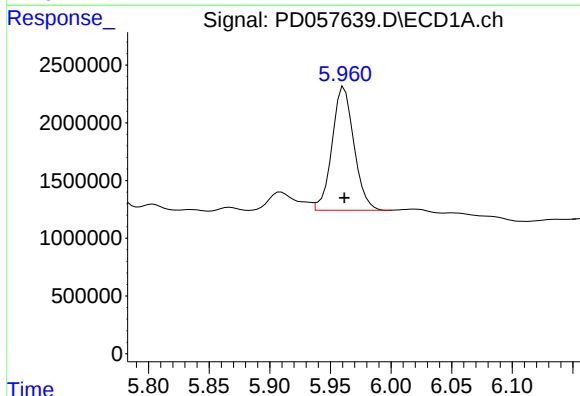


#27 Chlordane-5

R.T.: 5.961 min
Delta R.T.: 0.000 min
Response: 13420244
Conc: 500.00 ng/ml

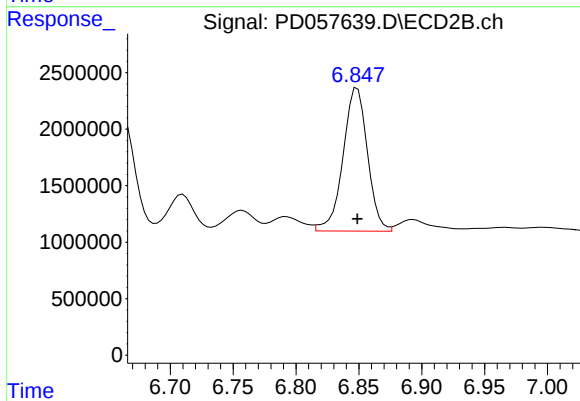

#27 Chlordane-5


R.T.: 6.849 min
Delta R.T.: 0.000 min
Response: 17160054
Conc: 500.00 ng/ml

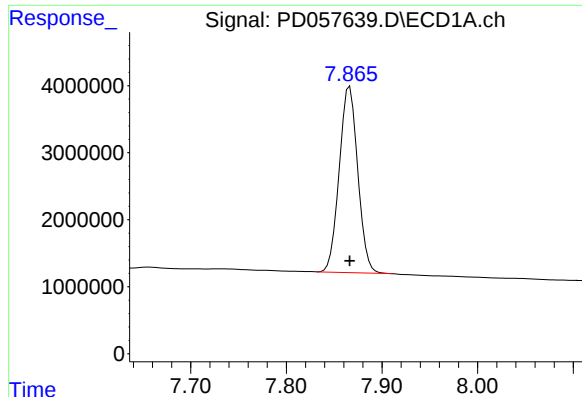

#28 Decachlorobiphenyl

R.T.: 7.866 min
Delta R.T.: 0.000 min
Response: 37419843
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

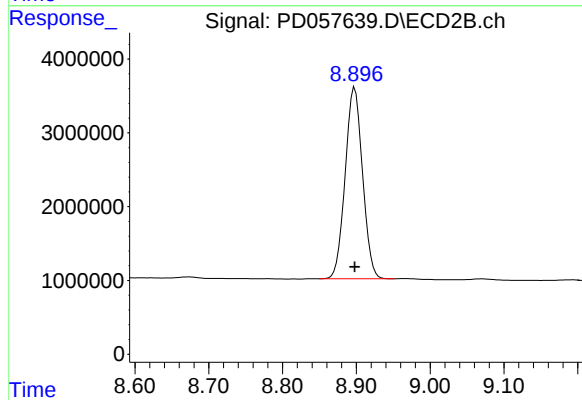

#28 Decachlorobiphenyl

R.T.: 8.898 min
Delta R.T.: 0.000 min
Response: 42375162
Conc: 50.00 ng/ml