

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032720\
 Data File : PD057650.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Mar 2020 15:16
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 28 04:12:47 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032720.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 27 14:08:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.231	3.895	15031265	17489659	21.053	22.293
28)	SA Decachlor...	7.873	8.901	17119640	20850412	22.485	23.706
Target Compounds							
7)	B delta-BHC	4.346	0.000	87026	0	0.084	N.D. #
8)	B Heptachlo...	4.870	5.728f	173661	1622673	0.205	1.619 #
9)	A Endosulfan I	0.000	6.098	0	3013621	N.D.	2.893 #
10)	B gamma-Chl...	0.000	5.965	0	3861910	N.D.	3.541 #
15)	B Endosulfa...	0.000	6.799f	0	778199	N.D.	0.770 #
23)	Chlordane-1	4.055	0.000	528358	0	21.227	N.D. #
25)	Chlordane-3	0.000	5.965	0	3861910	N.D.	26.509 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032720\
Data File : PD057650.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Mar 2020 15:16
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 28 04:12:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032720.M
Quant Title : GC Extractables
QLast Update : Fri Mar 27 14:08:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

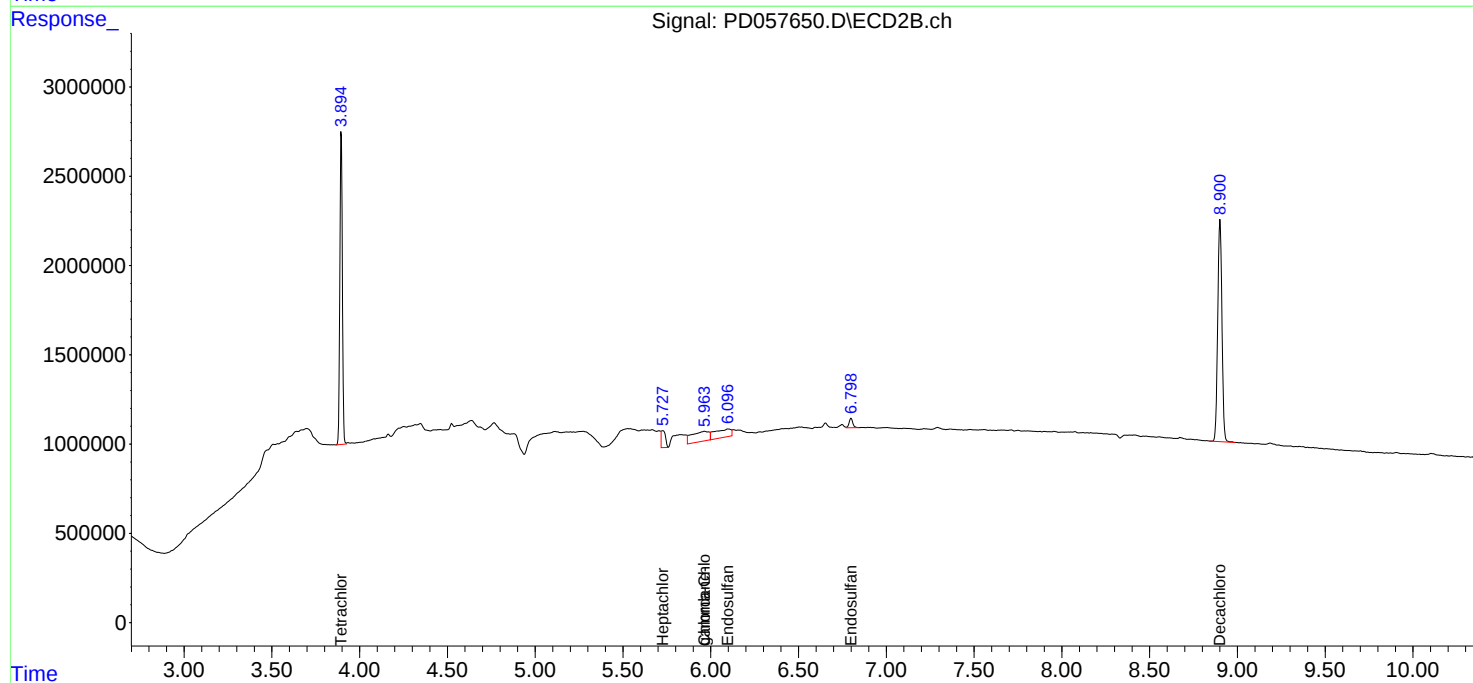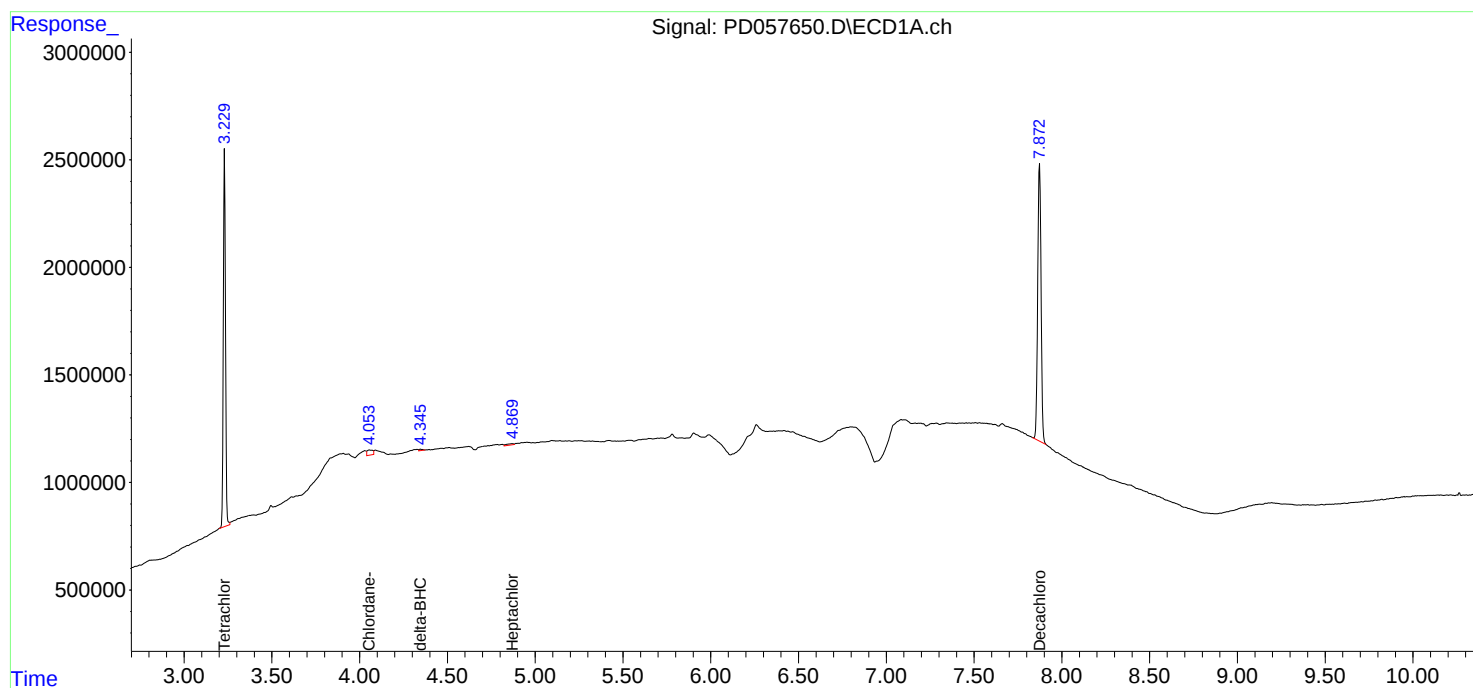


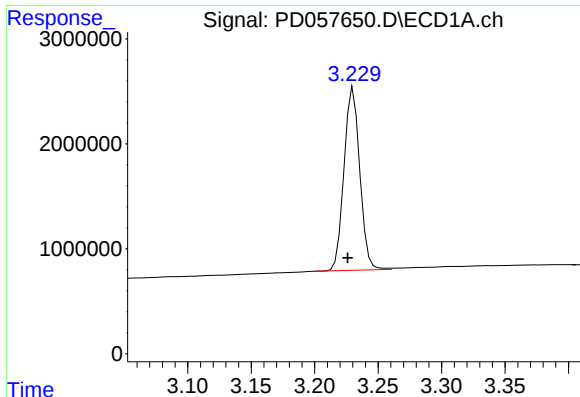

#1 Tetrachloro-m-xylene


R.T.: 3.231 min
Delta R.T.: 0.005 min
Response: 15031265
Conc: 21.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

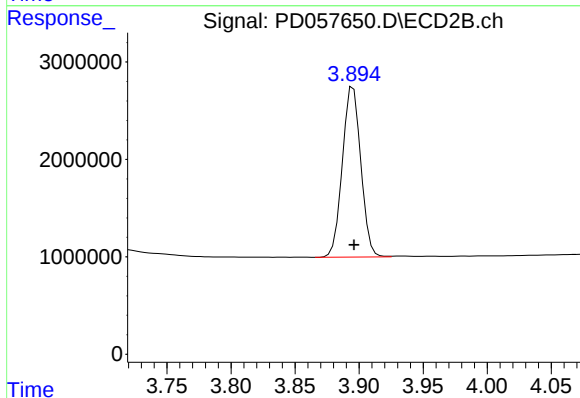


#1 Tetrachloro-m-xylene

R.T.: 3.895 min
Delta R.T.: 0.000 min
Response: 17489659
Conc: 22.29 ng/ml

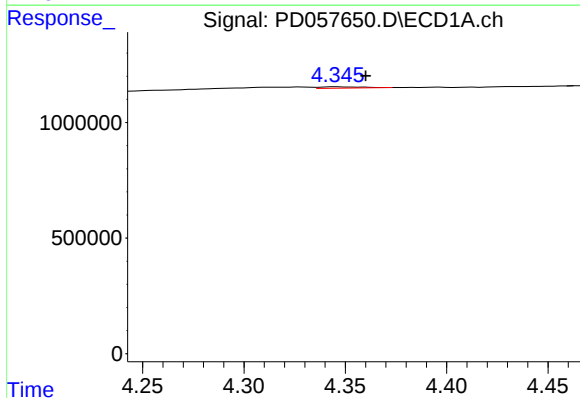


#7 delta-BHC

R.T.: 4.346 min
Delta R.T.: -0.014 min
Response: 87026
Conc: 0.08 ng/ml

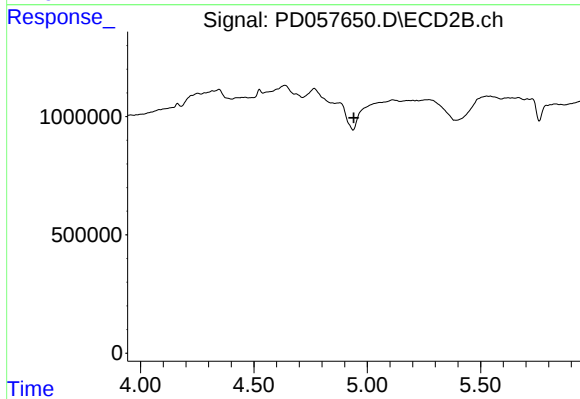

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.941 min
Response: 0
Conc: N.D.

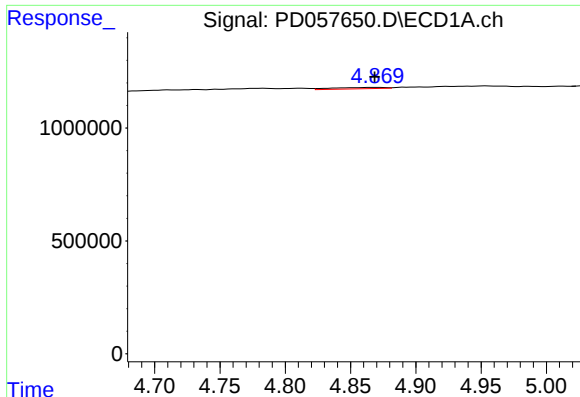

#8 Heptachlor epoxide


R.T.: 4.870 min
Delta R.T.: 0.001 min
Response: 173661
Conc: 0.20 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

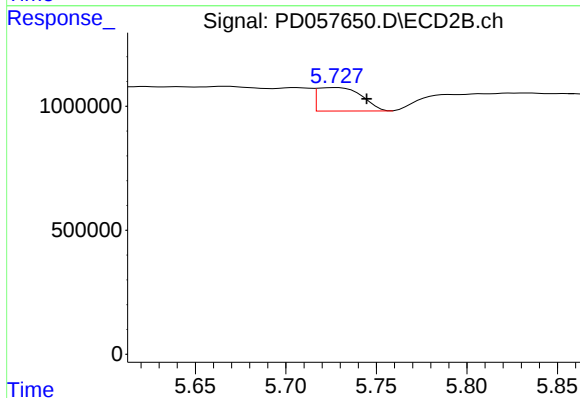


#8 Heptachlor epoxide

R.T.: 5.728 min
Delta R.T.: -0.017 min
Response: 1622673
Conc: 1.62 ng/ml

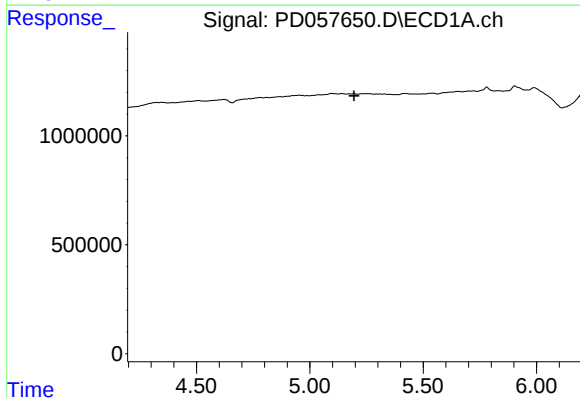


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.196 min
Response: 0
Conc: N.D.

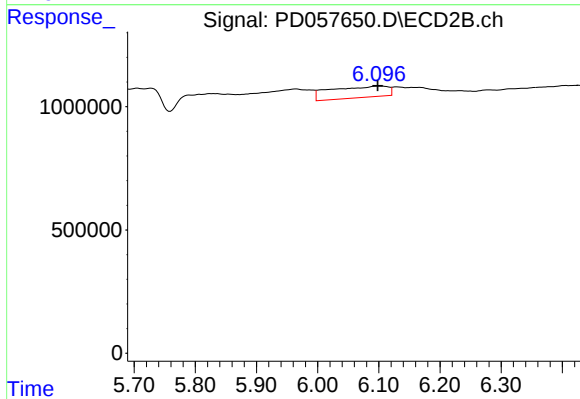

#9 Endosulfan I


R.T.: 6.098 min
Delta R.T.: 0.000 min
Response: 3013621
Conc: 2.89 ng/ml

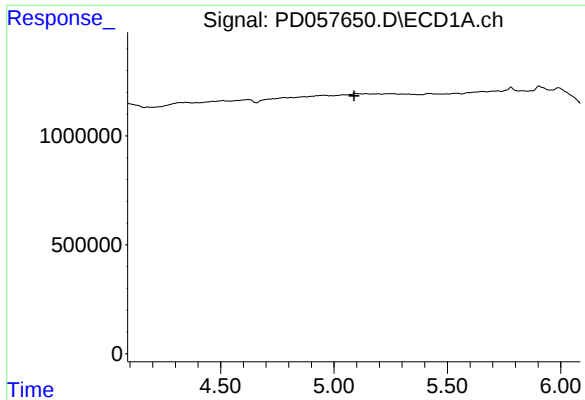

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.089 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

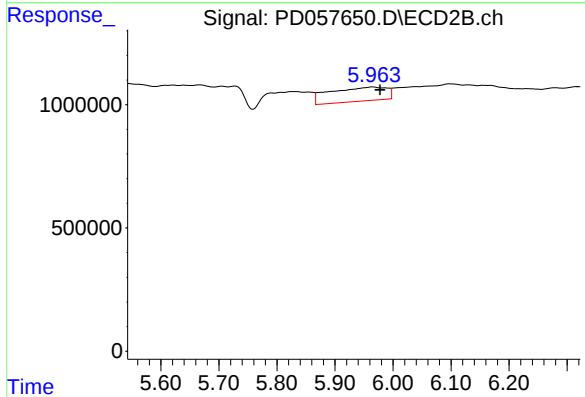


#10 gamma-Chlordane

R.T.: 5.965 min
Delta R.T.: -0.013 min
Response: 3861910
Conc: 3.54 ng/ml

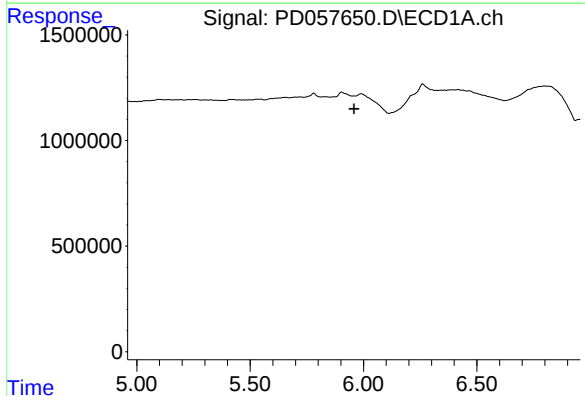


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 5.959 min
Response: 0
Conc: N.D.

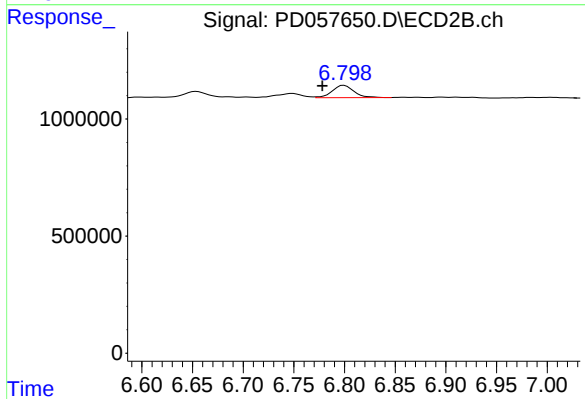

#15 Endosulfan II


R.T.: 6.799 min
Delta R.T.: 0.021 min
Response: 778199
Conc: 0.77 ng/ml

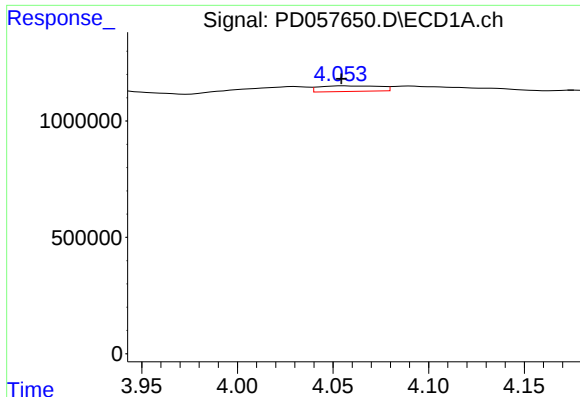

#23 Chlordane-1


R.T.: 4.055 min
Delta R.T.: 0.000 min
Response: 528358
Conc: 21.23 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

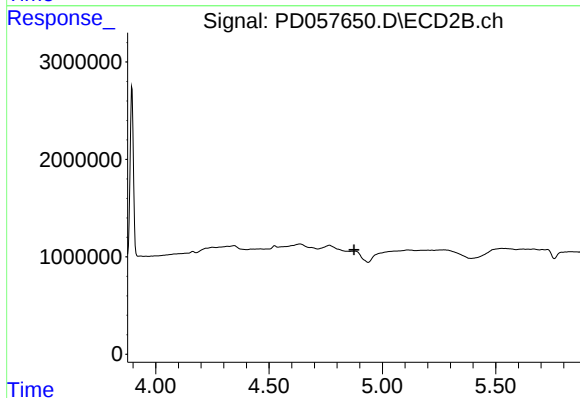


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.875 min
Response: 0
Conc: N.D.

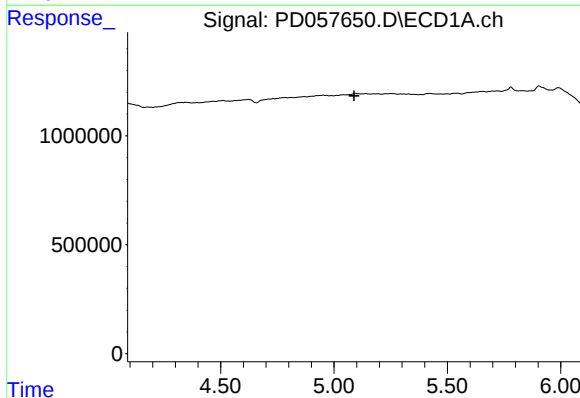


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.089 min
Response: 0
Conc: N.D.

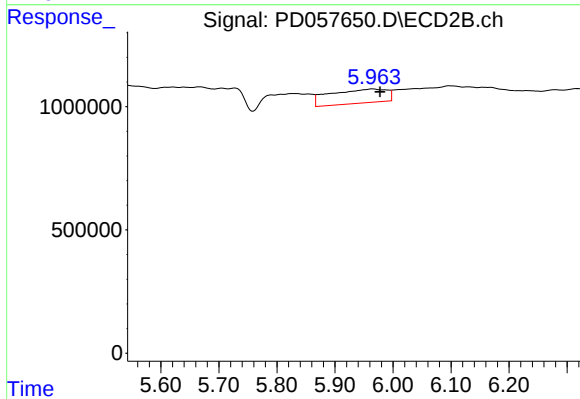

#25 Chlordane-3

R.T.: 5.965 min
Delta R.T.: -0.013 min
Response: 3861910
Conc: 26.51 ng/ml

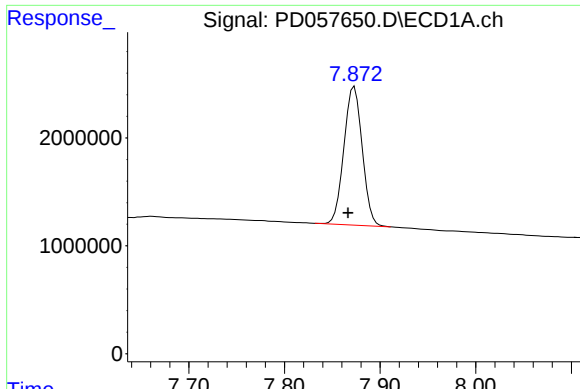

#28 Decachlorobiphenyl


R.T.: 7.873 min

Delta R.T.: 0.006 min

Response: 17119640

Conc: 22.48 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

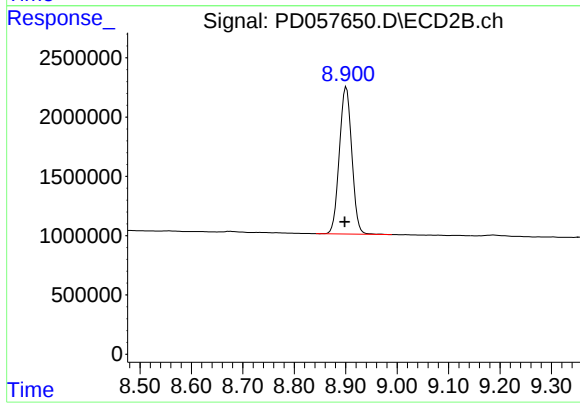

#28 Decachlorobiphenyl

R.T.: 8.901 min

Delta R.T.: 0.003 min

Response: 20850412

Conc: 23.71 ng/ml