

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032720\
 Data File : PD057655.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Mar 2020 16:30
 Operator : AJ\MA
 Sample : PB127349BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PB127349BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 28 04:13:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032720.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 27 14:08:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.230	3.896	14654158	17223012	20.524	21.953
28)	SA Decachlor...	7.872	8.901	16767310	20500767	22.022	23.309
Target Compounds							
2)	A alpha-BHC	3.641	0.000	113143	0	0.103	N.D. #
3)	MA gamma-BHC...	0.000	4.586f	0	101518	N.D.	0.088 #
4)	MA Heptachlor	0.000	5.063	0	4107659	N.D.	3.649 #
8)	B Heptachlo...	4.896f	0.000	133047	0	0.157	N.D. #
9)	A Endosulfan I	0.000	6.098	0	2877522	N.D.	2.763 #
10)	B gamma-Chl...	0.000	5.963	0	3105351	N.D.	2.848 #
13)	MA Dieldrin	0.000	6.367	0	60124	N.D.	0.057 #
14)	MA Endrin	5.710f	0.000	228853	0	0.315	N.D. #
15)	B Endosulfa...	0.000	6.800f	0	636989	N.D.	0.630 #
25)	Chlordane-3	0.000	5.963	0	3105351	N.D.	21.316 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032720\
Data File : PD057655.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Mar 2020 16:30
Operator : AJ\MA
Sample : PB127349BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PB127349BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 28 04:13:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032720.M
Quant Title : GC Extractables
QLast Update : Fri Mar 27 14:08:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

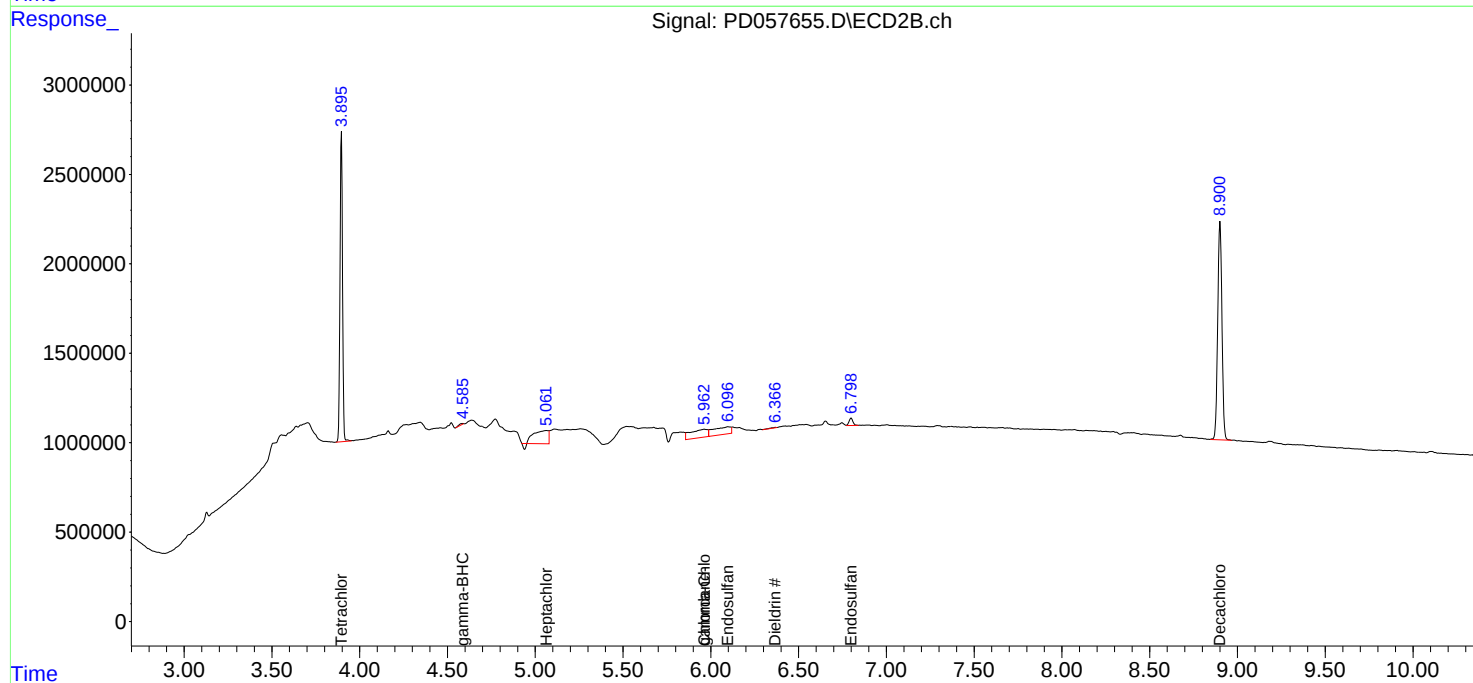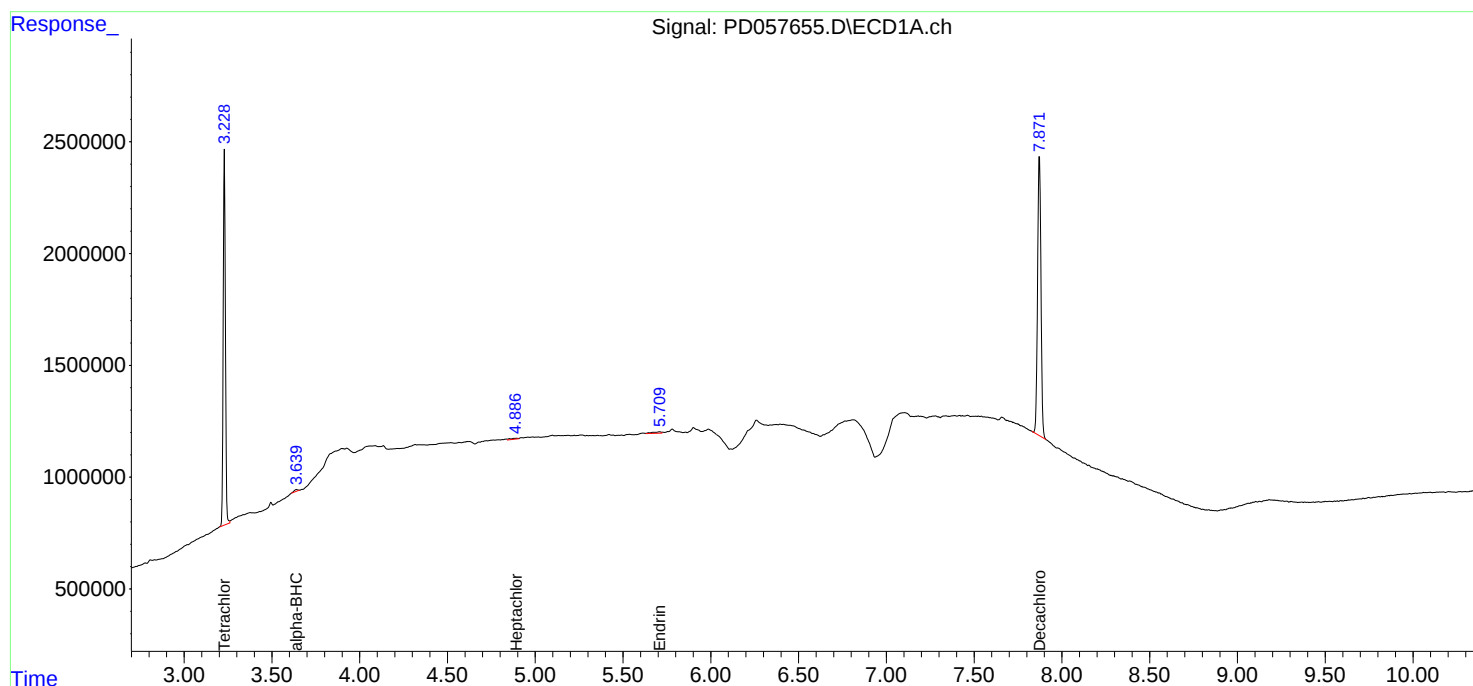


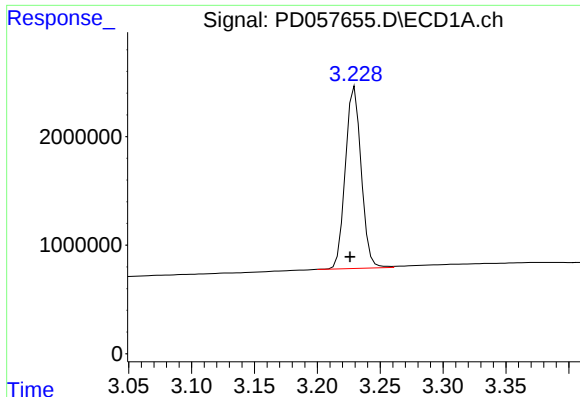

#1 Tetrachloro-m-xylene


R.T.: 3.230 min
Delta R.T.: 0.004 min
Response: 14654158
Conc: 20.52 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB127349BL

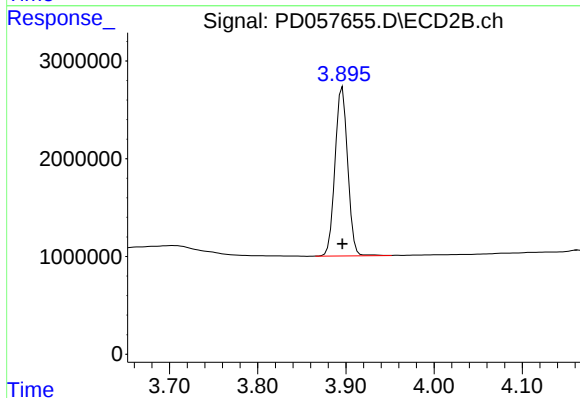


#1 Tetrachloro-m-xylene

R.T.: 3.896 min
Delta R.T.: 0.000 min
Response: 17223012
Conc: 21.95 ng/ml

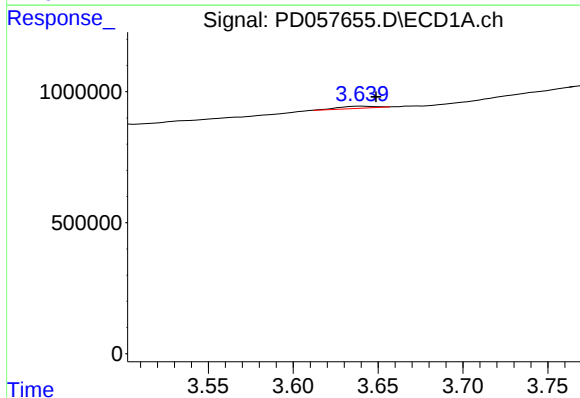


#2 alpha-BHC

R.T.: 3.641 min
Delta R.T.: -0.008 min
Response: 113143
Conc: 0.10 ng/ml

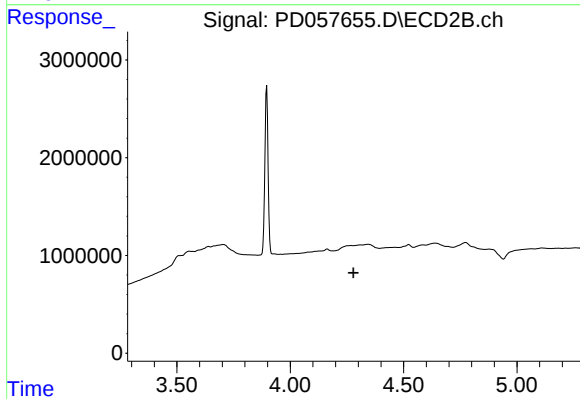

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.279 min
Response: 0
Conc: N.D.

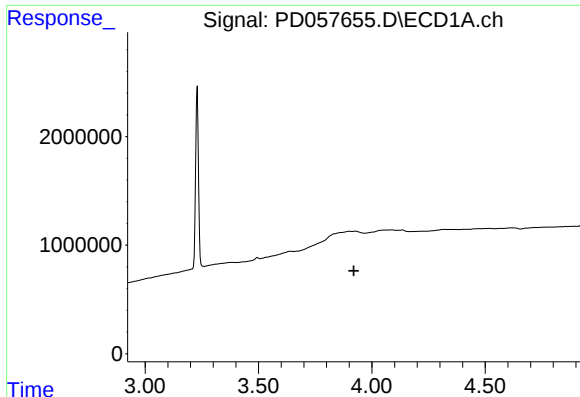

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 3.920 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB127349BL

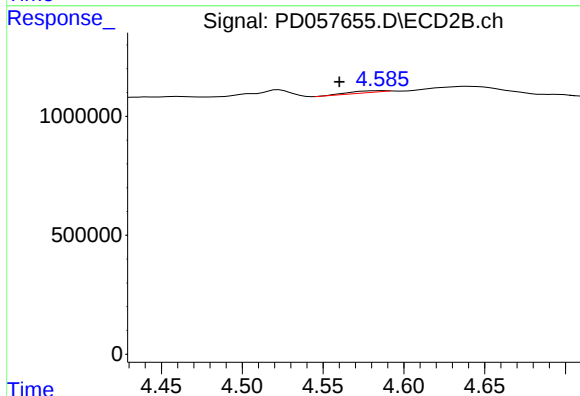


#3 gamma-BHC (Lindane)

R.T.: 4.586 min
Delta R.T.: 0.026 min
Response: 101518
Conc: 0.09 ng/ml

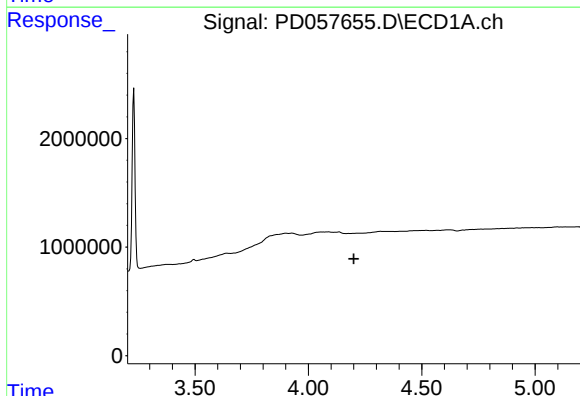


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.201 min
Response: 0
Conc: N.D.

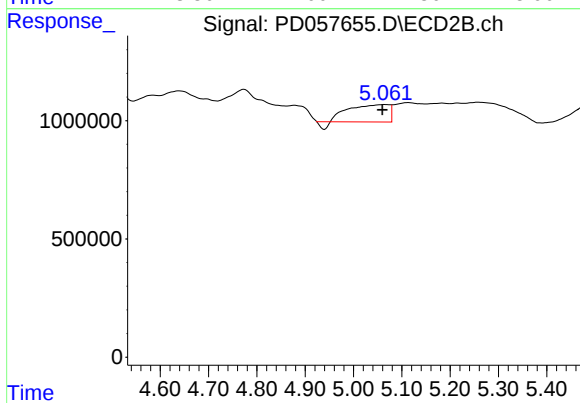

#4 Heptachlor


R.T.: 5.063 min
Delta R.T.: 0.003 min
Response: 4107659
Conc: 3.65 ng/ml

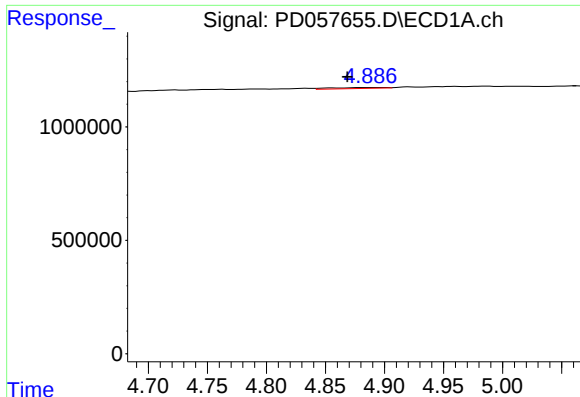

#8 Heptachlor epoxide


R.T.: 4.896 min
Delta R.T.: 0.027 min
Response: 133047
Conc: 0.16 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB127349BL

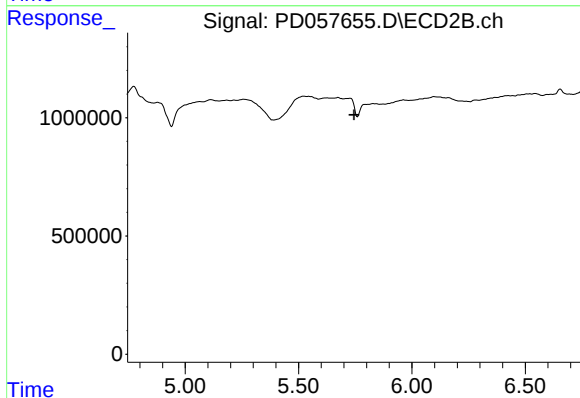


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.745 min
Response: 0
Conc: N.D.

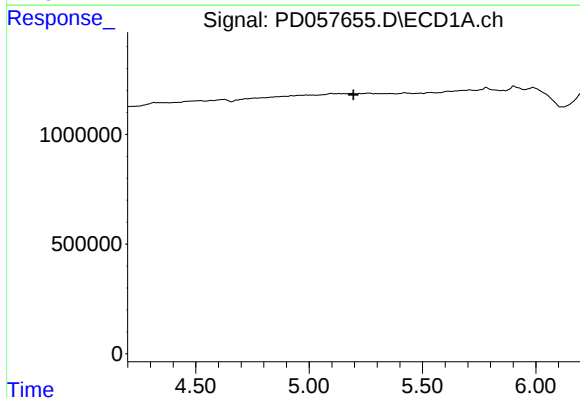


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.196 min
Response: 0
Conc: N.D.

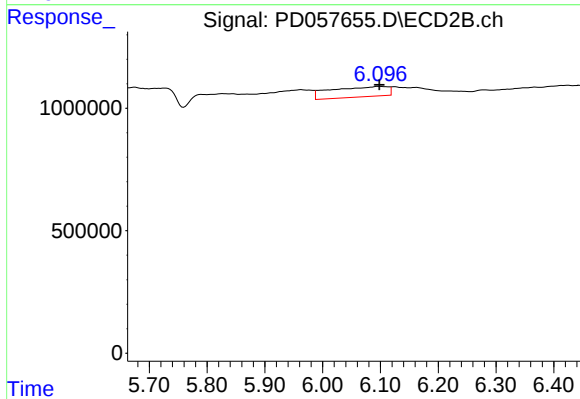

#9 Endosulfan I


R.T.: 6.098 min
Delta R.T.: 0.000 min
Response: 2877522
Conc: 2.76 ng/ml

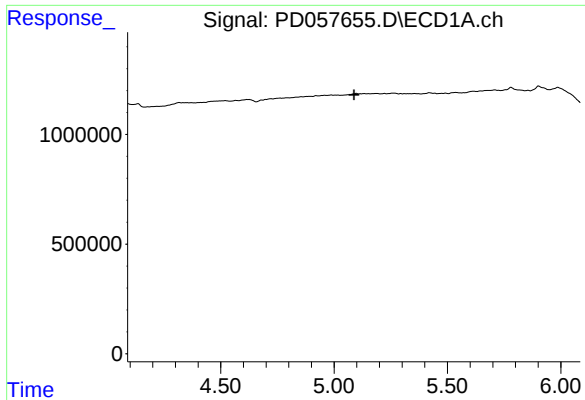

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.089 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB127349BL

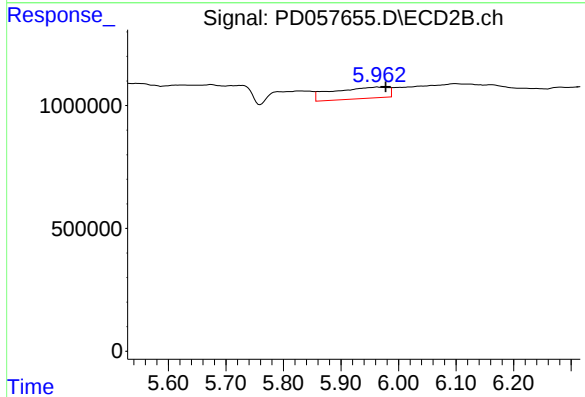


#10 gamma-Chlordane

R.T.: 5.963 min
Delta R.T.: -0.015 min
Response: 3105351
Conc: 2.85 ng/ml

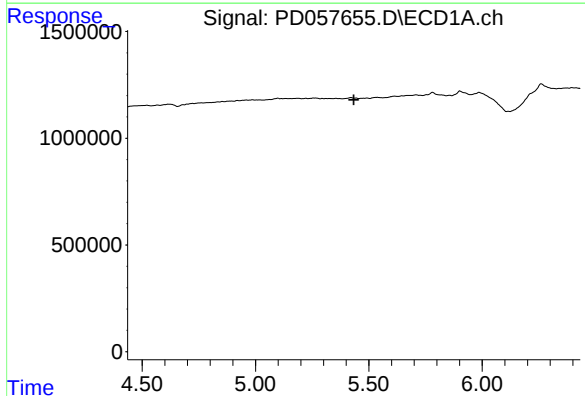


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 5.434 min
Response: 0
Conc: N.D.

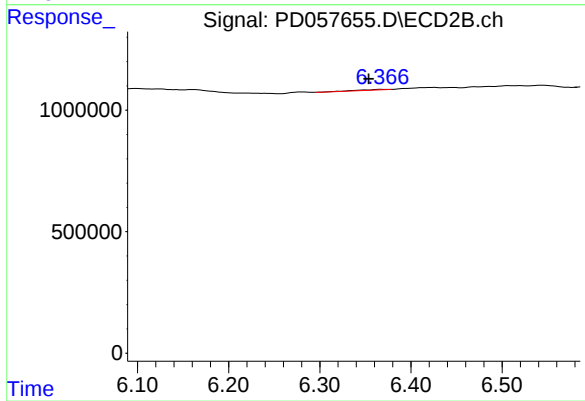

#13 Dieldrin


R.T.: 6.367 min
Delta R.T.: 0.014 min
Response: 60124
Conc: 0.06 ng/ml

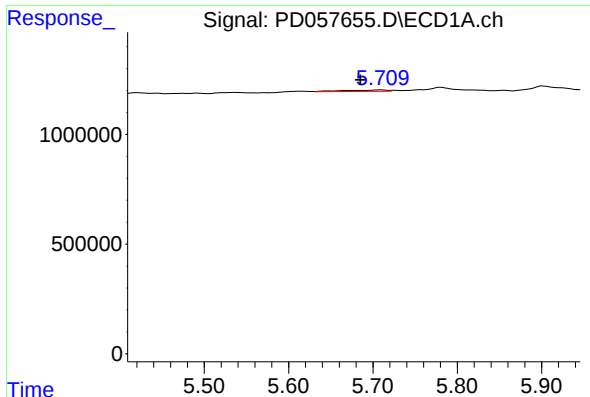

#14 Endrin


R.T.: 5.710 min
Delta R.T.: 0.025 min
Response: 228853
Conc: 0.31 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB127349BL

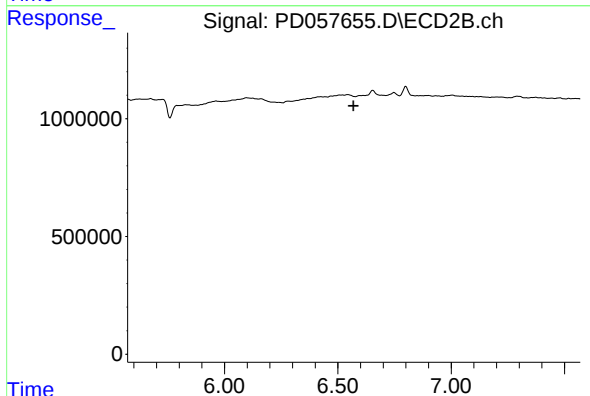


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.569 min
Response: 0
Conc: N.D.

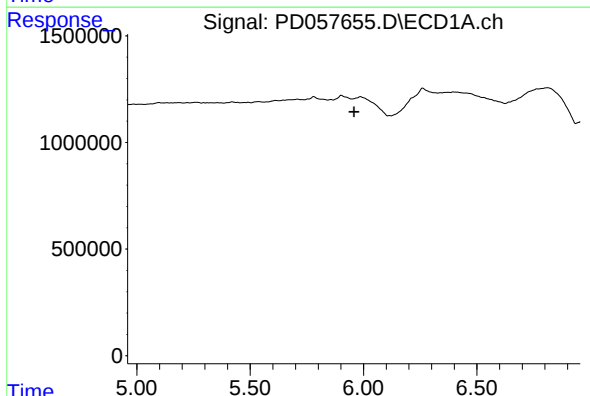


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.959 min
Response: 0
Conc: N.D.

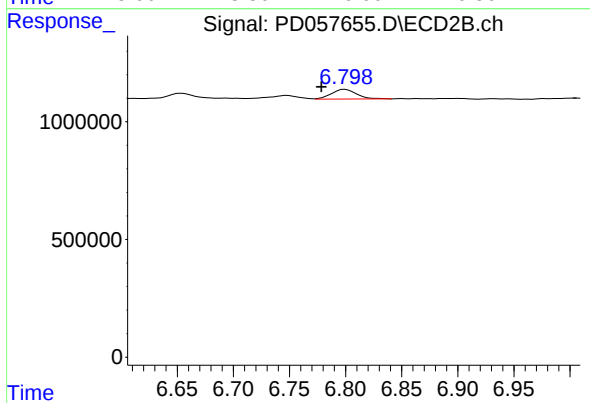

#15 Endosulfan II


R.T.: 6.800 min
Delta R.T.: 0.021 min
Response: 636989
Conc: 0.63 ng/ml

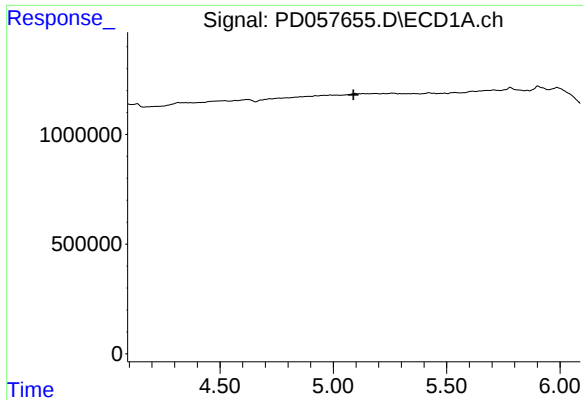

#25 Chlorine-3


R.T.: 0.000 min
Exp R.T.: 5.089 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB127349BL

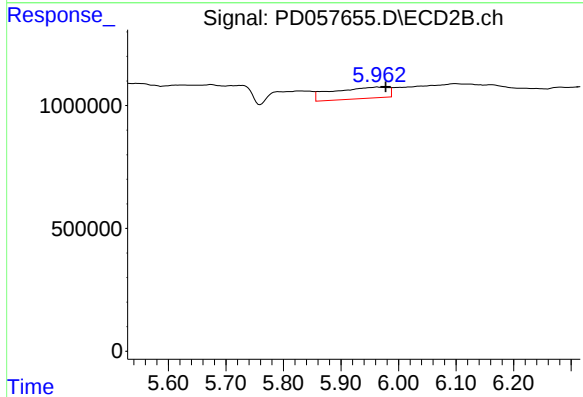


#25 Chlorine-3

R.T.: 5.963 min
Delta R.T.: -0.014 min
Response: 3105351
Conc: 21.32 ng/ml

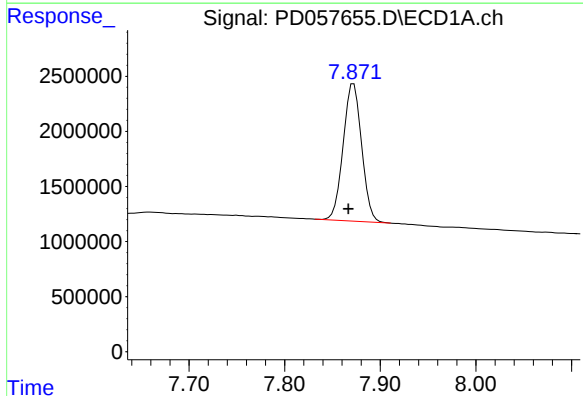

#28 Decachlorobiphenyl

R.T.: 7.872 min
Delta R.T.: 0.006 min
Response: 16767310
Conc: 22.02 ng/ml

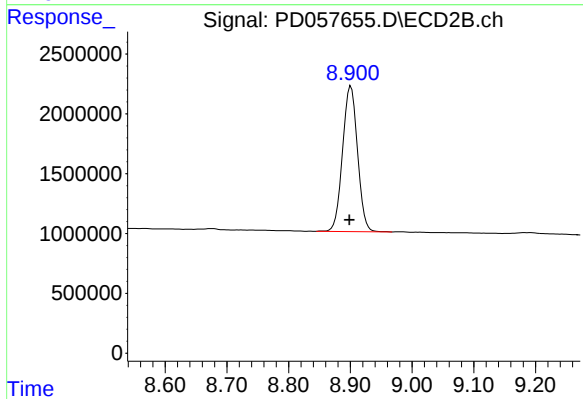

#28 Decachlorobiphenyl

R.T.: 8.901 min
Delta R.T.: 0.003 min
Response: 20500767
Conc: 23.31 ng/ml