

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032720\
 Data File : PD057664.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Mar 2020 18:36
 Operator : AJ\MA
 Sample : PB127350BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PB127350BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 28 04:15:15 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032720.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 27 14:08:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.227	3.897	15278932	18046804	21.400	23.003
28)	SA Decachlor...	7.866	8.898	17521265	21684417	23.012	24.655
Target Compounds							
3)	MA gamma-BHC...	3.932	0.000	1125836	0	1.046	N.D. #
8)	B Heptachlo...	0.000	5.737	0	1730136	N.D.	1.726 #
9)	A Endosulfan I	0.000	6.100	0	806558	N.D.	0.774 #
10)	B gamma-Chl...	5.111f	5.973	67321	1864971	0.073	1.710 #
11)	B alpha-Chl...	0.000	6.057	0	1170904	N.D.	1.057 #
14)	MA Endrin	5.705f	0.000	333317	0	0.459	N.D. #
15)	B Endosulfa...	0.000	6.800f	0	385270	N.D.	0.381 #
24)	Chlordane-2	4.518f	0.000	215100	0	7.503	N.D. #
25)	Chlordane-3	5.111f	5.973	67321	1864971	0.767	12.801 #
26)	Chlordane-4	0.000	6.057	0	1170904	N.D.	6.625 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032720\
Data File : PD057664.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Mar 2020 18:36
Operator : AJ\MA
Sample : PB127350BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PB127350BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 28 04:15:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032720.M
Quant Title : GC Extractables
QLast Update : Fri Mar 27 14:08:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

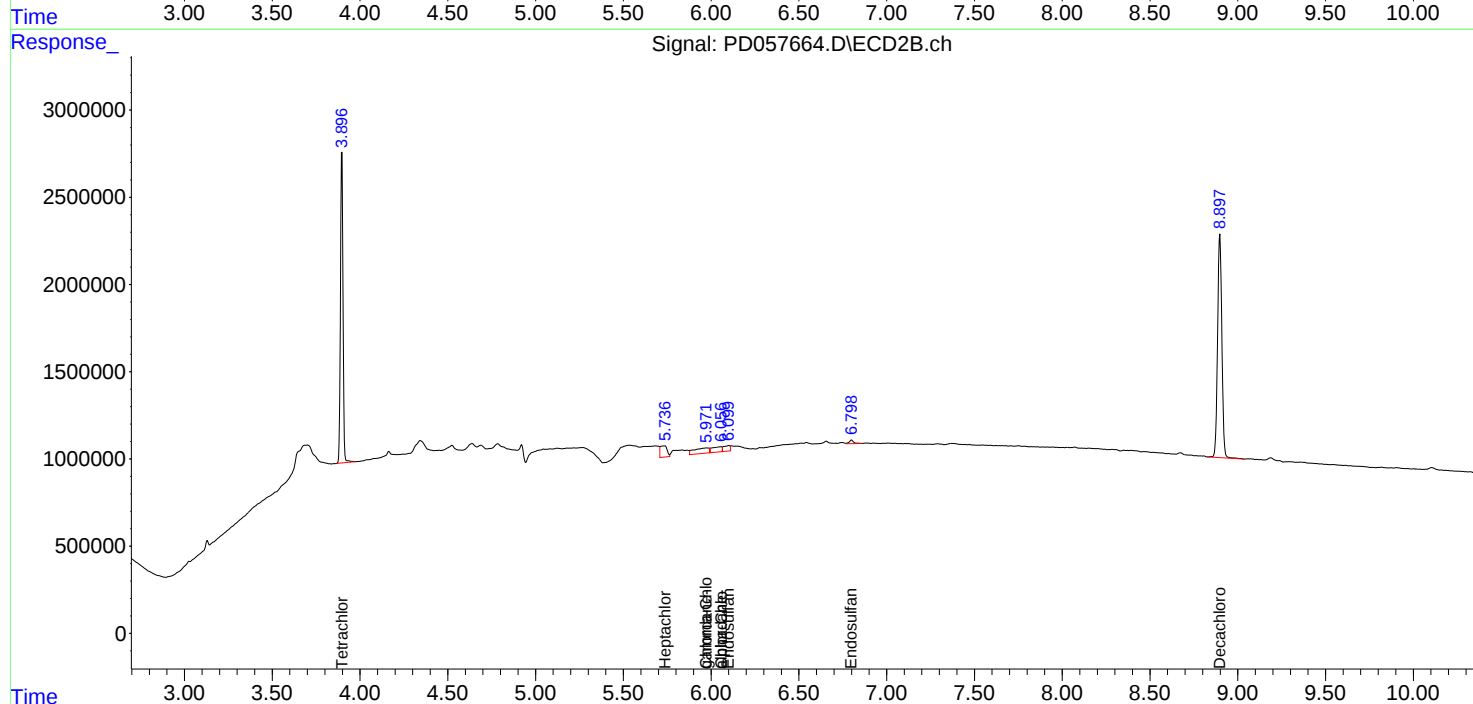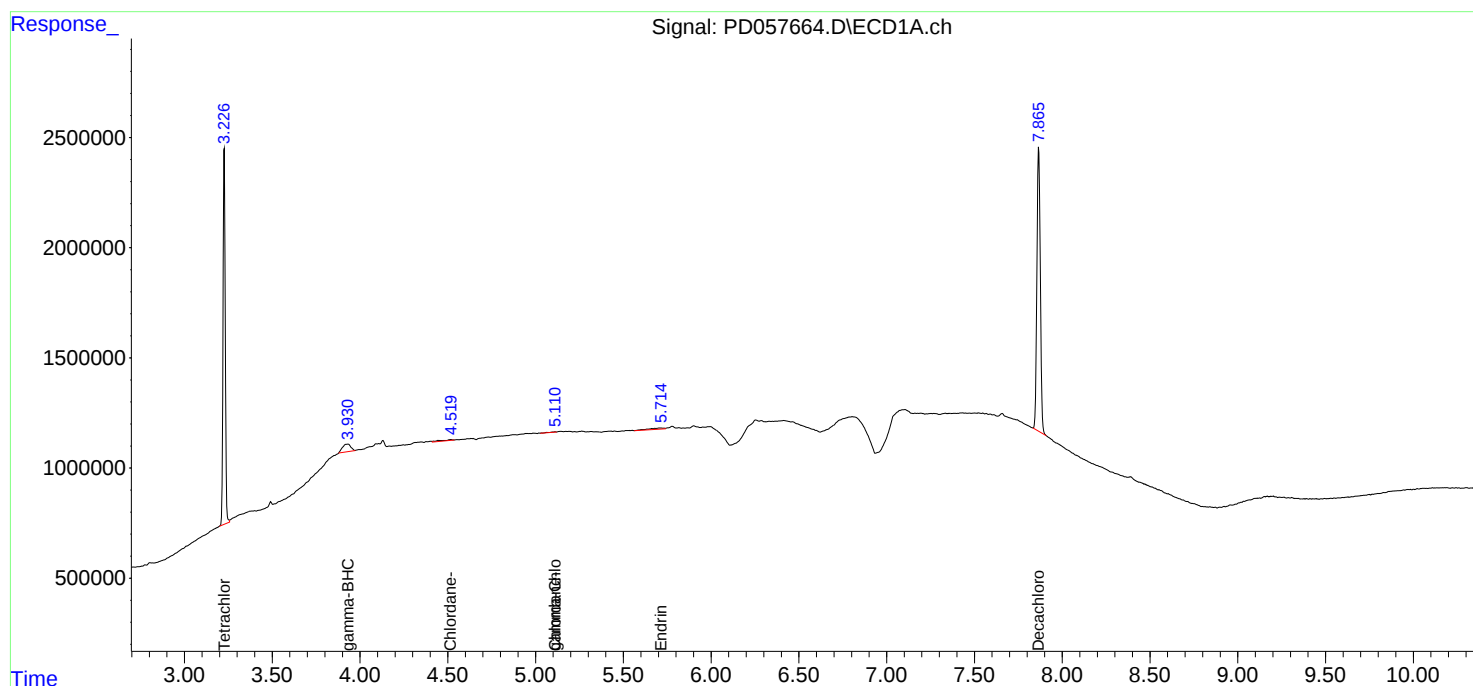


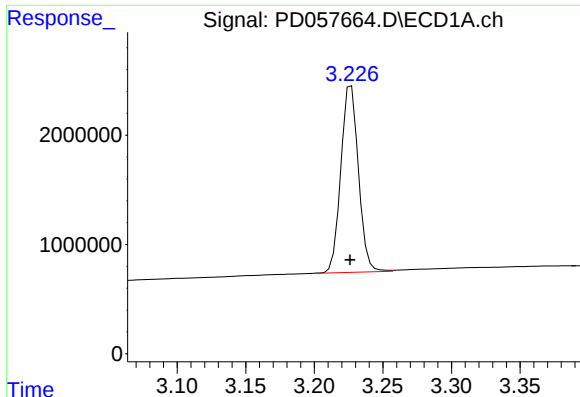

#1 Tetrachloro-m-xylene


R.T.: 3.227 min
Delta R.T.: 0.000 min
Response: 15278932
Conc: 21.40 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB127350BL

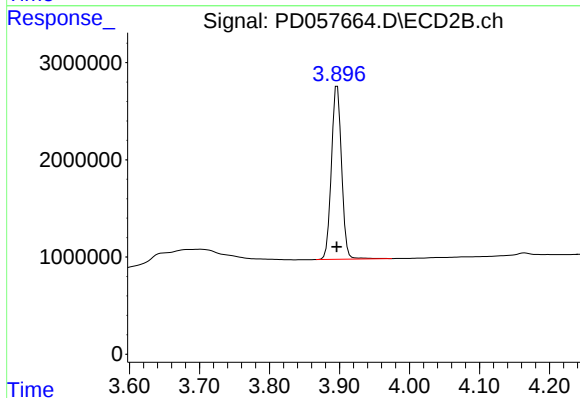


#1 Tetrachloro-m-xylene

R.T.: 3.897 min
Delta R.T.: 0.000 min
Response: 18046804
Conc: 23.00 ng/ml

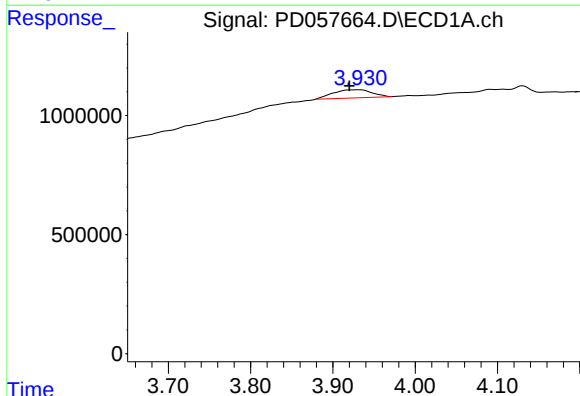


#3 gamma-BHC (Lindane)

R.T.: 3.932 min
Delta R.T.: 0.011 min
Response: 1125836
Conc: 1.05 ng/ml

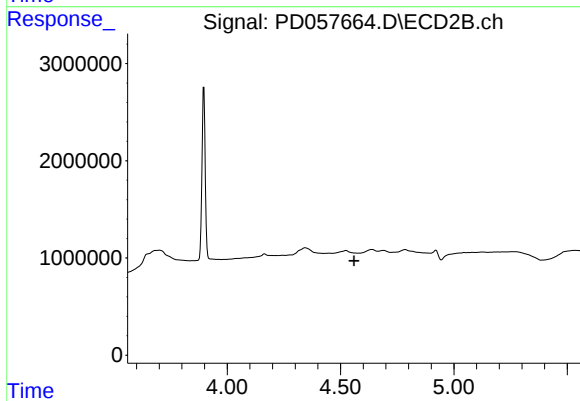

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.560 min
Response: 0
Conc: N.D.

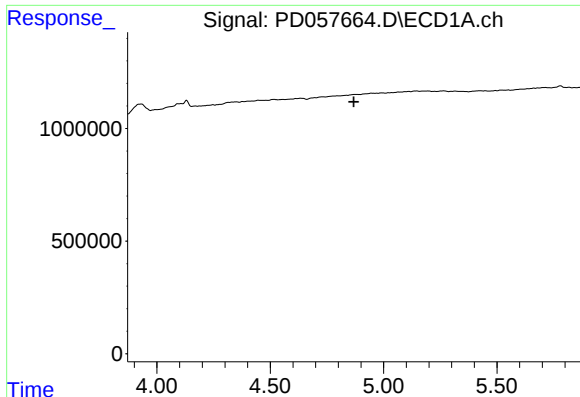

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.869 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB127350BL

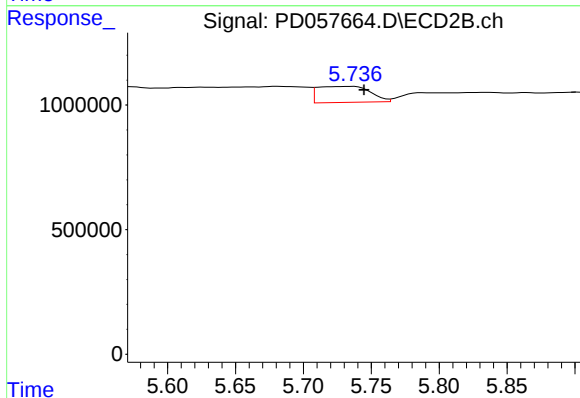


#8 Heptachlor epoxide

R.T.: 5.737 min
Delta R.T.: -0.008 min
Response: 1730136
Conc: 1.73 ng/ml

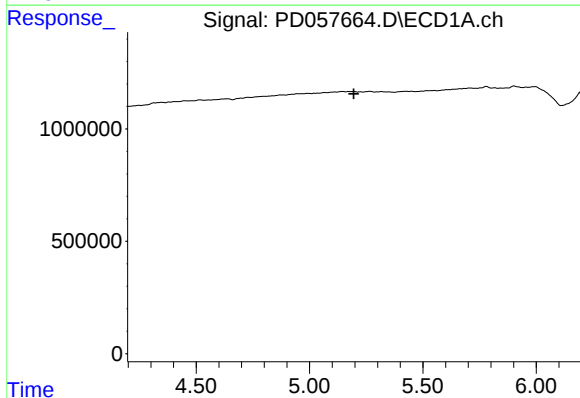


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.196 min
Response: 0
Conc: N.D.

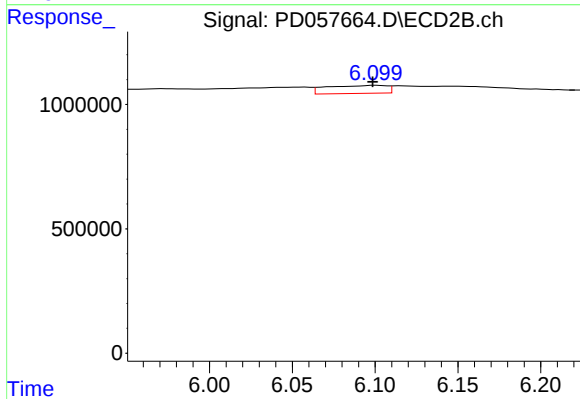

#9 Endosulfan I


R.T.: 6.100 min
Delta R.T.: 0.002 min
Response: 806558
Conc: 0.77 ng/ml

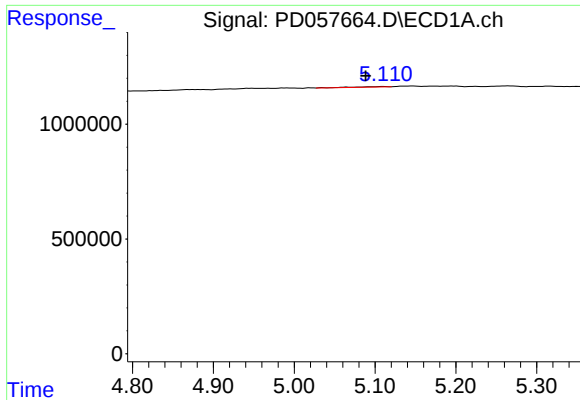

#10 gamma-Chlordane


R.T.: 5.111 min
Delta R.T.: 0.023 min
Response: 67321
Conc: 0.07 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB127350BL

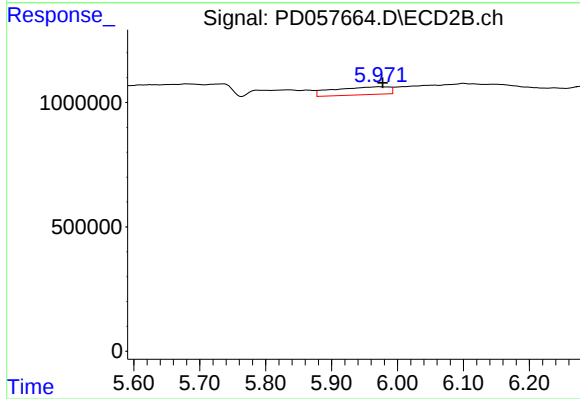


#10 gamma-Chlordane

R.T.: 5.973 min
Delta R.T.: -0.005 min
Response: 1864971
Conc: 1.71 ng/ml

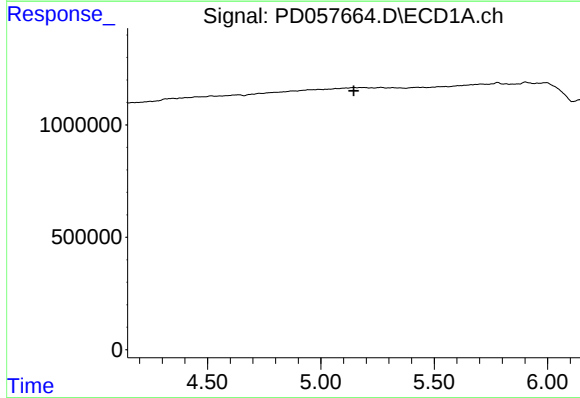


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.145 min
Response: 0
Conc: N.D.

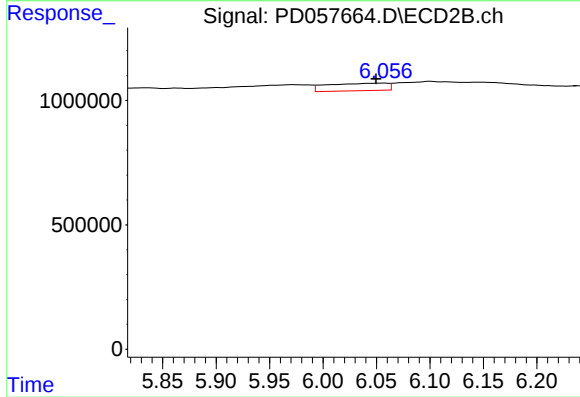

#11 alpha-Chlordane


R.T.: 6.057 min
Delta R.T.: 0.008 min
Response: 1170904
Conc: 1.06 ng/ml

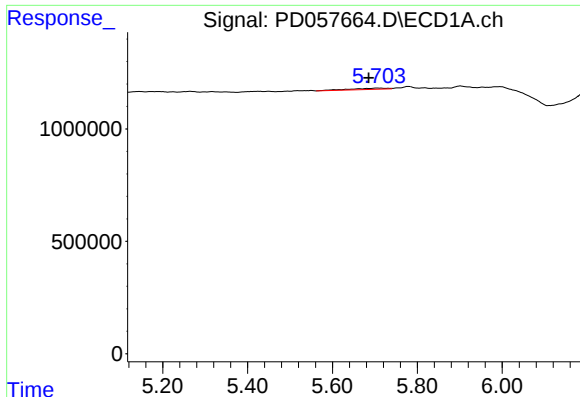

#14 Endrin


R.T.: 5.705 min
Delta R.T.: 0.019 min
Response: 333317
Conc: 0.46 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB127350BL

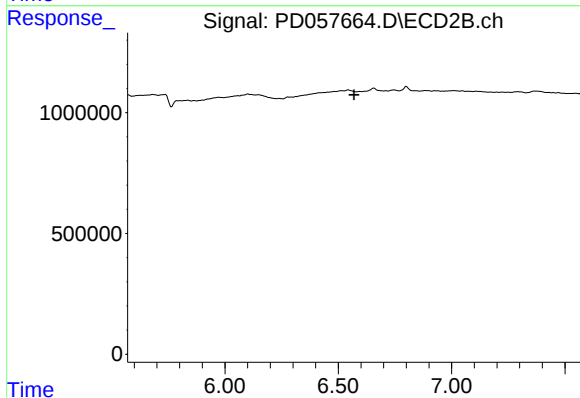


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.569 min
Response: 0
Conc: N.D.

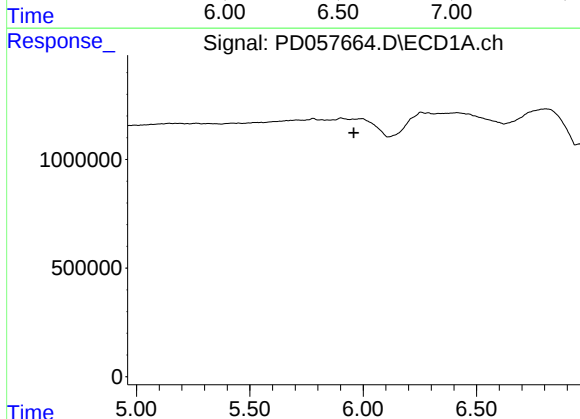


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.959 min
Response: 0
Conc: N.D.

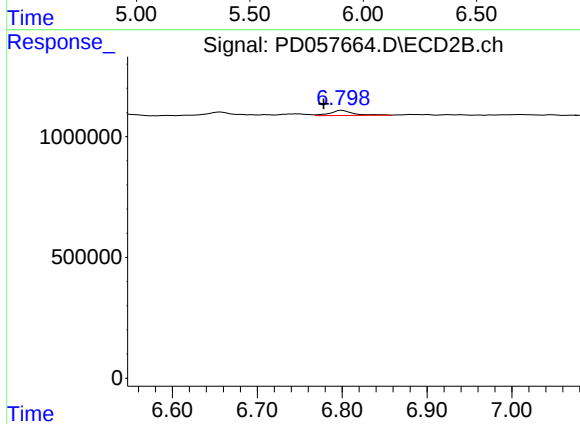

#15 Endosulfan II


R.T.: 6.800 min
Delta R.T.: 0.021 min
Response: 385270
Conc: 0.38 ng/ml

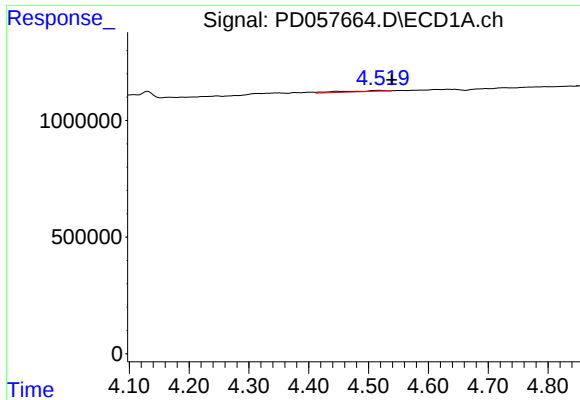

#24 Chlordane-2


R.T.: 4.518 min
Delta R.T.: -0.021 min
Response: 215100
Conc: 7.50 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB127350BL

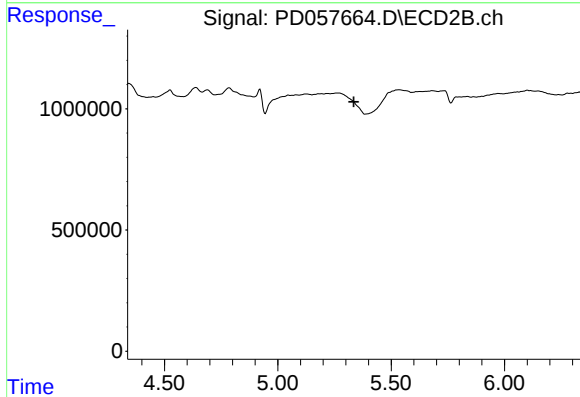


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.335 min
Response: 0
Conc: N.D.

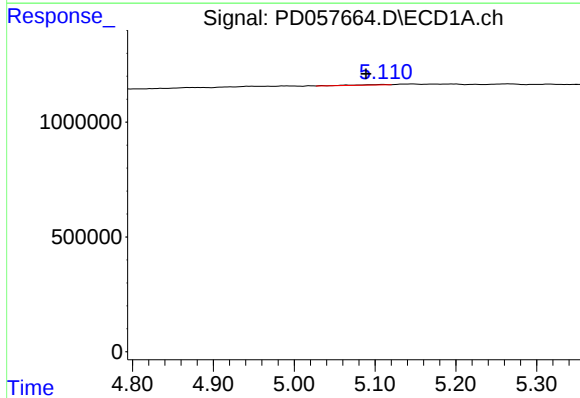


#25 Chlordane-3

R.T.: 5.111 min
Delta R.T.: 0.022 min
Response: 67321
Conc: 0.77 ng/ml

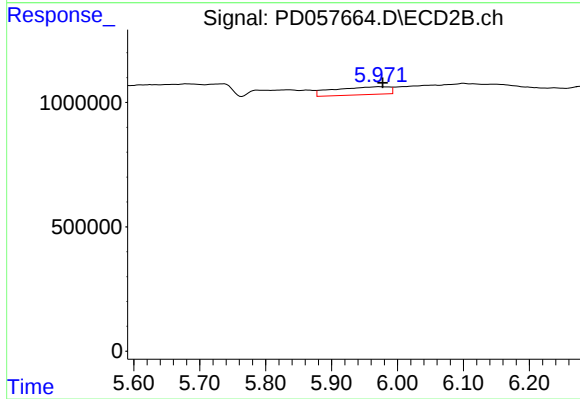

#25 Chlordane-3


R.T.: 5.973 min
Delta R.T.: -0.005 min
Response: 1864971
Conc: 12.80 ng/ml

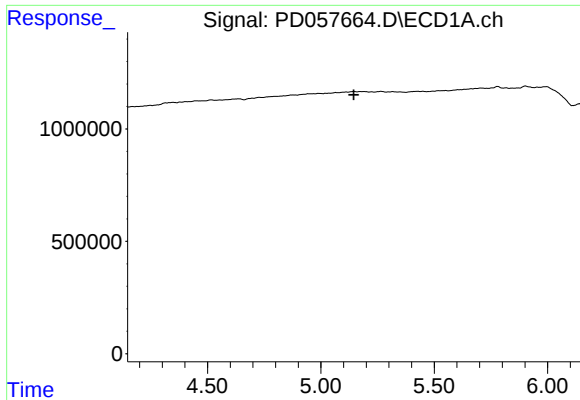

#26 Chlorodane-4


R.T.: 0.000 min
Exp R.T.: 5.145 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB127350BL

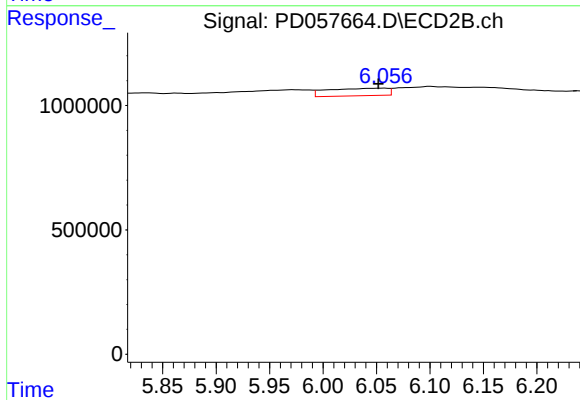


#26 Chlorodane-4

R.T.: 6.057 min
Delta R.T.: 0.005 min
Response: 1170904
Conc: 6.63 ng/ml

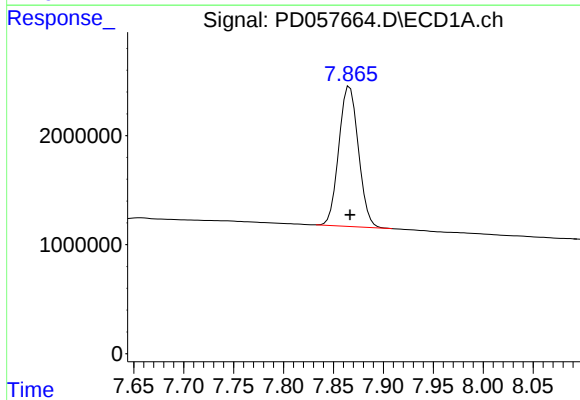

#28 Decachlorobiphenyl

R.T.: 7.866 min
Delta R.T.: 0.000 min
Response: 17521265
Conc: 23.01 ng/ml

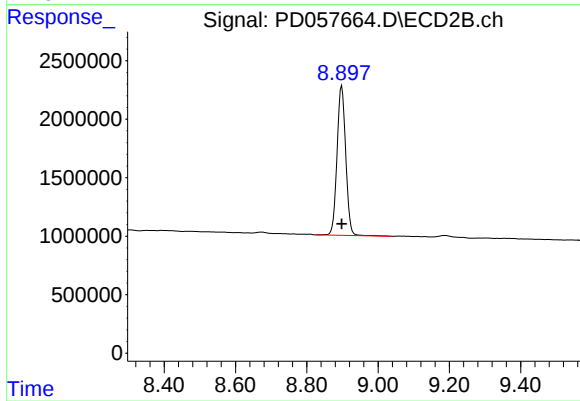

#28 Decachlorobiphenyl

R.T.: 8.898 min
Delta R.T.: 0.000 min
Response: 21684417
Conc: 24.65 ng/ml