

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032720\
 Data File : PD057668.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Mar 2020 19:32
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 28 04:15:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032720.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 27 14:08:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.227	3.897	15355200	18322157	21.506	23.354
28)	SA Decachlor...	7.867	8.899	17399111	21614884	22.852	24.575
Target Compounds							
3)	MA gamma-BHC...	3.926	0.000	1113271	0	1.034	N.D. #
4)	MA Heptachlor	0.000	5.078f	0	136154	N.D.	0.121 #
5)	MB Aldrin	4.451f	0.000	149480	0	0.152	N.D. #
8)	B Heptachlo...	4.852f	5.737	64628	1005613	0.076	1.003 #
9)	A Endosulfan I	0.000	6.101	0	1790251	N.D.	1.719 #
10)	B gamma-Chl...	5.108f	0.000	97242	0	0.106	N.D. #
15)	B Endosulfa...	0.000	6.799f	0	307756	N.D.	0.304 #
25)	Chlordane-3	5.108f	0.000	97242	0	1.108	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032720\
Data File : PD057668.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Mar 2020 19:32
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 28 04:15:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032720.M
Quant Title : GC Extractables
QLast Update : Fri Mar 27 14:08:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

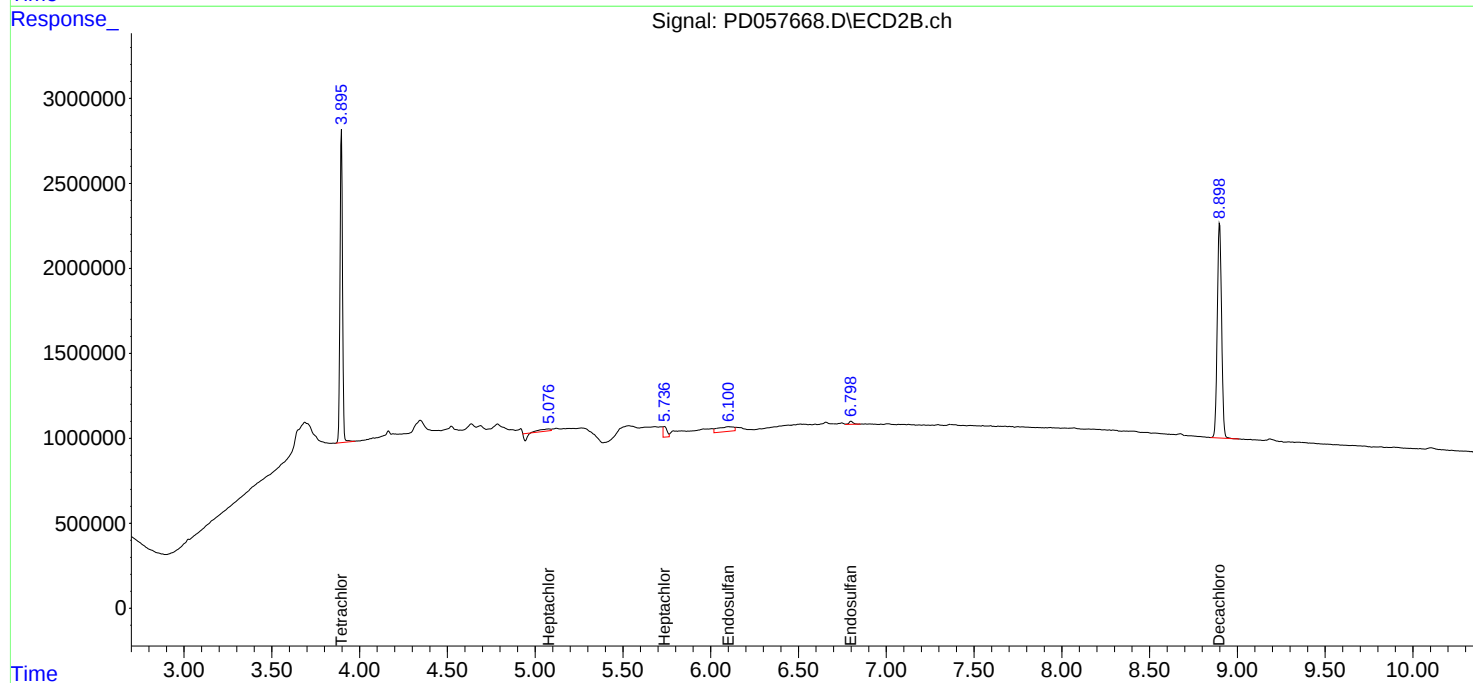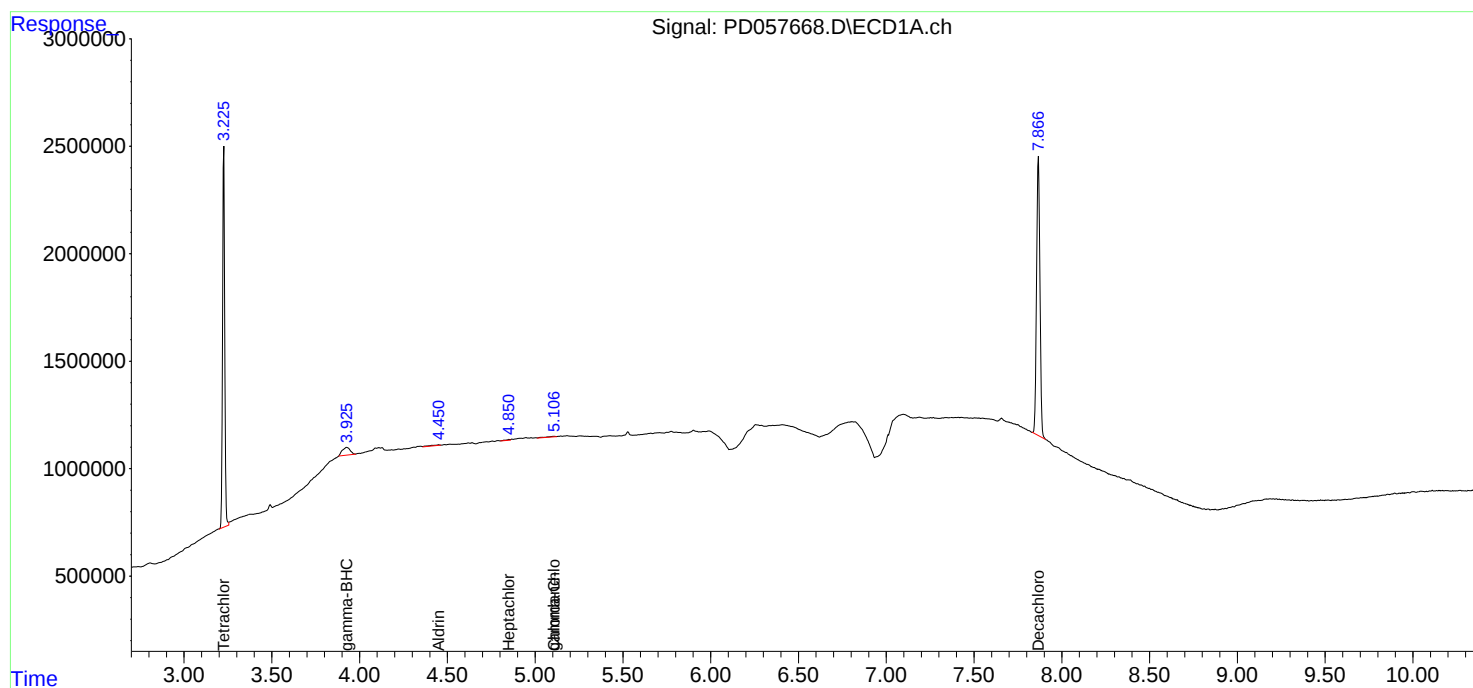


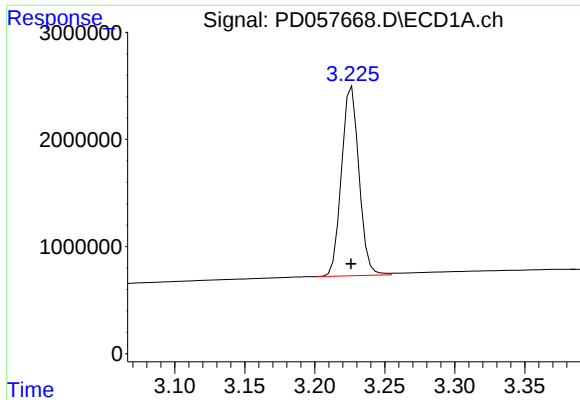

#1 Tetrachloro-m-xylene


R.T.: 3.227 min
Delta R.T.: 0.000 min
Response: 15355200
Conc: 21.51 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

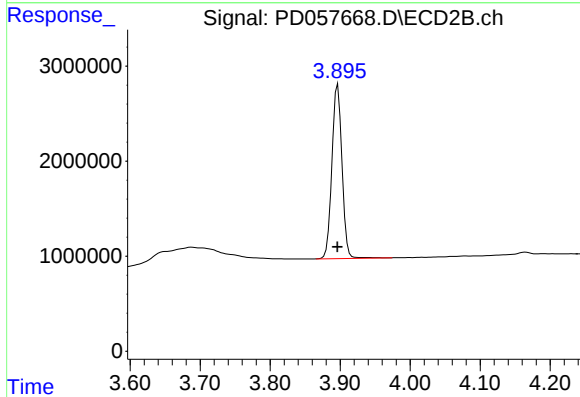


#1 Tetrachloro-m-xylene

R.T.: 3.897 min
Delta R.T.: 0.000 min
Response: 18322157
Conc: 23.35 ng/ml

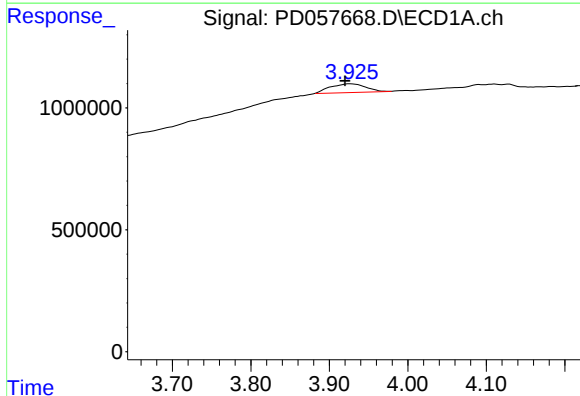


#3 gamma-BHC (Lindane)

R.T.: 3.926 min
Delta R.T.: 0.006 min
Response: 1113271
Conc: 1.03 ng/ml

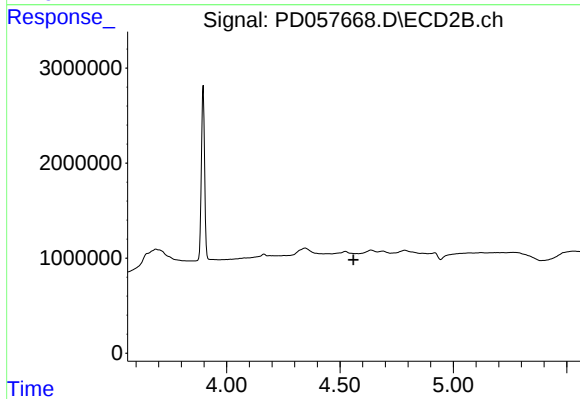

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.560 min
Response: 0
Conc: N.D.

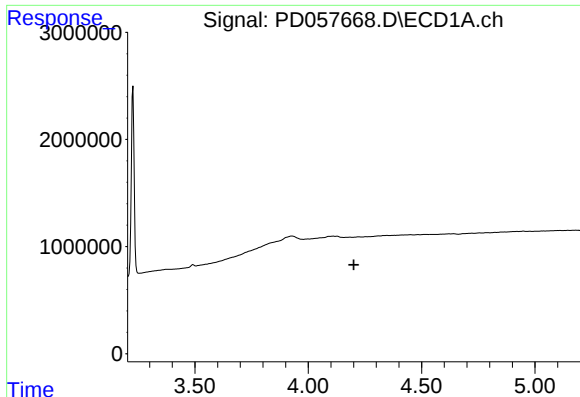

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.201 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

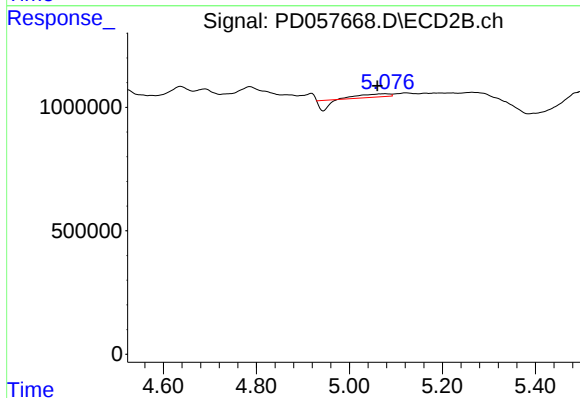


#4 Heptachlor

R.T.: 5.078 min
Delta R.T.: 0.018 min
Response: 136154
Conc: 0.12 ng/ml

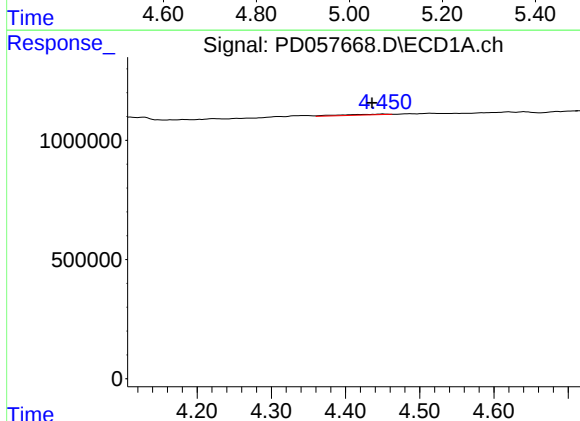


#5 Aldrin

R.T.: 4.451 min
Delta R.T.: 0.015 min
Response: 149480
Conc: 0.15 ng/ml

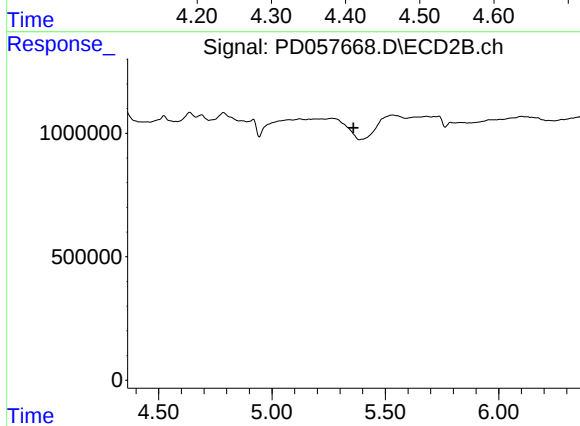

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.360 min
Response: 0
Conc: N.D.

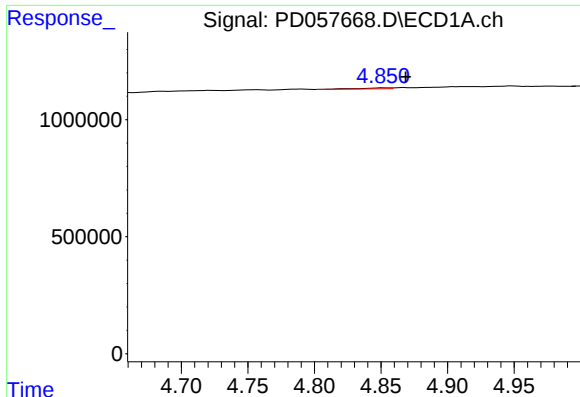

#8 Heptachlor epoxide


R.T.: 4.852 min
Delta R.T.: -0.017 min
Response: 64628
Conc: 0.08 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

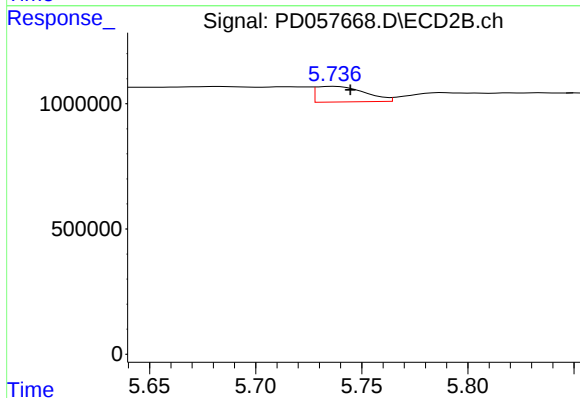


#8 Heptachlor epoxide

R.T.: 5.737 min
Delta R.T.: -0.007 min
Response: 1005613
Conc: 1.00 ng/ml

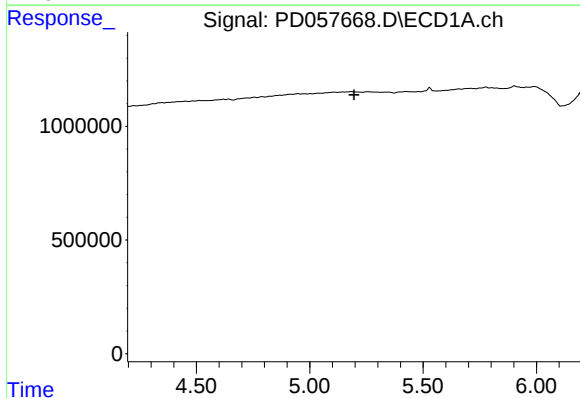


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.196 min
Response: 0
Conc: N.D.

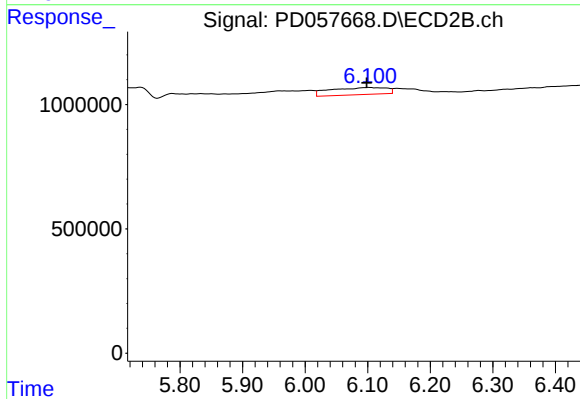

#9 Endosulfan I


R.T.: 6.101 min
Delta R.T.: 0.003 min
Response: 1790251
Conc: 1.72 ng/ml

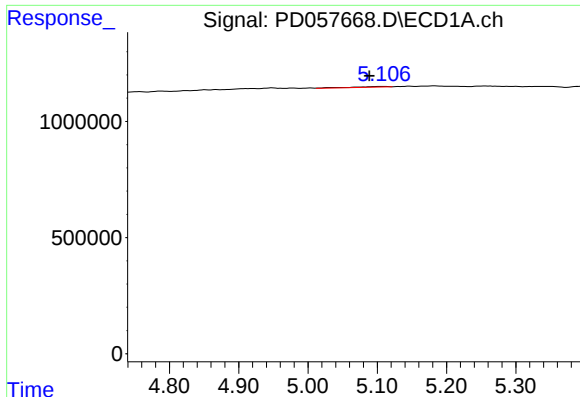

#10 gamma-Chlordane


R.T.: 5.108 min
Delta R.T.: 0.019 min
Response: 97242
Conc: 0.11 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

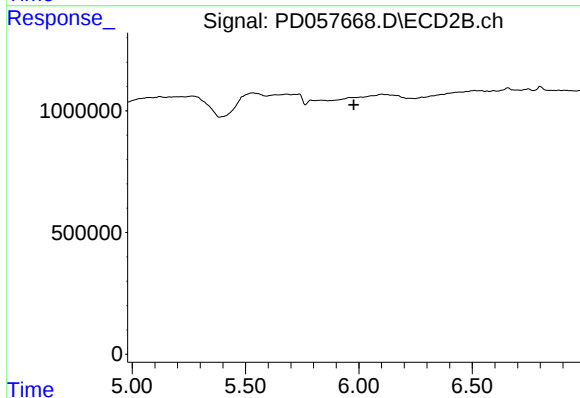


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.978 min
Response: 0
Conc: N.D.

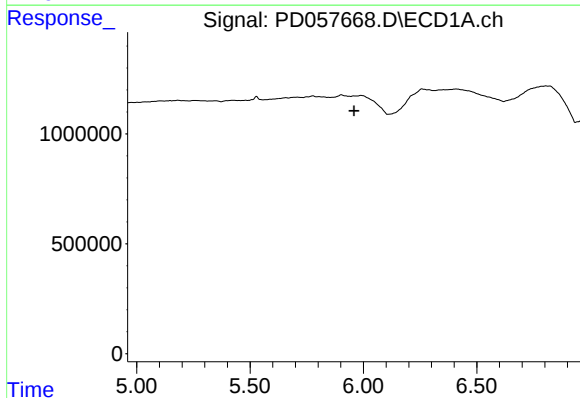


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.959 min
Response: 0
Conc: N.D.

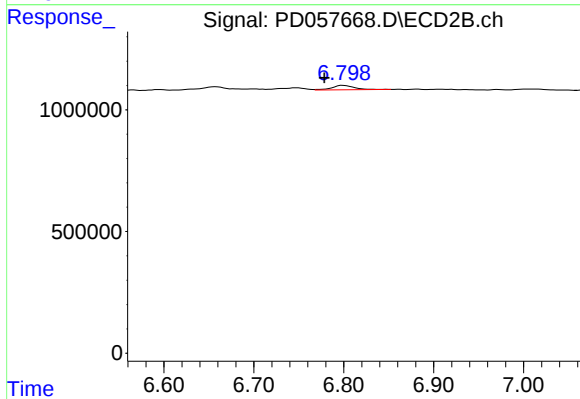

#15 Endosulfan II


R.T.: 6.799 min
Delta R.T.: 0.021 min
Response: 307756
Conc: 0.30 ng/ml

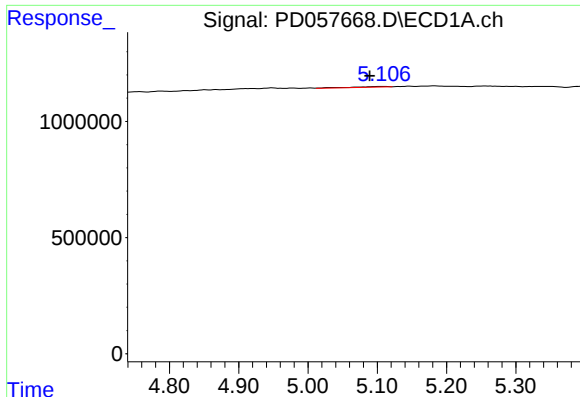

#25 Chlordane-3


R.T.: 5.108 min
Delta R.T.: 0.018 min
Response: 97242
Conc: 1.11 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

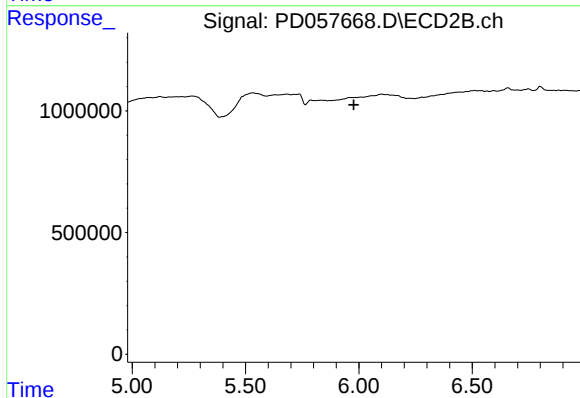


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.978 min
Response: 0
Conc: N.D.

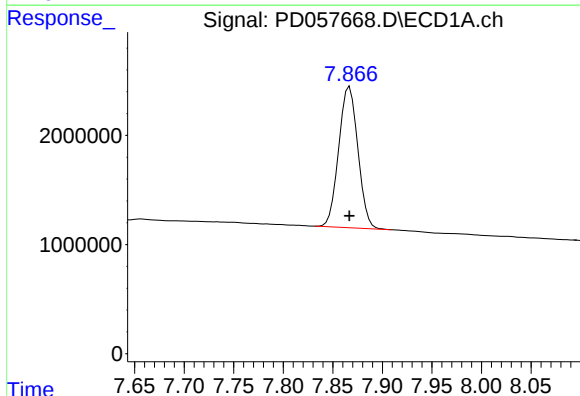

#28 Decachlorobiphenyl

R.T.: 7.867 min
Delta R.T.: 0.000 min
Response: 17399111
Conc: 22.85 ng/ml

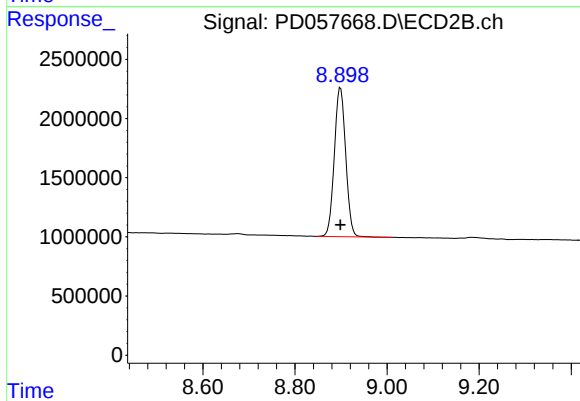

#28 Decachlorobiphenyl

R.T.: 8.899 min
Delta R.T.: 0.000 min
Response: 21614884
Conc: 24.58 ng/ml