

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032720\
 Data File : PD057643.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Mar 2020 13:33
 Operator : AJ\MA
 Sample : PTOXICC750
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PTOXICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 14:44:07 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX032720.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 27 14:39:47 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.226	3.896	55390049	61642142	77.821	76.493
7) SA Decachlor...	7.866	8.898	57640781	65512332	75.283	73.751
Target Compounds						
2) Toxaphene-1	5.614	6.445	6820166	8906420	800.194	785.223
3) Toxaphene-2	5.990	6.738	11241063	9783234	775.594	714.644
4) Toxaphene-3	6.230	7.023	10520415	21681142	762.536	764.044
5) Toxaphene-4	6.368	7.107	4982730	13405069	834.529	753.442
6) Toxaphene-5	6.649	7.520	4279927	12852155	834.183	750.245

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032720\
Data File : PD057643.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Mar 2020 13:33
Operator : AJ\MA
Sample : PTOXICC750
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 14:44:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX032720.M
Quant Title : GC Extractables
QLast Update : Fri Mar 27 14:39:47 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

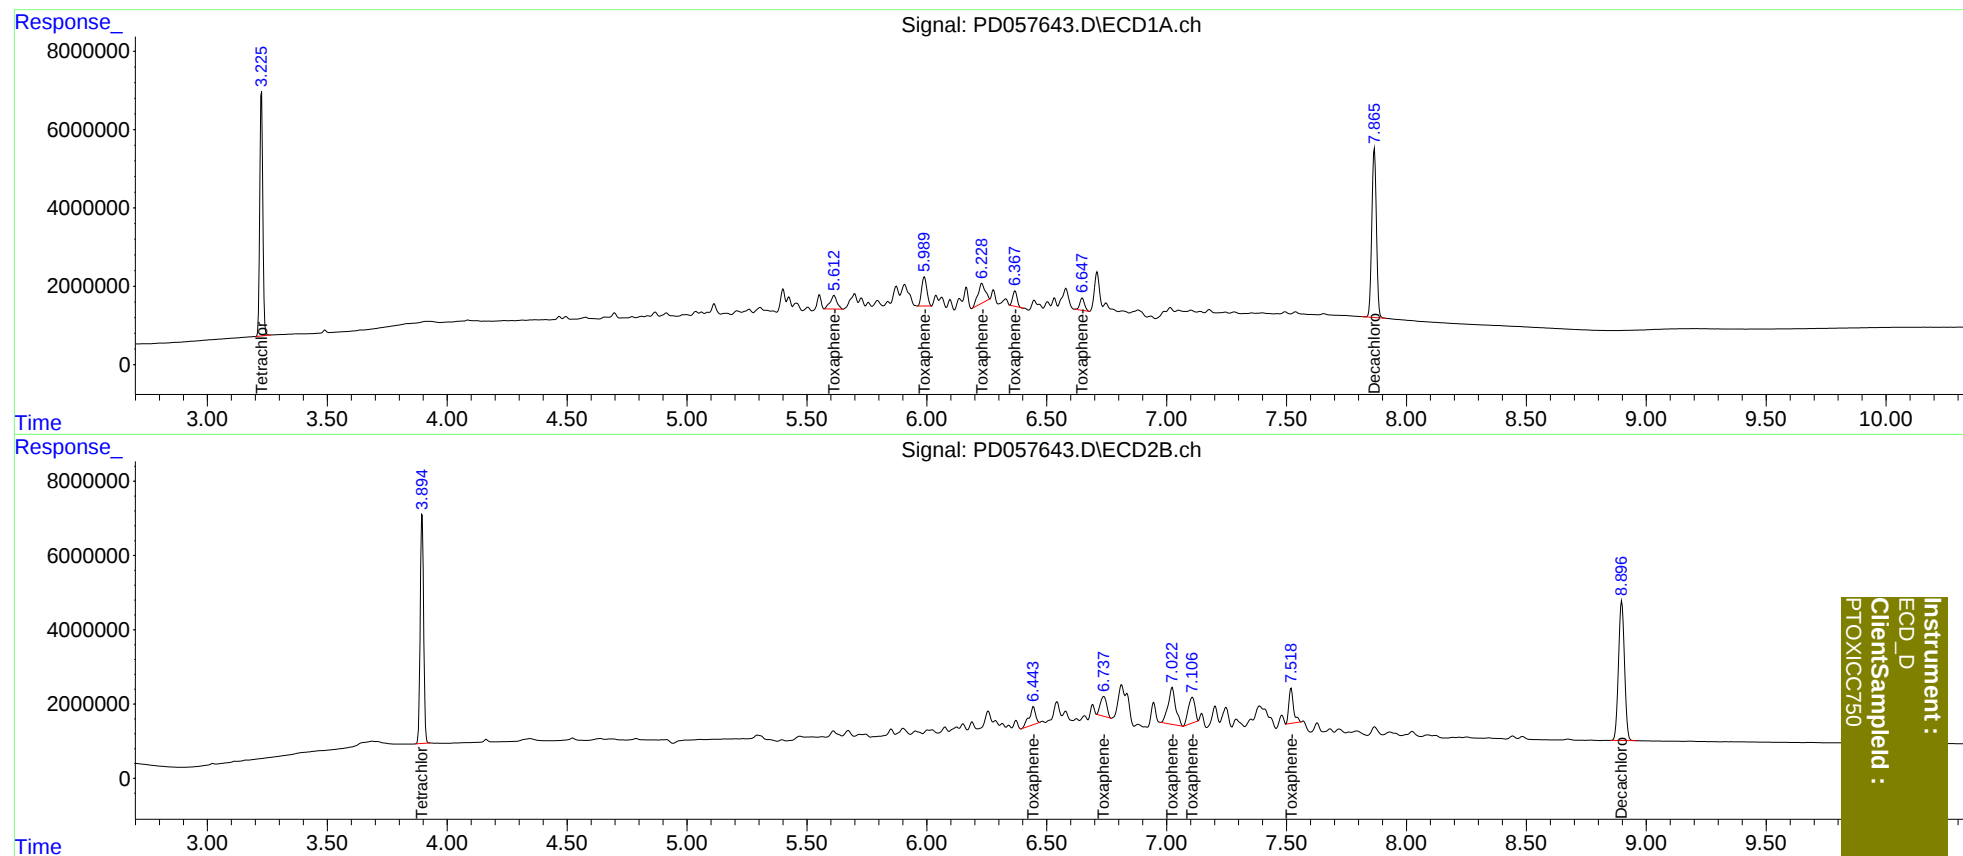

Instrument :
ECD_D
Client Sample :
PTOXICC750