

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032720\
 Data File : PD057671.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Mar 2020 20:56
 Operator : AJ\MA
 Sample : PTOXCCC500
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PTOXCCC500

Manual Integrations
 APPROVED

mohammad
 3/31/2020 3:17:31 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 28 04:20:02 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX032720.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 27 15:53:27 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.227	3.896	35103167	41699778	49.279	52.155
7) SA Decachlor...	7.867	8.899	38721316	46479666	50.062	51.768
Target Compounds						
2) Toxaphene-1	5.615	6.445	4347810	6036796	506.196	533.855
3) Toxaphene-2	5.990	6.738	7251295	6921504	499.011	534.773
4) Toxaphene-3	6.232	7.025	7364268	14788162	506.544	543.008
5) Toxaphene-4	6.367	7.109	3317710	9214575	539.154m	550.727
6) Toxaphene-5	6.650	7.520	2643508	9039477	522.418	554.055

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032720\
Data File : PD057671.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Mar 2020 20:56
Operator : AJ\MA
Sample : PTOXCCC500
Misc :
ALS Vial : 22 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 28 04:20:02 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX032720.M
Quant Title : GC Extractables
QLast Update : Fri Mar 27 15:53:27 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

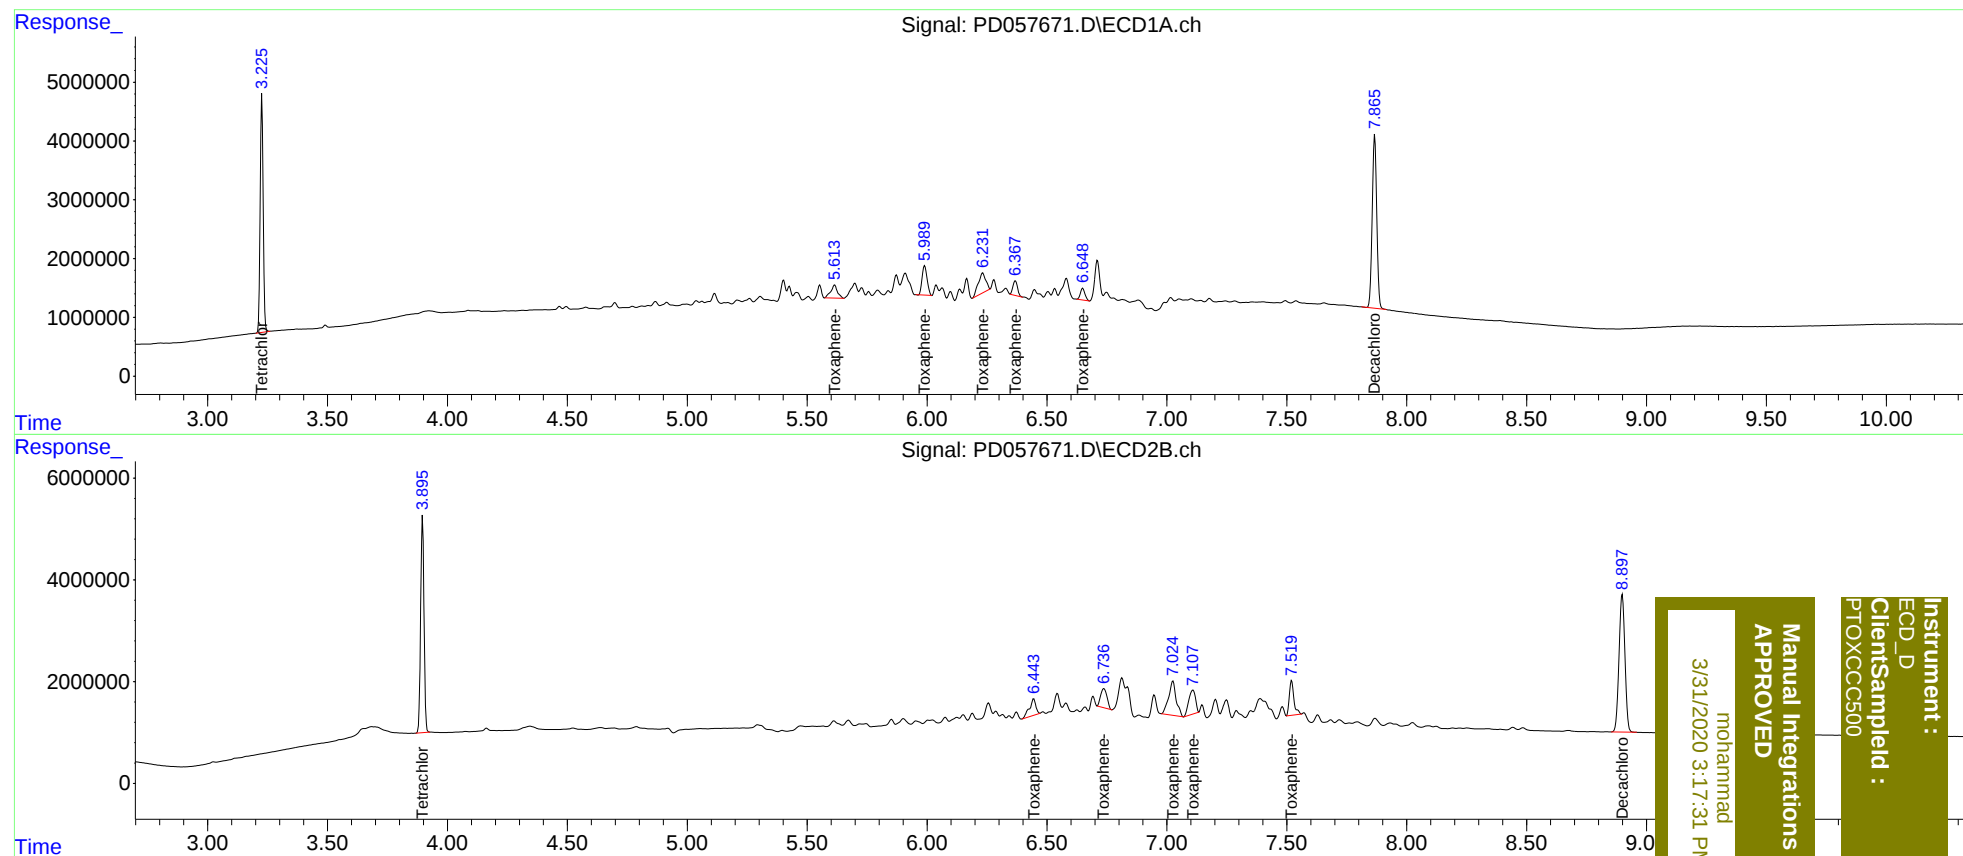

Manual Integrations
APPROVED

mohammad
3/31/2020 3:17:31 PM

Instrument :
ECD_D
ClientSampled :
PTOXCCC500