

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032720\
 Data File : PD057637.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Mar 2020 12:09
 Operator : AJ\MA
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 14:00:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032720.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 27 13:59:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.226	3.896	77281607	78062826	101.272	100.123
28)	SA Decachlor...	7.866	8.898	72702273	80597860	97.144	95.100
Target Compounds							
23)	Chlordane-1	4.056	4.875	24561609	31400288	995.902	1014.835
24)	Chlordane-2	4.540	5.338	27204368	35264101	965.405	941.725
25)	Chlordane-3	5.089	5.978	88454409	145.1E6	1028.792	1010.655
26)	Chlordane-4	5.145	6.051	81586451	172.7E6	1032.310	997.816
27)	Chlordane-5	5.961	6.849	27001280	34352955	1005.991	1000.957



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032720\
Data File : PD057637.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Mar 2020 12:09
Operator : AJ\MA
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 14:00:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032720.M
Quant Title : GC Extractables
QLast Update : Fri Mar 27 13:59:30 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

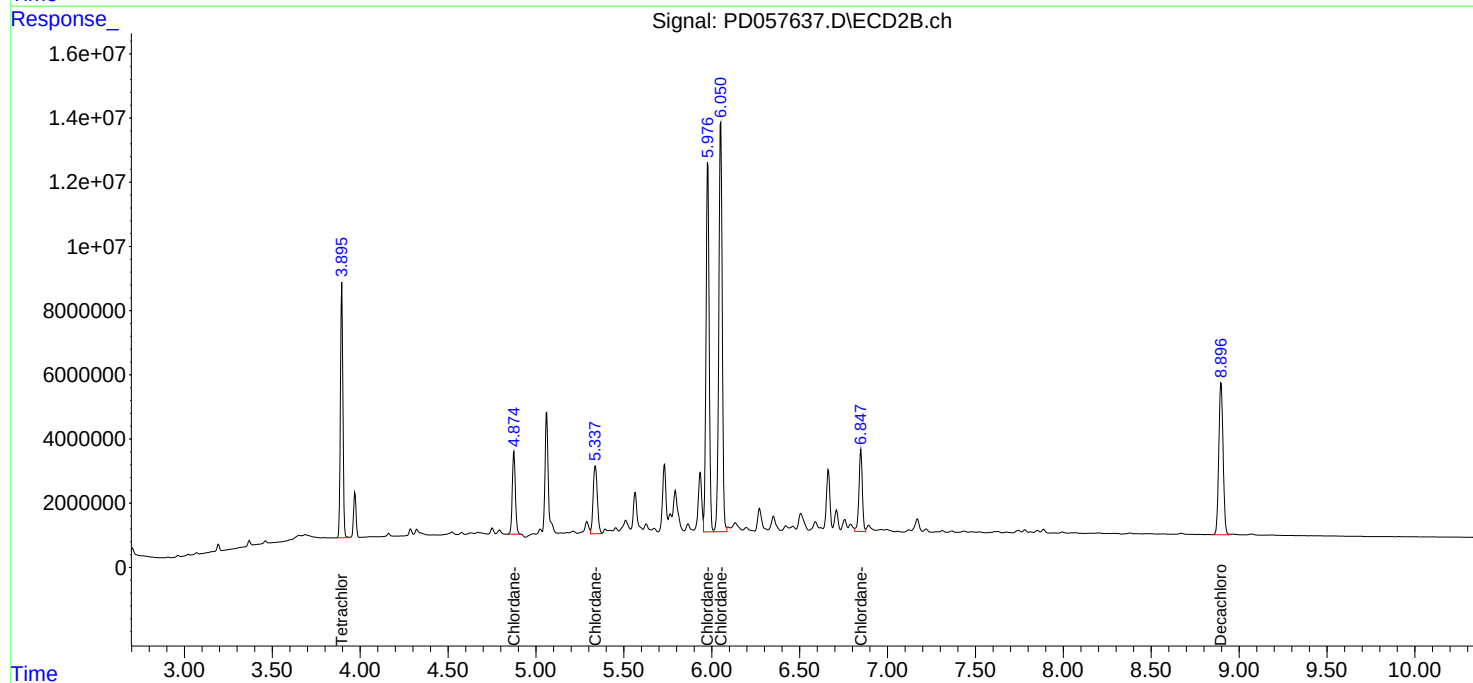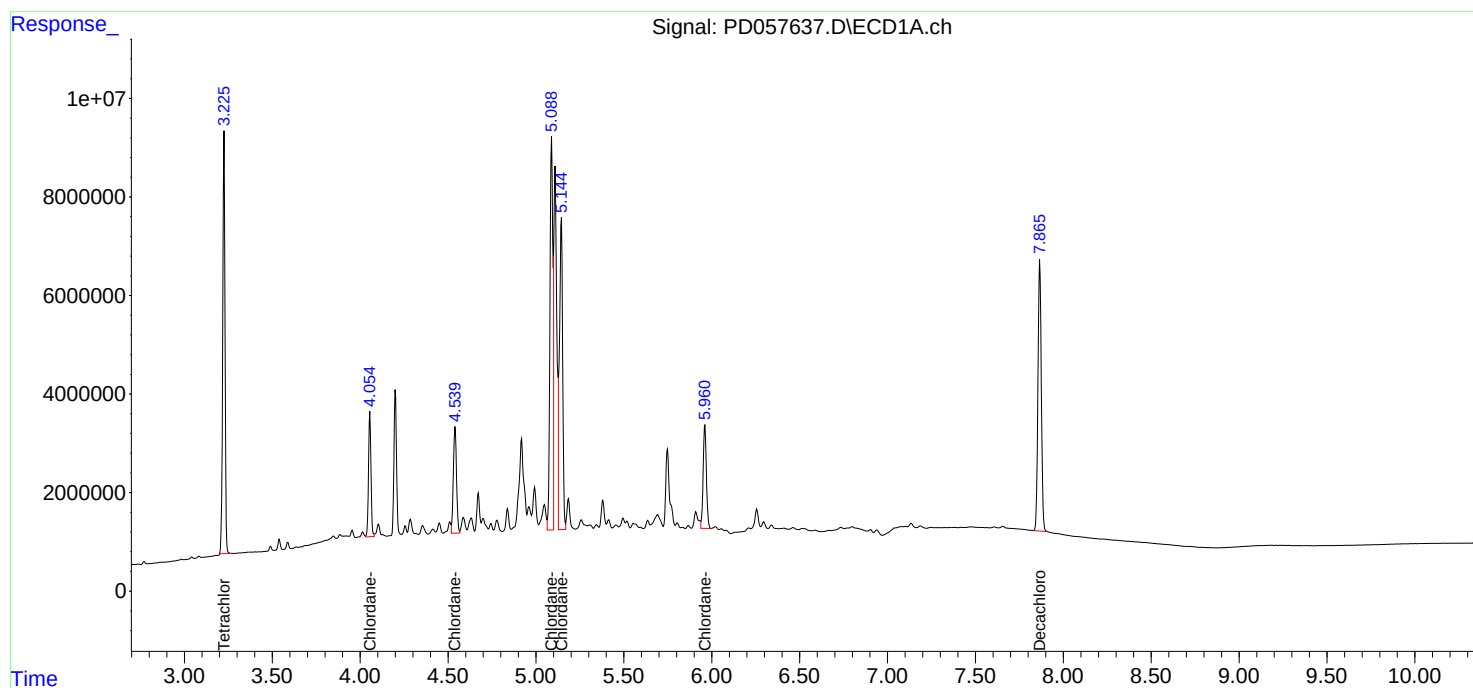


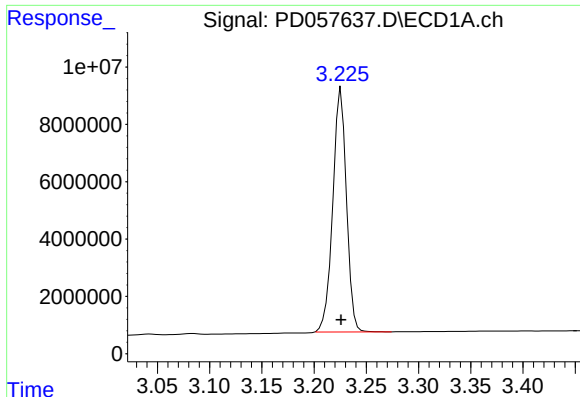

#1 Tetrachloro-m-xylene


R.T.: 3.226 min
Delta R.T.: 0.000 min
Response: 77281607
Conc: 101.27 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

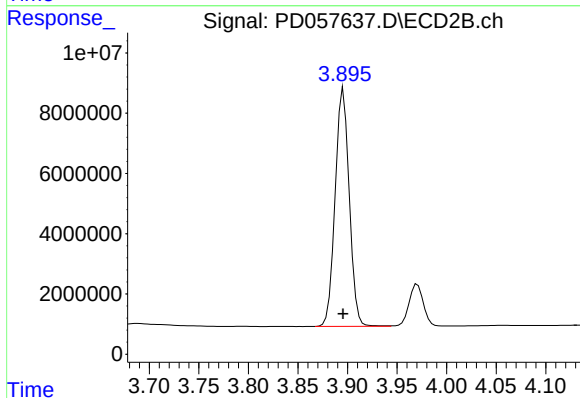


#1 Tetrachloro-m-xylene

R.T.: 3.896 min
Delta R.T.: 0.000 min
Response: 78062826
Conc: 100.12 ng/ml

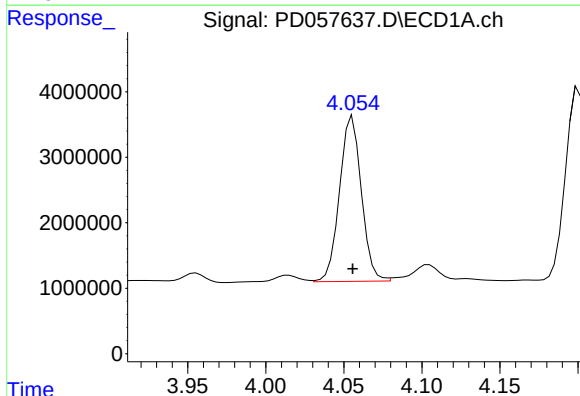


#23 Chlordane-1

R.T.: 4.056 min
Delta R.T.: 0.000 min
Response: 24561609
Conc: 995.90 ng/ml

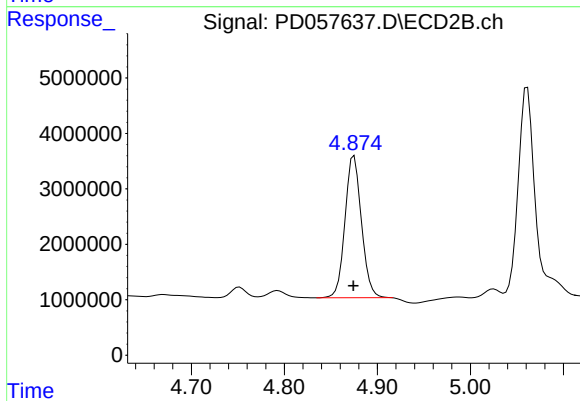

#23 Chlordane-1


R.T.: 4.875 min
Delta R.T.: 0.000 min
Response: 31400288
Conc: 1014.83 ng/ml

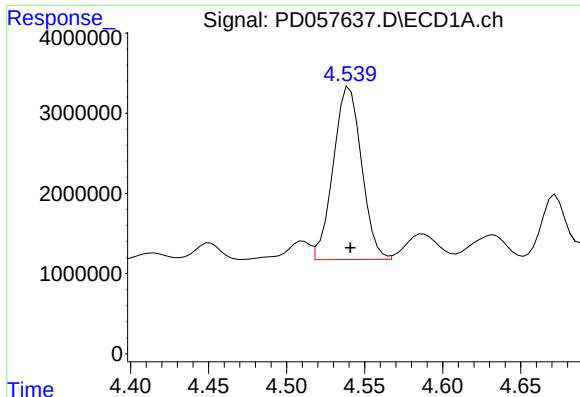

#24 Chlordane-2


R.T.: 4.540 min
Delta R.T.: 0.000 min
Response: 27204368
Conc: 965.40 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

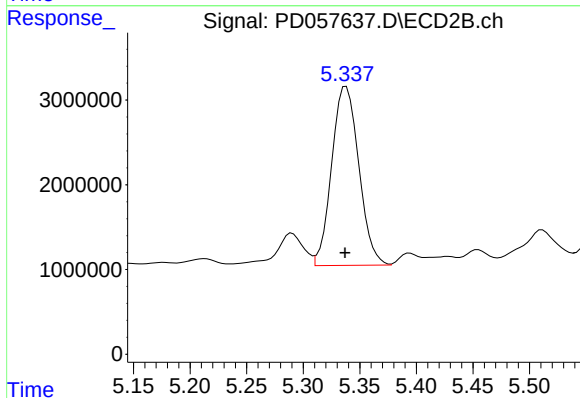


#24 Chlordane-2

R.T.: 5.338 min
Delta R.T.: 0.000 min
Response: 35264101
Conc: 941.73 ng/ml

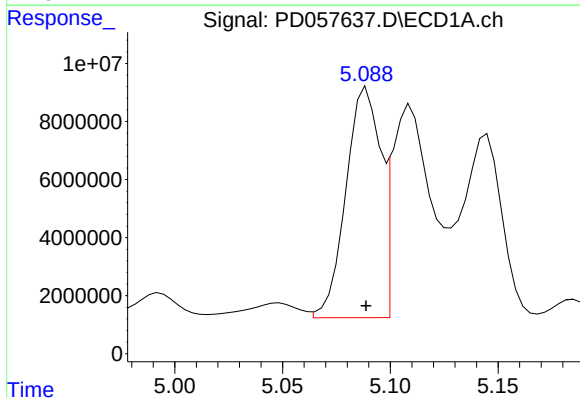


#25 Chlordane-3

R.T.: 5.089 min
Delta R.T.: 0.000 min
Response: 88454409
Conc: 1028.79 ng/ml

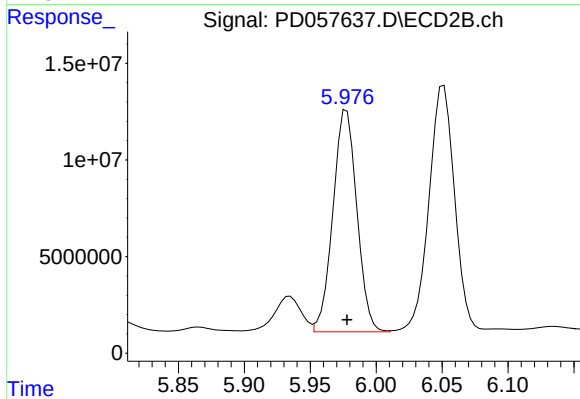

#25 Chlordane-3


R.T.: 5.978 min
Delta R.T.: 0.000 min
Response: 145093364
Conc: 1010.66 ng/ml

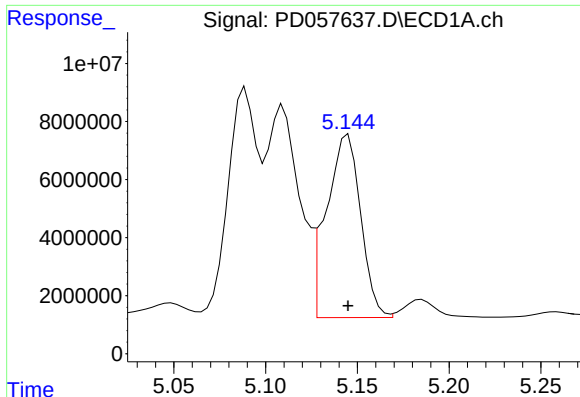

#26 Chlordane-4


R.T.: 5.145 min
Delta R.T.: 0.000 min
Response: 81586451
Conc: 1032.31 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

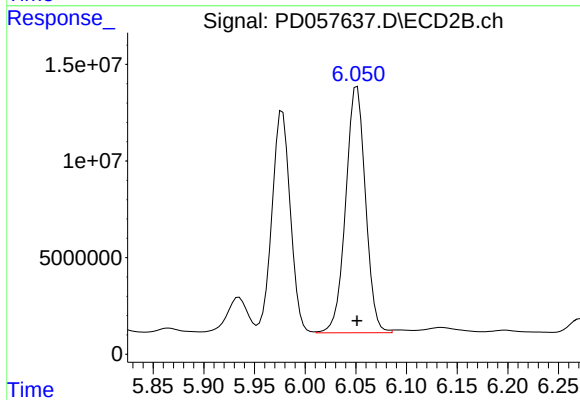


#26 Chlordane-4

R.T.: 6.051 min
Delta R.T.: 0.000 min
Response: 172716181
Conc: 997.82 ng/ml

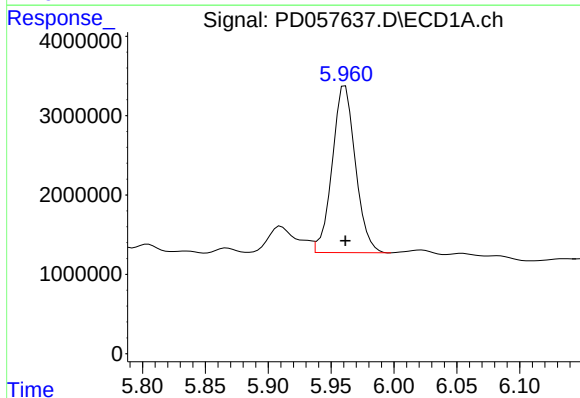


#27 Chlordane-5

R.T.: 5.961 min
Delta R.T.: 0.000 min
Response: 27001280
Conc: 1005.99 ng/ml

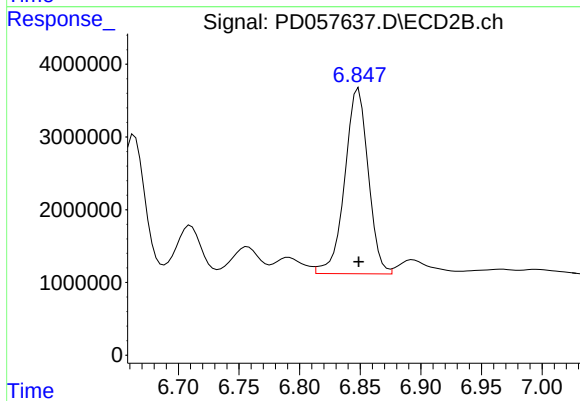

#27 Chlordane-5


R.T.: 6.849 min
Delta R.T.: 0.000 min
Response: 34352955
Conc: 1000.96 ng/ml

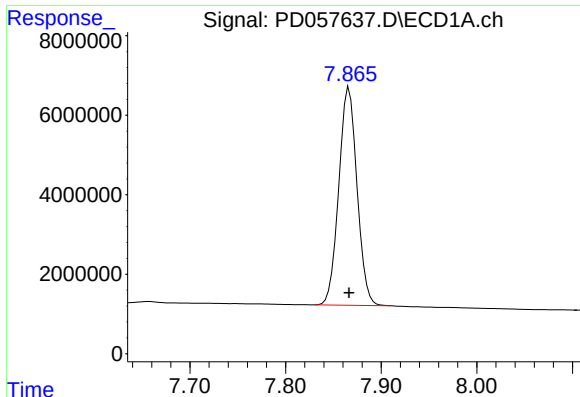

#28 Decachlorobiphenyl

R.T.: 7.866 min
Delta R.T.: 0.000 min
Response: 72702273
Conc: 97.14 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

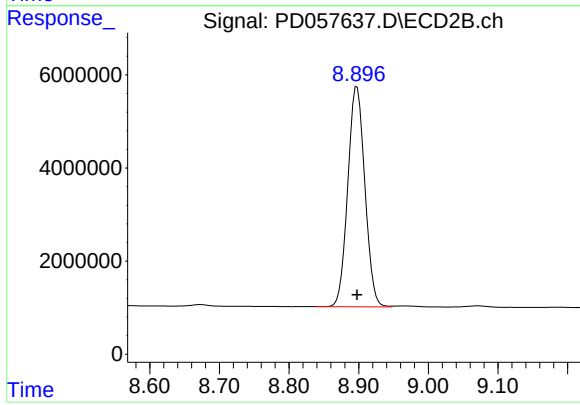

#28 Decachlorobiphenyl

R.T.: 8.898 min
Delta R.T.: 0.000 min
Response: 80597860
Conc: 95.10 ng/ml