

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032720\
 Data File : PD057648.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Mar 2020 14:43
 Operator : AJ\MA
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD032720CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 14:57:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032720.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 27 14:08:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.226	3.896	36293338	38487062	50.832	49.057
28)	SA Decachlor...	7.866	8.898	36975323	42301538	48.563	48.096
Target Compounds							
23)	Chlordane-1	4.056	4.876	11635661	15080690	467.477	492.007
24)	Chlordane-2	4.541	5.338	13566027	18252637	473.196	492.385
25)	Chlordane-3	5.089	5.978	41756792	69875560	475.698	479.635
26)	Chlordane-4	5.145	6.052	38110321	84146249	471.261	476.134
27)	Chlordane-5	5.962	6.850	13355873	16636575	501.042	499.751



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032720\
Data File : PD057648.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Mar 2020 14:43
Operator : AJ\MA
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD032720CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 14:57:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032720.M
Quant Title : GC Extractables
QLast Update : Fri Mar 27 14:08:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

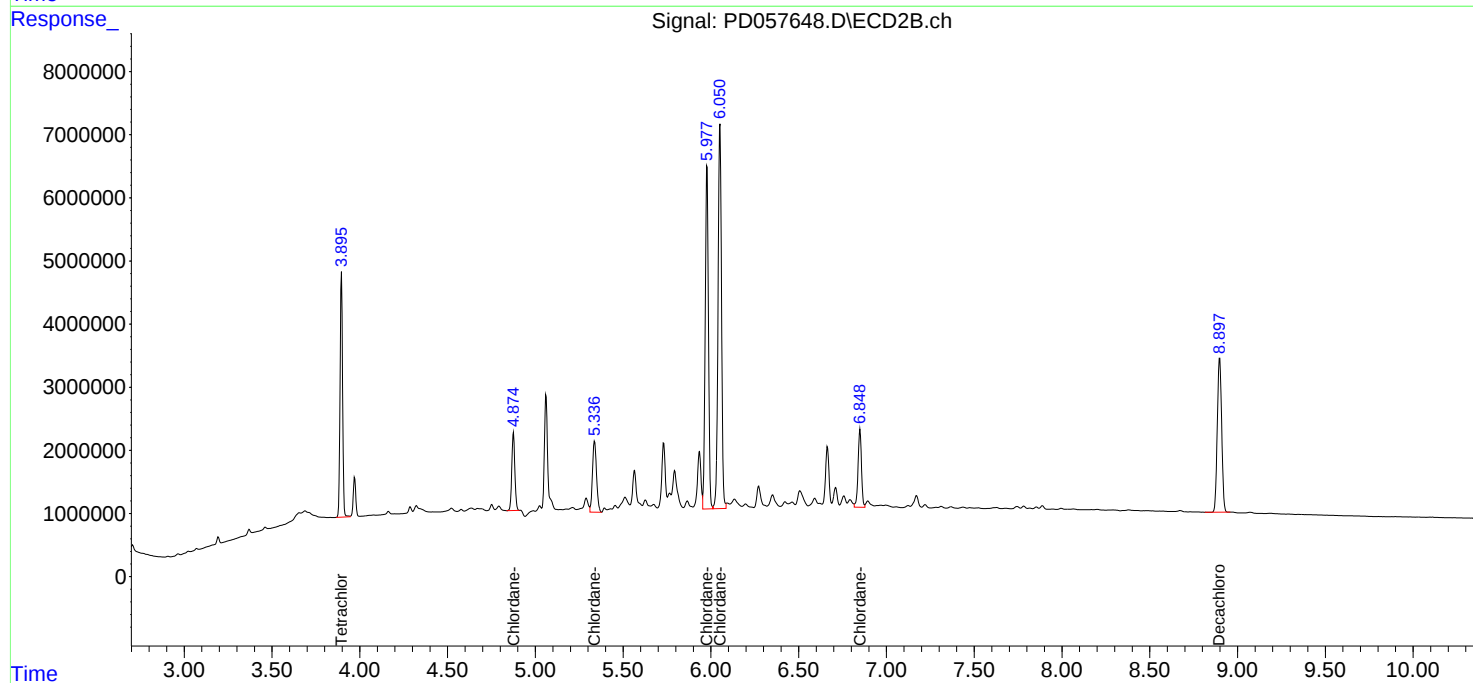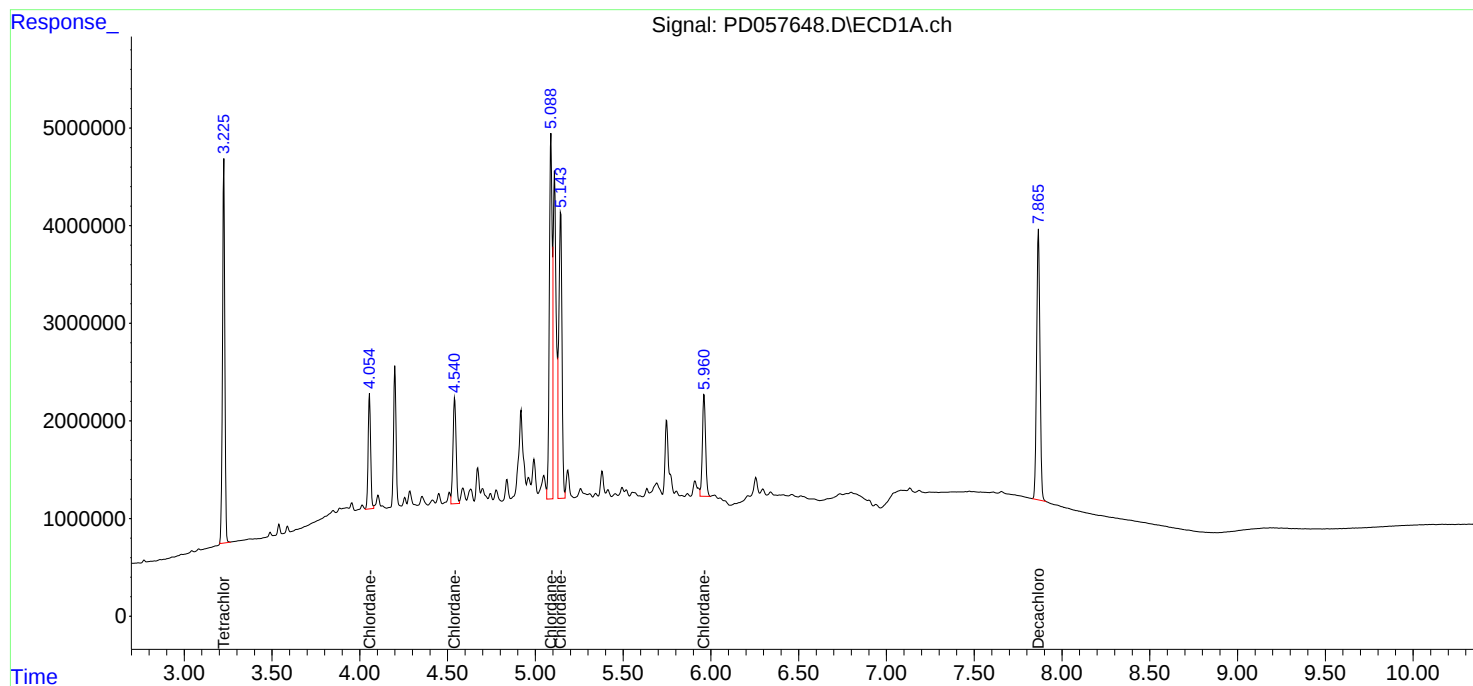


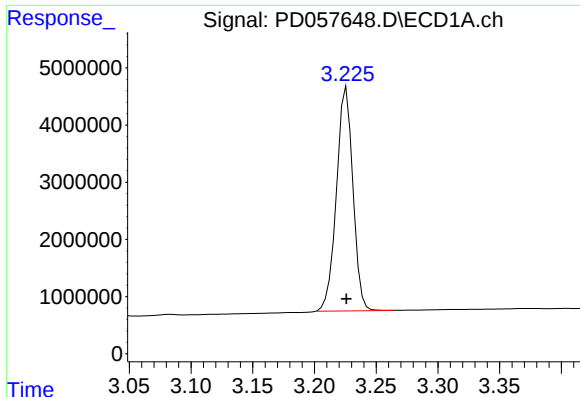

#1 Tetrachloro-m-xylene


R.T.: 3.226 min
Delta R.T.: 0.000 min
Response: 36293338
Conc: 50.83 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD032720CHLOR

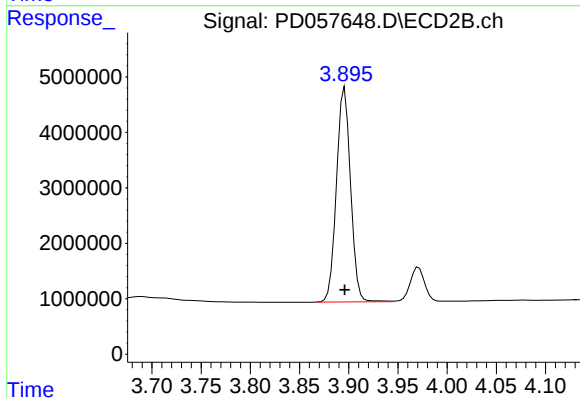


#1 Tetrachloro-m-xylene

R.T.: 3.896 min
Delta R.T.: 0.000 min
Response: 38487062
Conc: 49.06 ng/ml

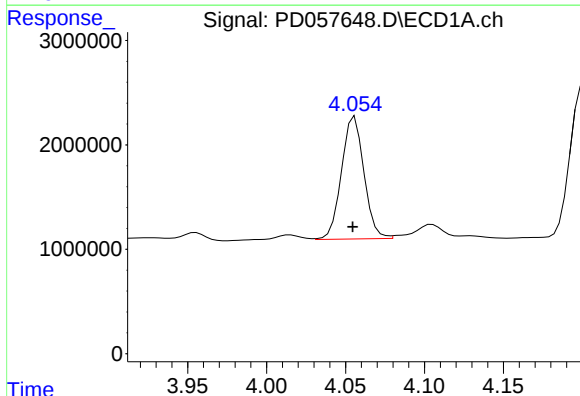


#23 Chlordane-1

R.T.: 4.056 min
Delta R.T.: 0.001 min
Response: 11635661
Conc: 467.48 ng/ml

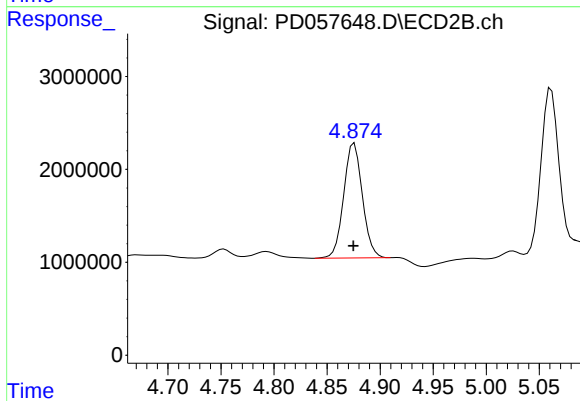

#23 Chlordane-1


R.T.: 4.876 min
Delta R.T.: 0.000 min
Response: 15080690
Conc: 492.01 ng/ml

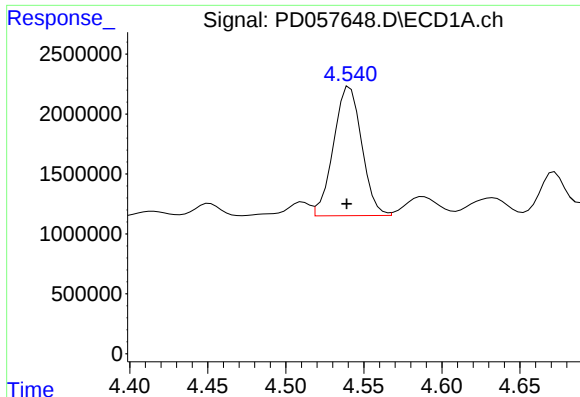

#24 Chlordane-2


R.T.: 4.541 min
Delta R.T.: 0.002 min
Response: 13566027
Conc: 473.20 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD032720CHLOR

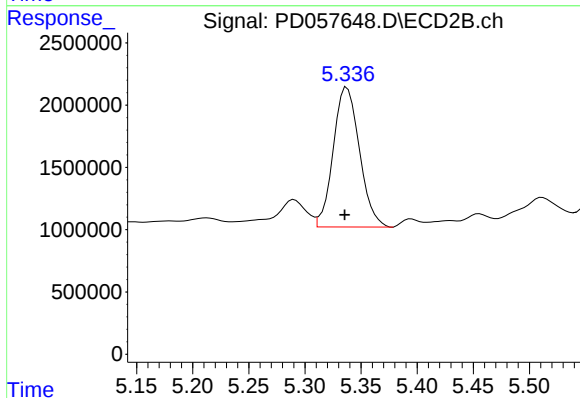


#24 Chlordane-2

R.T.: 5.338 min
Delta R.T.: 0.002 min
Response: 18252637
Conc: 492.38 ng/ml

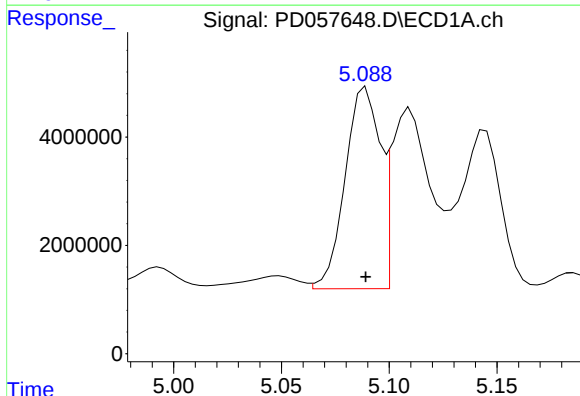


#25 Chlordane-3

R.T.: 5.089 min
Delta R.T.: 0.000 min
Response: 41756792
Conc: 475.70 ng/ml

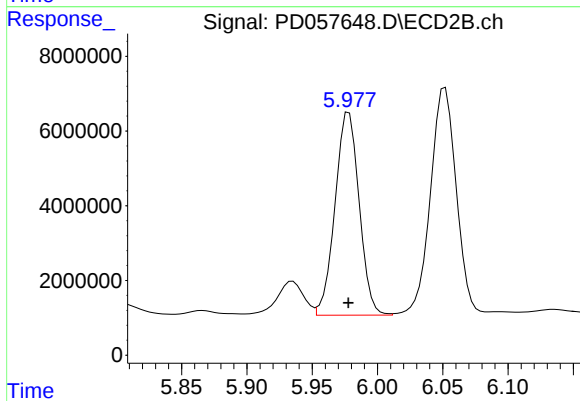

#25 Chlordane-3


R.T.: 5.978 min
Delta R.T.: 0.000 min
Response: 69875560
Conc: 479.63 ng/ml

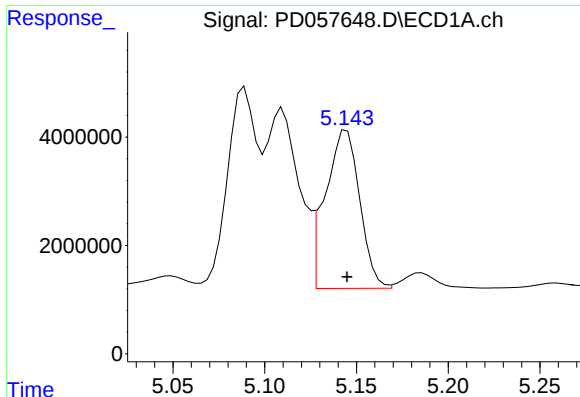

#26 Chlordane-4


R.T.: 5.145 min
Delta R.T.: 0.000 min
Response: 38110321
Conc: 471.26 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD032720CHLOR

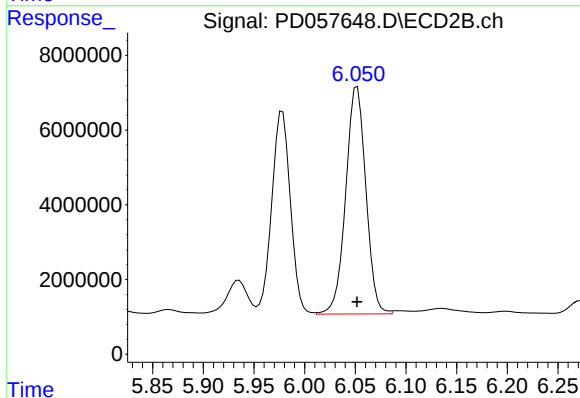


#26 Chlordane-4

R.T.: 6.052 min
Delta R.T.: 0.000 min
Response: 84146249
Conc: 476.13 ng/ml

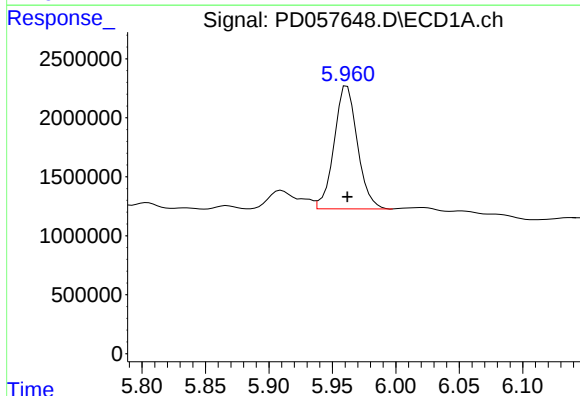


#27 Chlordane-5

R.T.: 5.962 min
Delta R.T.: 0.000 min
Response: 13355873
Conc: 501.04 ng/ml

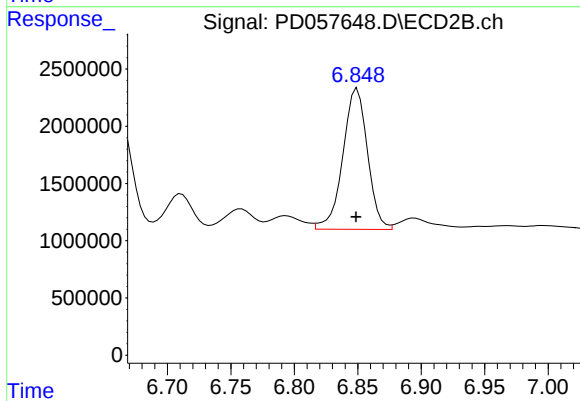

#27 Chlordane-5


R.T.: 6.850 min
Delta R.T.: 0.000 min
Response: 16636575
Conc: 499.75 ng/ml

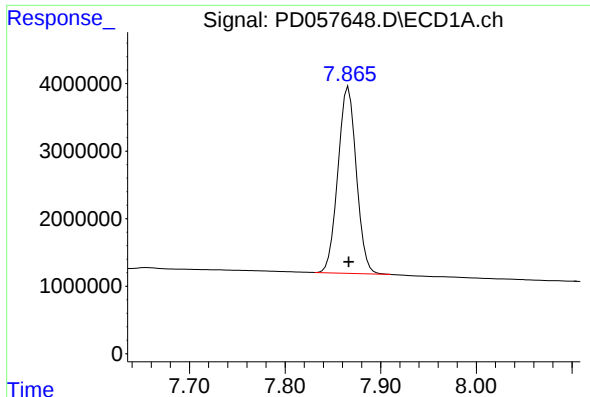

#28 Decachlorobiphenyl

R.T.: 7.866 min
Delta R.T.: 0.000 min
Response: 36975323
Conc: 48.56 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD032720CHLOR

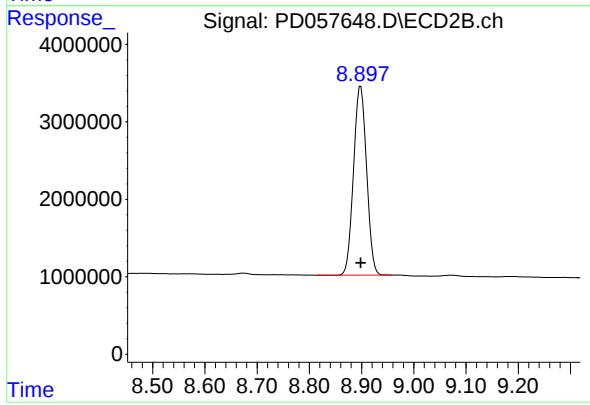

#28 Decachlorobiphenyl

R.T.: 8.898 min
Delta R.T.: 0.000 min
Response: 42301538
Conc: 48.10 ng/ml