

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032720\
 Data File : PD057660.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Mar 2020 17:40
 Operator : AJ\MA
 Sample : L1798-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PT-CHLR-WP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 28 04:14:42 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032720.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 27 14:08:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.224	3.896	21968374	17521053	30.769	22.333 #
28)	SA Decachlor...	7.867	8.899	17906644	21042506	23.518	23.925
Target Compounds							
23)	Chlordane-1	4.056	4.875	77477521	101.5E6	3112.754	3311.970
24)	Chlordane-2	4.540	5.338	78985464	105.0E6	2755.088	2833.434
25)	Chlordane-3	5.089	5.978	266.6E6	390.2E6	3037.037	2678.682
26)	Chlordane-4	5.145	6.052	241.8E6	448.5E6	2990.309	2537.961
27)	Chlordane-5	5.962	6.850	76794734	101.7E6	2880.936	3055.132



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032720\
Data File : PD057660.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Mar 2020 17:40
Operator : AJ\MA
Sample : L1798-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PT-CHLR-WP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 28 04:14:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032720.M
Quant Title : GC Extractables
QLast Update : Fri Mar 27 14:08:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

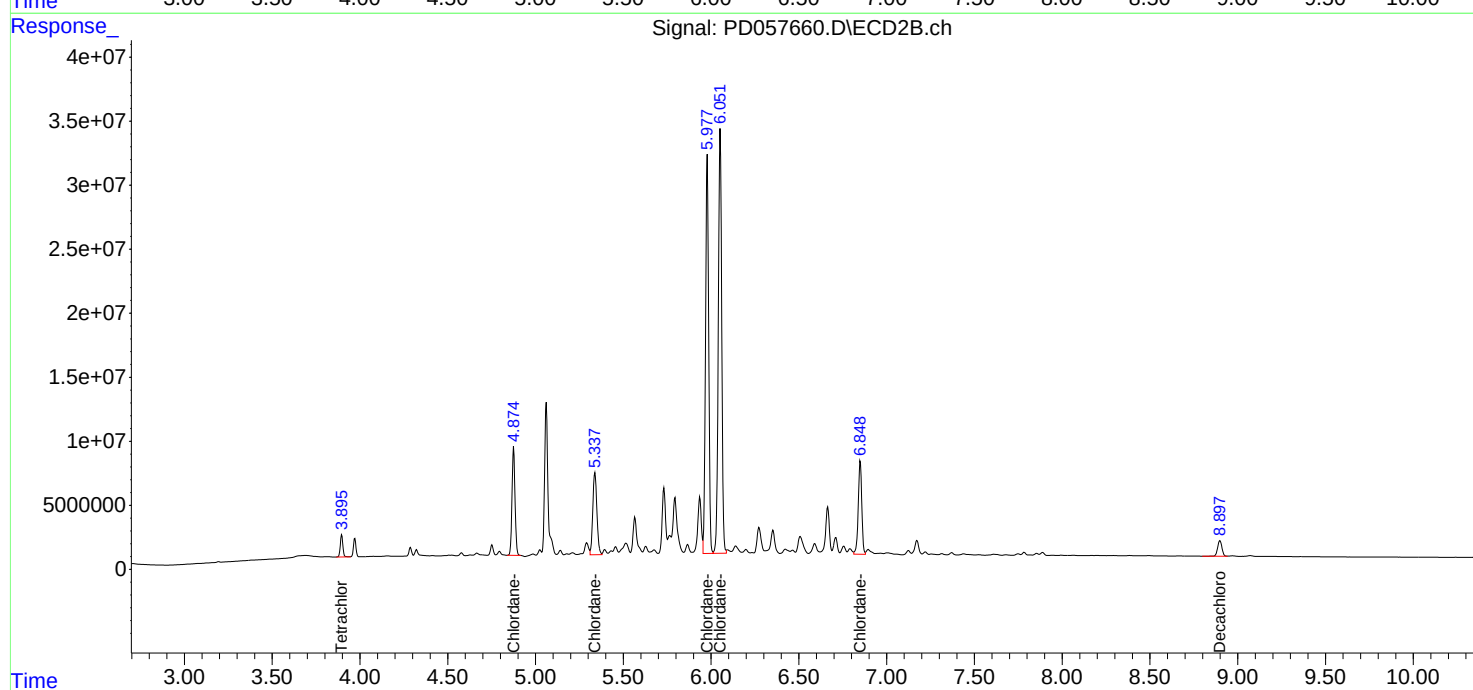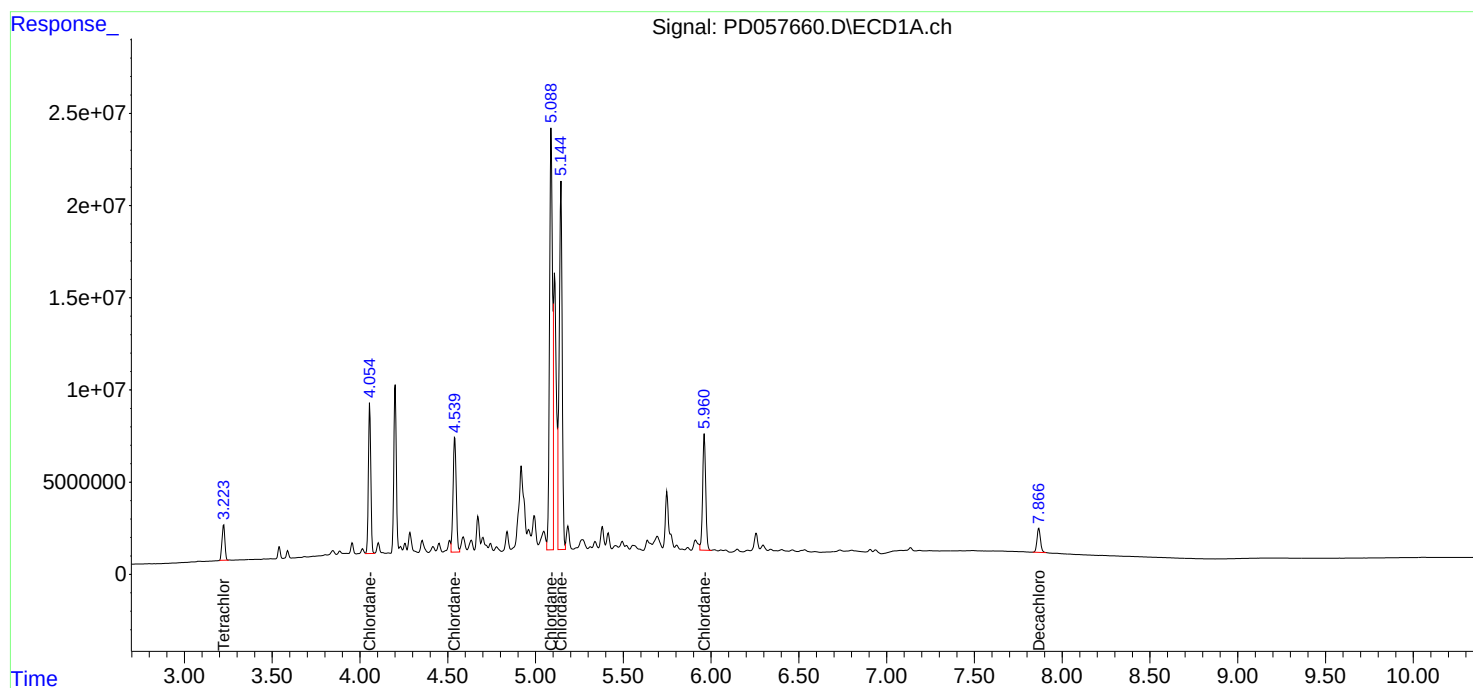


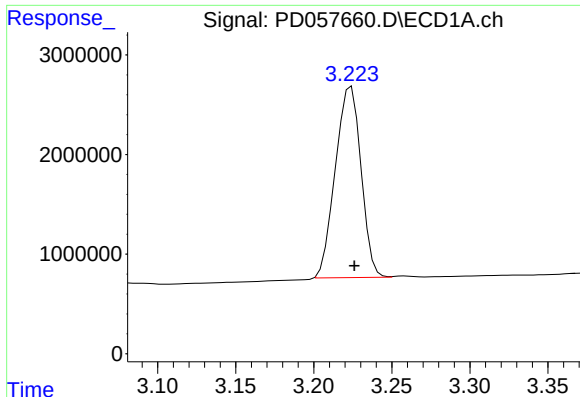

#1 Tetrachloro-m-xylene


R.T.: 3.224 min
Delta R.T.: -0.002 min
Response: 21968374
Conc: 30.77 ng/ml

Instrument :
ECD_D
ClientSampleId :
PT-CHLR-WP

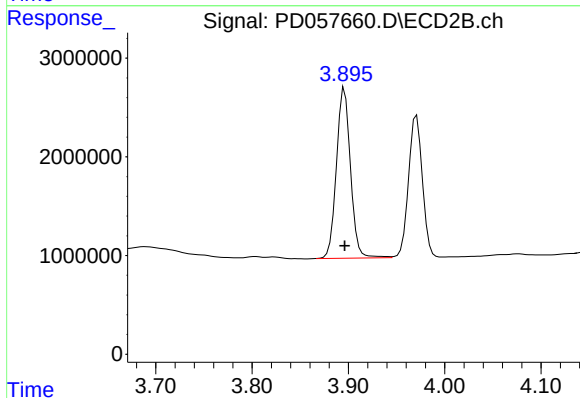


#1 Tetrachloro-m-xylene

R.T.: 3.896 min
Delta R.T.: 0.000 min
Response: 17521053
Conc: 22.33 ng/ml

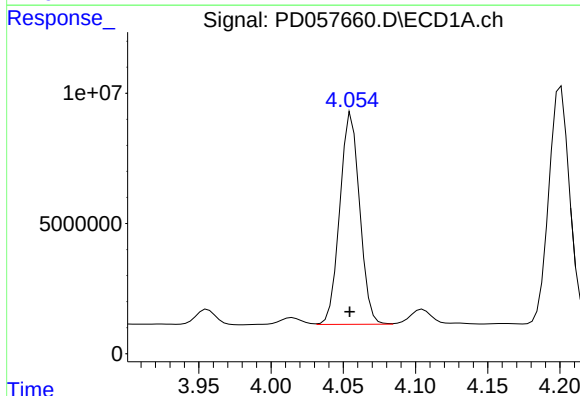


#23 Chlordane-1

R.T.: 4.056 min
Delta R.T.: 0.001 min
Response: 77477521
Conc: 3112.75 ng/ml

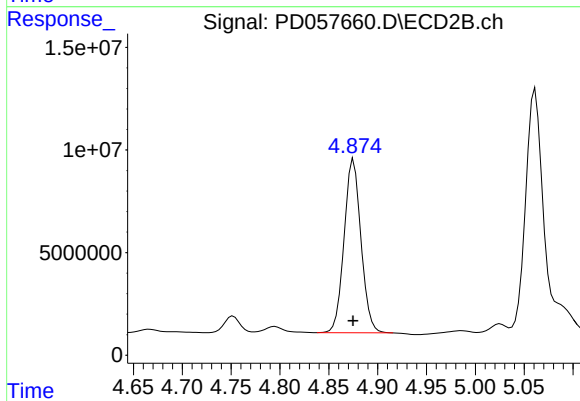

#23 Chlordane-1


R.T.: 4.875 min
Delta R.T.: 0.000 min
Response: 101516456
Conc: 3311.97 ng/ml

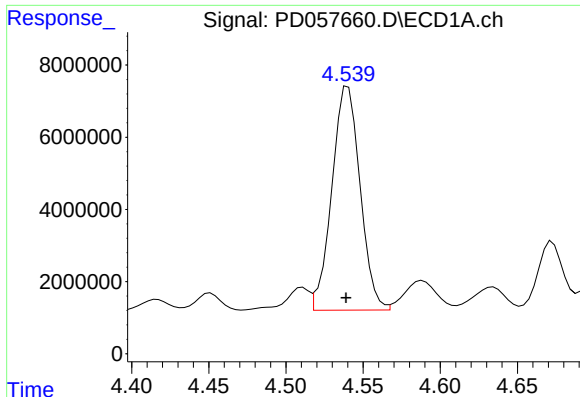

#24 Chlordane-2


R.T.: 4.540 min
Delta R.T.: 0.001 min
Response: 78985464
Conc: 2755.09 ng/ml

Instrument :
ECD_D
ClientSampleId :
PT-CHLR-WP

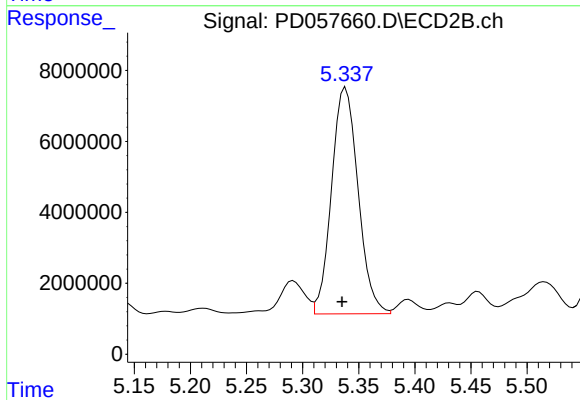


#24 Chlordane-2

R.T.: 5.338 min
Delta R.T.: 0.003 min
Response: 105034987
Conc: 2833.43 ng/ml

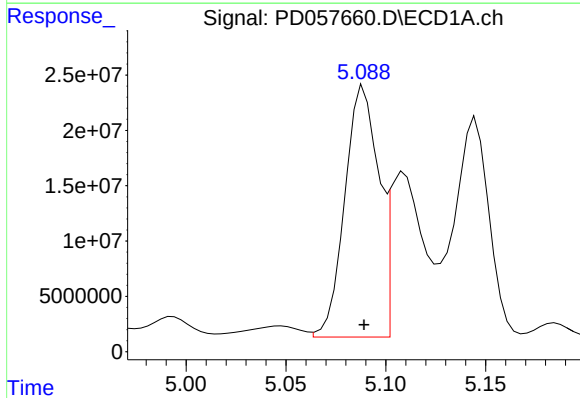


#25 Chlordane-3

R.T.: 5.089 min
Delta R.T.: 0.000 min
Response: 266591053
Conc: 3037.04 ng/ml

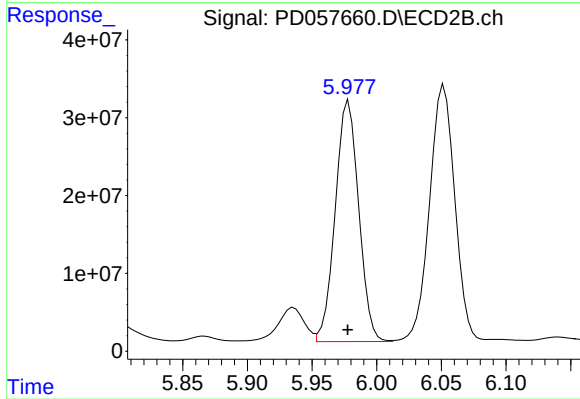

#25 Chlordane-3


R.T.: 5.978 min
Delta R.T.: 0.000 min
Response: 390243492
Conc: 2678.68 ng/ml

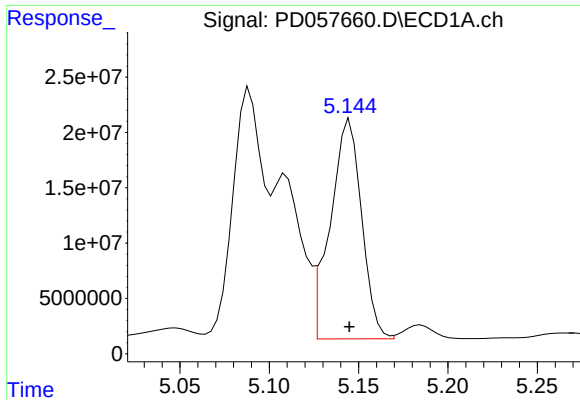

#26 Chlordane-4


R.T.: 5.145 min
Delta R.T.: 0.000 min
Response: 241822964
Conc: 2990.31 ng/ml

Instrument :
ECD_D
ClientSampleId :
PT-CHLR-WP

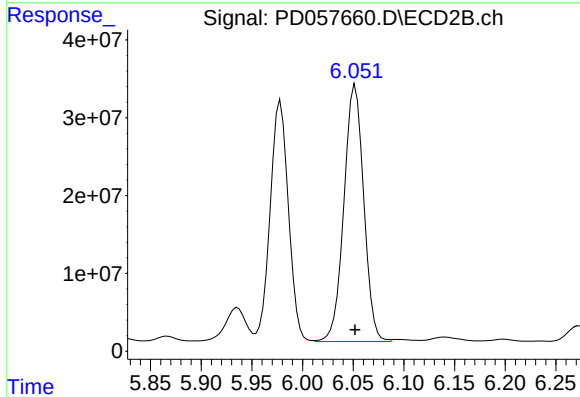


#26 Chlordane-4

R.T.: 6.052 min
Delta R.T.: 0.000 min
Response: 448529515
Conc: 2537.96 ng/ml

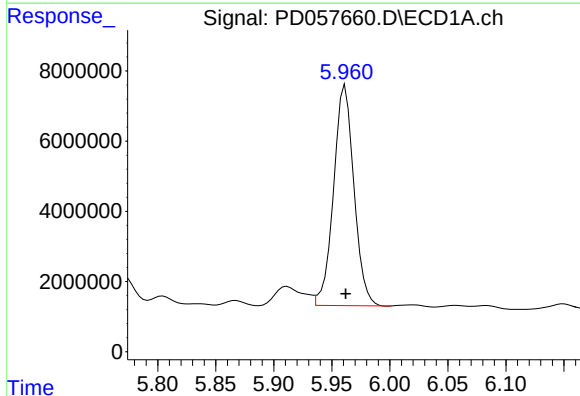


#27 Chlordane-5

R.T.: 5.962 min
Delta R.T.: 0.000 min
Response: 76794734
Conc: 2880.94 ng/ml

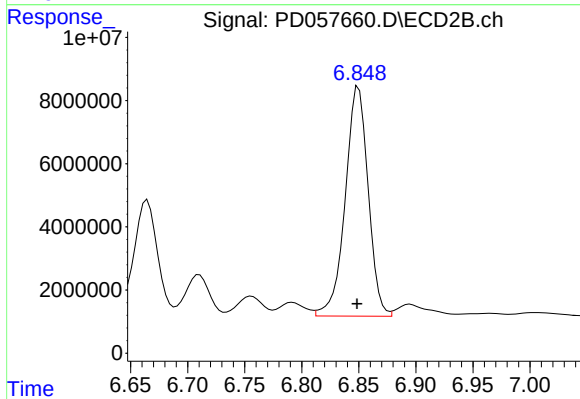

#27 Chlordane-5


R.T.: 6.850 min
Delta R.T.: 0.001 min
Response: 101704487
Conc: 3055.13 ng/ml

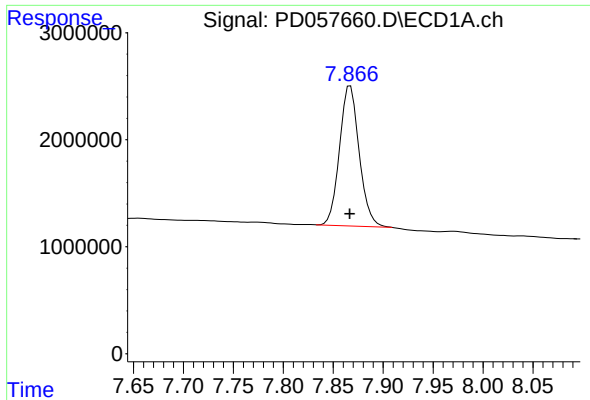

#28 Decachlorobiphenyl

R.T.: 7.867 min
Delta R.T.: 0.000 min
Response: 17906644
Conc: 23.52 ng/ml

Instrument :
ECD_D
ClientSampleId :
PT-CHLR-WP

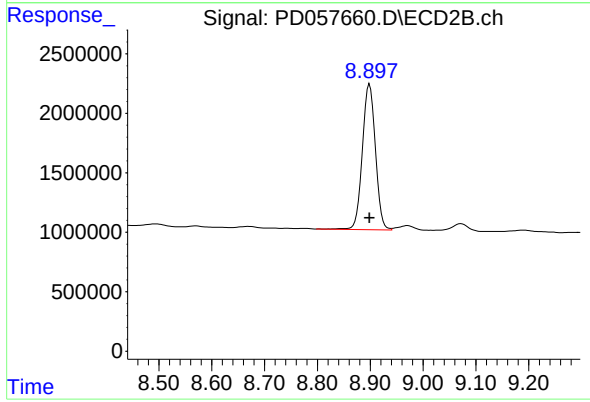

#28 Decachlorobiphenyl

R.T.: 8.899 min
Delta R.T.: 0.000 min
Response: 21042506
Conc: 23.92 ng/ml