

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD032720\  
 Data File : PD057668.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2020 19:32  
 Operator : AJ\MA  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_D  
 ClientSampleId :  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 28 04:15:40 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD032720.M  
 Quant Title : GC Extractables  
 QLast Update : Fri Mar 27 14:08:11 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

|                             | Compound        | RT#1  | RT#2  | Resp#1   | Resp#2   | ng/ml  | ng/ml  |
|-----------------------------|-----------------|-------|-------|----------|----------|--------|--------|
| -----                       |                 |       |       |          |          |        |        |
| System Monitoring Compounds |                 |       |       |          |          |        |        |
| 1)                          | SA Tetrachlo... | 3.227 | 3.897 | 15355200 | 18322157 | 21.506 | 23.354 |
| 28)                         | SA Decachlor... | 7.867 | 8.899 | 17399111 | 21614884 | 22.852 | 24.575 |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD032720\  
Data File : PD057668.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 27 Mar 2020 19:32  
Operator : AJ\MA  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
I.BLK

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Mar 28 04:15:40 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD032720.M  
Quant Title : GC Extractables  
QLast Update : Fri Mar 27 14:08:11 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

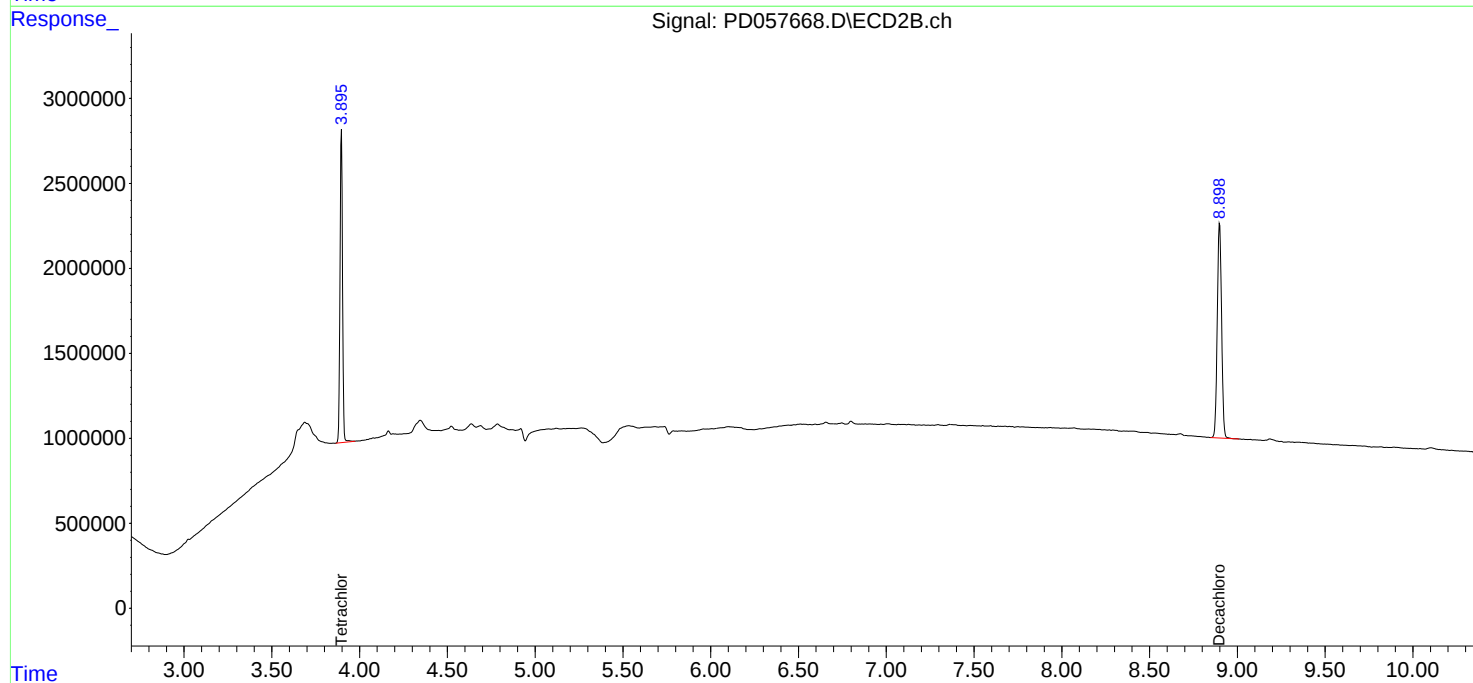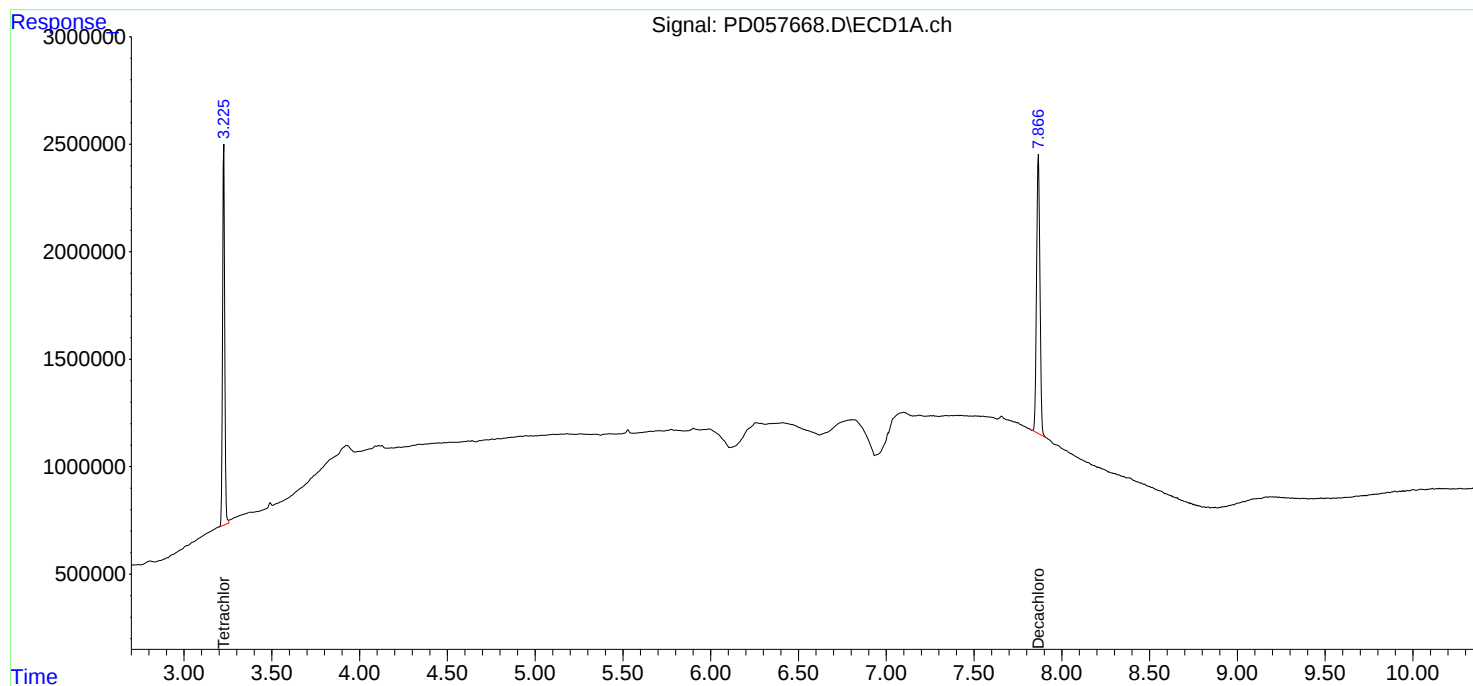


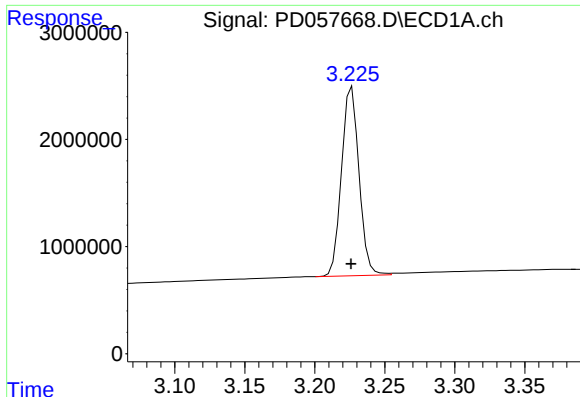

#1 Tetrachloro-m-xylene


R.T.: 3.227 min  
Delta R.T.: 0.000 min  
Response: 15355200  
Conc: 21.51 ng/ml

Instrument :  
ECD\_D  
ClientSampleId :  
I.BLK

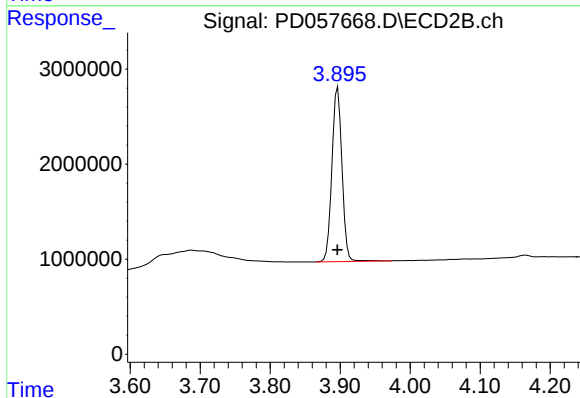


#1 Tetrachloro-m-xylene

R.T.: 3.897 min  
Delta R.T.: 0.000 min  
Response: 18322157  
Conc: 23.35 ng/ml

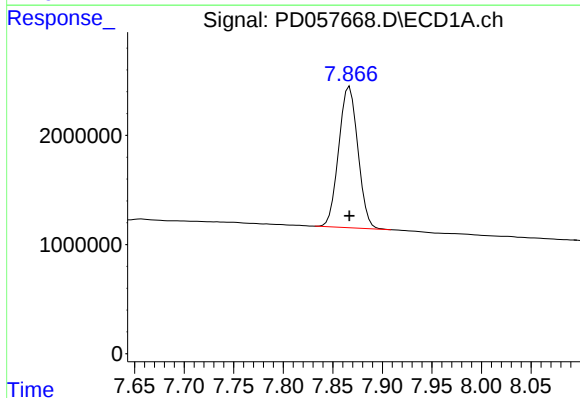

#28 Decachlorobiphenyl

R.T.: 7.867 min  
Delta R.T.: 0.000 min  
Response: 17399111  
Conc: 22.85 ng/ml

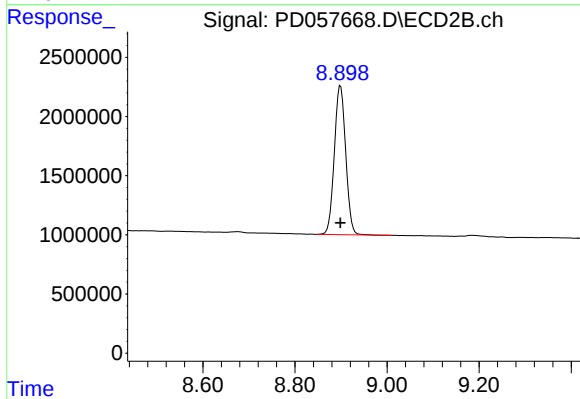

#28 Decachlorobiphenyl

R.T.: 8.899 min  
Delta R.T.: 0.000 min  
Response: 21614884  
Conc: 24.58 ng/ml