

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032819\
 Data File : PD052246.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Mar 2019 16:58
 Operator : AJ\SJ
 Sample : PIBLK06
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK07

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 01:35:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032519CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 25 18:59:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.222	4.043	32375142	598.8E6	22.809	20.580
27) SA Decachlor...	7.819	9.157	56229016	552.1E6	35.909	35.764
Target Compounds						
6) B beta-BHC	0.000	4.931f	0	21409685	N.D.	1.167


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032819\
Data File : PD052246.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Mar 2019 16:58
Operator : AJ\SJ
Sample : PIBLK06
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PIBLK07

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 01:35:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032519CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 25 18:59:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

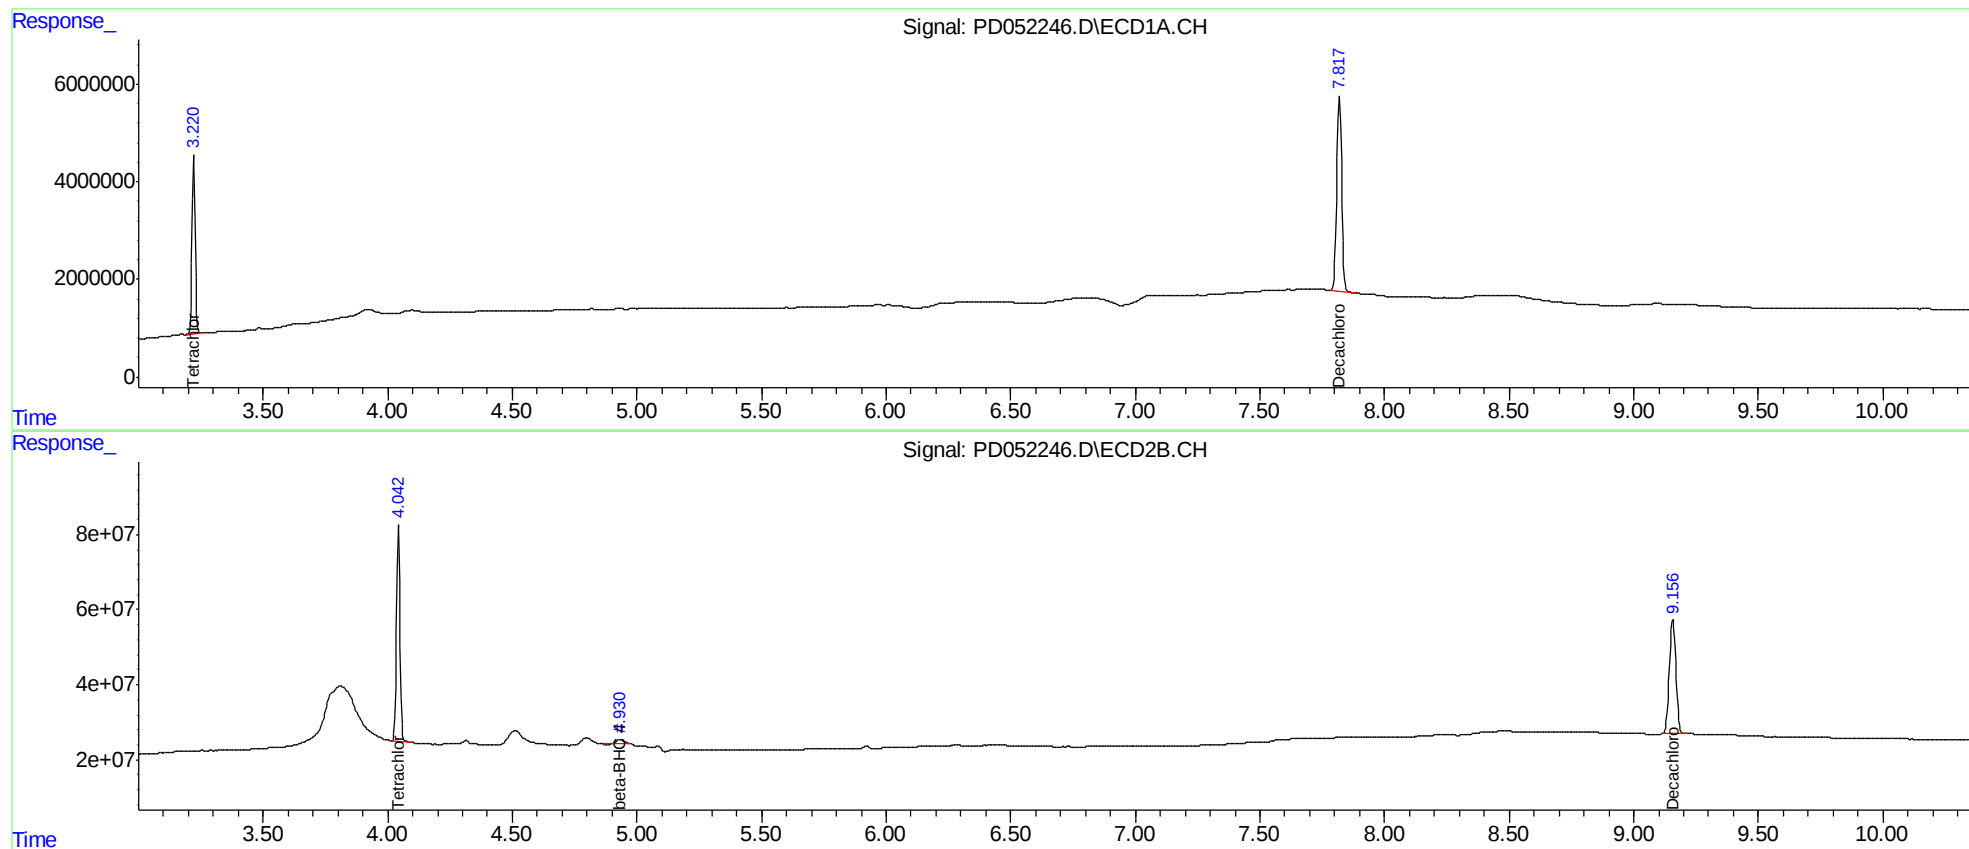


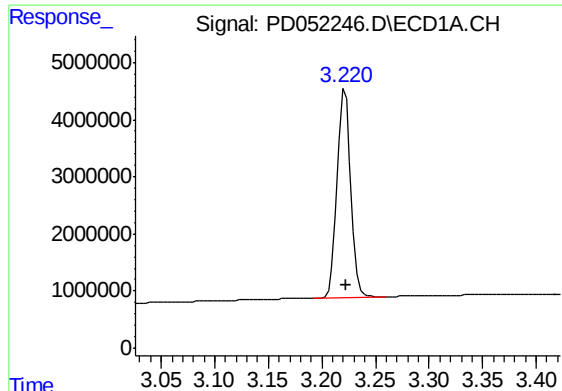

#1 Tetrachloro-m-xylene


R.T.: 3.222 min
Delta R.T.: 0.000 min
Response: 32375142
Conc: 22.81 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK07

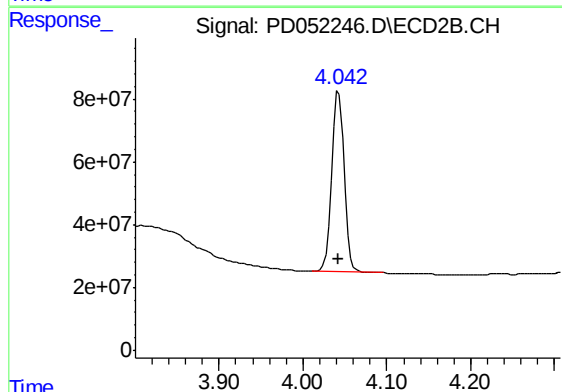


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 598828173
Conc: 20.58 ng/ml

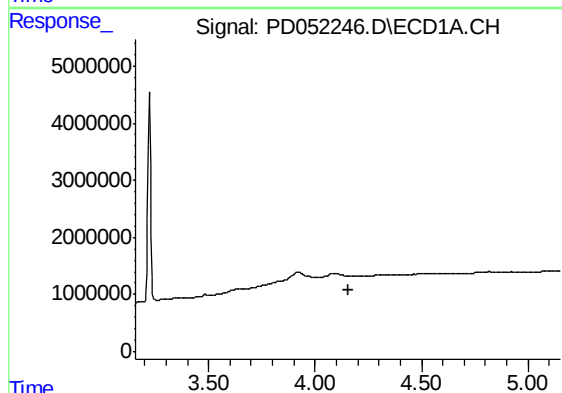


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.154 min
Response: 0
Conc: N.D.

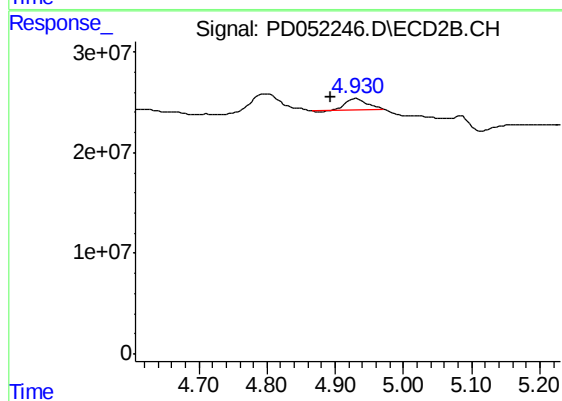

#6 beta-BHC


R.T.: 4.931 min
Delta R.T.: 0.038 min
Response: 21409685
Conc: 1.17 ng/ml

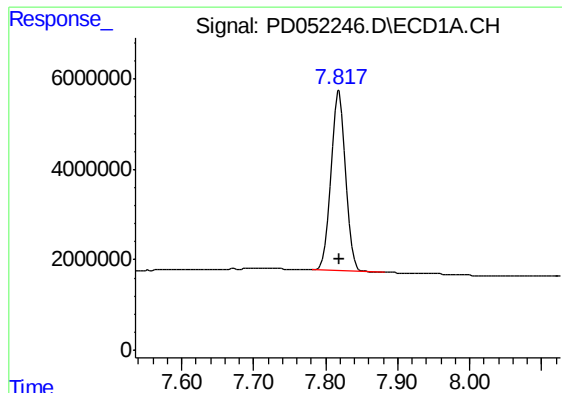

#27 Decachlorobiphenyl

R.T.: 7.819 min
Delta R.T.: 0.000 min
Response: 56229016
Conc: 35.91 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK07

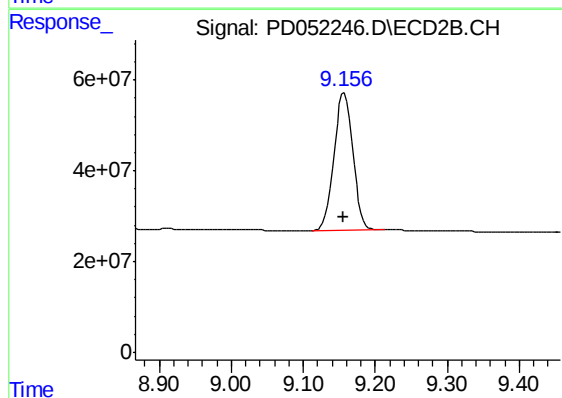

#27 Decachlorobiphenyl

R.T.: 9.157 min
Delta R.T.: 0.001 min
Response: 552077069
Conc: 35.76 ng/ml