

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032819\
 Data File : PD052248.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Mar 2019 17:40
 Operator : AJ\SJ
 Sample : PB118312BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PBLK12

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 01:36:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032519CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 25 18:59:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1) SA	Tetrachlo...	3.221	4.042	29302993	569.8E6	20.644	19.582
27) SA	Decachlor...	7.817	9.154	48594078	495.8E6	31.033	32.118
Target Compounds							
6) B	beta-BHC	0.000	4.931f	0 28411157	N.D.		1.548
8) B	Heptachlo...	0.000	5.919	0 13340196	N.D.		0.392
9) A	Endosulfan I	0.000	6.283	0 8895172	N.D.		0.284
10) B	trans-Chl...	0.000	6.135	0 12425908	N.D.		0.366
11) B	cis-Chlor...	0.000	6.283f	0 8895172	N.D.		0.274


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032819\
Data File : PD052248.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Mar 2019 17:40
Operator : AJ\SJ
Sample : PB118312BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PBLK12

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 01:36:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032519CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 25 18:59:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

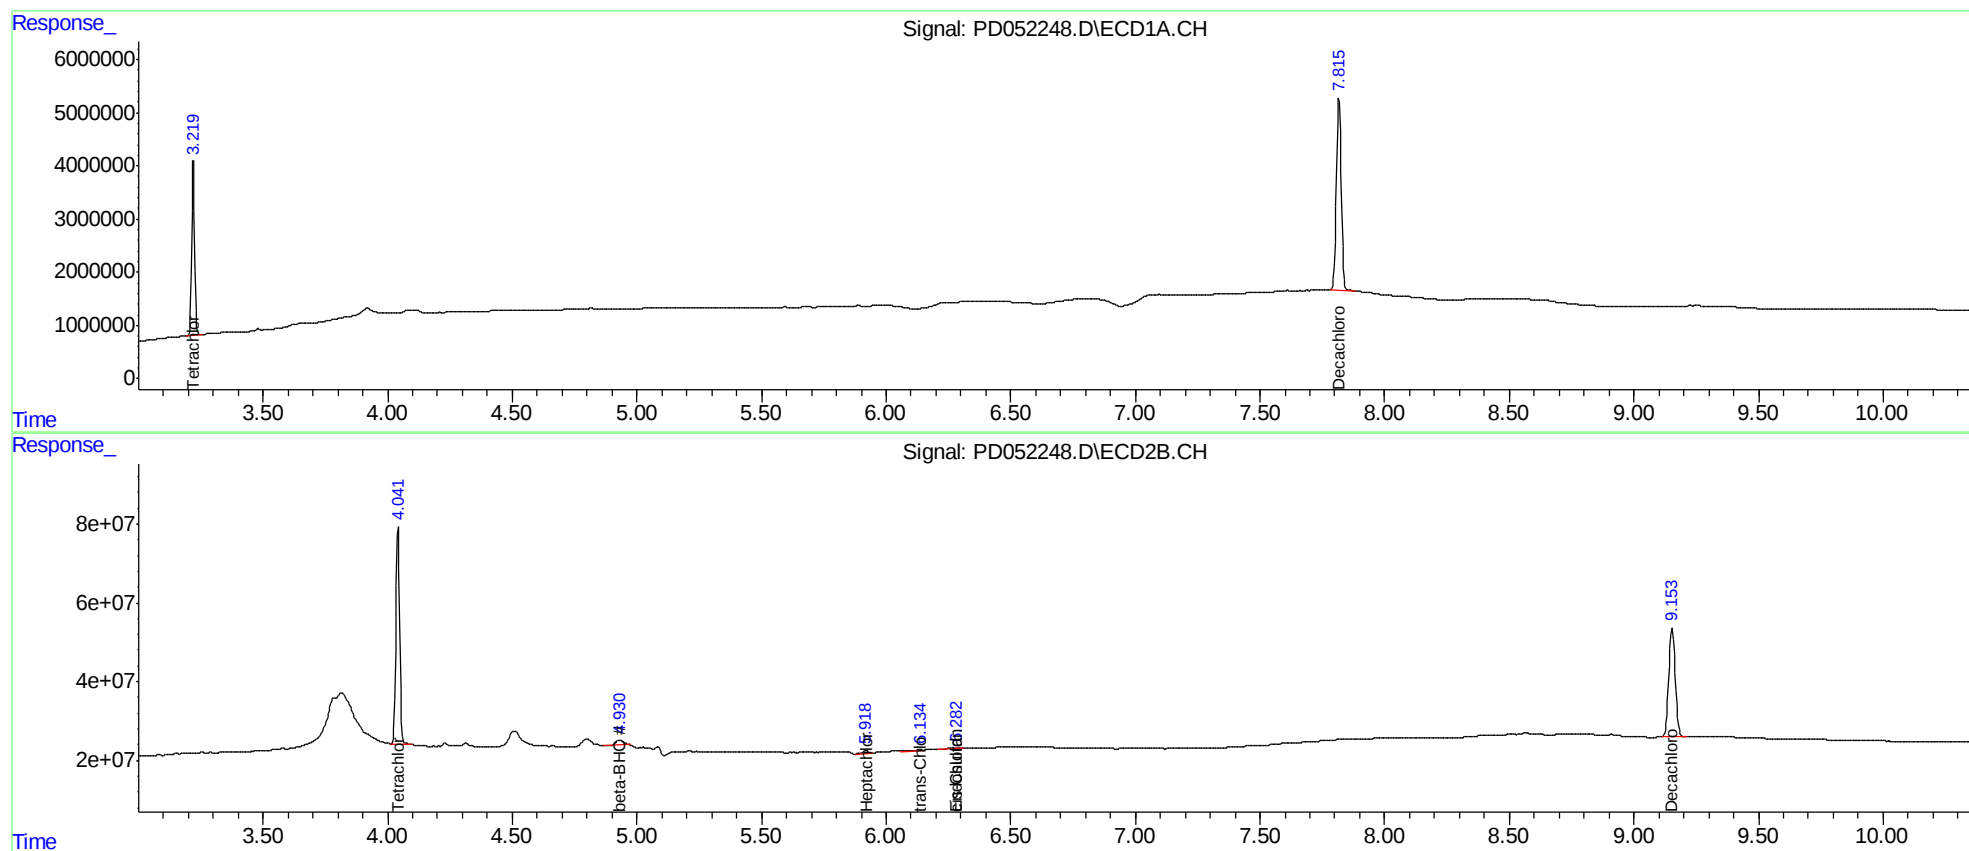


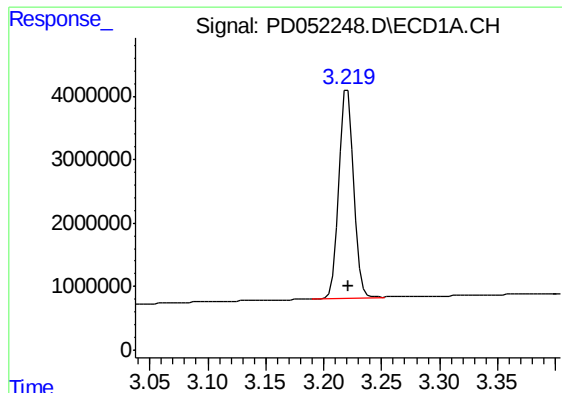

#1 Tetrachloro-m-xylene


R.T.: 3.221 min
Delta R.T.: -0.001 min
Response: 29302993
Conc: 20.64 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK12

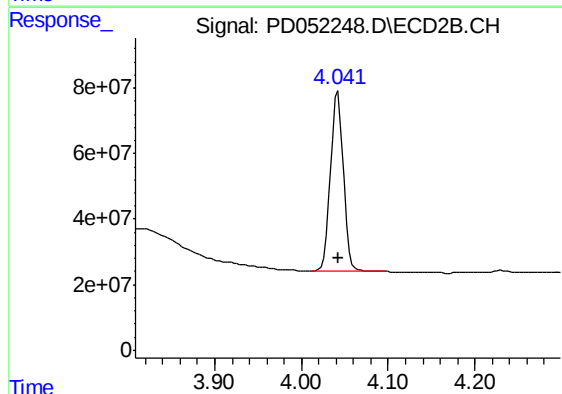


#1 Tetrachloro-m-xylene

R.T.: 4.042 min
Delta R.T.: 0.000 min
Response: 569781303
Conc: 19.58 ng/ml

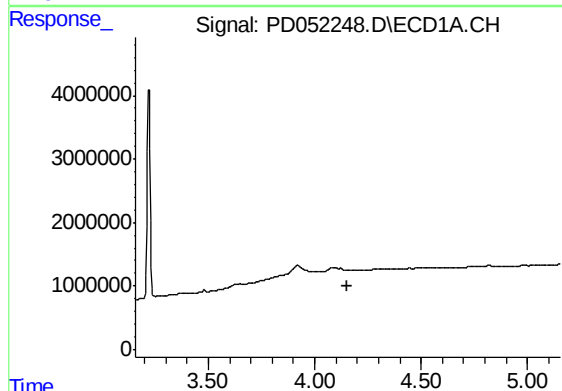


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.154 min
Response: 0
Conc: N.D.

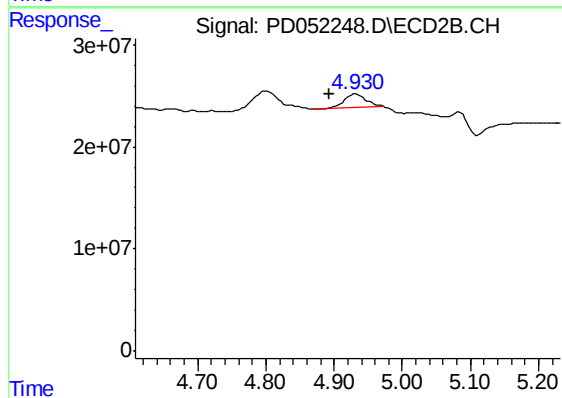

#6 beta-BHC


R.T.: 4.931 min
Delta R.T.: 0.038 min
Response: 28411157
Conc: 1.55 ng/ml

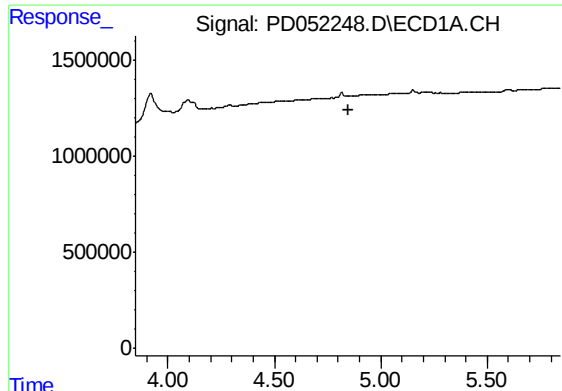

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.846 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PBLK12

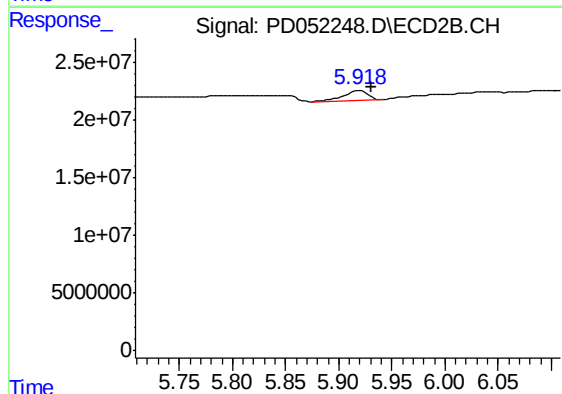


#8 Heptachlor epoxide

R.T.: 5.919 min
Delta R.T.: -0.011 min
Response: 13340196
Conc: 0.39 ng/ml

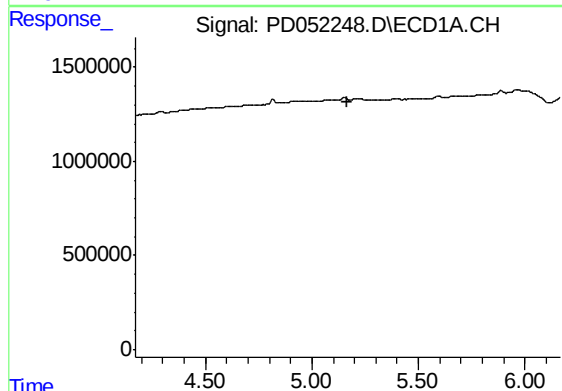


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.168 min
Response: 0
Conc: N.D.

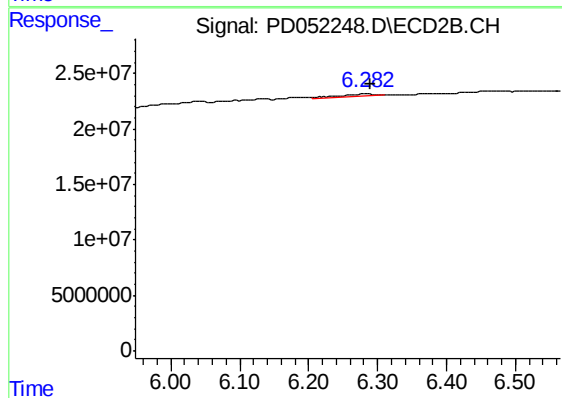

#9 Endosulfan I


R.T.: 6.283 min
Delta R.T.: -0.006 min
Response: 8895172
Conc: 0.28 ng/ml

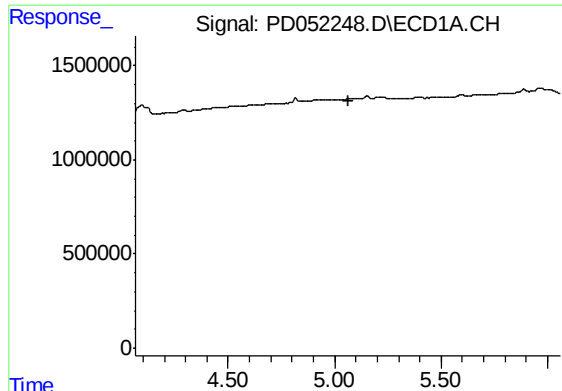

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.063 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PBLK12

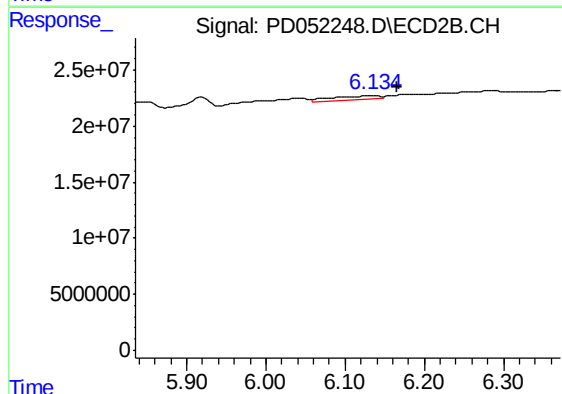


#10 trans-Chlordane

R.T.: 6.135 min
Delta R.T.: -0.030 min
Response: 12425908
Conc: 0.37 ng/ml

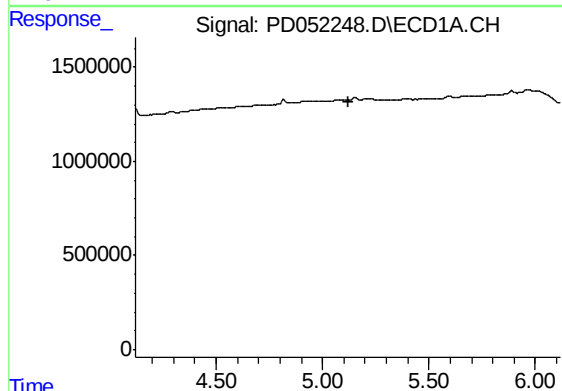


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.119 min
Response: 0
Conc: N.D.

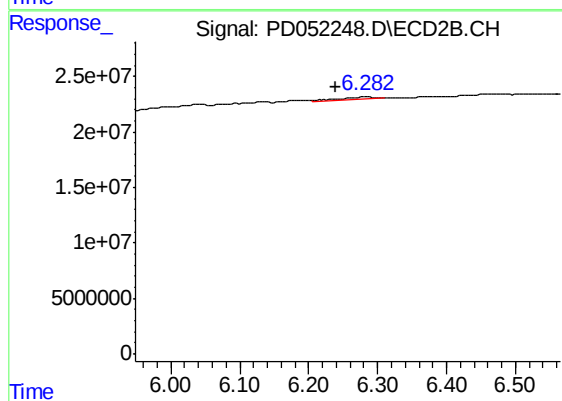

#11 cis-Chlordane


R.T.: 6.283 min
Delta R.T.: 0.045 min
Response: 8895172
Conc: 0.27 ng/ml

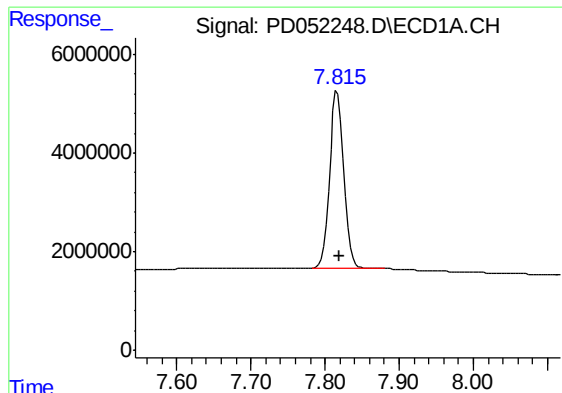

#27 Decachlorobiphenyl

R.T.: 7.817 min
Delta R.T.: -0.002 min
Response: 48594078
Conc: 31.03 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK12

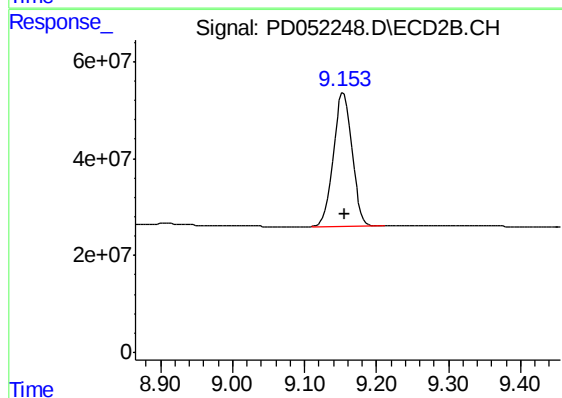

#27 Decachlorobiphenyl

R.T.: 9.154 min
Delta R.T.: -0.002 min
Response: 495798915
Conc: 32.12 ng/ml