

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032819\
 Data File : PD052250.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Mar 2019 18:09
 Operator : AJ\SJ
 Sample : K2068-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BF5M7

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 01:36:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032519CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 25 18:59:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.221	4.042	28662216	485.1E6	20.193	16.673
27)	SA Decachlor...	7.818	9.154	32112783	341.5E6	20.508	22.122
Target Compounds							
2)	A alpha-BHC	0.000	4.405f	0	169.3E6	N.D.	3.872
3)	MA gamma-BHC...	0.000	4.686f	0	63794900	N.D.	1.606
4)	MA Heptachlor	0.000	5.254	0	48514284	N.D.	1.210
6)	B beta-BHC	0.000	4.934f	0	20667282	N.D.	1.126
7)	B delta-BHC	0.000	5.072f	0	31935416	N.D.	0.805
8)	B Heptachlo...	0.000	5.911	0	65812491	N.D.	1.932
9)	A Endosulfan I	0.000	6.283	0	9690546	N.D.	0.309
10)	B trans-Chl...	0.000	6.178	0	70804309	N.D.	2.085
11)	B cis-Chlor...	0.000	6.235	0	42825682	N.D.	1.319
13)	MA Dieldrin	0.000	6.526	0	17381609	N.D.	0.558
15)	B Endosulfa...	0.000	6.983	0	19471490	N.D.	0.768


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032819\
Data File : PD052250.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Mar 2019 18:09
Operator : AJ\SJ
Sample : K2068-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
BF5M7

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 01:36:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032519CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 25 18:59:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

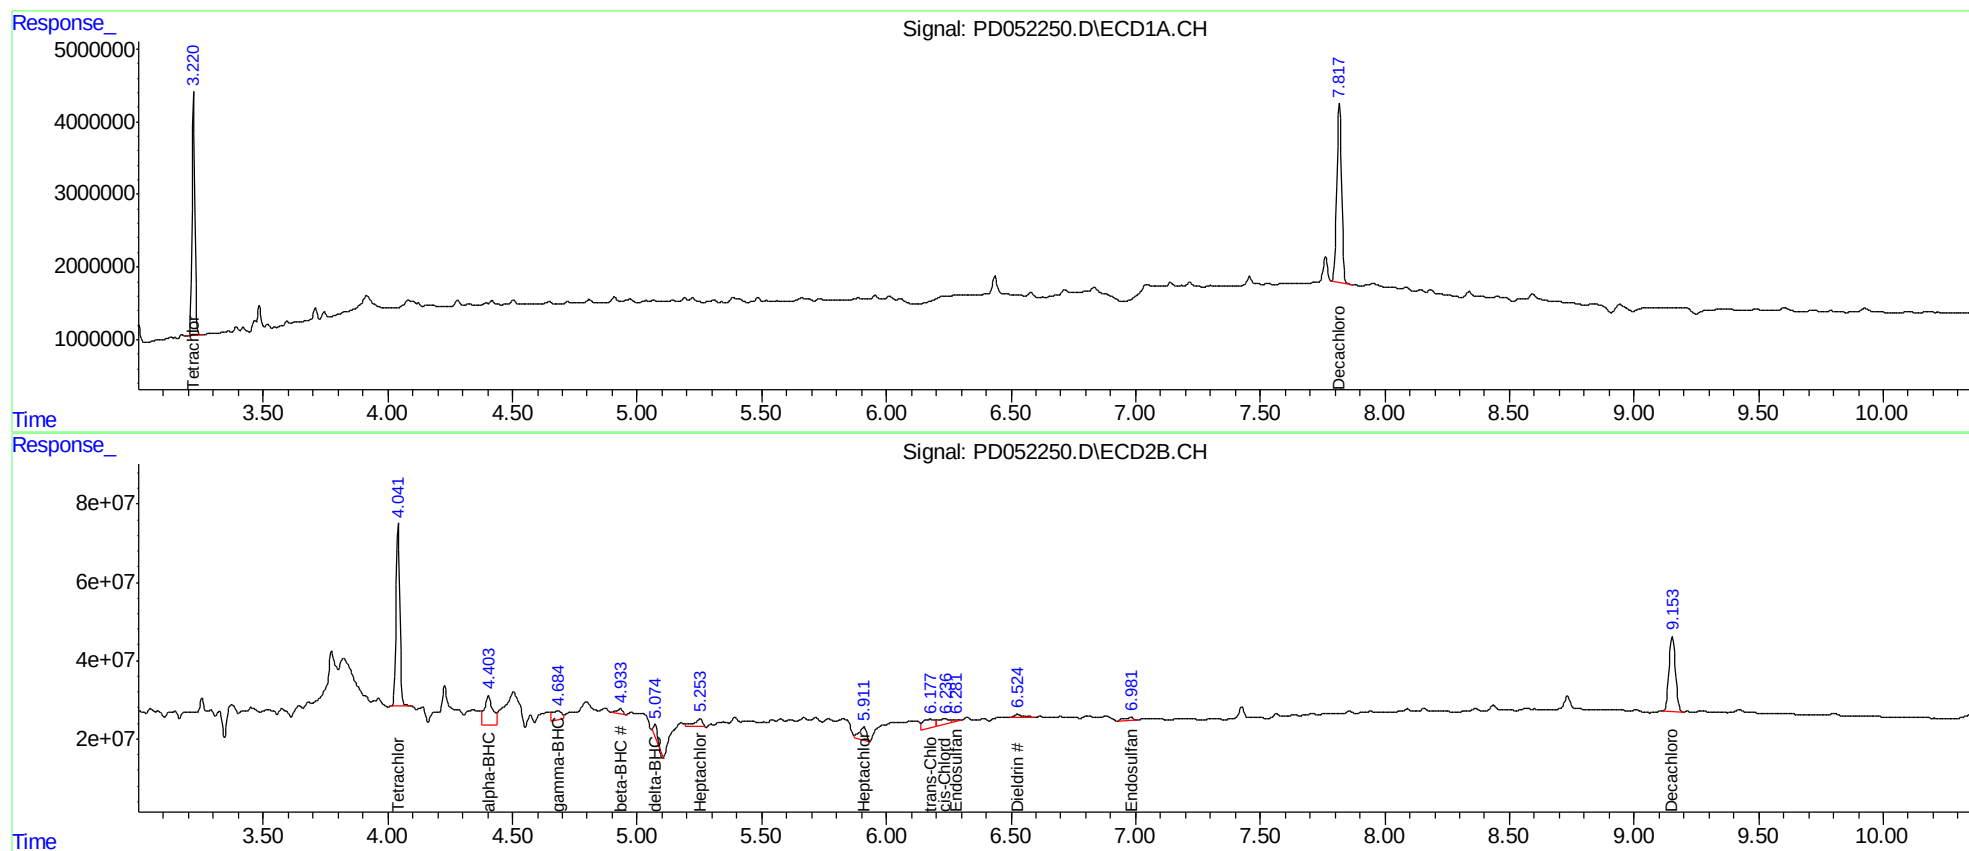


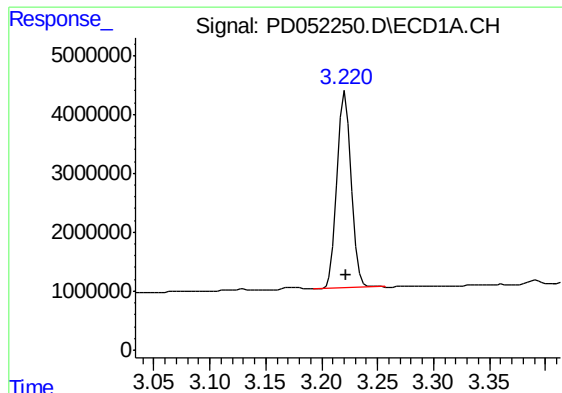

#1 Tetrachloro-m-xylene


R.T.: 3.221 min
Delta R.T.: 0.000 min
Response: 28662216
Conc: 20.19 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF5M7

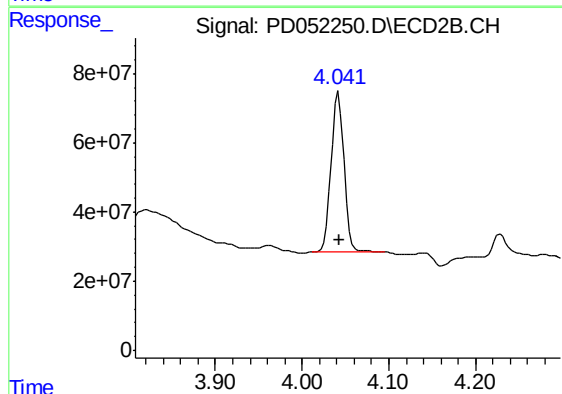


#1 Tetrachloro-m-xylene

R.T.: 4.042 min
Delta R.T.: 0.000 min
Response: 485146962
Conc: 16.67 ng/ml

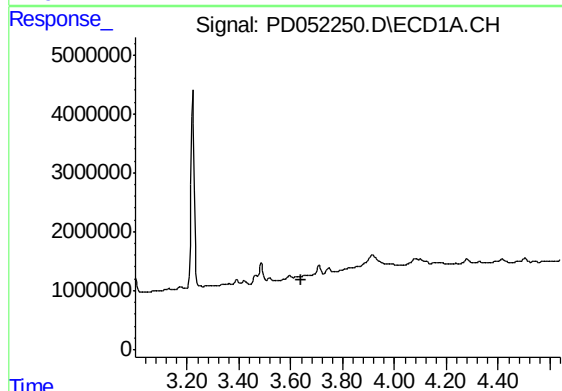


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.641 min
Response: 0
Conc: N.D.

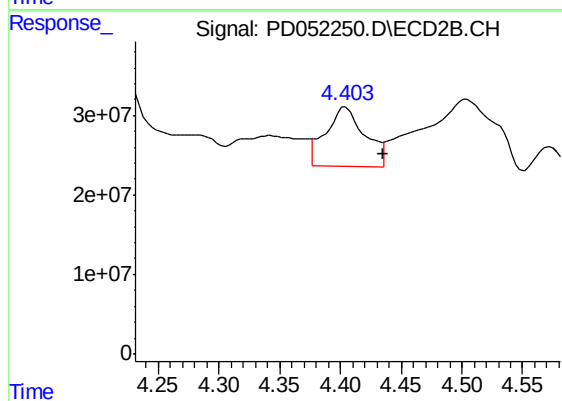

#2 alpha-BHC


R.T.: 4.405 min
Delta R.T.: -0.031 min
Response: 169317772
Conc: 3.87 ng/ml

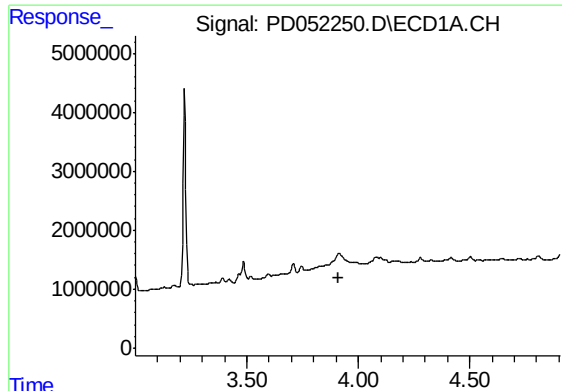

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 3.910 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5M7

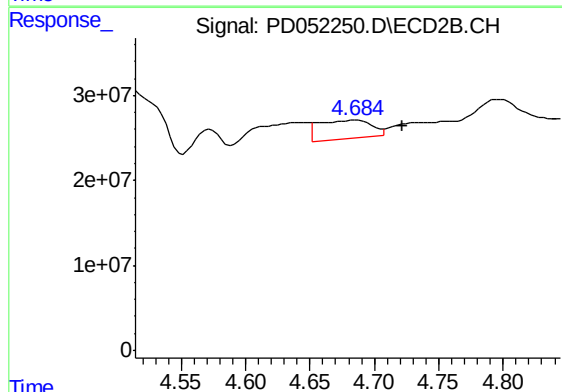


#3 gamma-BHC (Lindane)

R.T.: 4.686 min
Delta R.T.: -0.036 min
Response: 63794900
Conc: 1.61 ng/ml

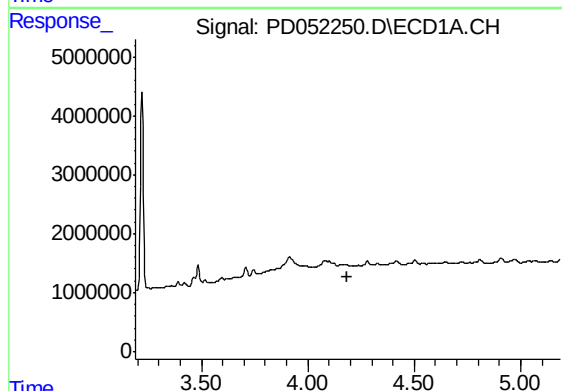


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.187 min
Response: 0
Conc: N.D.

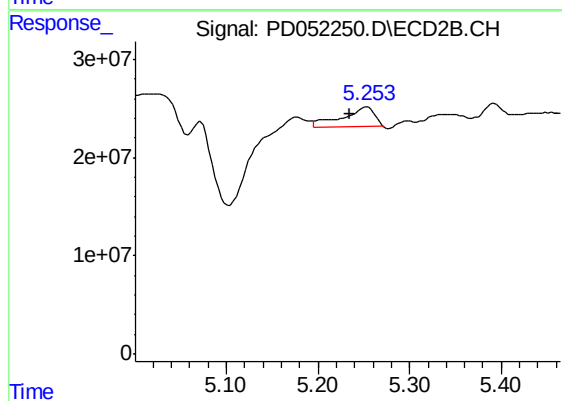

#4 Heptachlor


R.T.: 5.254 min
Delta R.T.: 0.019 min
Response: 48514284
Conc: 1.21 ng/ml

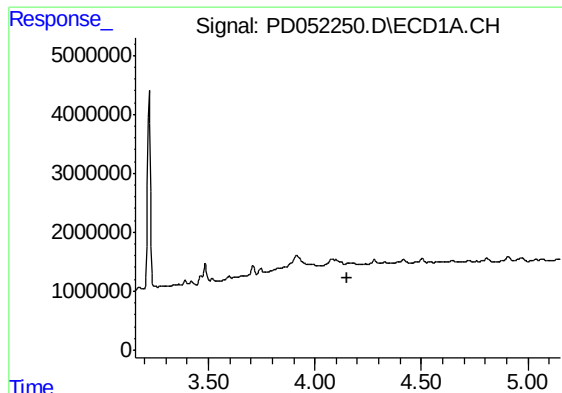

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.154 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5M7

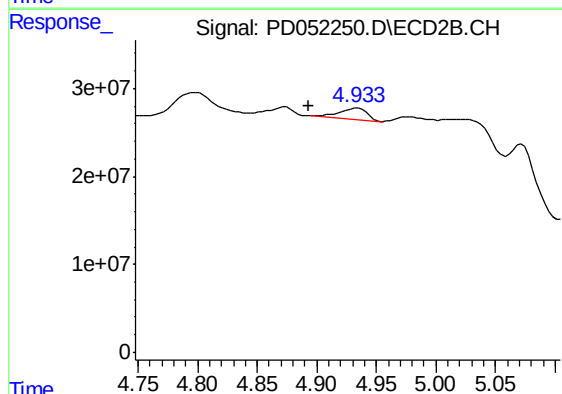


#6 beta-BHC

R.T.: 4.934 min
Delta R.T.: 0.041 min
Response: 20667282
Conc: 1.13 ng/ml

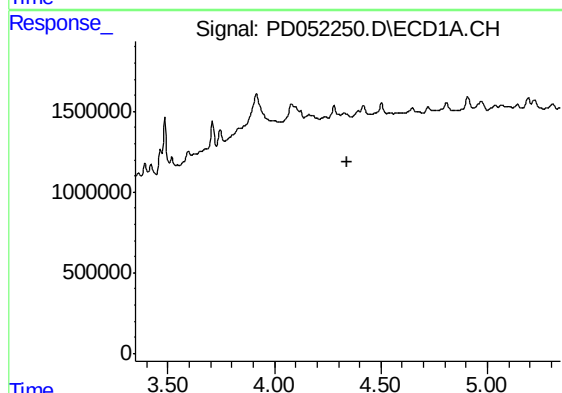


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.344 min
Response: 0
Conc: N.D.

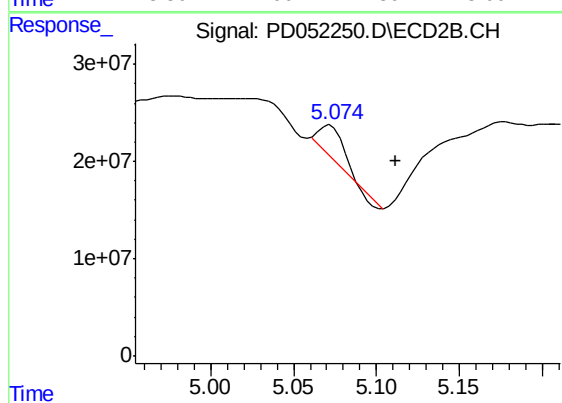

#7 delta-BHC


R.T.: 5.072 min
Delta R.T.: -0.040 min
Response: 31935416
Conc: 0.80 ng/ml

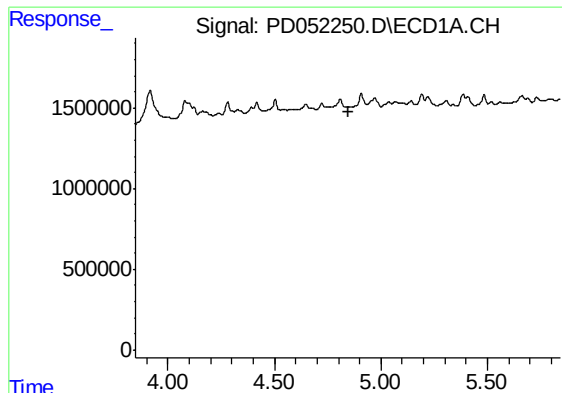

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.846 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5M7

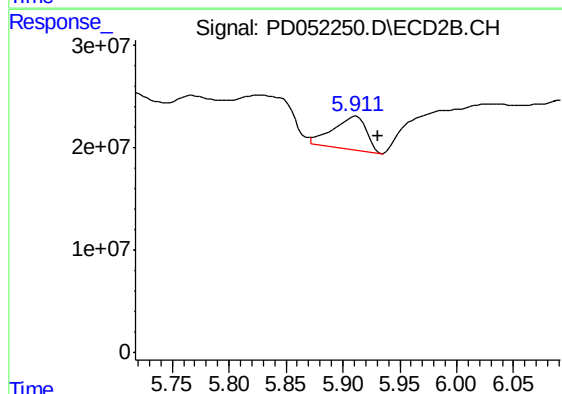


#8 Heptachlor epoxide

R.T.: 5.911 min
Delta R.T.: -0.019 min
Response: 65812491
Conc: 1.93 ng/ml

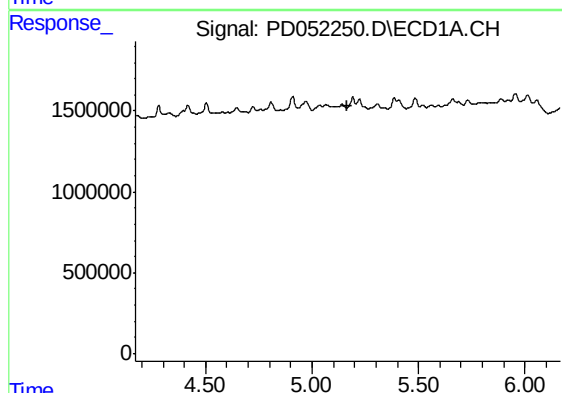


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.168 min
Response: 0
Conc: N.D.

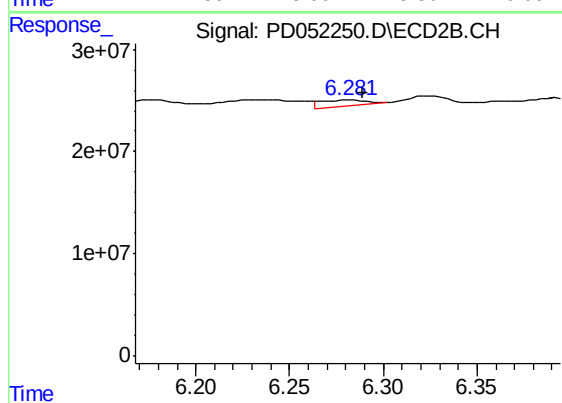

#9 Endosulfan I


R.T.: 6.283 min
Delta R.T.: -0.007 min
Response: 9690546
Conc: 0.31 ng/ml

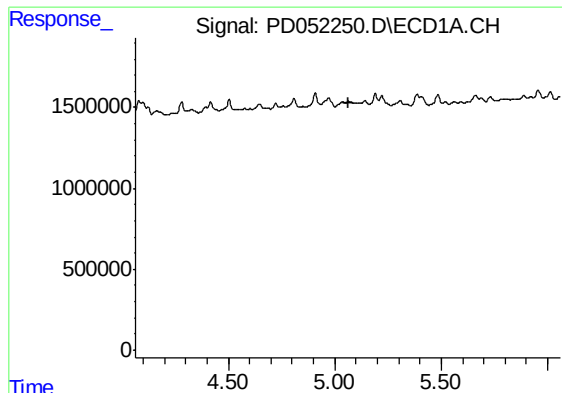

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.063 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5M7

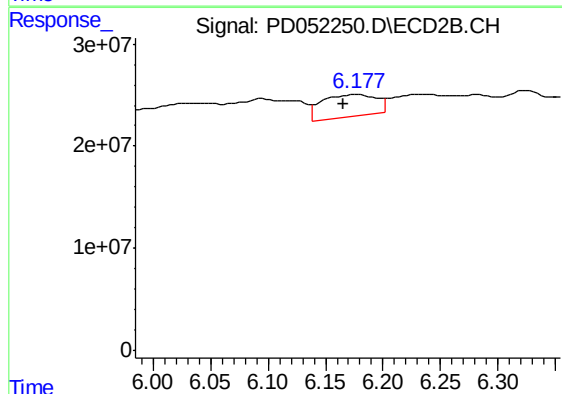


#10 trans-Chlordane

R.T.: 6.178 min
Delta R.T.: 0.012 min
Response: 70804309
Conc: 2.08 ng/ml

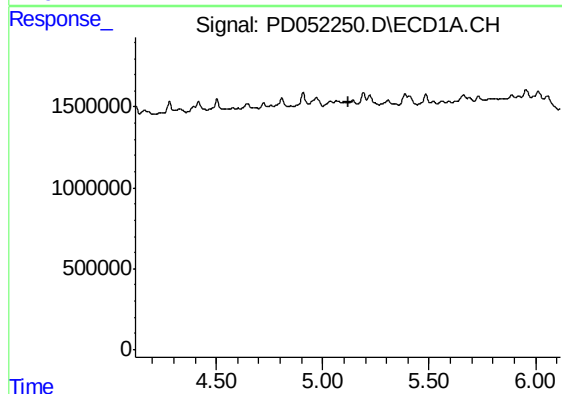


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.119 min
Response: 0
Conc: N.D.

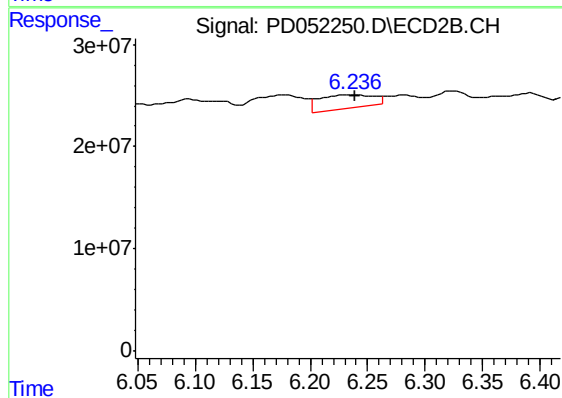

#11 cis-Chlordane


R.T.: 6.235 min
Delta R.T.: -0.004 min
Response: 42825682
Conc: 1.32 ng/ml

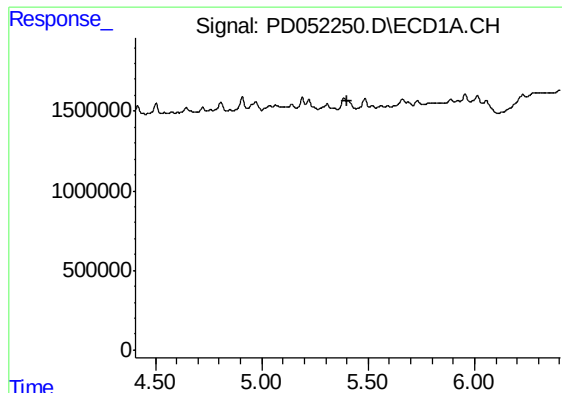

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 5.404 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5M7

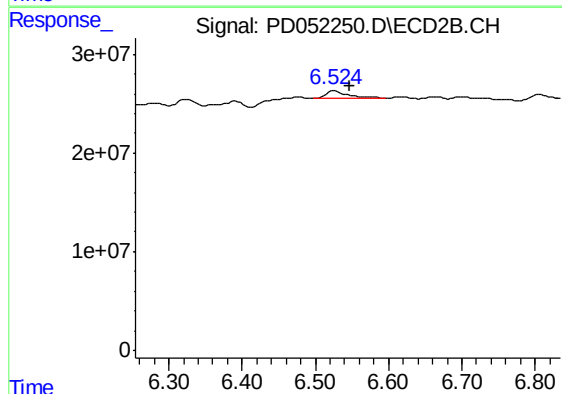


#13 Dieldrin

R.T.: 6.526 min
Delta R.T.: -0.022 min
Response: 17381609
Conc: 0.56 ng/ml

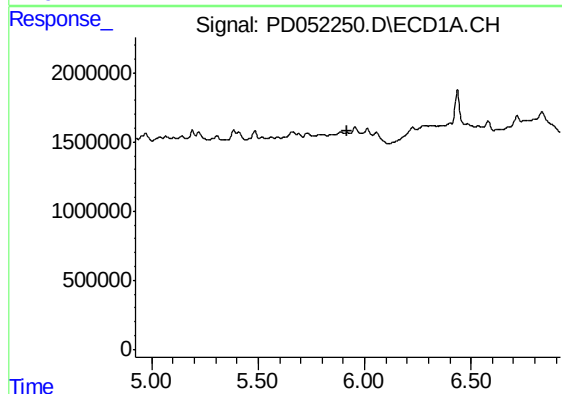


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 5.920 min
Response: 0
Conc: N.D.

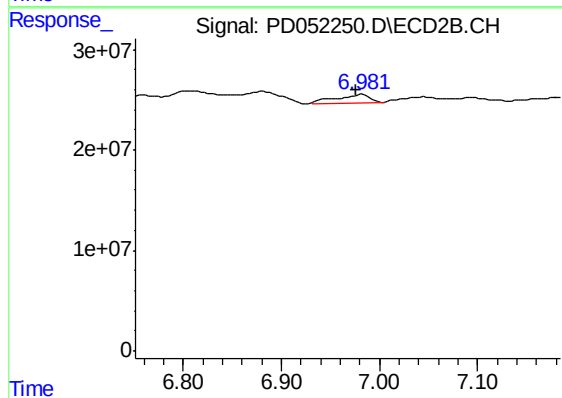

#15 Endosulfan II


R.T.: 6.983 min
Delta R.T.: 0.007 min
Response: 19471490
Conc: 0.77 ng/ml

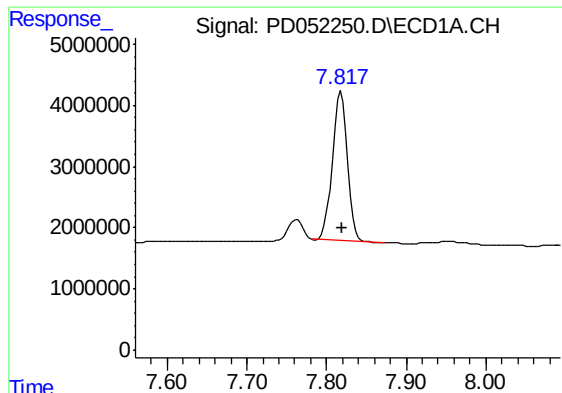

#27 Decachlorobiphenyl

R.T.: 7.818 min
Delta R.T.: -0.001 min
Response: 32112783
Conc: 20.51 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF5M7

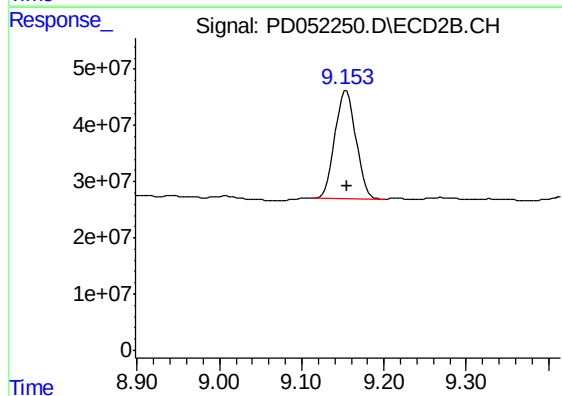

#27 Decachlorobiphenyl

R.T.: 9.154 min
Delta R.T.: -0.002 min
Response: 341484409
Conc: 22.12 ng/ml