

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032819\
 Data File : PD052257.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Mar 2019 19:48
 Operator : AJ\SJ
 Sample : K2068-17
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BF5L1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 01:38:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032519CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 25 18:59:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.221	4.042	22732290	462.9E6	16.015	15.907
27)	SA Decachlor...	7.817	9.154	31212138	340.5E6	19.933	22.055
Target Compounds							
2)	A alpha-BHC	0.000	4.405f	0 14079120	N.D.	0.322	
3)	MA gamma-BHC...	3.921	0.000	9181456	0 4.097	N.D.	#
6)	B beta-BHC	0.000	4.934f	0 16354607	N.D.	0.891	
8)	B Heptachlo...	0.000	5.909	0 64850949	N.D.	1.904	
9)	A Endosulfan I	0.000	6.264	0 62673702	N.D.	1.999	
10)	B trans-Chl...	0.000	6.125f	0 80475785	N.D.	2.370	
11)	B cis-Chlor...	0.000	6.264	0 62673702	N.D.	1.930	
15)	B Endosulfa...	0.000	6.974	0 53667771	N.D.	2.117	


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032819\
Data File : PD052257.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Mar 2019 19:48
Operator : AJ\SJ
Sample : K2068-17
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
BF5L1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 01:38:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032519CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 25 18:59:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

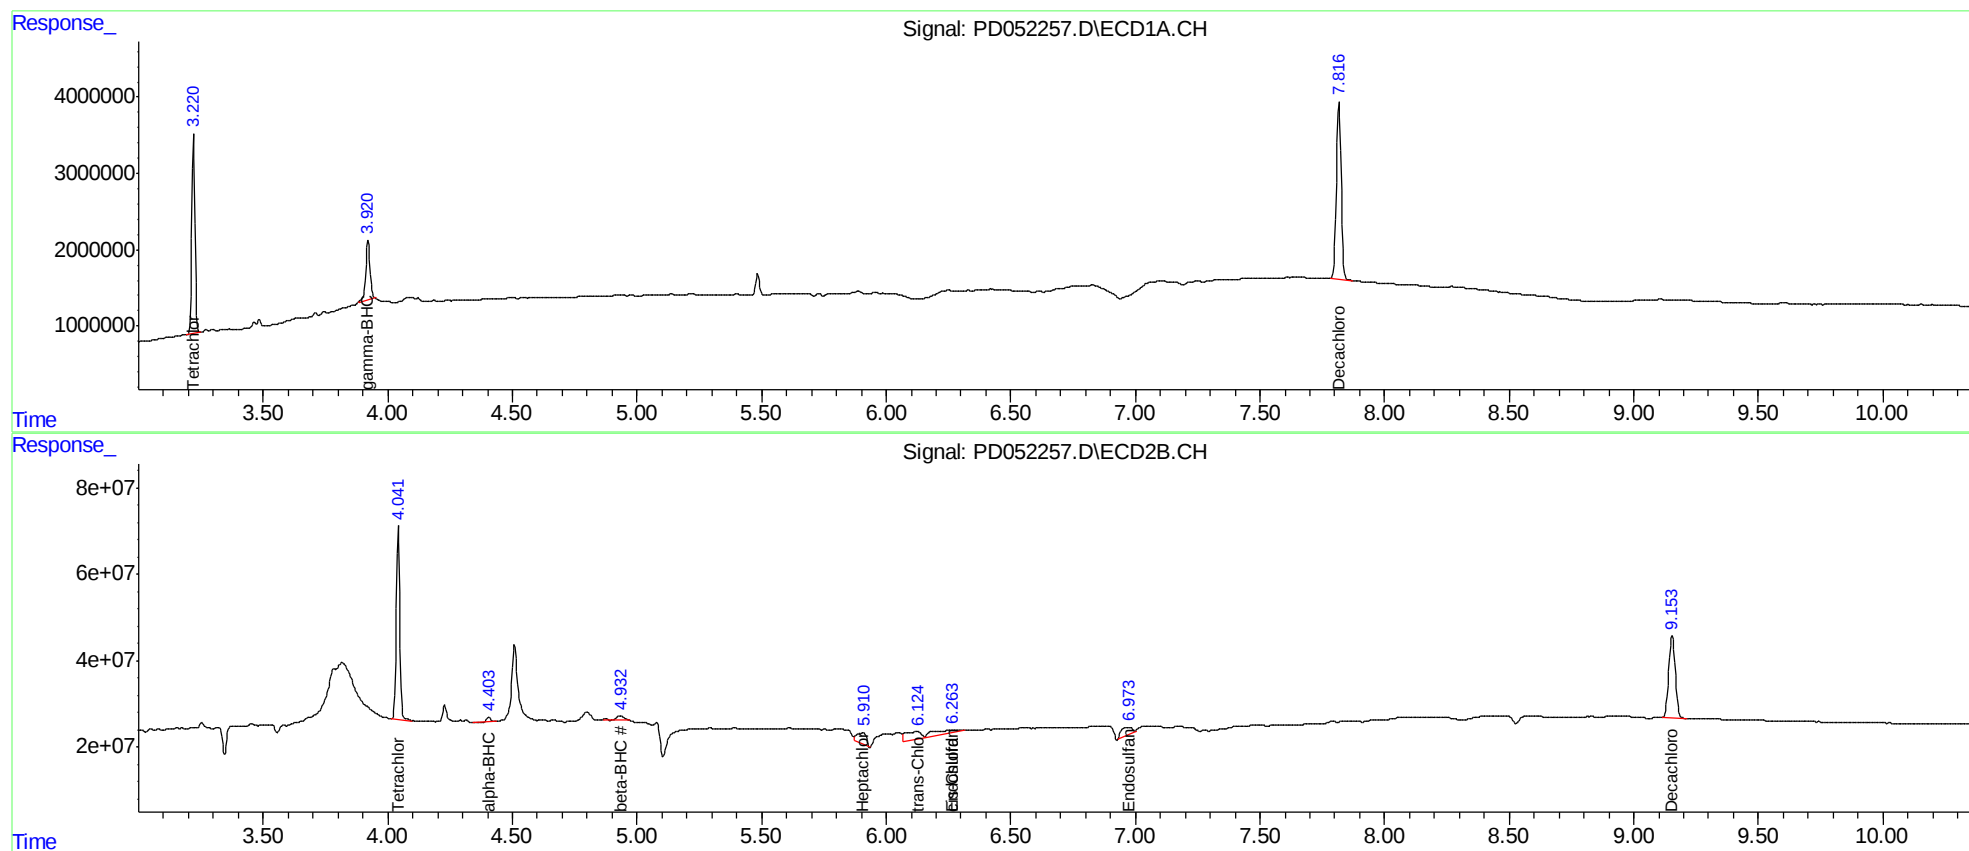


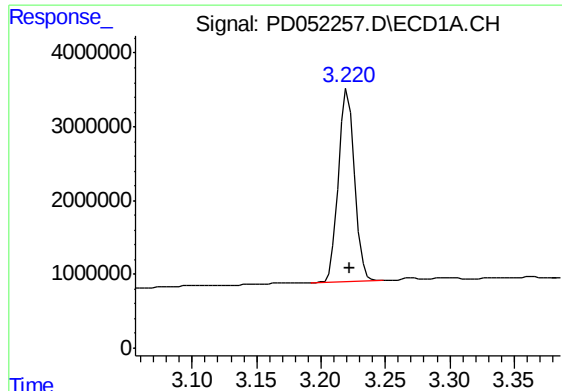

#1 Tetrachloro-m-xylene


R.T.: 3.221 min
Delta R.T.: -0.001 min
Response: 22732290
Conc: 16.02 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF5L1

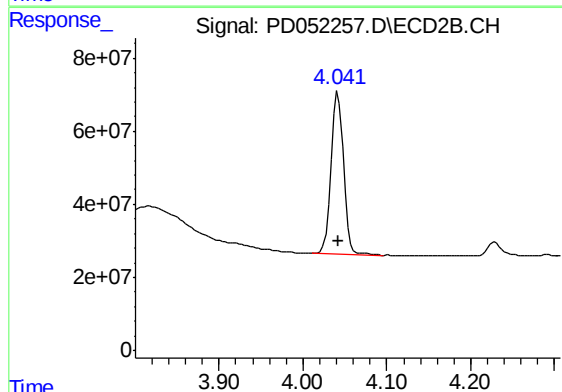


#1 Tetrachloro-m-xylene

R.T.: 4.042 min
Delta R.T.: 0.000 min
Response: 462856010
Conc: 15.91 ng/ml

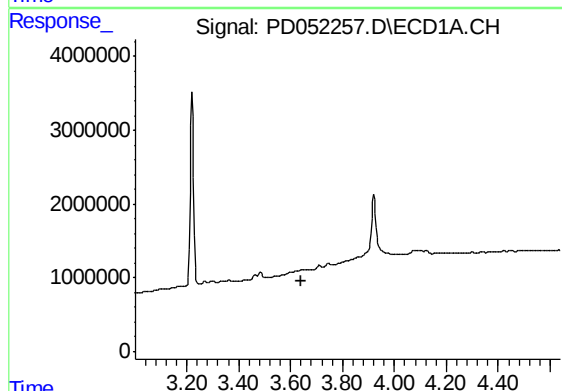


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.641 min
Response: 0
Conc: N.D.

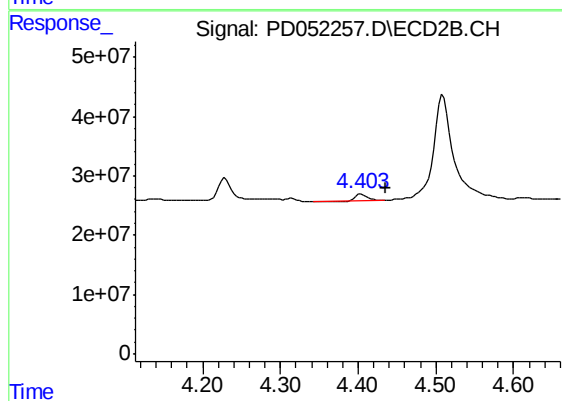

#2 alpha-BHC


R.T.: 4.405 min
Delta R.T.: -0.030 min
Response: 14079120
Conc: 0.32 ng/ml

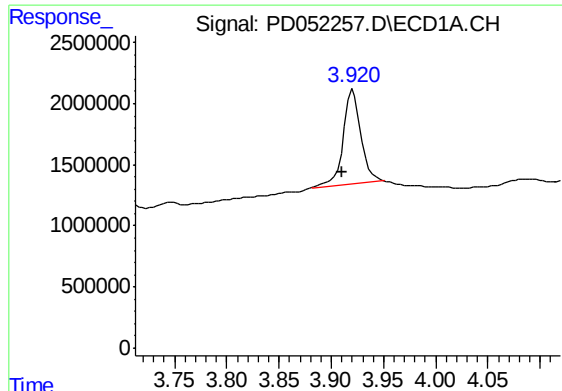

#3 gamma-BHC (Lindane)


R.T.: 3.921 min
Delta R.T.: 0.011 min
Response: 9181456
Conc: 4.10 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF5L1

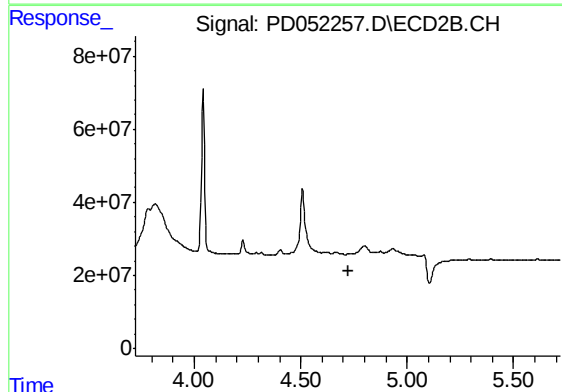


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.722 min
Response: 0
Conc: N.D.

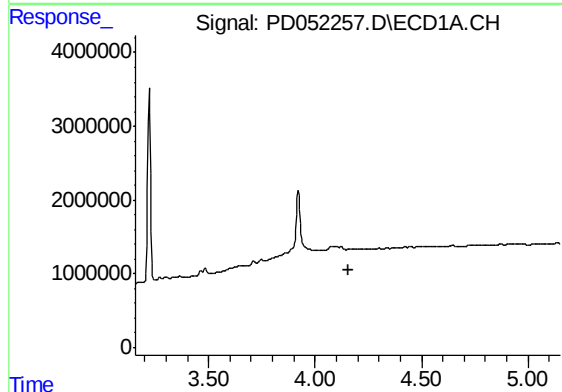


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.154 min
Response: 0
Conc: N.D.

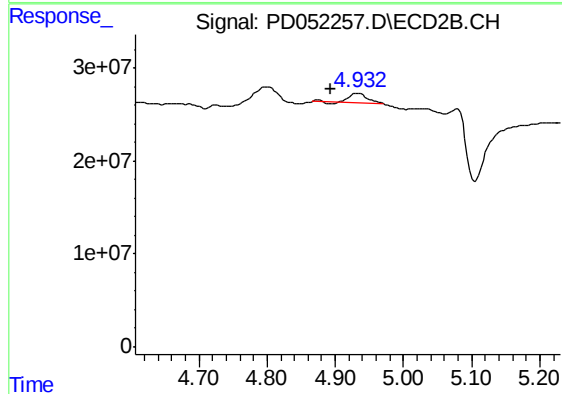

#6 beta-BHC


R.T.: 4.934 min
Delta R.T.: 0.041 min
Response: 16354607
Conc: 0.89 ng/ml

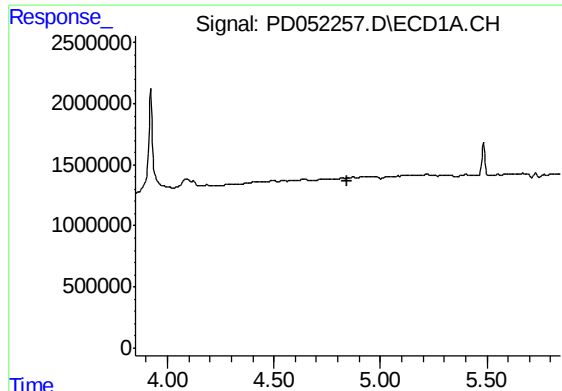

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.846 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5L1

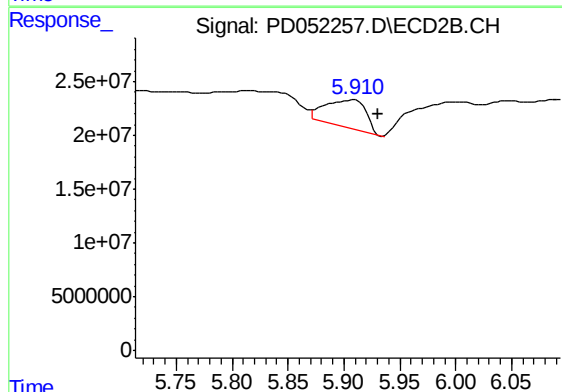


#8 Heptachlor epoxide

R.T.: 5.909 min
Delta R.T.: -0.022 min
Response: 64850949
Conc: 1.90 ng/ml

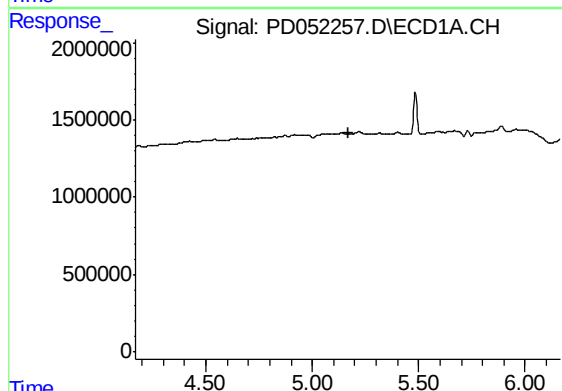


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.168 min
Response: 0
Conc: N.D.

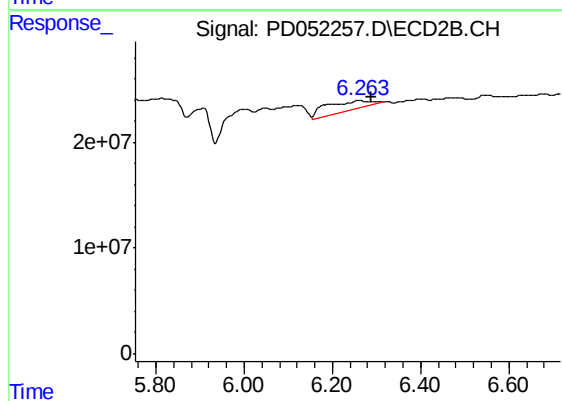

#9 Endosulfan I


R.T.: 6.264 min
Delta R.T.: -0.025 min
Response: 62673702
Conc: 2.00 ng/ml

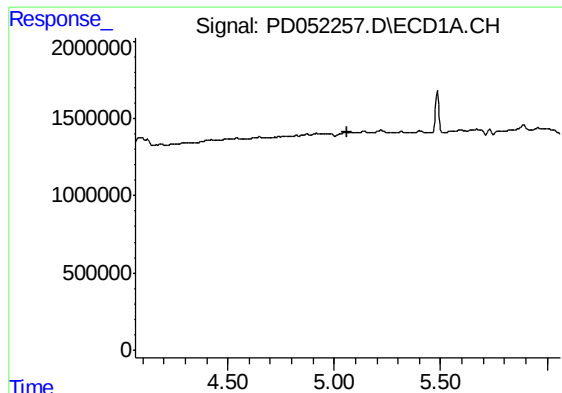

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.063 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5L1

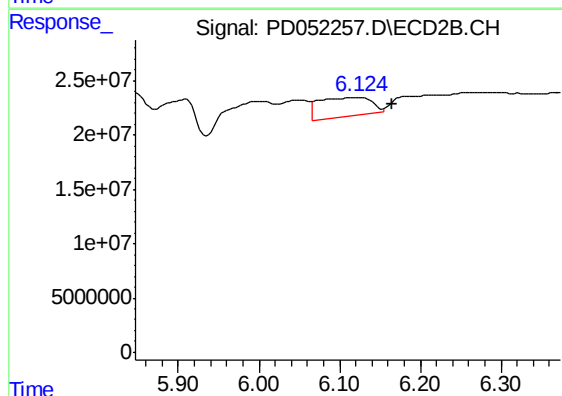


#10 trans-Chlordane

R.T.: 6.125 min
Delta R.T.: -0.040 min
Response: 80475785
Conc: 2.37 ng/ml

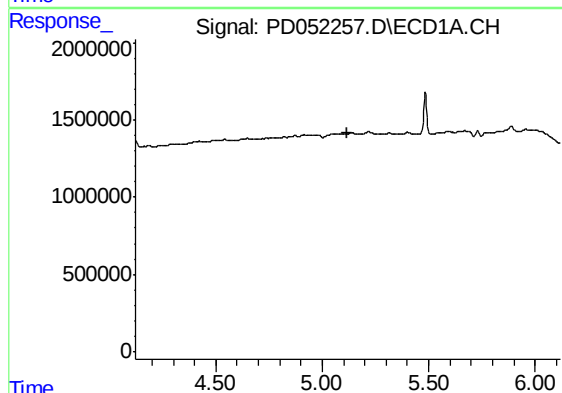


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.119 min
Response: 0
Conc: N.D.

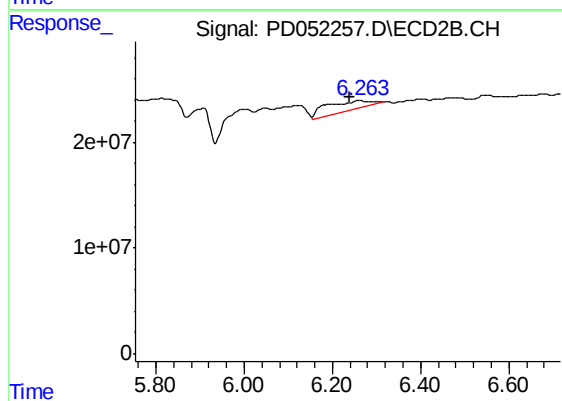

#11 cis-Chlordane


R.T.: 6.264 min
Delta R.T.: 0.026 min
Response: 62673702
Conc: 1.93 ng/ml

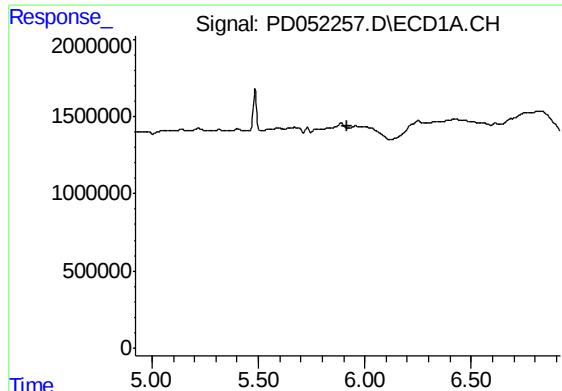

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.920 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5L1

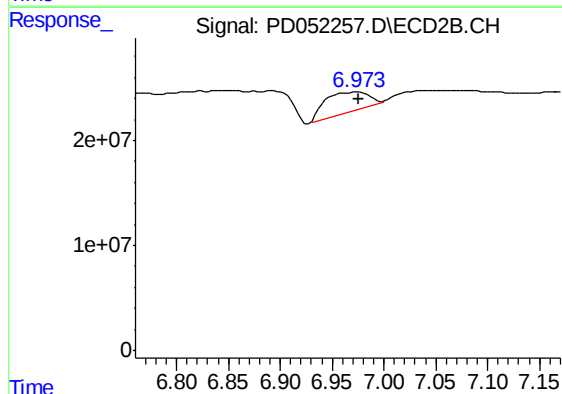


#15 Endosulfan II

R.T.: 6.974 min
Delta R.T.: -0.002 min
Response: 53667771
Conc: 2.12 ng/ml

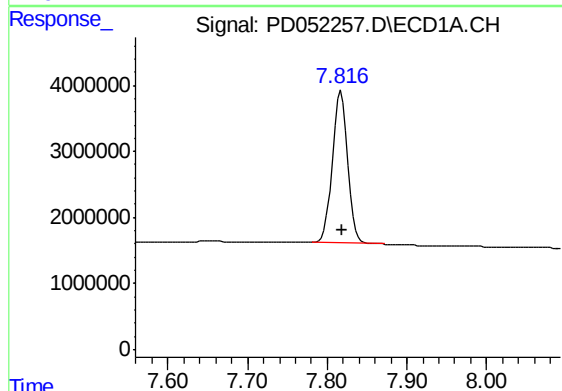

#27 Decachlorobiphenyl

R.T.: 7.817 min
Delta R.T.: -0.002 min
Response: 31212138
Conc: 19.93 ng/ml

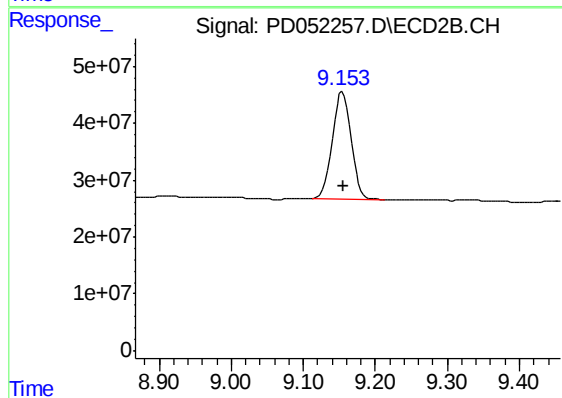

#27 Decachlorobiphenyl

R.T.: 9.154 min
Delta R.T.: -0.001 min
Response: 340453192
Conc: 22.05 ng/ml