

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032819\
 Data File : PD052259.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Mar 2019 20:16
 Operator : AJ\SJ
 Sample : K2068-24
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BF5K5

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 01:39:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032519CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 25 18:59:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1) SA	Tetrachlo...	3.221	4.042	16679682	342.6E6	11.751	11.775
27) SA	Decachlor...	7.816	9.154	19713053	216.6E6	12.589	14.034
Target Compounds							
2) A	alpha-BHC	0.000	4.405f	0	31169722	N.D.	0.713
6) B	beta-BHC	0.000	4.935f	0	5306675	N.D.	0.289
9) A	Endosulfan I	0.000	6.324	0	1991038	N.D.	<MDL
10) B	trans-Chl...	0.000	6.183	0	18693385	N.D.	0.550
11) B	cis-Chlor...	0.000	6.254	0	37221790	N.D.	1.146
15) B	Endosulfa...	0.000	6.983	0	11039003	N.D.	0.435


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032819\
Data File : PD052259.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Mar 2019 20:16
Operator : AJ\SJ
Sample : K2068-24
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
BF5K5

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 01:39:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032519CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 25 18:59:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

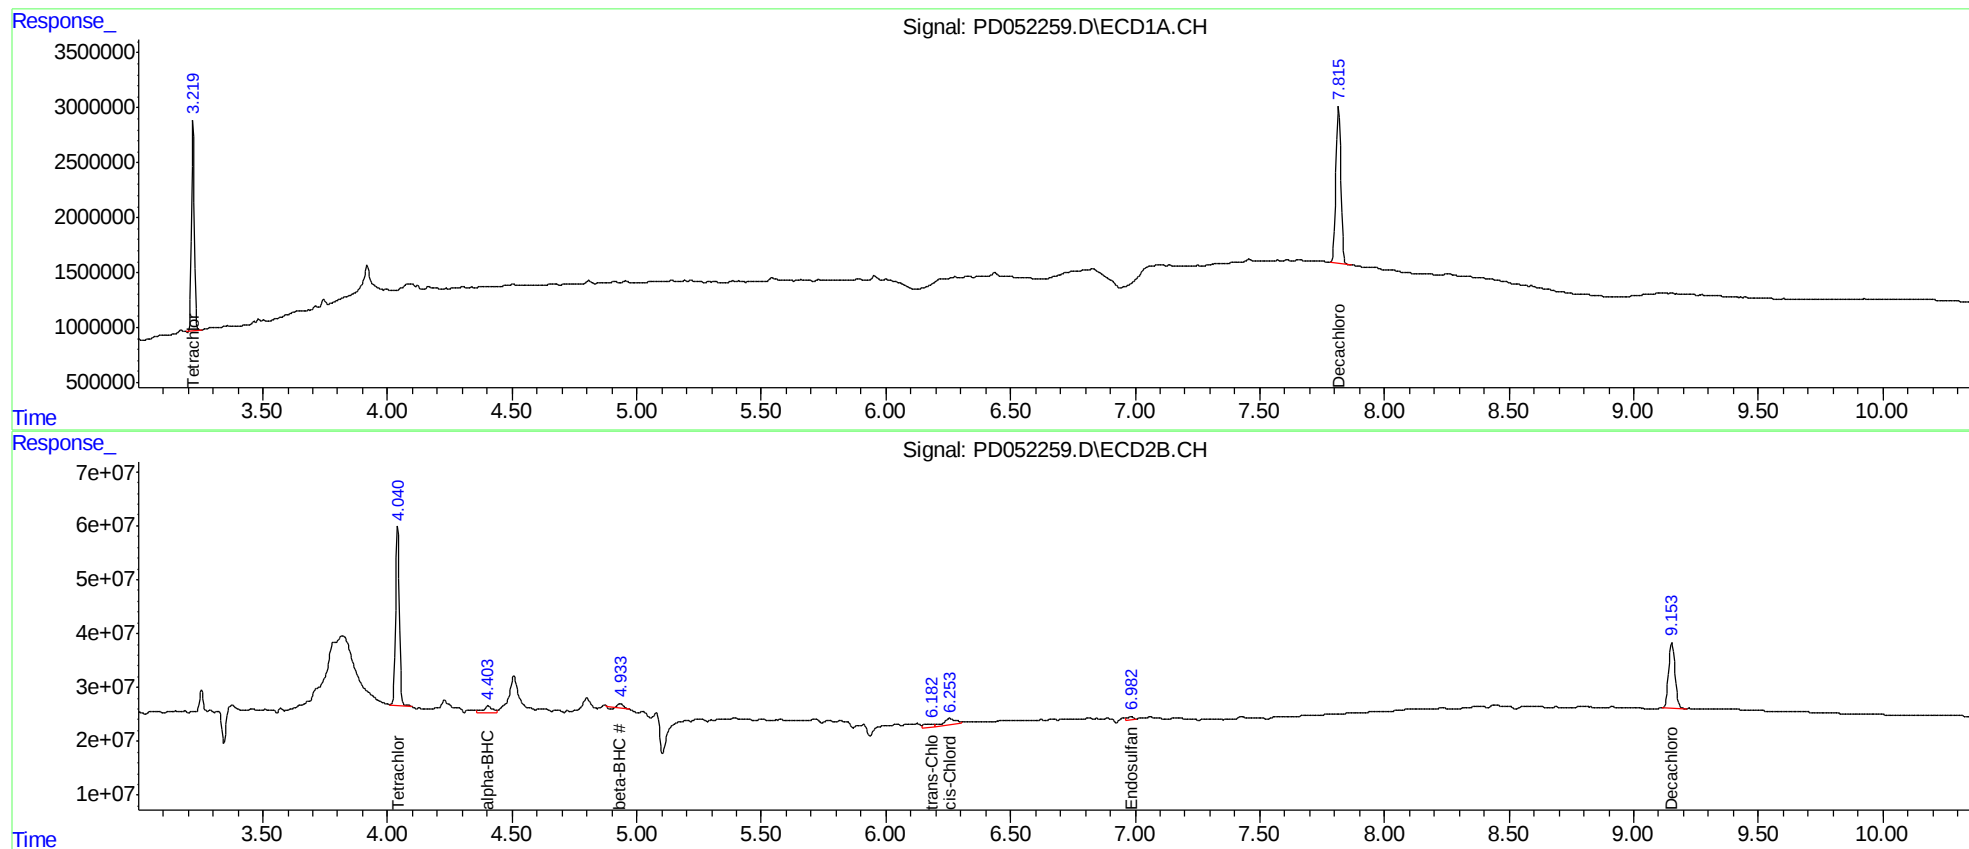


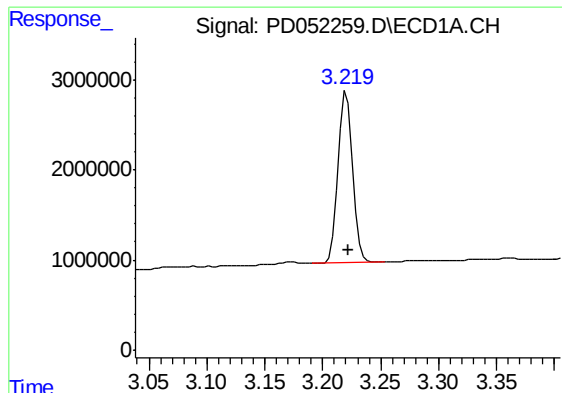

#1 Tetrachloro-m-xylene


R.T.: 3.221 min
Delta R.T.: -0.001 min
Response: 16679682
Conc: 11.75 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF5K5

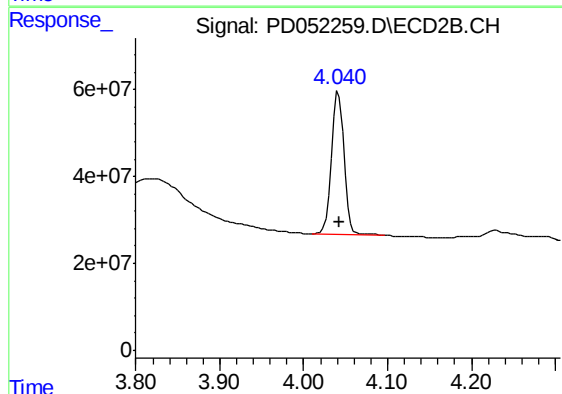


#1 Tetrachloro-m-xylene

R.T.: 4.042 min
Delta R.T.: -0.001 min
Response: 342610279
Conc: 11.77 ng/ml

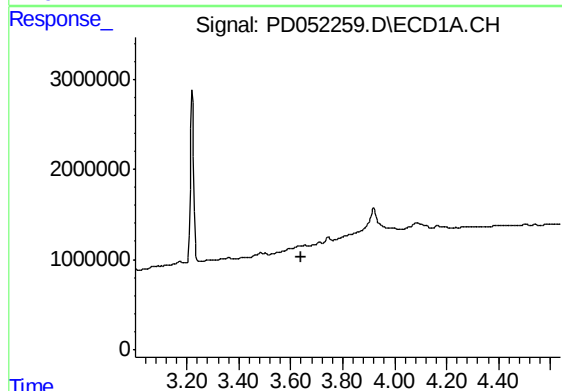


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.641 min
Response: 0
Conc: N.D.

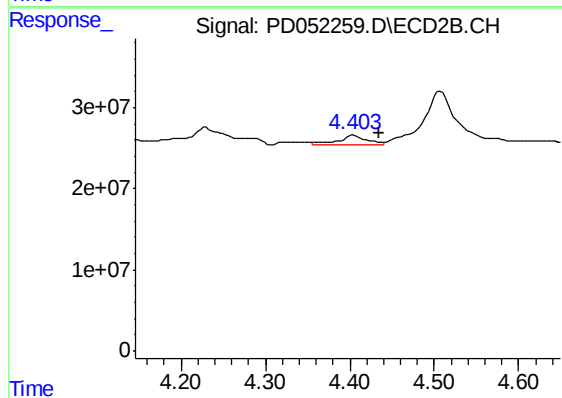

#2 alpha-BHC


R.T.: 4.405 min
Delta R.T.: -0.030 min
Response: 31169722
Conc: 0.71 ng/ml

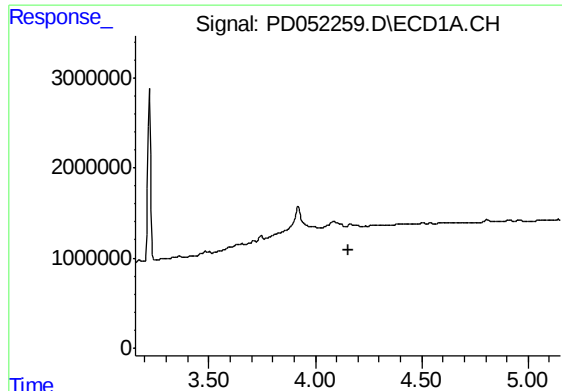

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.154 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5K5

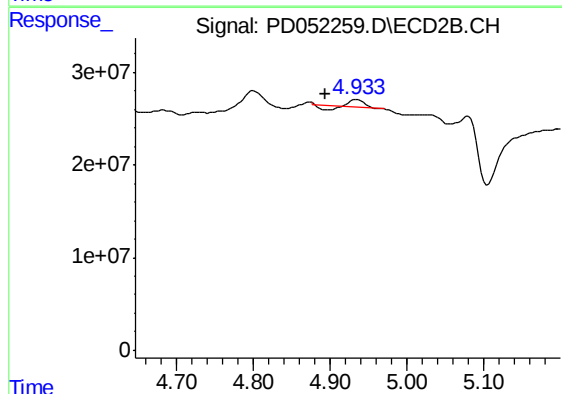


#6 beta-BHC

R.T.: 4.935 min
Delta R.T.: 0.041 min
Response: 5306675
Conc: 0.29 ng/ml

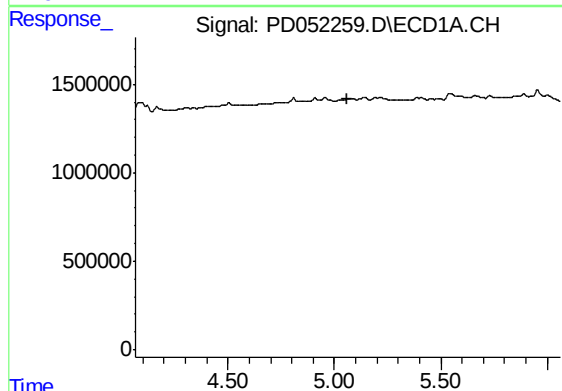


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.063 min
Response: 0
Conc: N.D.

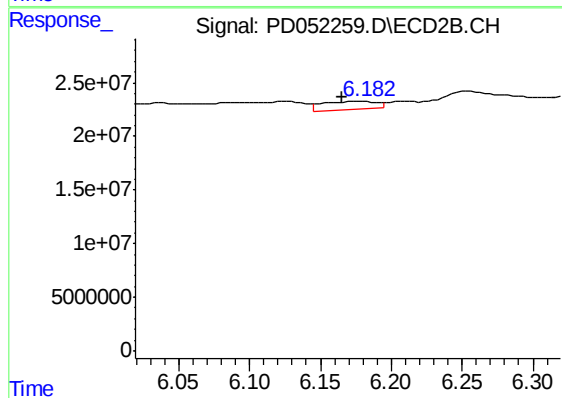

#10 trans-Chlordane


R.T.: 6.183 min
Delta R.T.: 0.018 min
Response: 18693385
Conc: 0.55 ng/ml

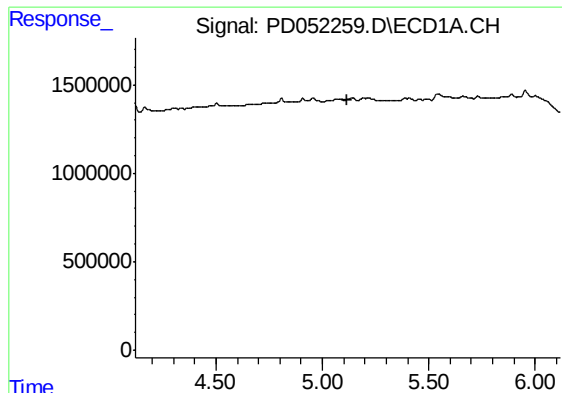

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.119 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5K5

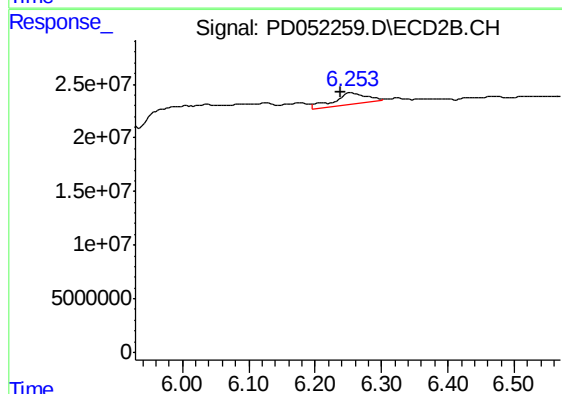


#11 cis-Chlordane

R.T.: 6.254 min
Delta R.T.: 0.016 min
Response: 37221790
Conc: 1.15 ng/ml

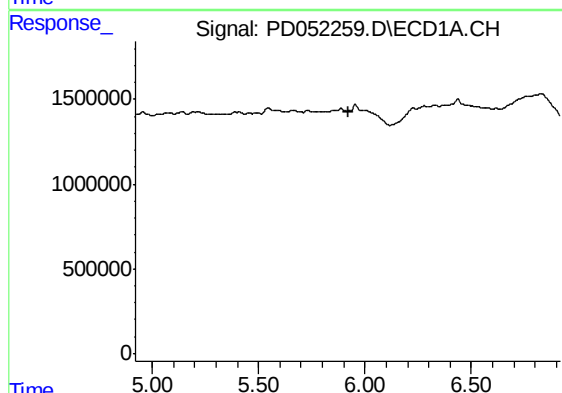


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.920 min
Response: 0
Conc: N.D.

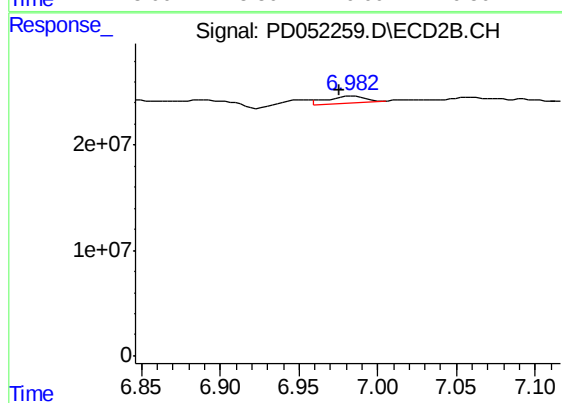

#15 Endosulfan II


R.T.: 6.983 min
Delta R.T.: 0.007 min
Response: 11039003
Conc: 0.44 ng/ml

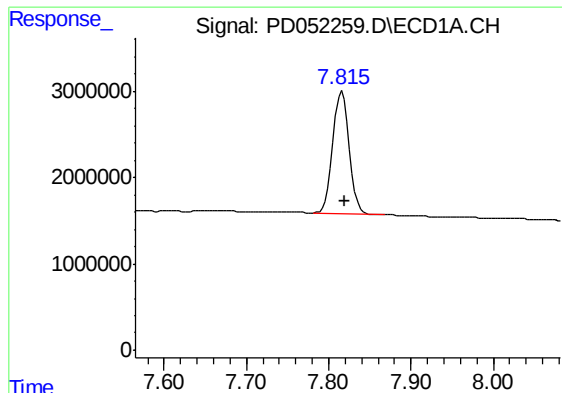

#27 Decachlorobiphenyl

R.T.: 7.816 min
Delta R.T.: -0.003 min
Response: 19713053
Conc: 12.59 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF5K5

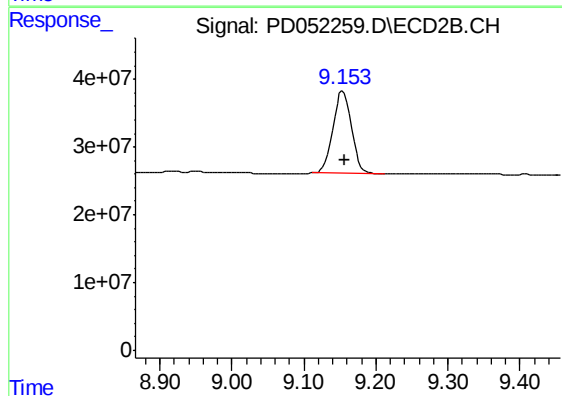

#27 Decachlorobiphenyl

R.T.: 9.154 min
Delta R.T.: -0.002 min
Response: 216633215
Conc: 14.03 ng/ml