

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032819\
 Data File : PD052260.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Mar 2019 20:30
 Operator : AJ\SJ
 Sample : PIBLK07
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK08

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 01:39:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032519CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 25 18:59:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.221	4.042	32656453	630.5E6	23.007	21.668
27)	SA Decachlor...	7.817	9.155	56745105	623.1E6	36.239	40.362
Target Compounds							
6)	B beta-BHC	0.000	4.933f	0 24873410	N.D.		1.356
8)	B Heptachlo...	0.000	5.921	0 49986101	N.D.		1.467
10)	B trans-Chl...	0.000	6.172	0 13128349	N.D.		0.387
11)	B cis-Chlor...	0.000	6.172f	0 13128349	N.D.		0.404


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032819\
Data File : PD052260.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Mar 2019 20:30
Operator : AJ\SJ
Sample : PIBLK07
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PIBLK08

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 01:39:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032519CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 25 18:59:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

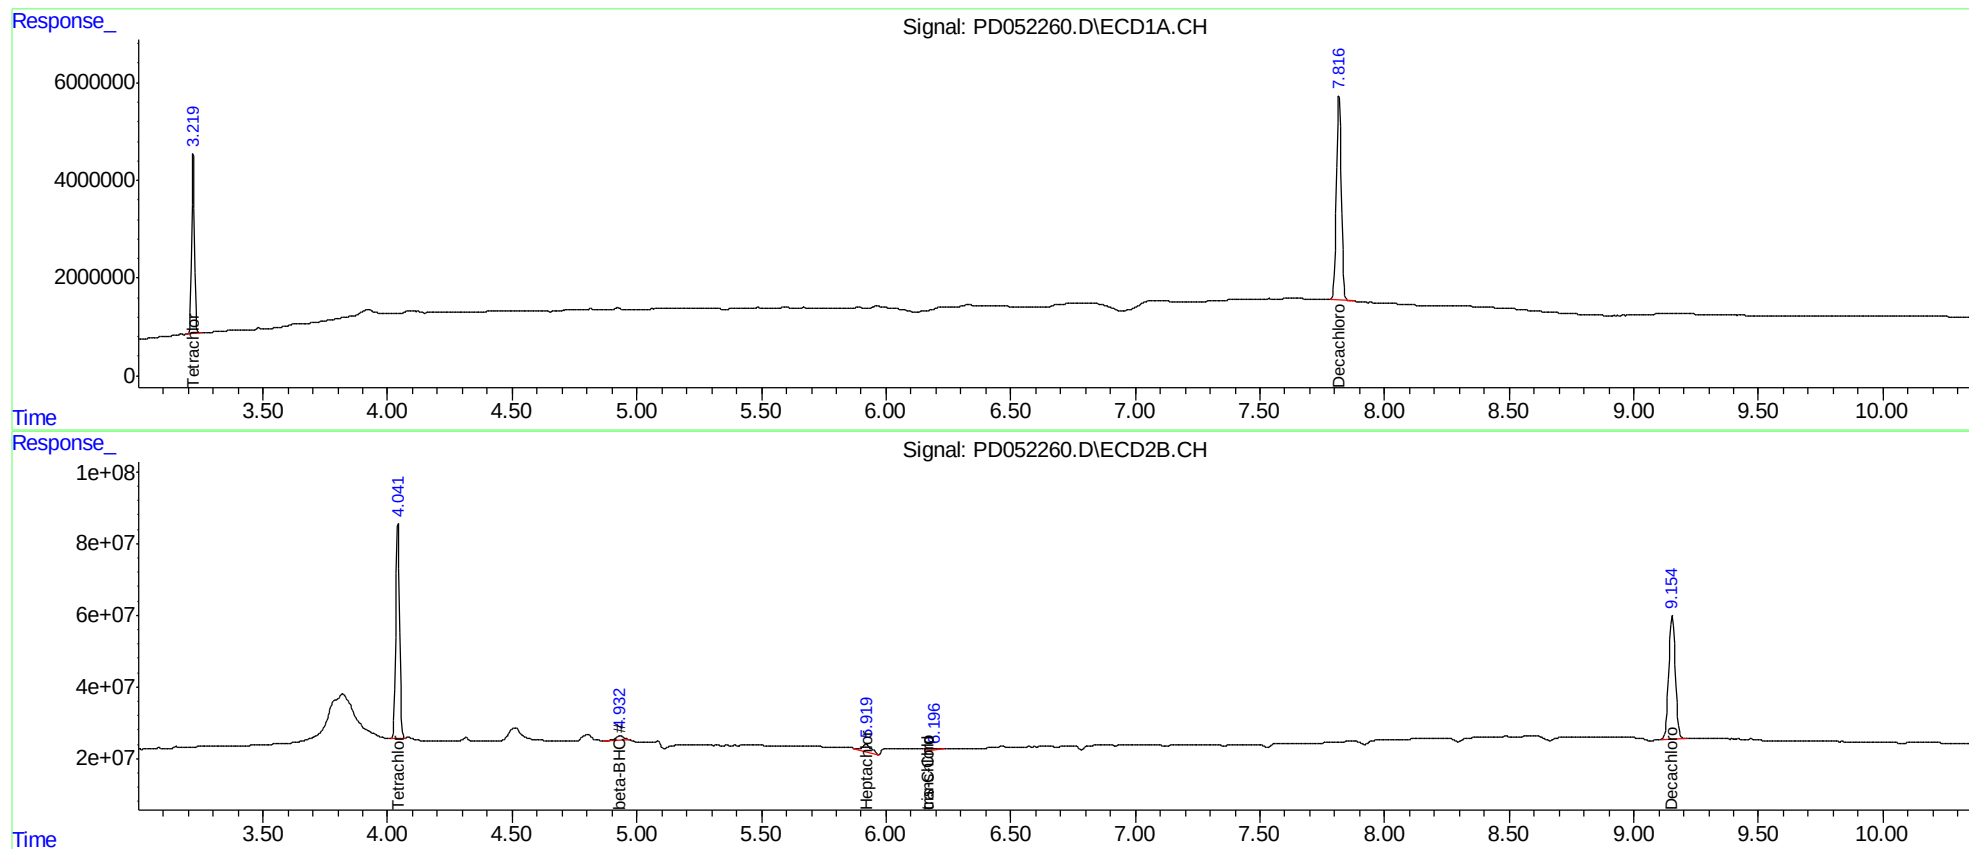


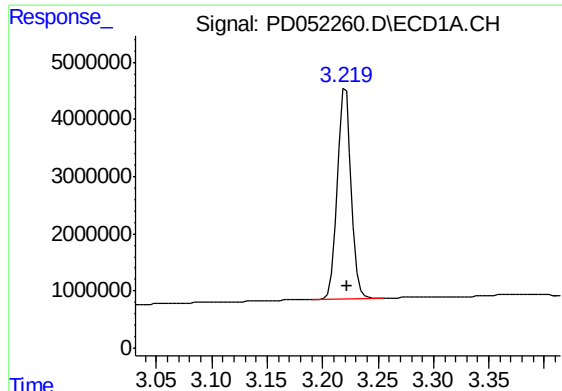

#1 Tetrachloro-m-xylene


R.T.: 3.221 min
Delta R.T.: -0.001 min
Response: 32656453
Conc: 23.01 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK08

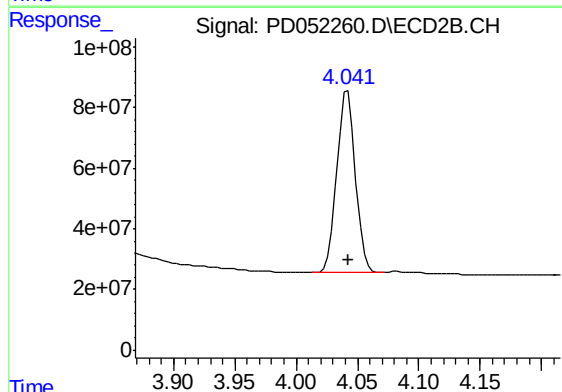


#1 Tetrachloro-m-xylene

R.T.: 4.042 min
Delta R.T.: 0.000 min
Response: 630491550
Conc: 21.67 ng/ml

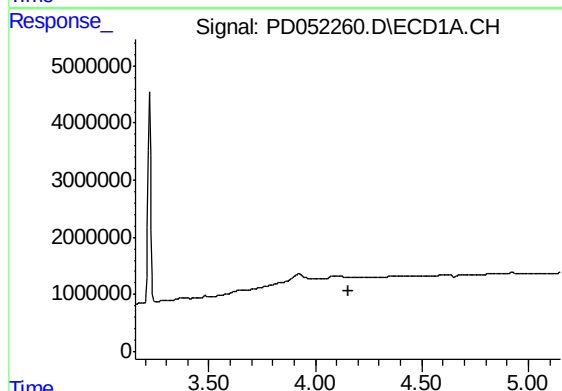


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.154 min
Response: 0
Conc: N.D.

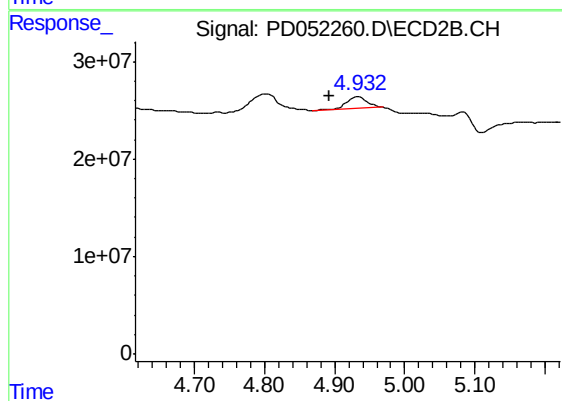

#6 beta-BHC


R.T.: 4.933 min
Delta R.T.: 0.040 min
Response: 24873410
Conc: 1.36 ng/ml

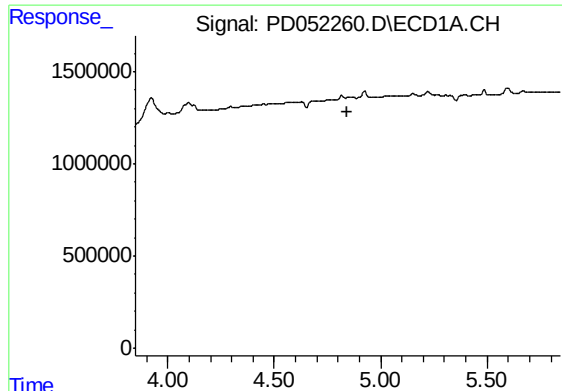

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.846 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PIBLK08

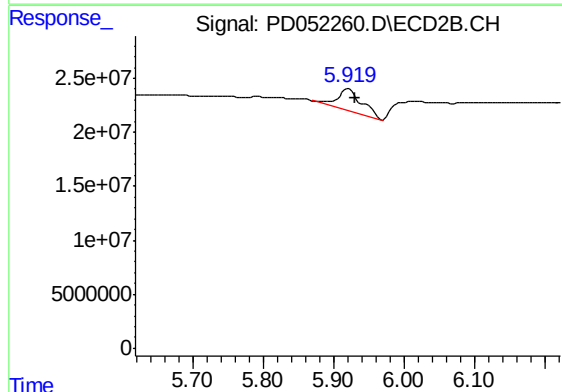


#8 Heptachlor epoxide

R.T.: 5.921 min
Delta R.T.: -0.010 min
Response: 49986101
Conc: 1.47 ng/ml

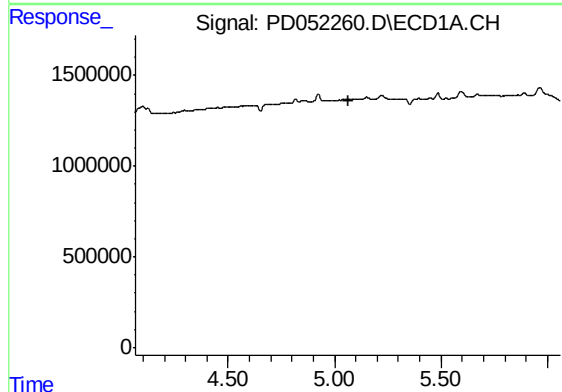


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.063 min
Response: 0
Conc: N.D.

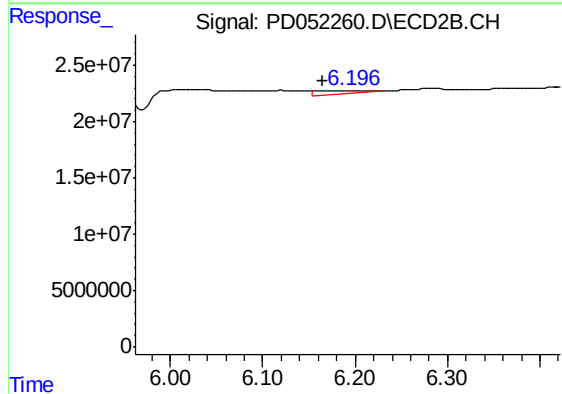

#10 trans-Chlordane


R.T.: 6.172 min
Delta R.T.: 0.006 min
Response: 13128349
Conc: 0.39 ng/ml

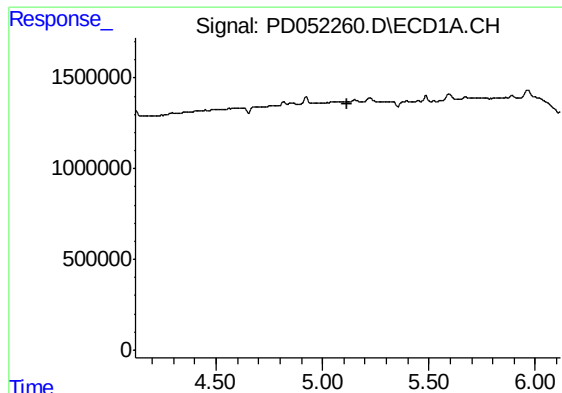

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.119 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PIBLK08

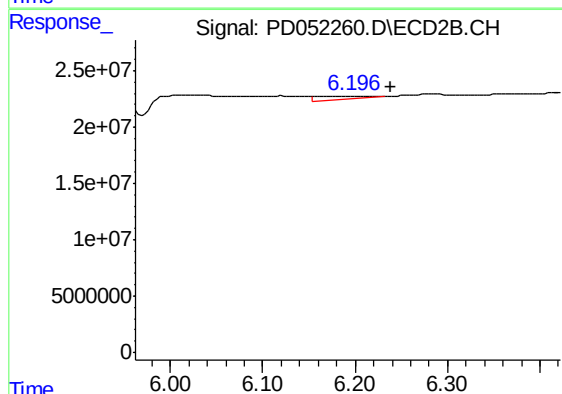


#11 cis-Chlordane

R.T.: 6.172 min
Delta R.T.: -0.066 min
Response: 13128349
Conc: 0.40 ng/ml

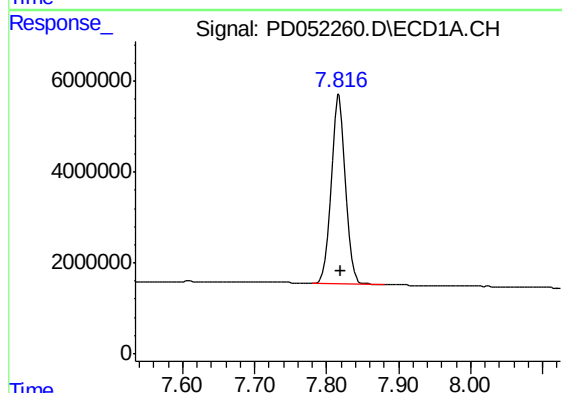

#27 Decachlorobiphenyl

R.T.: 7.817 min
Delta R.T.: -0.002 min
Response: 56745105
Conc: 36.24 ng/ml

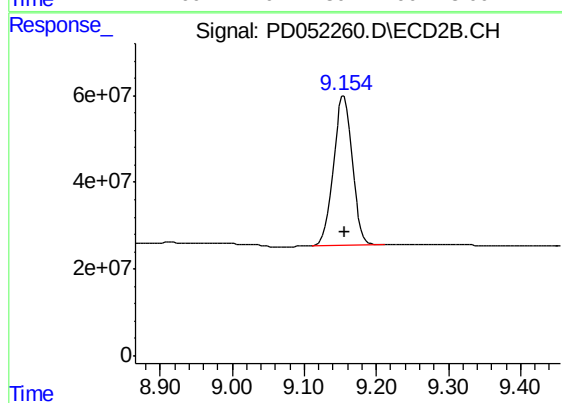

#27 Decachlorobiphenyl

R.T.: 9.155 min
Delta R.T.: 0.000 min
Response: 623051898
Conc: 40.36 ng/ml