

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032819\
 Data File : PD052265.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Mar 2019 21:41
 Operator : AJ\SJ
 Sample : K2068-04
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BF5M3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 01:41:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032519CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 25 18:59:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.221	4.042	28728828	538.7E6	20.240	18.513
27)	SA Decachlor...	7.817	9.154	36923323	407.8E6	23.580	26.418
Target Compounds							
2)	A alpha-BHC	0.000	4.404f	0	139.2E6	N.D.	3.183
3)	MA gamma-BHC...	0.000	4.682f	0	23013141	N.D.	0.579
4)	MA Heptachlor	0.000	5.262f	0	9176266	N.D.	0.229
6)	B beta-BHC	0.000	4.935f	0	29733387	N.D.	1.620
7)	B delta-BHC	0.000	5.079f	0	53463996	N.D.	1.347
9)	A Endosulfan I	0.000	6.256	0	30417120	N.D.	0.970
10)	B trans-Chl...	0.000	6.174	0	56402587	N.D.	1.661
11)	B cis-Chlor...	0.000	6.256	0	30417120	N.D.	0.937
15)	B Endosulfa...	0.000	6.982	0	15348206	N.D.	0.605


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032819\
Data File : PD052265.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Mar 2019 21:41
Operator : AJ\SJ
Sample : K2068-04
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
BF5M3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 01:41:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032519CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 25 18:59:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

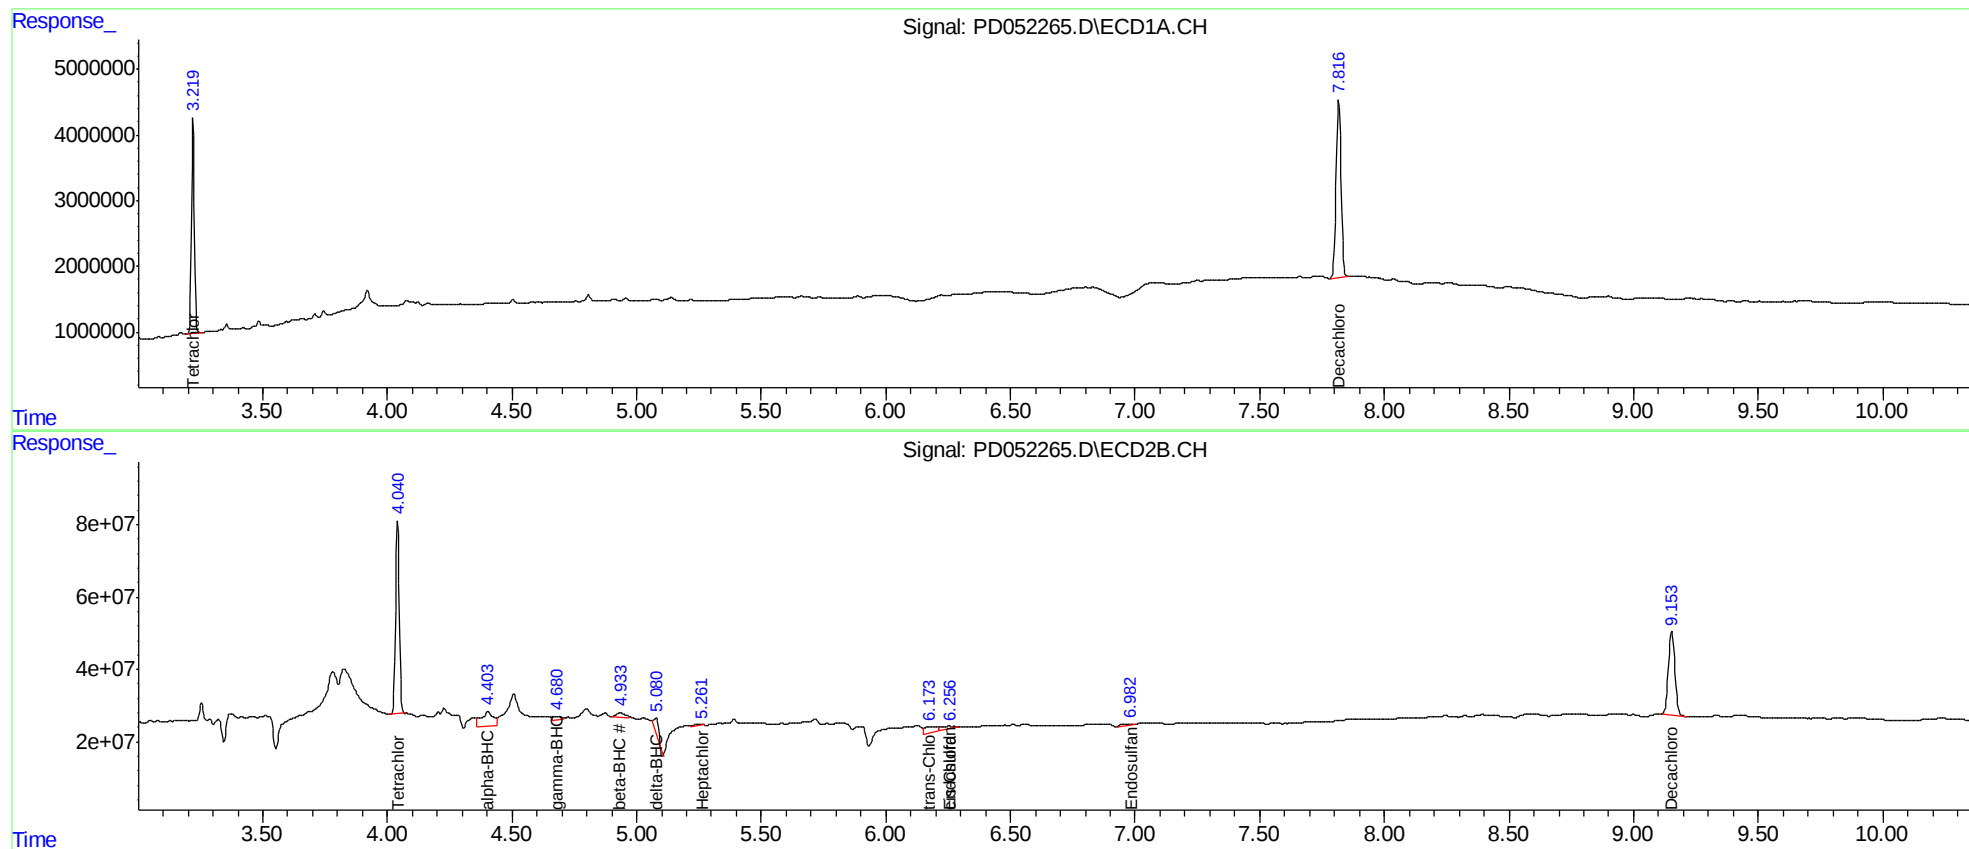


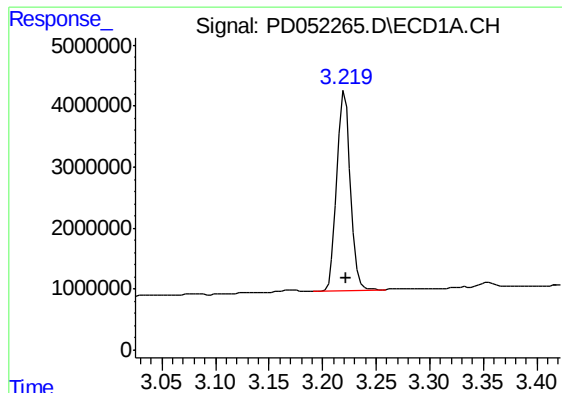

#1 Tetrachloro-m-xylene


R.T.: 3.221 min
Delta R.T.: -0.001 min
Response: 28728828
Conc: 20.24 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF5M3

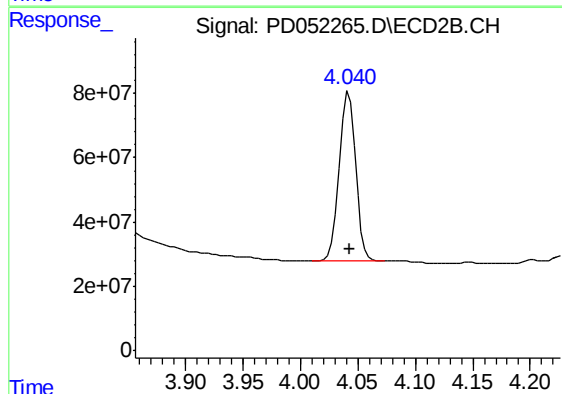


#1 Tetrachloro-m-xylene

R.T.: 4.042 min
Delta R.T.: -0.001 min
Response: 538683423
Conc: 18.51 ng/ml

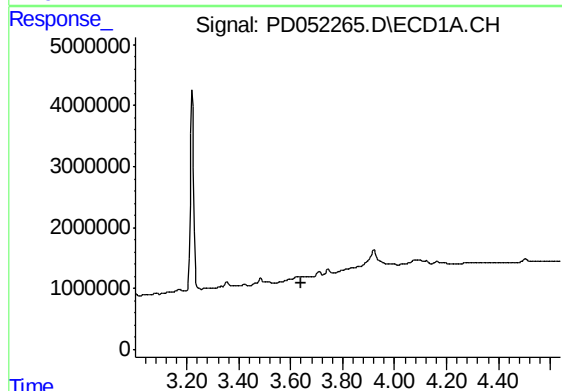


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.641 min
Response: 0
Conc: N.D.

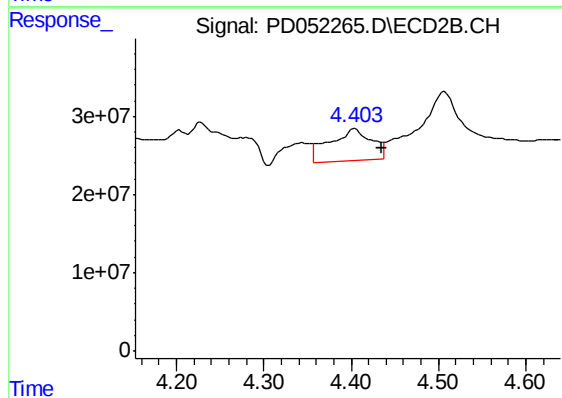

#2 alpha-BHC


R.T.: 4.404 min
Delta R.T.: -0.031 min
Response: 139204066
Conc: 3.18 ng/ml

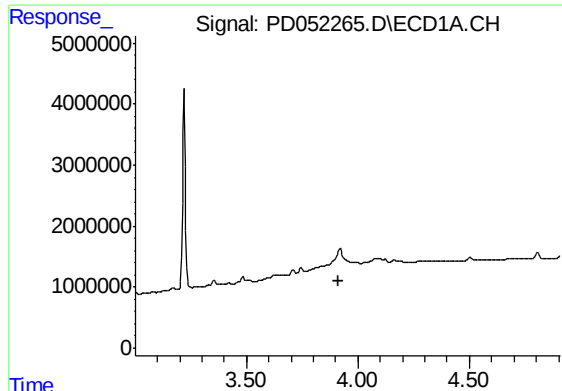

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 3.910 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5M3

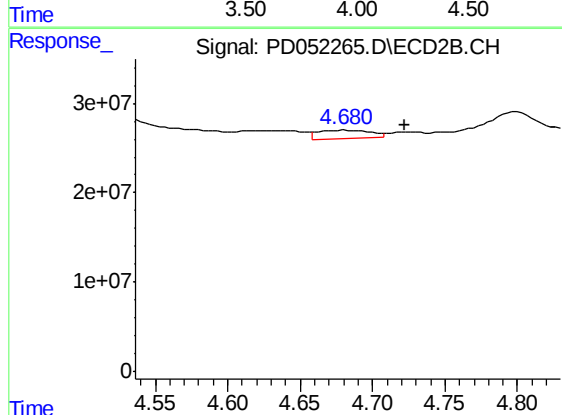


#3 gamma-BHC (Lindane)

R.T.: 4.682 min
Delta R.T.: -0.040 min
Response: 23013141
Conc: 0.58 ng/ml

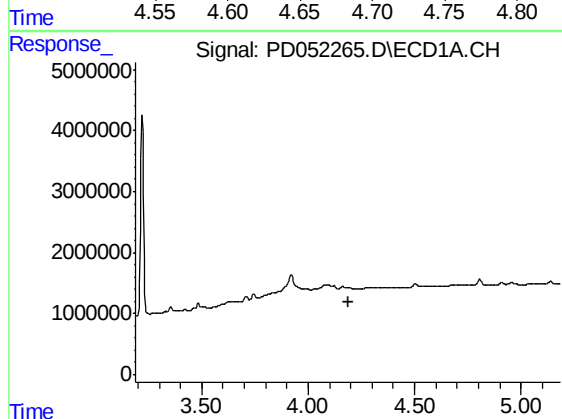


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.187 min
Response: 0
Conc: N.D.

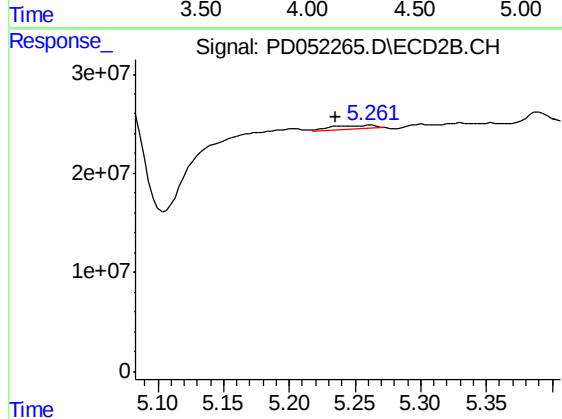

#4 Heptachlor


R.T.: 5.262 min
Delta R.T.: 0.027 min
Response: 9176266
Conc: 0.23 ng/ml

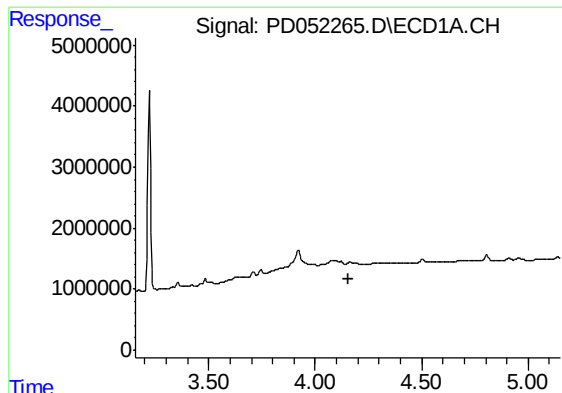

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.154 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5M3

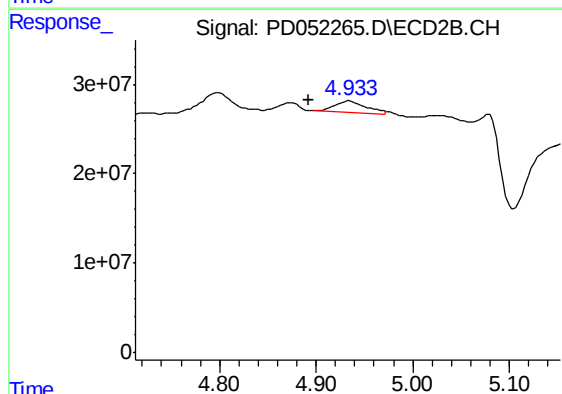


#6 beta-BHC

R.T.: 4.935 min
Delta R.T.: 0.042 min
Response: 29733387
Conc: 1.62 ng/ml

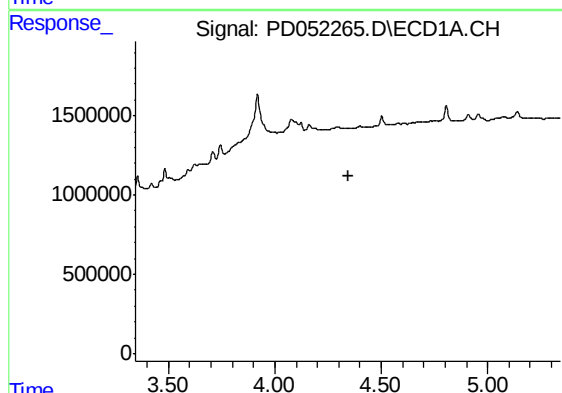


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.344 min
Response: 0
Conc: N.D.

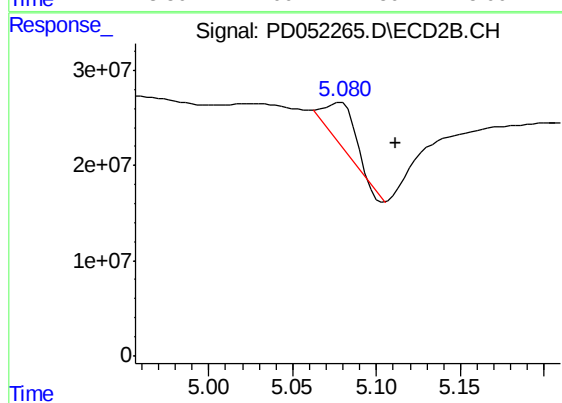

#7 delta-BHC


R.T.: 5.079 min
Delta R.T.: -0.033 min
Response: 53463996
Conc: 1.35 ng/ml

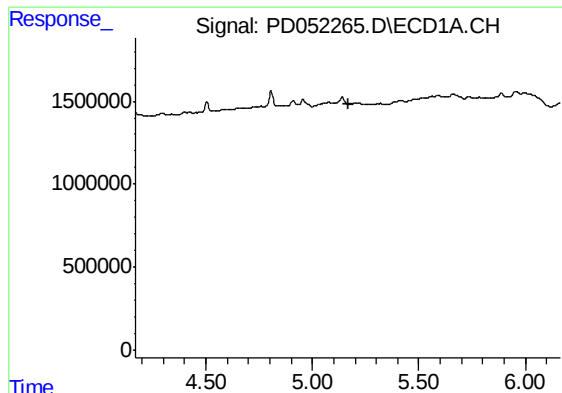

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.168 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5M3

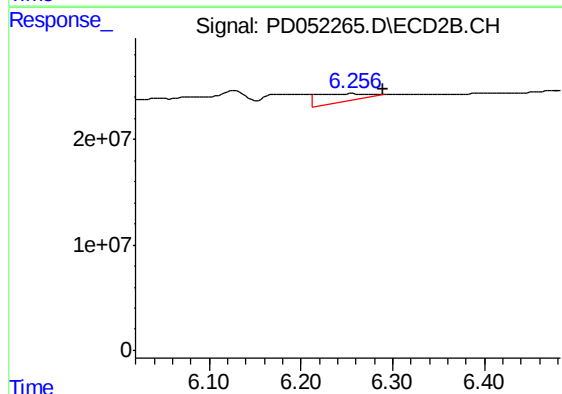


#9 Endosulfan I

R.T.: 6.256 min
Delta R.T.: -0.033 min
Response: 30417120
Conc: 0.97 ng/ml

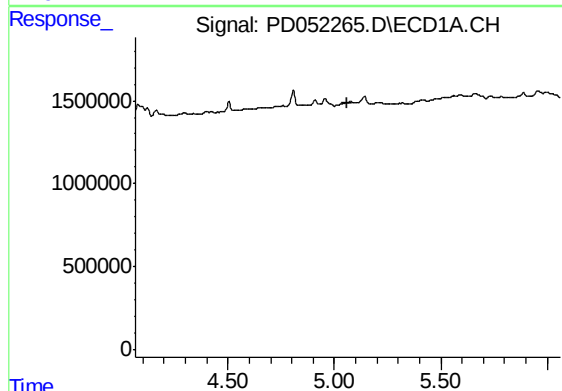


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.063 min
Response: 0
Conc: N.D.

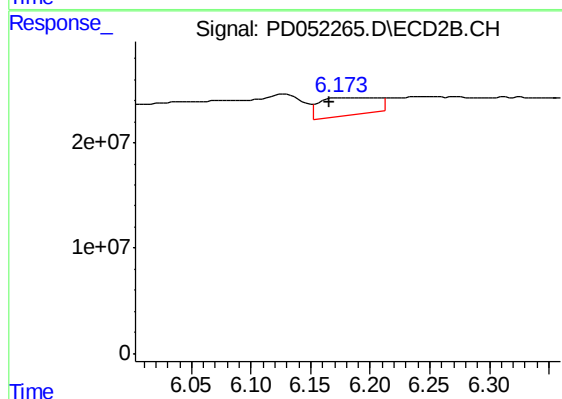

#10 trans-Chlordane


R.T.: 6.174 min
Delta R.T.: 0.009 min
Response: 56402587
Conc: 1.66 ng/ml

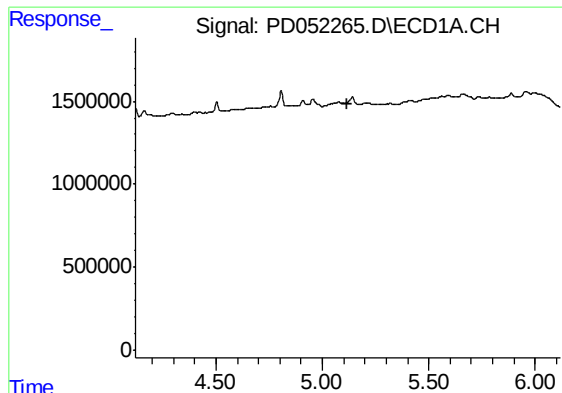

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.119 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5M3

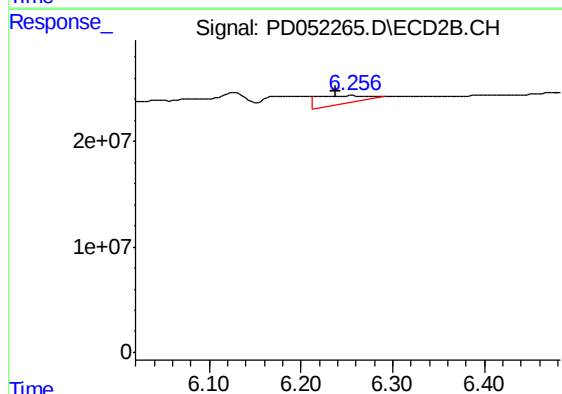


#11 cis-Chlordane

R.T.: 6.256 min
Delta R.T.: 0.018 min
Response: 30417120
Conc: 0.94 ng/ml

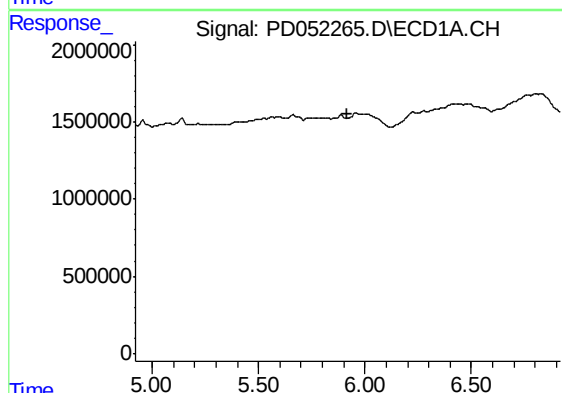


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.920 min
Response: 0
Conc: N.D.

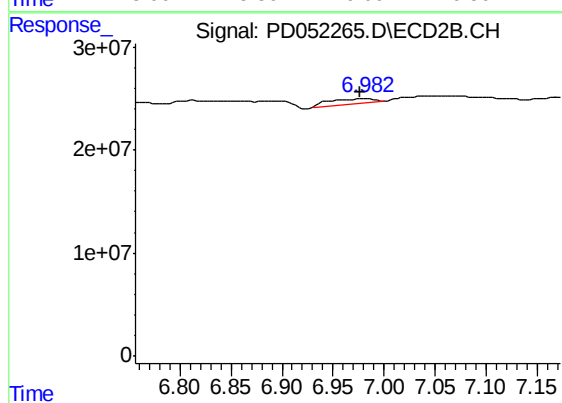

#15 Endosulfan II


R.T.: 6.982 min
Delta R.T.: 0.006 min
Response: 15348206
Conc: 0.61 ng/ml

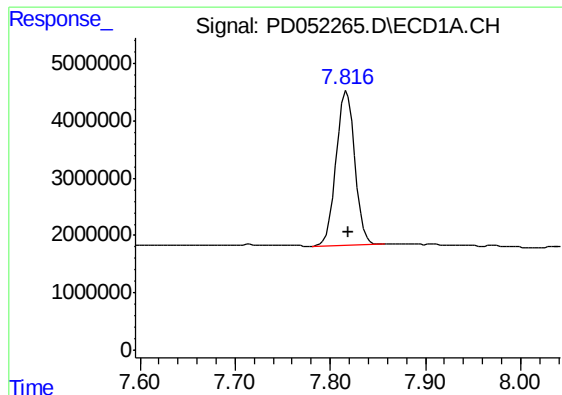

#27 Decachlorobiphenyl

R.T.: 7.817 min
Delta R.T.: -0.002 min
Response: 36923323
Conc: 23.58 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF5M3

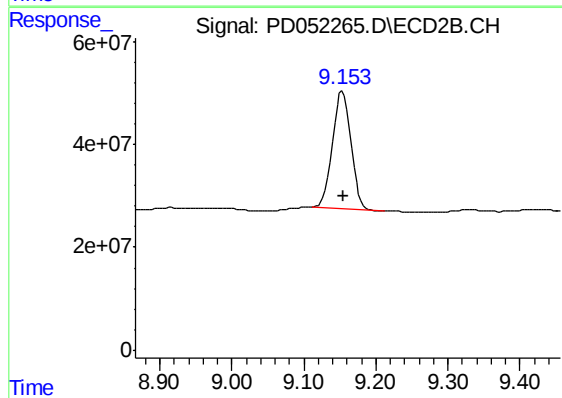

#27 Decachlorobiphenyl

R.T.: 9.154 min
Delta R.T.: -0.002 min
Response: 407806201
Conc: 26.42 ng/ml