

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032819\
 Data File : PD052269.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Mar 2019 22:38
 Operator : AJ\SJ
 Sample : K2068-07
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BFC97

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 01:42:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032519CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 25 18:59:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.221	4.042	38996724	680.7E6	27.473	23.394
27)	SA Decachlor...	7.816	9.155	53171850	565.9E6	33.957	36.662
Target Compounds							
2)	A alpha-BHC	0.000	4.404f	0 73194736	N.D.		1.674
6)	B beta-BHC	0.000	4.936f	0 36253167	N.D.		1.976
7)	B delta-BHC	0.000	5.080f	0 57575328	N.D.		1.451
9)	A Endosulfan I	0.000	6.246f	0 10358169	N.D.		0.330
10)	B trans-Chl...	0.000	6.167	0 27853648	N.D.		0.820
11)	B cis-Chlor...	0.000	6.246	0 10358169	N.D.		0.319
15)	B Endosulfa...	0.000	6.975	0 18813148	N.D.		0.742


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032819\
Data File : PD052269.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Mar 2019 22:38
Operator : AJ\SJ
Sample : K2068-07
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
BFC97

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 01:42:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032519CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 25 18:59:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

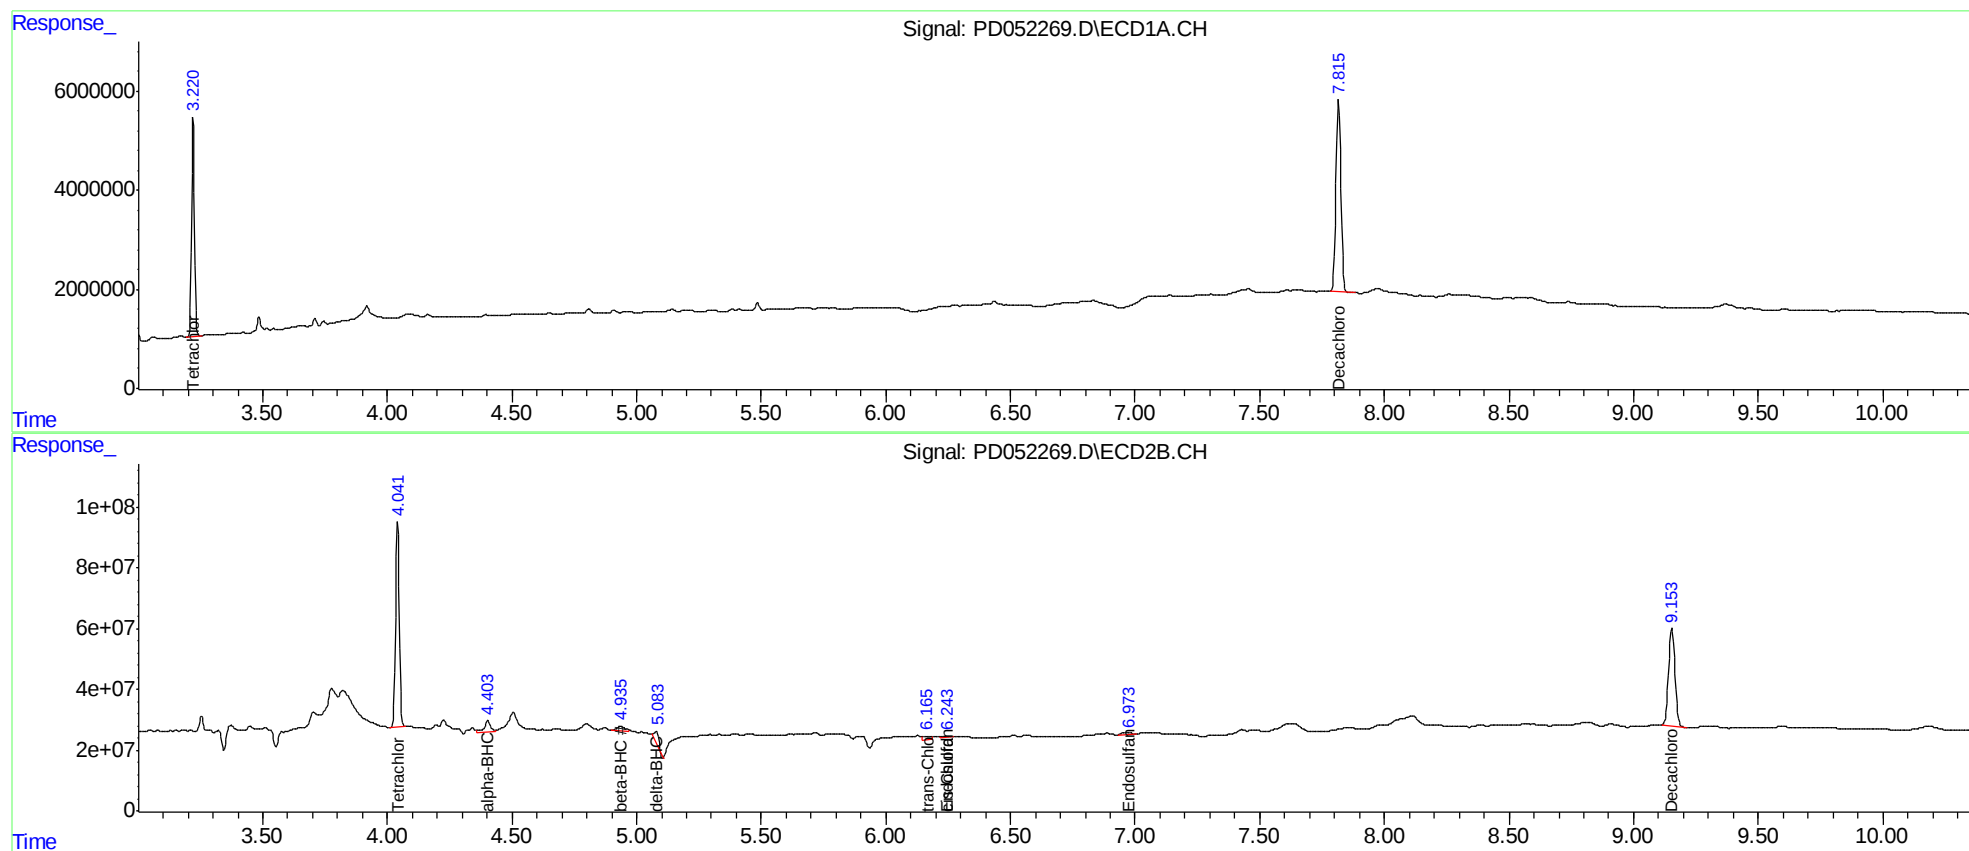


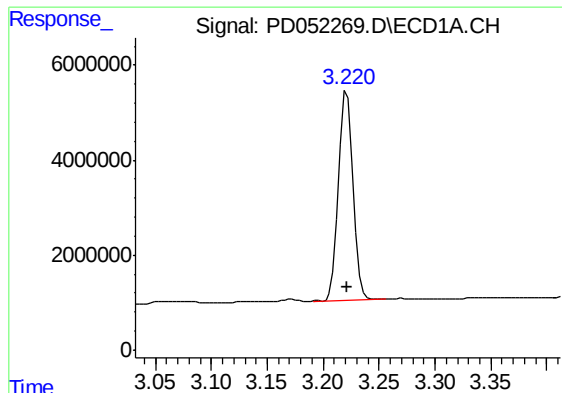

#1 Tetrachloro-m-xylene


R.T.: 3.221 min
Delta R.T.: 0.000 min
Response: 38996724
Conc: 27.47 ng/ml

Instrument :
ECD_D
ClientSampleId :
BFC97

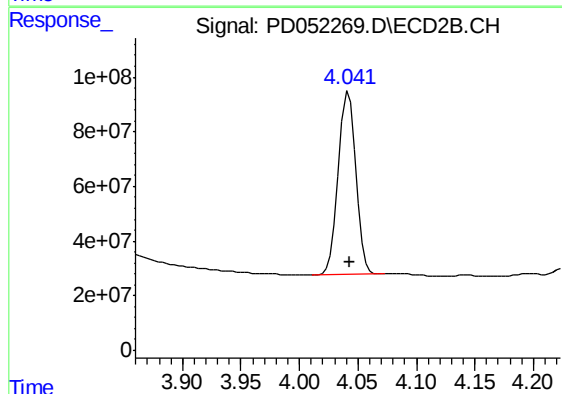


#1 Tetrachloro-m-xylene

R.T.: 4.042 min
Delta R.T.: 0.000 min
Response: 680691348
Conc: 23.39 ng/ml

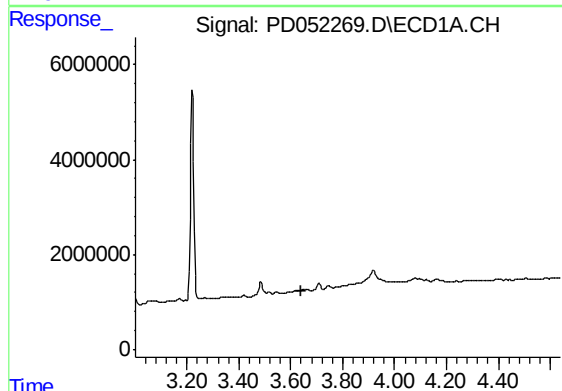


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.641 min
Response: 0
Conc: N.D.

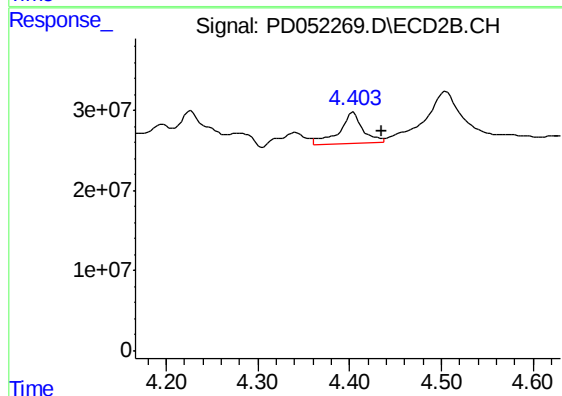

#2 alpha-BHC


R.T.: 4.404 min
Delta R.T.: -0.031 min
Response: 73194736
Conc: 1.67 ng/ml

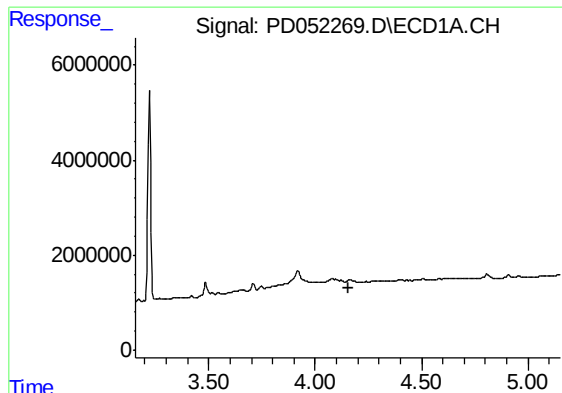

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.154 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BFC97

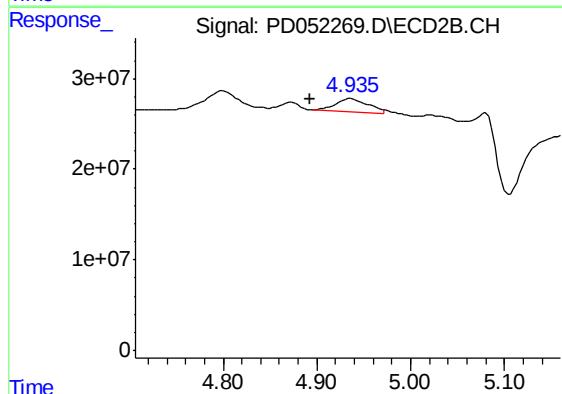


#6 beta-BHC

R.T.: 4.936 min
Delta R.T.: 0.043 min
Response: 36253167
Conc: 1.98 ng/ml

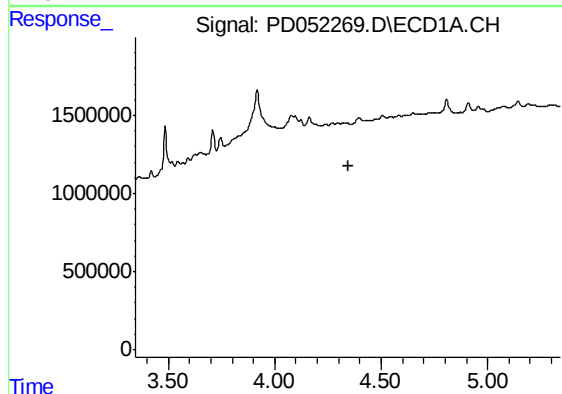


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.344 min
Response: 0
Conc: N.D.

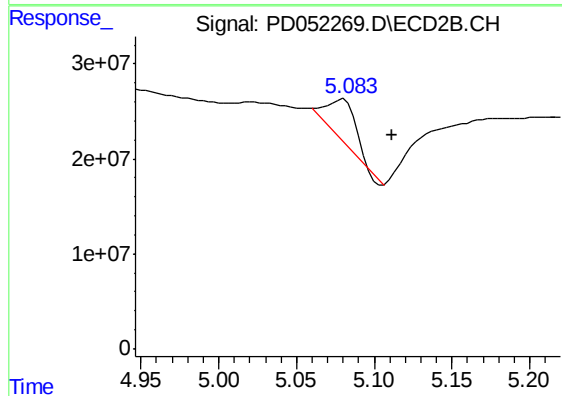

#7 delta-BHC


R.T.: 5.080 min
Delta R.T.: -0.032 min
Response: 57575328
Conc: 1.45 ng/ml

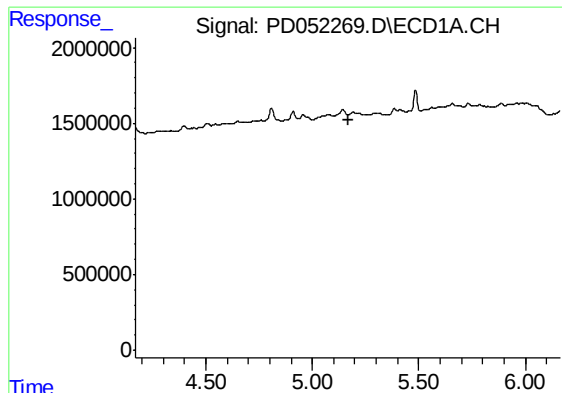

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.168 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BFC97

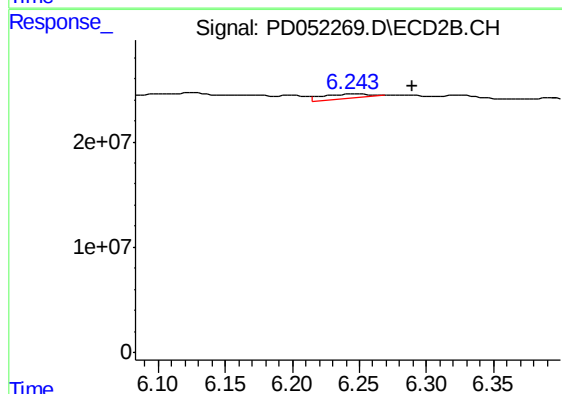


#9 Endosulfan I

R.T.: 6.246 min
Delta R.T.: -0.044 min
Response: 10358169
Conc: 0.33 ng/ml

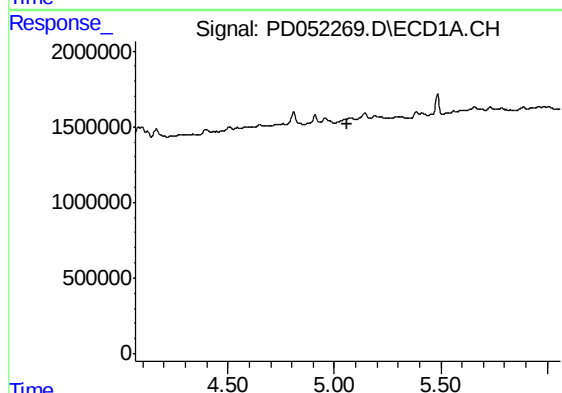


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.063 min
Response: 0
Conc: N.D.

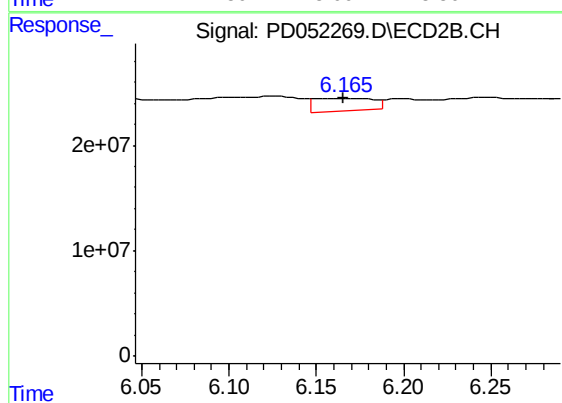

#10 trans-Chlordane


R.T.: 6.167 min
Delta R.T.: 0.000 min
Response: 27853648
Conc: 0.82 ng/ml

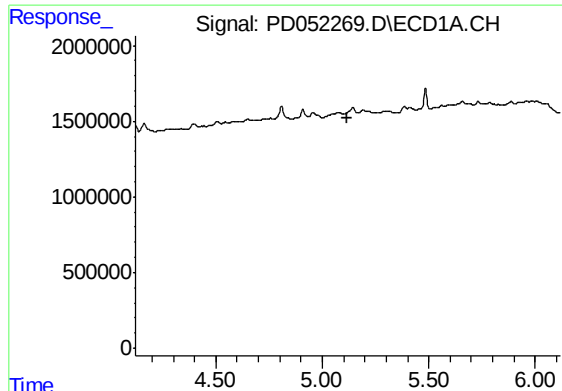

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.119 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BFC97

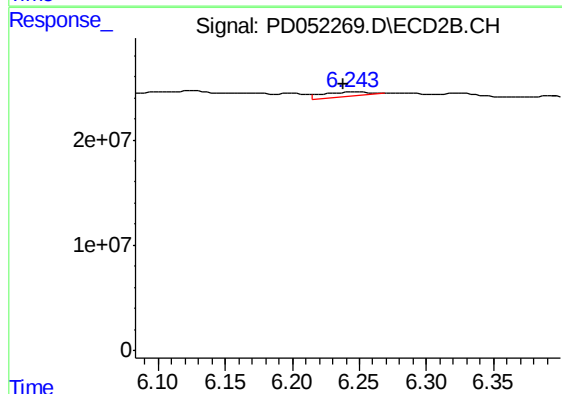


#11 cis-Chlordane

R.T.: 6.246 min
Delta R.T.: 0.007 min
Response: 10358169
Conc: 0.32 ng/ml

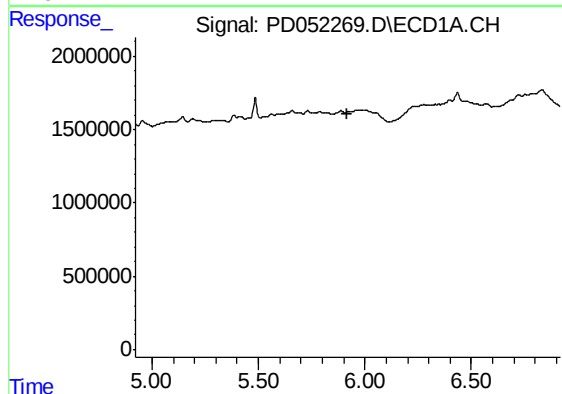


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 5.920 min
Response: 0
Conc: N.D.

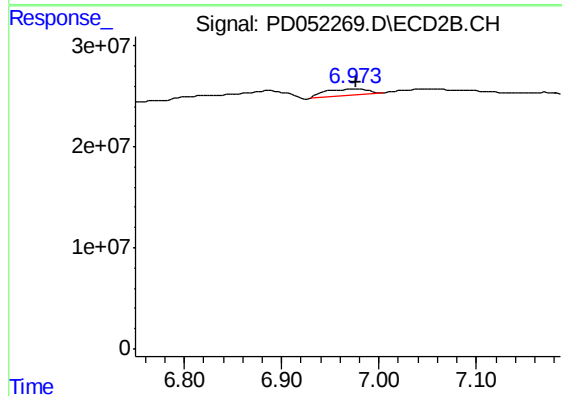

#15 Endosulfan II


R.T.: 6.975 min
Delta R.T.: -0.002 min
Response: 18813148
Conc: 0.74 ng/ml

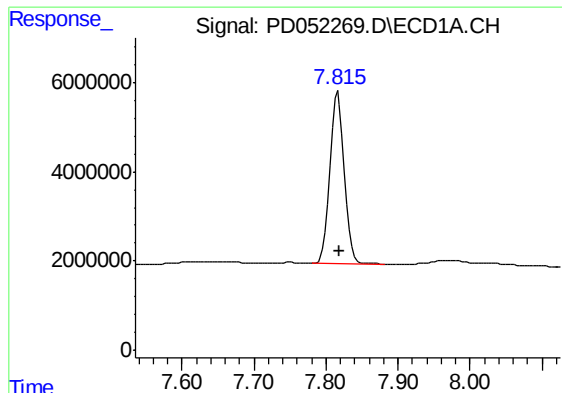

#27 Decachlorobiphenyl

R.T.: 7.816 min
Delta R.T.: -0.003 min
Response: 53171850
Conc: 33.96 ng/ml

Instrument :
ECD_D
ClientSampleId :
BFC97

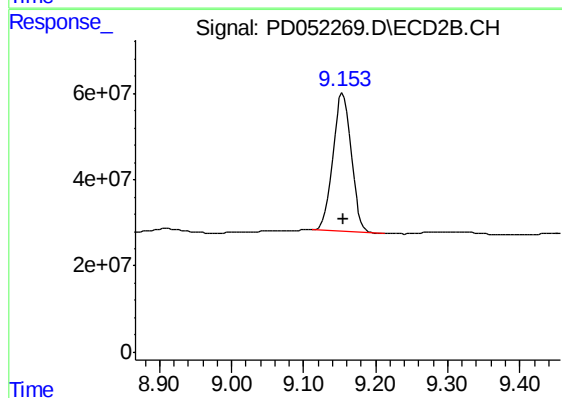

#27 Decachlorobiphenyl

R.T.: 9.155 min
Delta R.T.: -0.001 min
Response: 565943499
Conc: 36.66 ng/ml