

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032819\
 Data File : PD052270.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Mar 2019 22:52
 Operator : AJ\SJ
 Sample : K2068-18
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BF5M4

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 01:42:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032519CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 25 18:59:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.221	4.042	25891447	492.7E6	18.241	16.932
27)	SA Decachlor...	7.818	9.155	34954180	369.2E6	22.323	23.916
Target Compounds							
2)	A alpha-BHC	0.000	4.405f	0	108.9E6	N.D.	2.490
3)	MA gamma-BHC...	0.000	4.756f	0	17964207	N.D.	0.452
4)	MA Heptachlor	0.000	5.253	0	22205407	N.D.	0.554
6)	B beta-BHC	0.000	4.935f	0	8016905	N.D.	0.437
9)	A Endosulfan I	0.000	6.245f	0	14100166	N.D.	0.450
10)	B trans-Chl...	0.000	6.155	0	43638924	N.D.	1.285
11)	B cis-Chlor...	0.000	6.245	0	14100166	N.D.	0.434
13)	MA Dieldrin	0.000	6.525	0	20489655	N.D.	0.657
15)	B Endosulfa...	0.000	6.986	0	21636728	N.D.	0.853


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032819\
Data File : PD052270.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Mar 2019 22:52
Operator : AJ\SJ
Sample : K2068-18
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
BF5M4

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 01:42:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032519CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 25 18:59:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

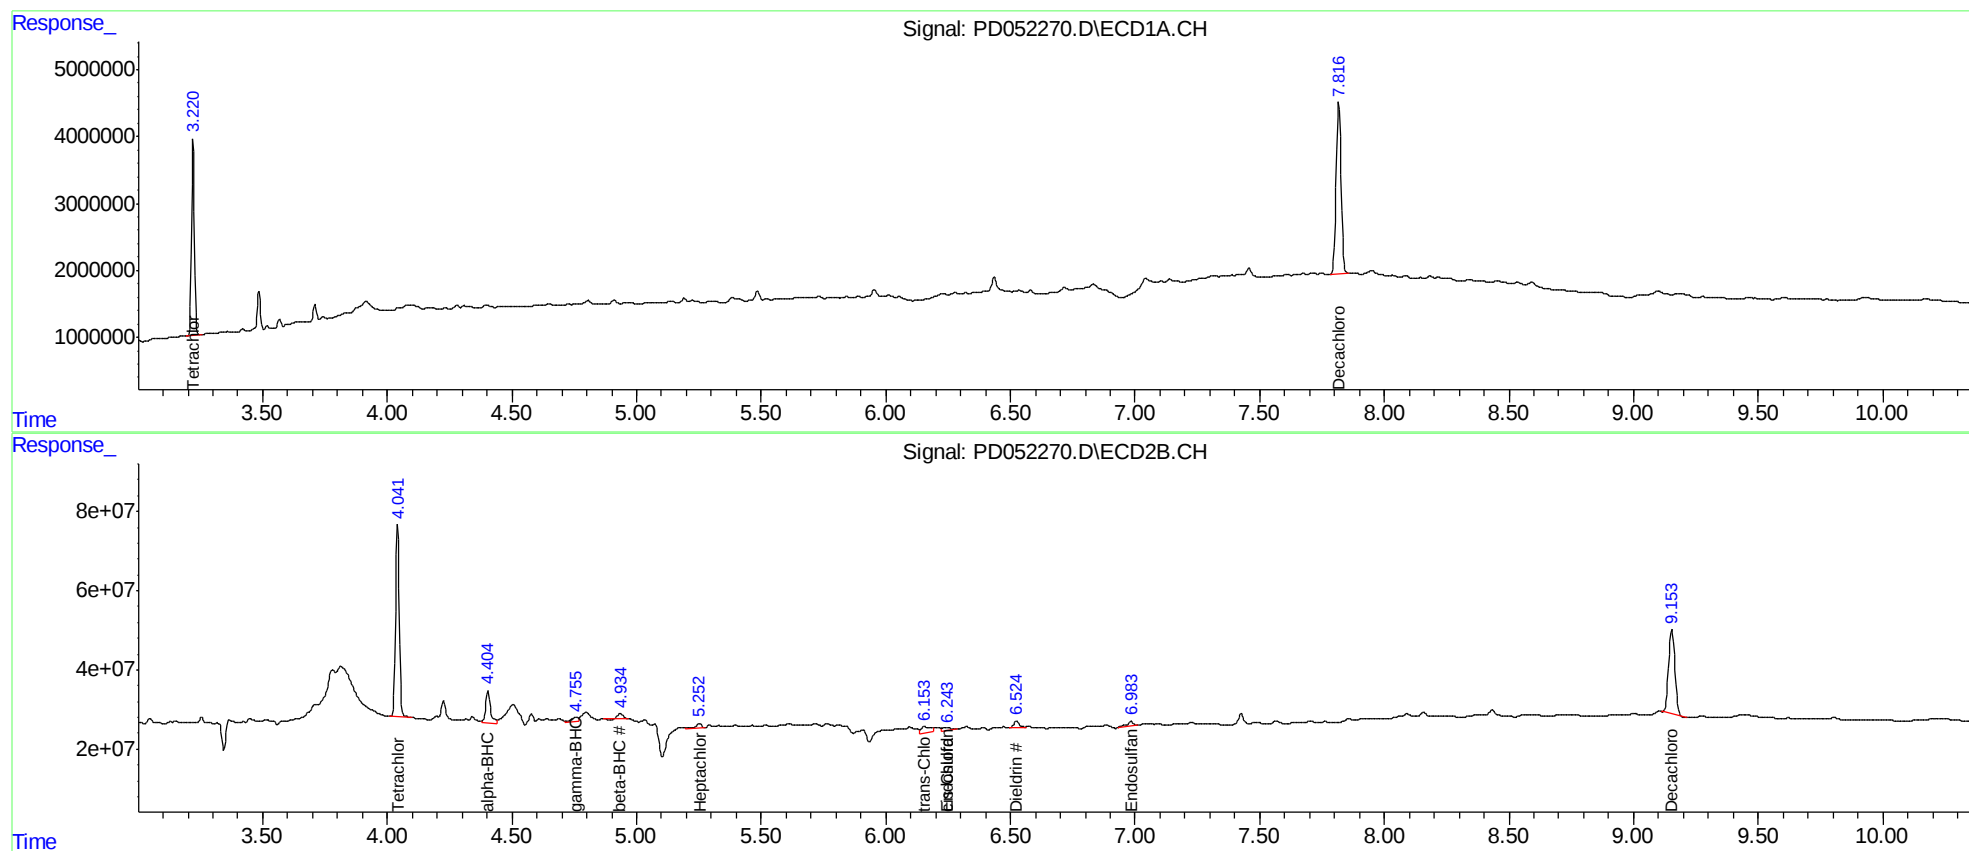


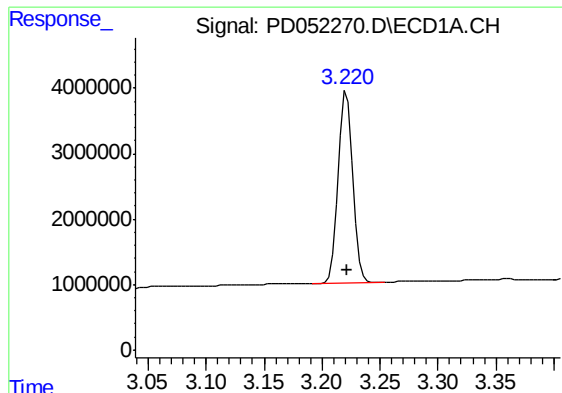

#1 Tetrachloro-m-xylene


R.T.: 3.221 min
Delta R.T.: 0.000 min
Response: 25891447
Conc: 18.24 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF5M4

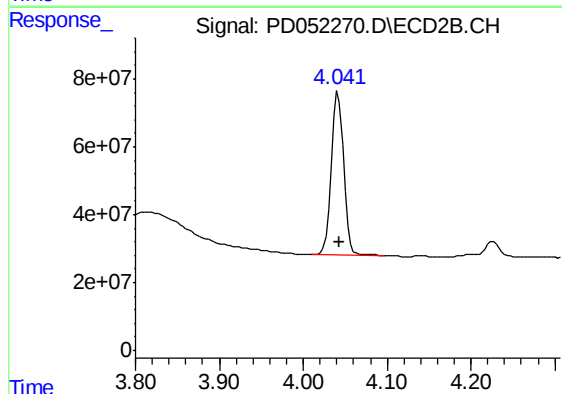


#1 Tetrachloro-m-xylene

R.T.: 4.042 min
Delta R.T.: 0.000 min
Response: 492682740
Conc: 16.93 ng/ml

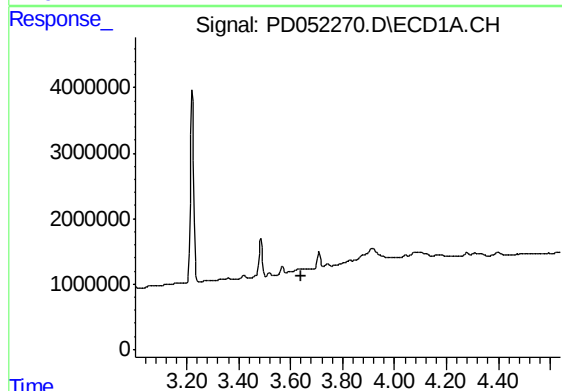


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.641 min
Response: 0
Conc: N.D.

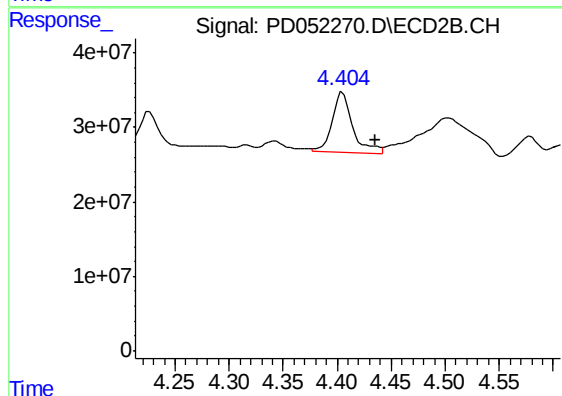

#2 alpha-BHC


R.T.: 4.405 min
Delta R.T.: -0.030 min
Response: 108883103
Conc: 2.49 ng/ml

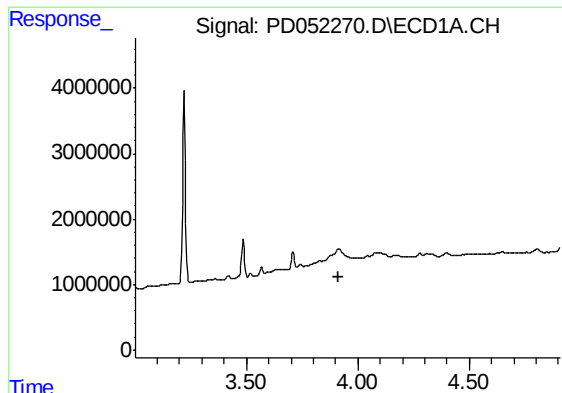

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 3.910 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5M4

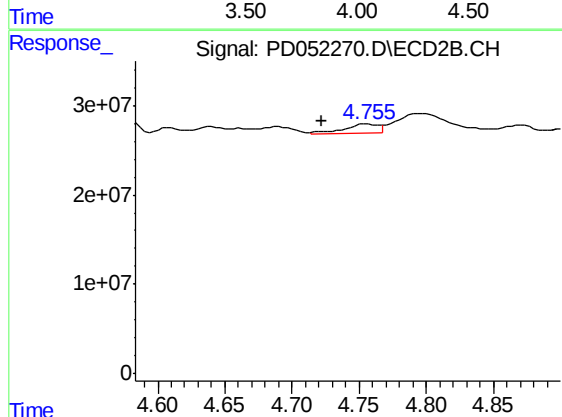


#3 gamma-BHC (Lindane)

R.T.: 4.756 min
Delta R.T.: 0.034 min
Response: 17964207
Conc: 0.45 ng/ml

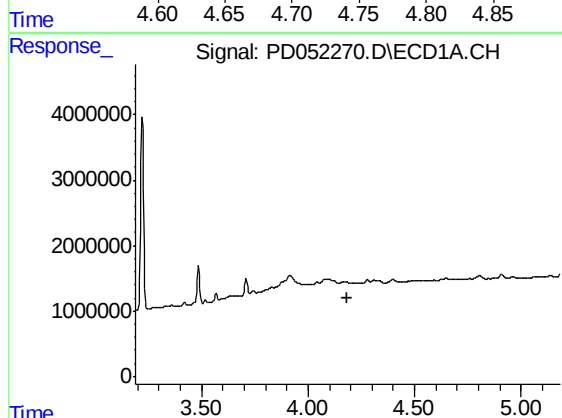


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.187 min
Response: 0
Conc: N.D.

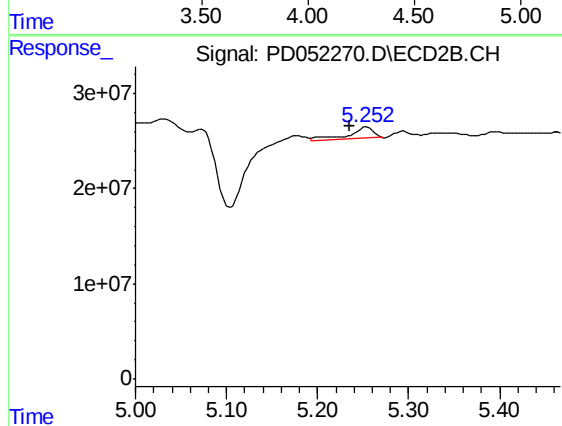

#4 Heptachlor


R.T.: 5.253 min
Delta R.T.: 0.018 min
Response: 22205407
Conc: 0.55 ng/ml

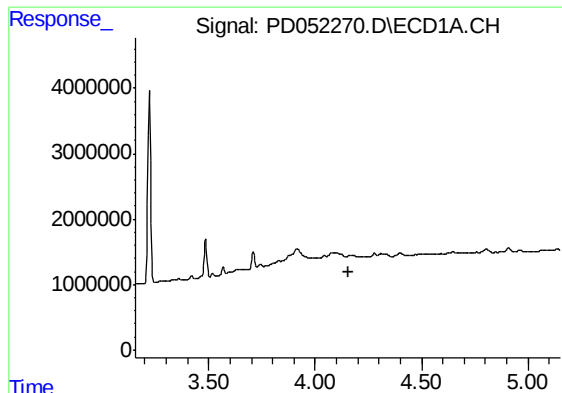

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.154 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5M4

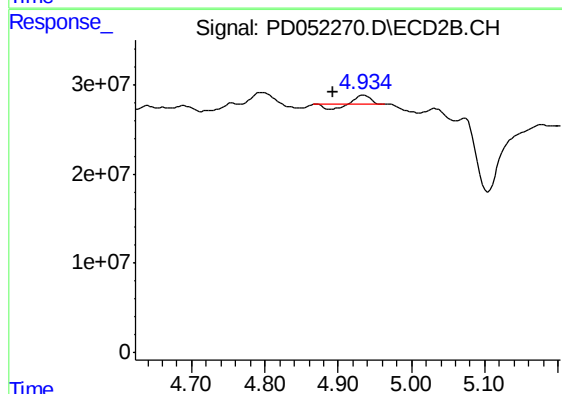


#6 beta-BHC

R.T.: 4.935 min
Delta R.T.: 0.042 min
Response: 8016905
Conc: 0.44 ng/ml

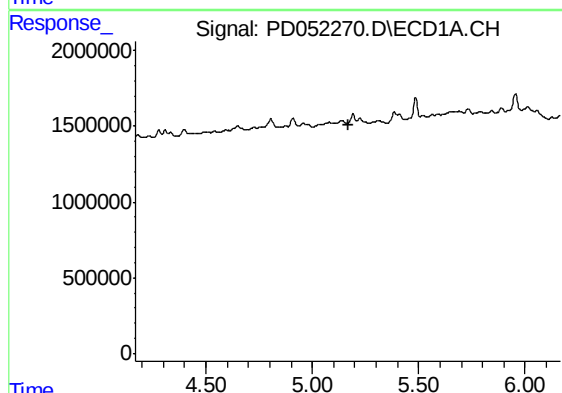


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.168 min
Response: 0
Conc: N.D.

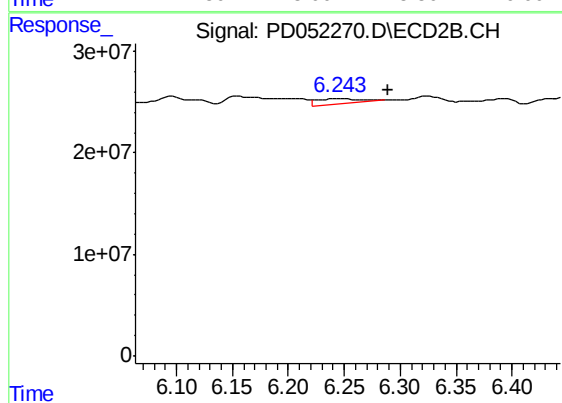

#9 Endosulfan I


R.T.: 6.245 min
Delta R.T.: -0.044 min
Response: 14100166
Conc: 0.45 ng/ml

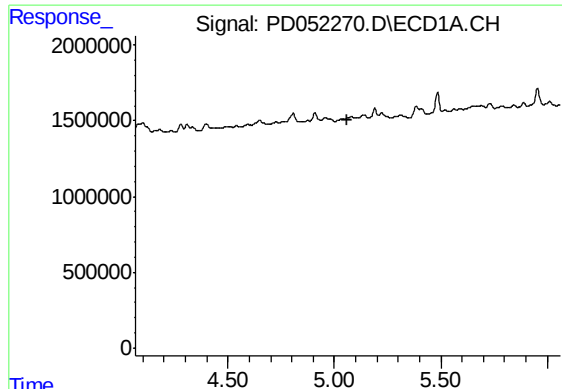

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.063 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5M4

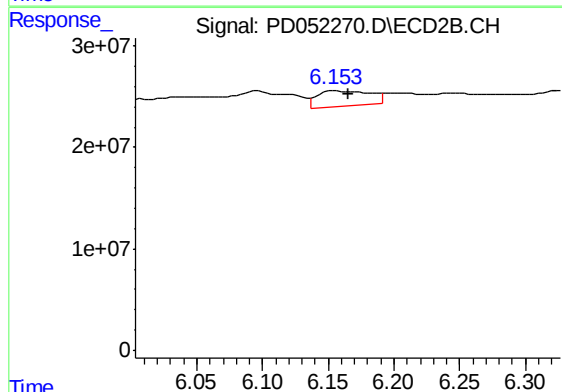


#10 trans-Chlordane

R.T.: 6.155 min
Delta R.T.: -0.011 min
Response: 43638924
Conc: 1.28 ng/ml

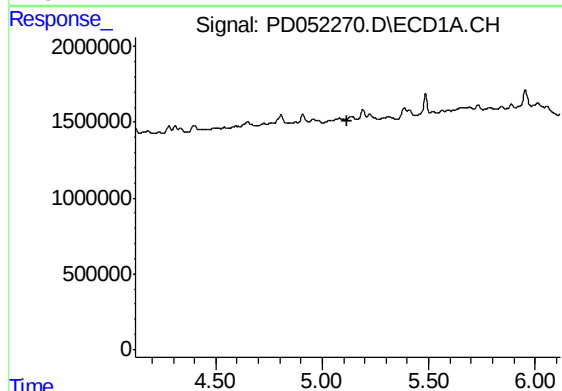


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.119 min
Response: 0
Conc: N.D.

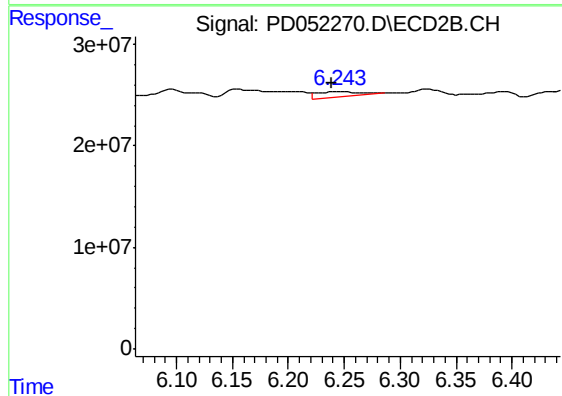

#11 cis-Chlordane


R.T.: 6.245 min
Delta R.T.: 0.007 min
Response: 14100166
Conc: 0.43 ng/ml

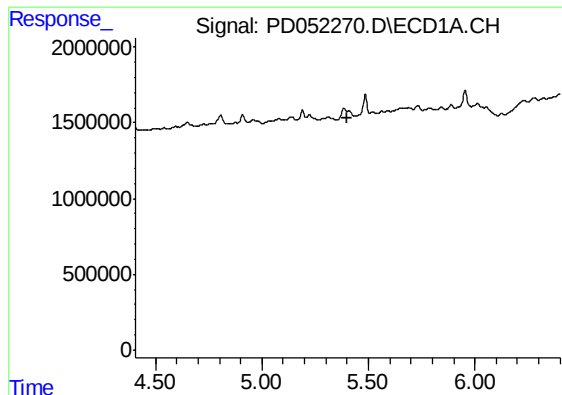

#13 Dielddrin


R.T.: 0.000 min
Exp R.T.: 5.404 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5M4

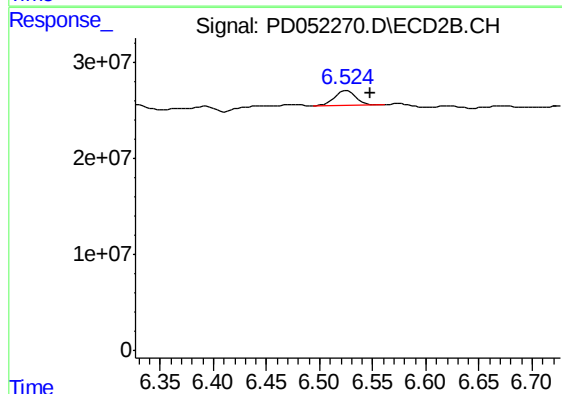


#13 Dielddrin

R.T.: 6.525 min
Delta R.T.: -0.022 min
Response: 20489655
Conc: 0.66 ng/ml

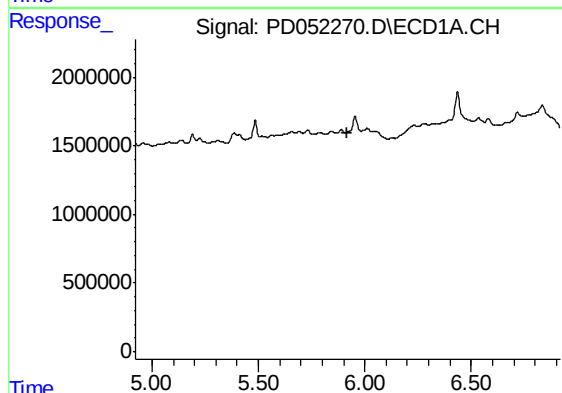


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 5.920 min
Response: 0
Conc: N.D.

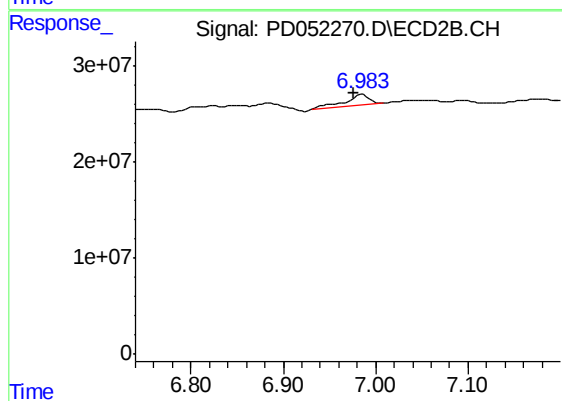

#15 Endosulfan II


R.T.: 6.986 min
Delta R.T.: 0.010 min
Response: 21636728
Conc: 0.85 ng/ml

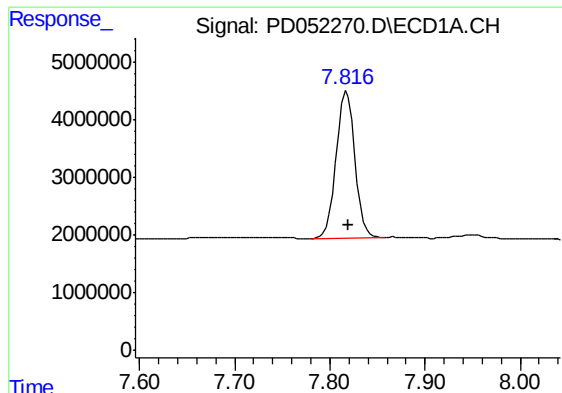

#27 Decachlorobiphenyl

R.T.: 7.818 min
Delta R.T.: -0.002 min
Response: 34954180
Conc: 22.32 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF5M4

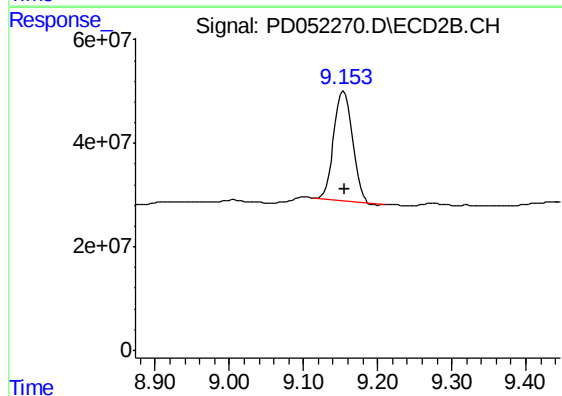

#27 Decachlorobiphenyl

R.T.: 9.155 min
Delta R.T.: -0.001 min
Response: 369185567
Conc: 23.92 ng/ml