

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032819\
 Data File : PD052275.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Mar 2019 00:17
 Operator : AJ\SJ
 Sample : PIBLK08
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK09

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 01:44:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032519CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 25 18:59:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1) SA	Tetrachlo...	3.221	4.042	33353055	630.1E6	23.497	21.654
27) SA	Decachlor...	7.817	9.154	54637219	563.5E6	34.893	36.505
Target Compounds							
6) B	beta-BHC	0.000	4.934f	0 28740201	N.D.		1.566
8) B	Heptachlo...	0.000	5.922	0 97697794	N.D.		2.868
10) B	trans-Chl...	0.000	6.176	0 65134450	N.D.		1.918
11) B	cis-Chlor...	0.000	6.176f	0 65134450	N.D.		2.006


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032819\
Data File : PD052275.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Mar 2019 00:17
Operator : AJ\SJ
Sample : PIBLK08
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PIBLK09

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 01:44:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032519CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 25 18:59:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

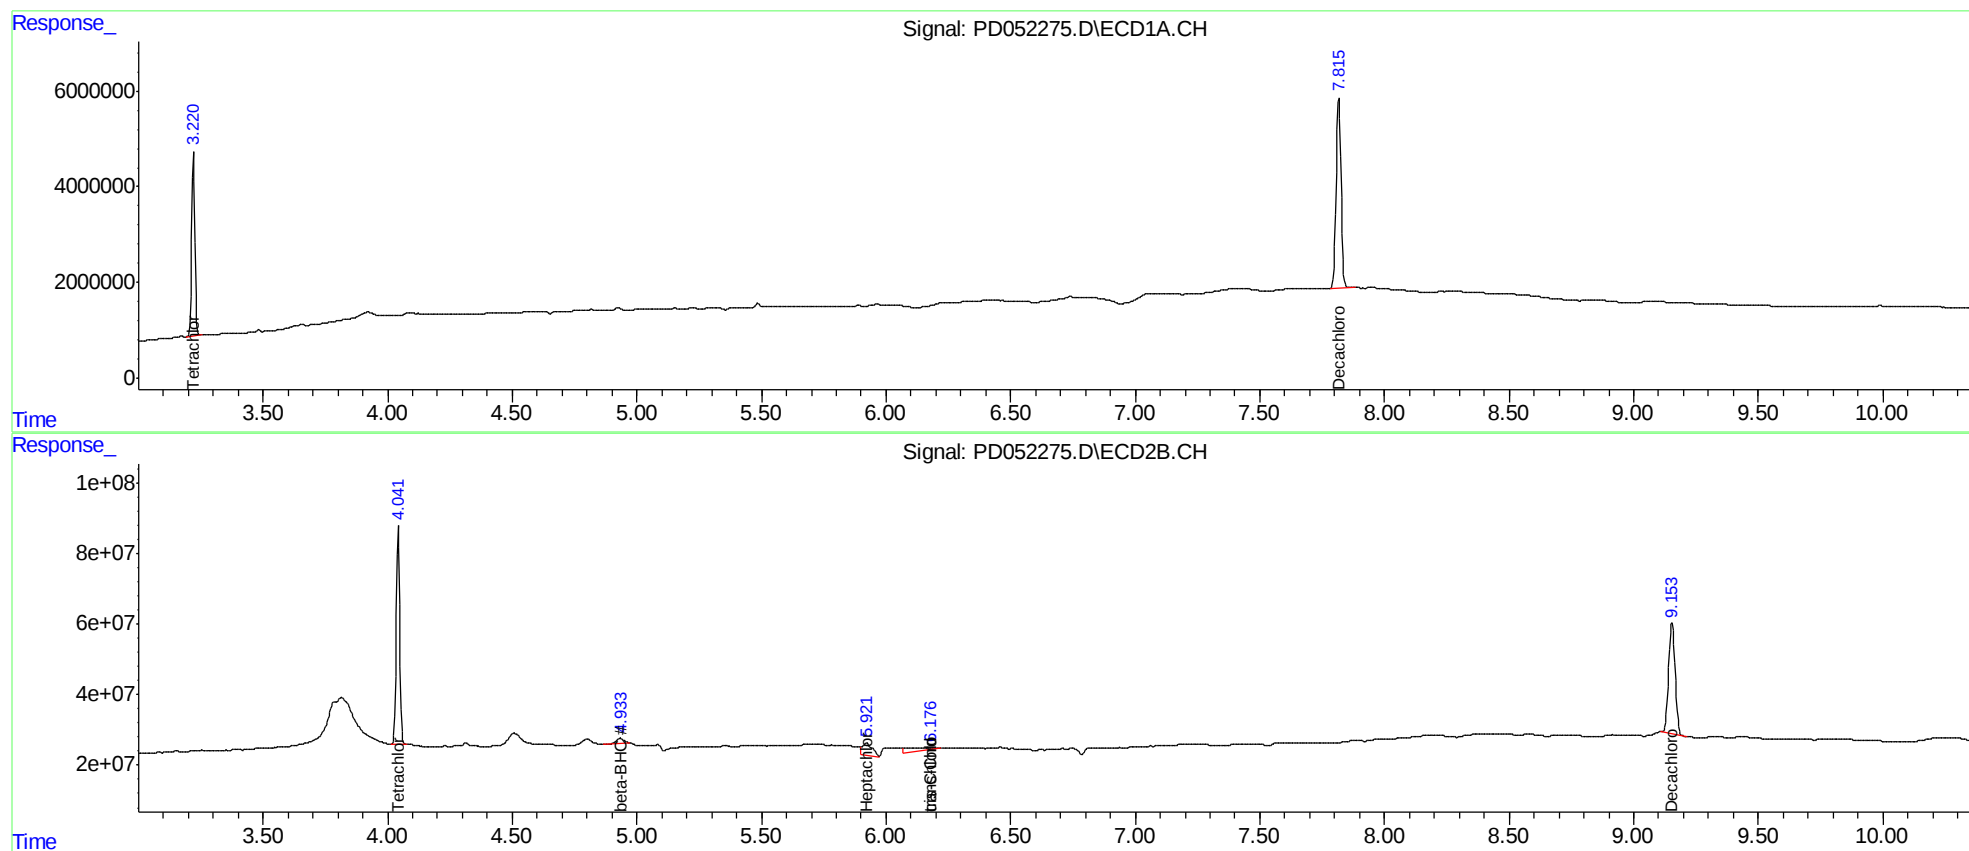


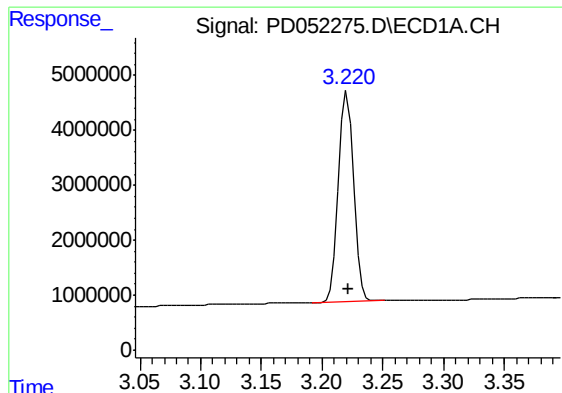

#1 Tetrachloro-m-xylene


R.T.: 3.221 min
Delta R.T.: -0.001 min
Response: 33353055
Conc: 23.50 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK09

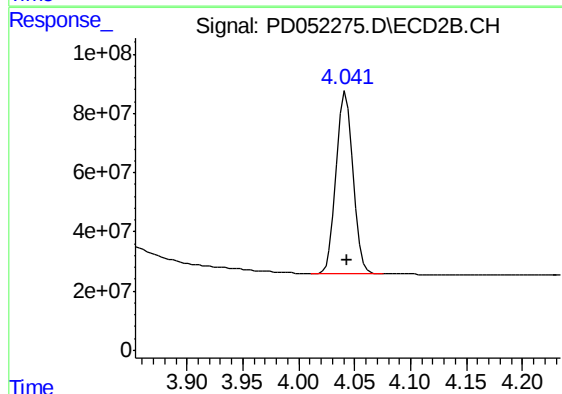


#1 Tetrachloro-m-xylene

R.T.: 4.042 min
Delta R.T.: 0.000 min
Response: 630068980
Conc: 21.65 ng/ml

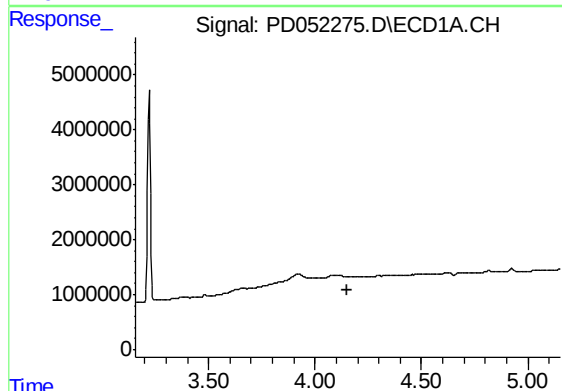


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.154 min
Response: 0
Conc: N.D.

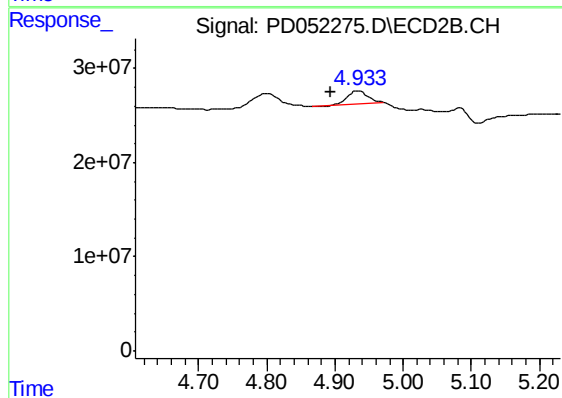

#6 beta-BHC


R.T.: 4.934 min
Delta R.T.: 0.041 min
Response: 28740201
Conc: 1.57 ng/ml

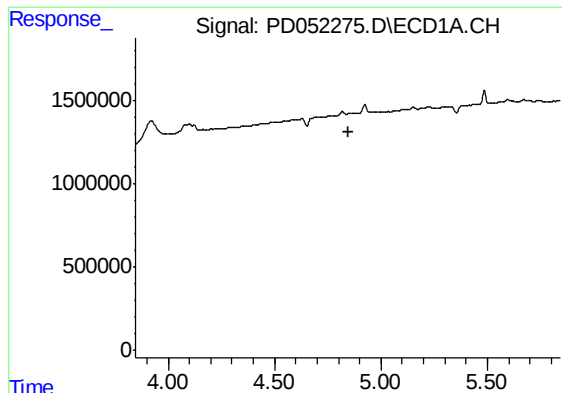

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.846 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PIBLK09

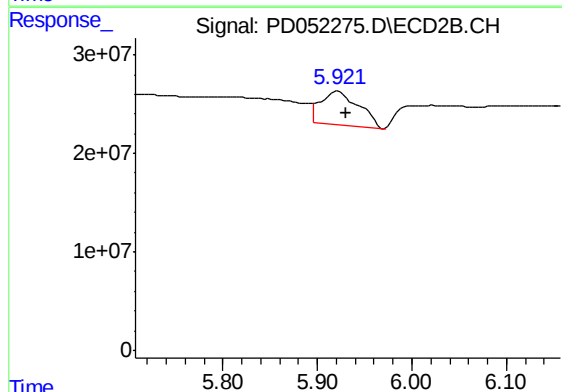


#8 Heptachlor epoxide

R.T.: 5.922 min
Delta R.T.: -0.009 min
Response: 97697794
Conc: 2.87 ng/ml

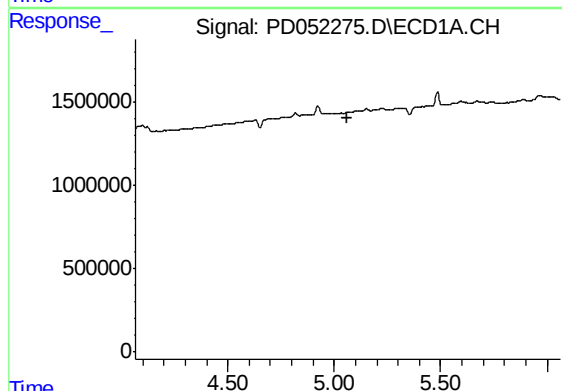


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.063 min
Response: 0
Conc: N.D.

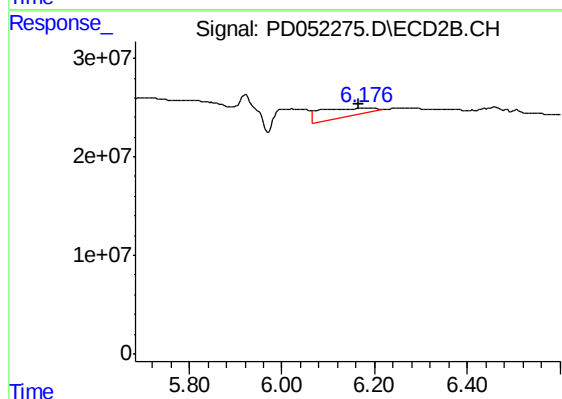

#10 trans-Chlordane


R.T.: 6.176 min
Delta R.T.: 0.010 min
Response: 65134450
Conc: 1.92 ng/ml

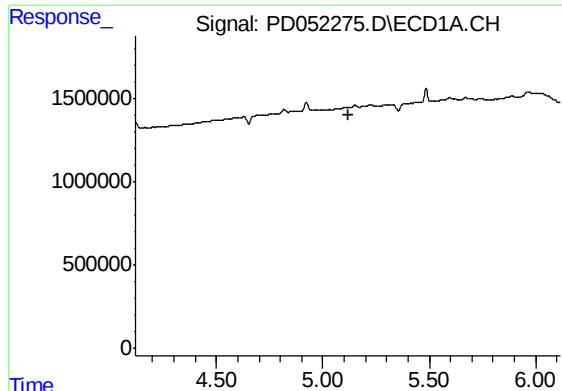

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.119 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PIBLK09

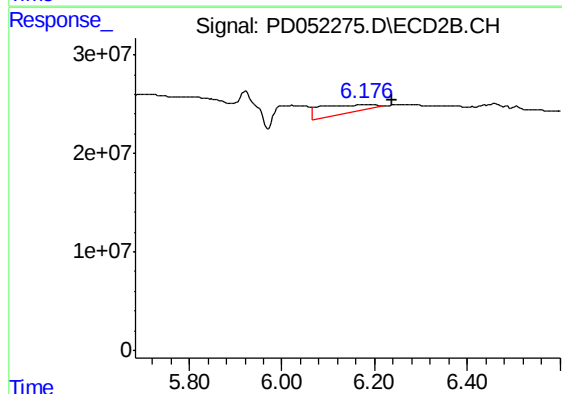


#11 cis-Chlordane

R.T.: 6.176 min
Delta R.T.: -0.063 min
Response: 65134450
Conc: 2.01 ng/ml

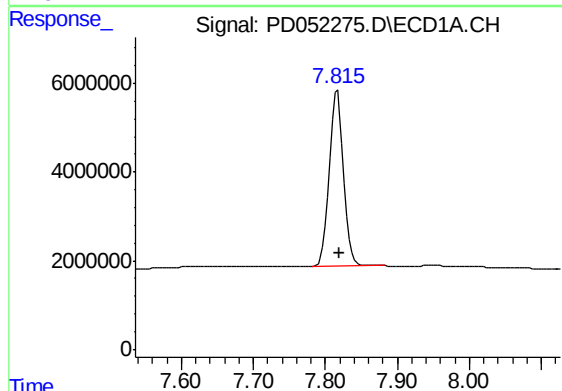

#27 Decachlorobiphenyl

R.T.: 7.817 min
Delta R.T.: -0.003 min
Response: 54637219
Conc: 34.89 ng/ml

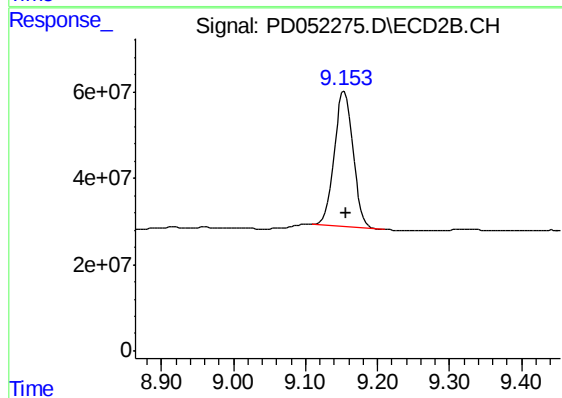

#27 Decachlorobiphenyl

R.T.: 9.154 min
Delta R.T.: -0.002 min
Response: 563517199
Conc: 36.50 ng/ml