

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032822\
 Data File : PD068790.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Mar 2022 10:08
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 28 15:43:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 03:30:32 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.454	4.174	24954213	218.5E6	20.552	22.854
28)	SA Decachlor...	8.216	9.374	27178136	131.7E6	21.512	23.236
Target Compounds							
3)	MA gamma-BHC...	0.000	4.890f	0	418822	N.D.	0.033 #
4)	MA Heptachlor	0.000	5.380	0	380599	N.D.	0.032 #
6)	B beta-BHC	4.394f	5.009f	154519	3397026	0.208	0.619 #
7)	B delta-BHC	0.000	5.229f	0	652927	N.D.	0.054 #
8)	B Heptachlo...	0.000	6.089	0	168900	N.D.	0.016 #
11)	B alpha-Chl...	0.000	6.383f	0	605427	N.D.	0.061 #
21)	B Endrin ke...	0.000	7.969	0	4245497	N.D.	0.548 #
26)	Chlordane-4	0.000	6.383f	0	605427	N.D.	0.389 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032822\
Data File : PD068790.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Mar 2022 10:08
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 28 15:43:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 03:30:32 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

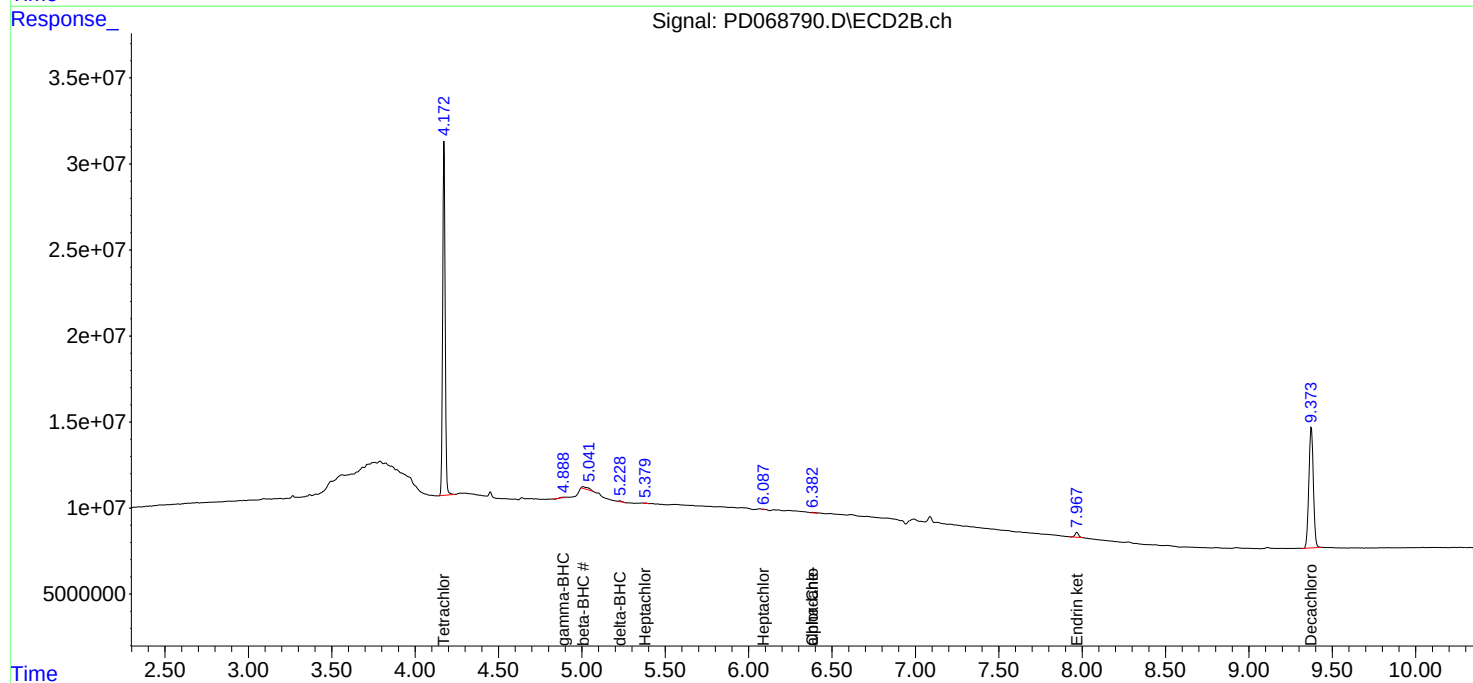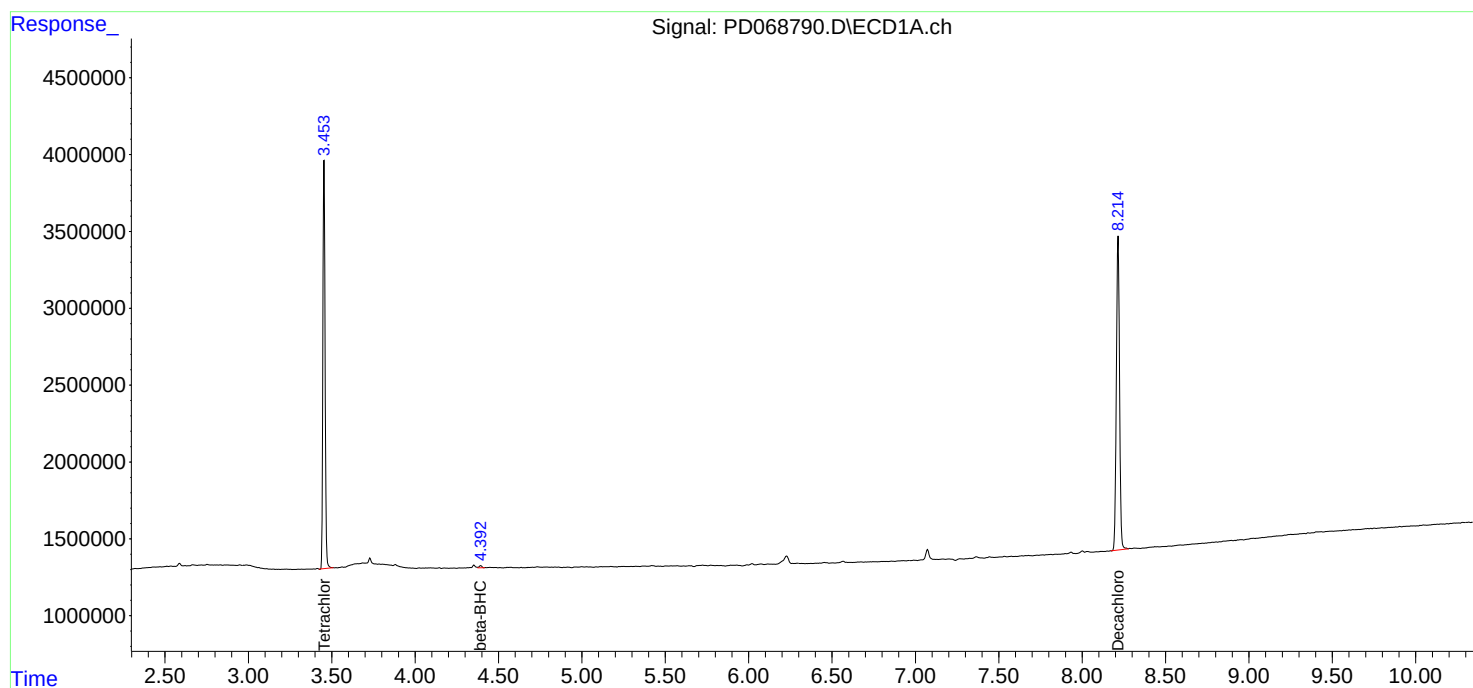


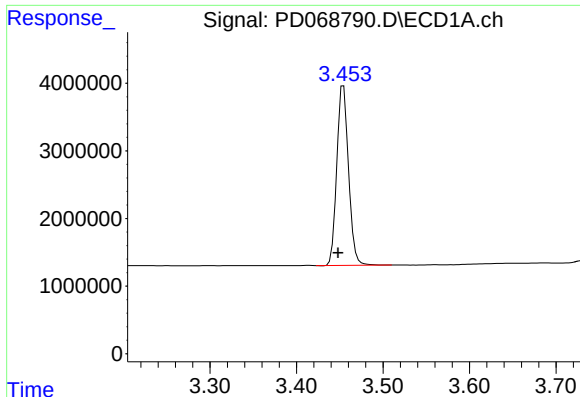

#1 Tetrachloro-m-xylene


R.T.: 3.454 min
Delta R.T.: 0.006 min
Response: 24954213
Conc: 20.55 ng/ml

Instrument :
ECD_D
ClientSampleId :

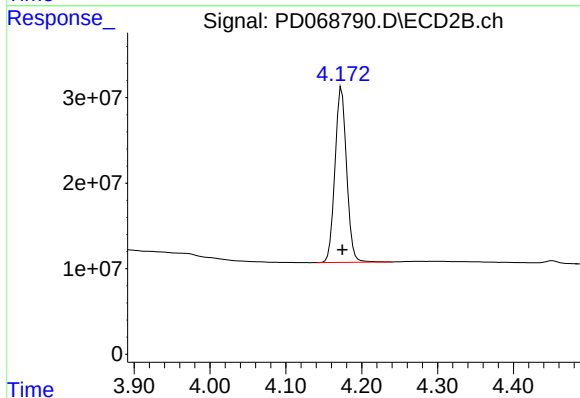


#1 Tetrachloro-m-xylene

R.T.: 4.174 min
Delta R.T.: -0.001 min
Response: 218499886
Conc: 22.85 ng/ml

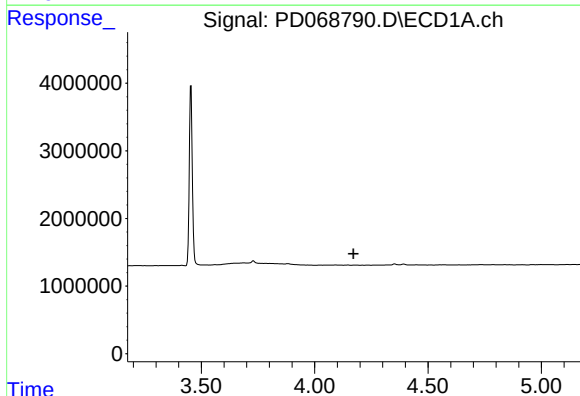


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.172 min
Response: 0
Conc: N.D.

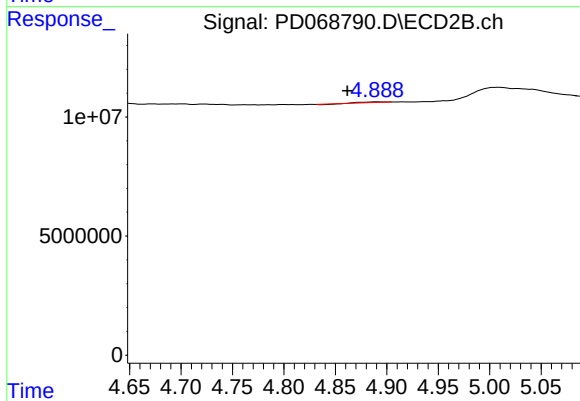

#3 gamma-BHC (Lindane)


R.T.: 4.890 min
Delta R.T.: 0.028 min
Response: 418822
Conc: 0.03 ng/ml

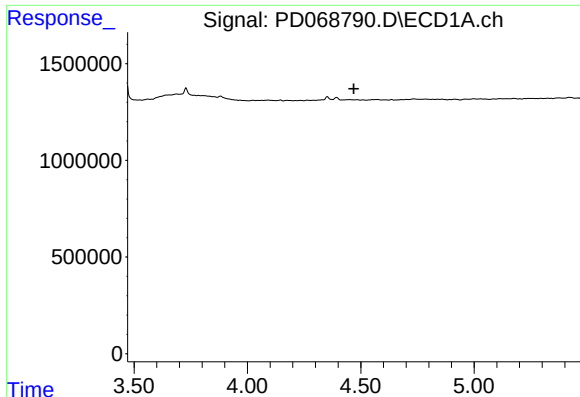

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.470 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

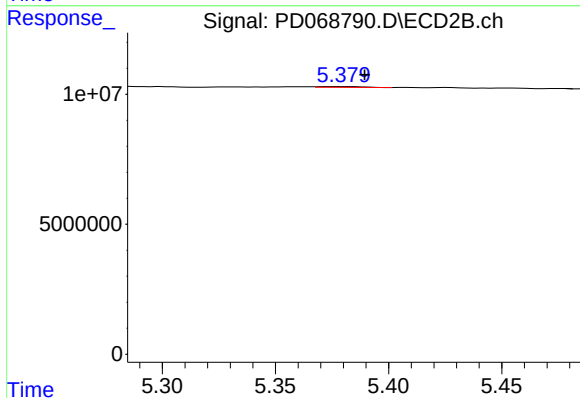


#4 Heptachlor

R.T.: 5.380 min
Delta R.T.: -0.009 min
Response: 380599
Conc: 0.03 ng/ml

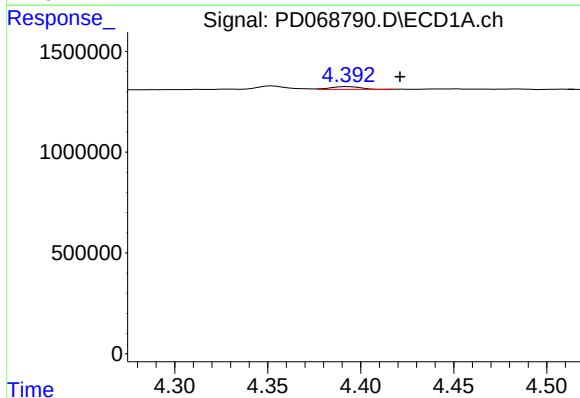


#6 beta-BHC

R.T.: 4.394 min
Delta R.T.: -0.028 min
Response: 154519
Conc: 0.21 ng/ml

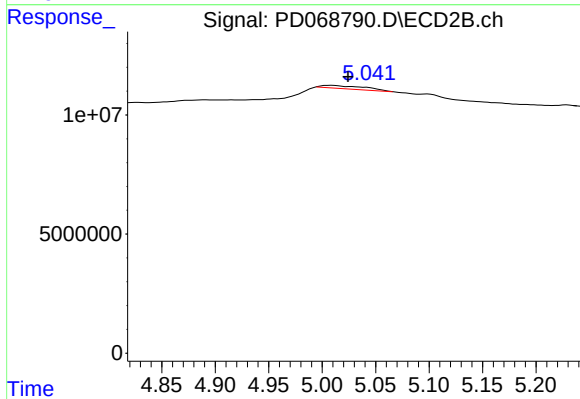

#6 beta-BHC


R.T.: 5.009 min
Delta R.T.: -0.016 min
Response: 3397026
Conc: 0.62 ng/ml

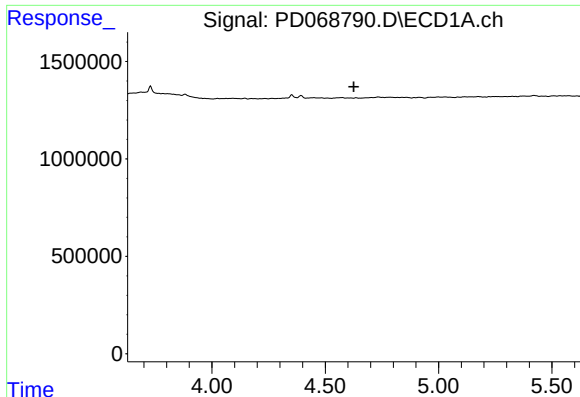

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.626 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

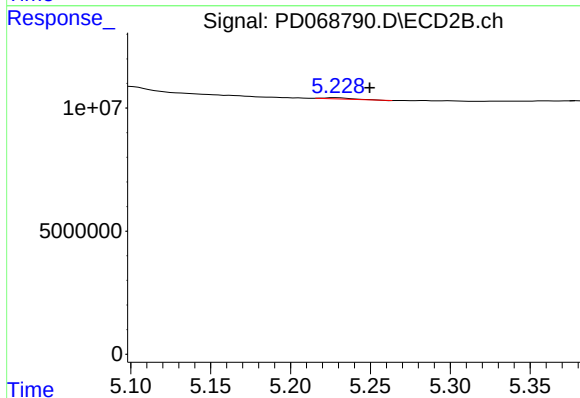


#7 delta-BHC

R.T.: 5.229 min
Delta R.T.: -0.021 min
Response: 652927
Conc: 0.05 ng/ml

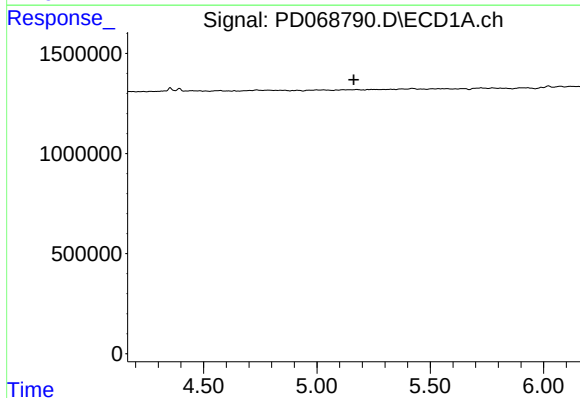


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.162 min
Response: 0
Conc: N.D.

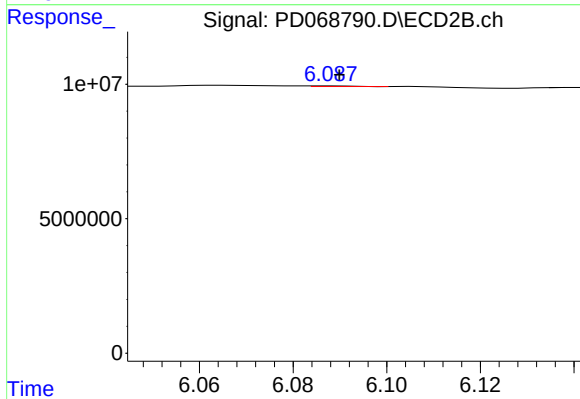

#8 Heptachlor epoxide


R.T.: 6.089 min
Delta R.T.: -0.001 min
Response: 168900
Conc: 0.02 ng/ml

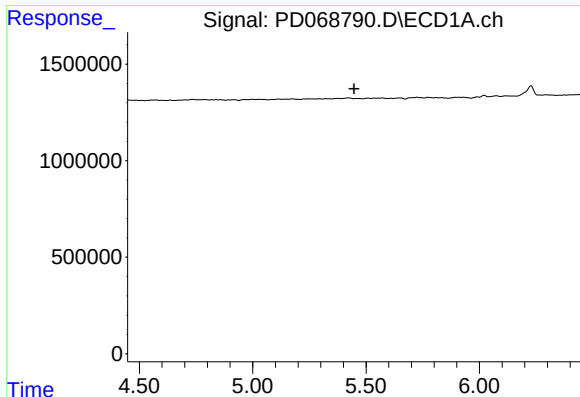

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.447 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

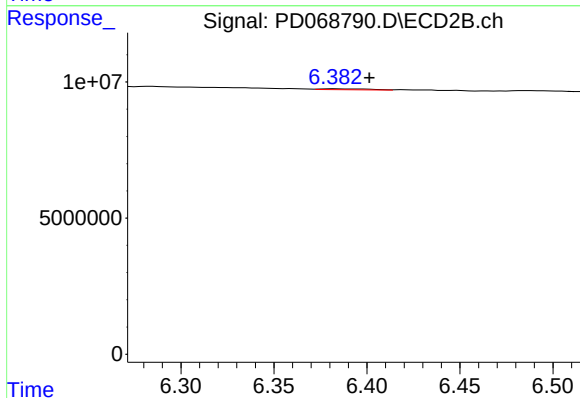


#11 alpha-Chlordane

R.T.: 6.383 min
Delta R.T.: -0.018 min
Response: 605427
Conc: 0.06 ng/ml

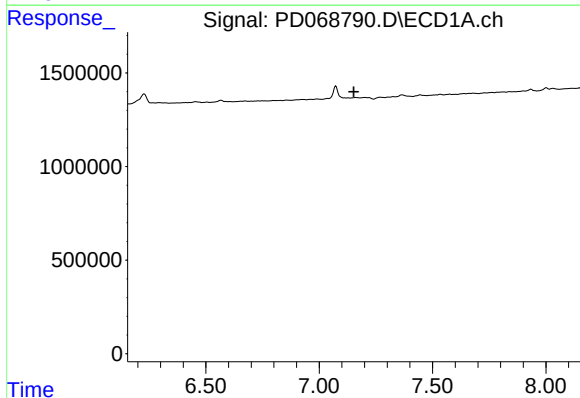


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 7.153 min
Response: 0
Conc: N.D.

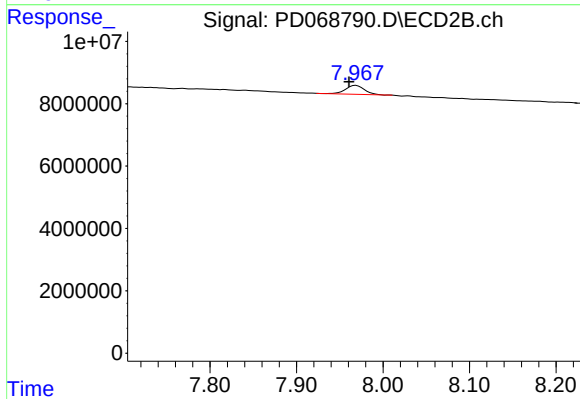

#21 Endrin ketone


R.T.: 7.969 min
Delta R.T.: 0.008 min
Response: 4245497
Conc: 0.55 ng/ml

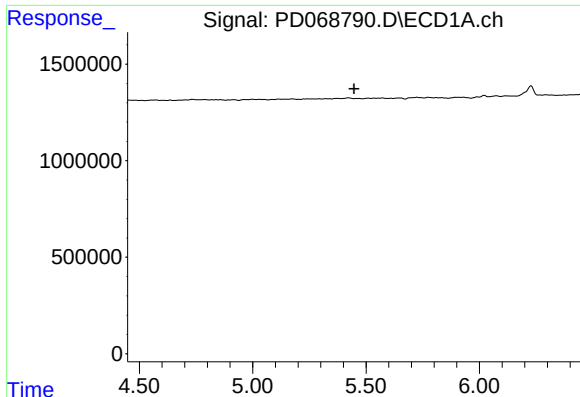

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.447 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

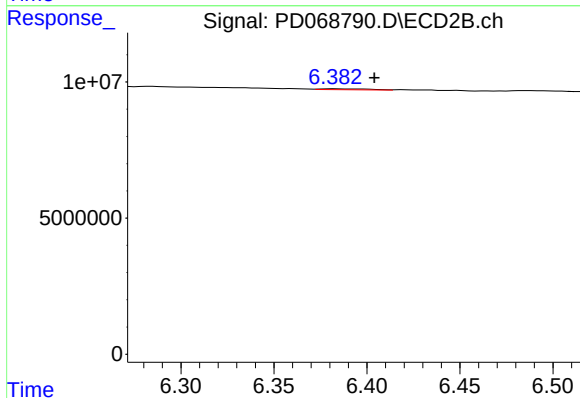


#26 Chlordane-4

R.T.: 6.383 min
Delta R.T.: -0.021 min
Response: 605427
Conc: 0.39 ng/ml

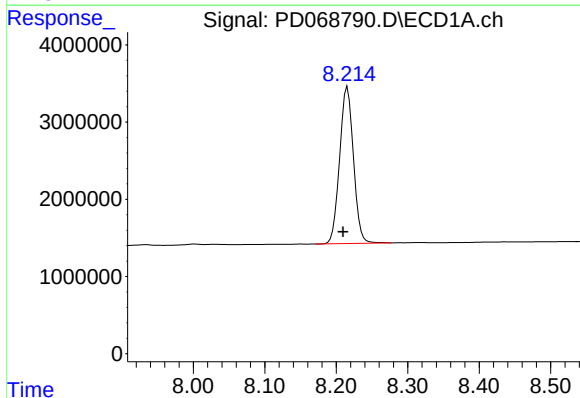

#28 Decachlorobiphenyl

R.T.: 8.216 min
Delta R.T.: 0.006 min
Response: 27178136
Conc: 21.51 ng/ml

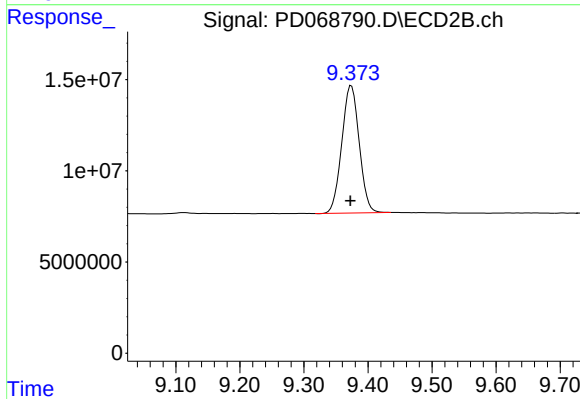

#28 Decachlorobiphenyl

R.T.: 9.374 min
Delta R.T.: 0.002 min
Response: 131673915
Conc: 23.24 ng/ml