

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032822\
 Data File : PD068800.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Mar 2022 13:53
 Operator : AR\AJ
 Sample : PB143676BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 01:45:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 03:30:32 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.453	4.174	22200592	194.4E6	18.285	20.329
28)	SA Decachlor...	8.213	9.374	26216779	127.8E6	20.751	22.555
Target Compounds							
4)	MA Heptachlor	0.000	5.380	0	56734	N.D.	0.005 #
6)	B beta-BHC	4.392f	0.000	336639	0	0.452	N.D. #
7)	B delta-BHC	0.000	5.230f	0	1452366	N.D.	0.121 #
8)	B Heptachlo...	0.000	6.084	0	906346	N.D.	0.087 #
9)	A Endosulfan I	0.000	6.468f	0	147374	N.D.	0.016 #
10)	B gamma-Chl...	5.416f	0.000	184807	0	0.122	N.D. #
11)	B alpha-Chl...	5.416f	0.000	184807	0	0.124	N.D. #
21)	B Endrin ke...	0.000	7.969	0	2726398	N.D.	0.352 #
25)	Chlordane-3	5.416f	0.000	184807	0	1.325	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032822\
Data File : PD068800.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Mar 2022 13:53
Operator : AR\AJ
Sample : PB143676BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 01:45:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 03:30:32 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

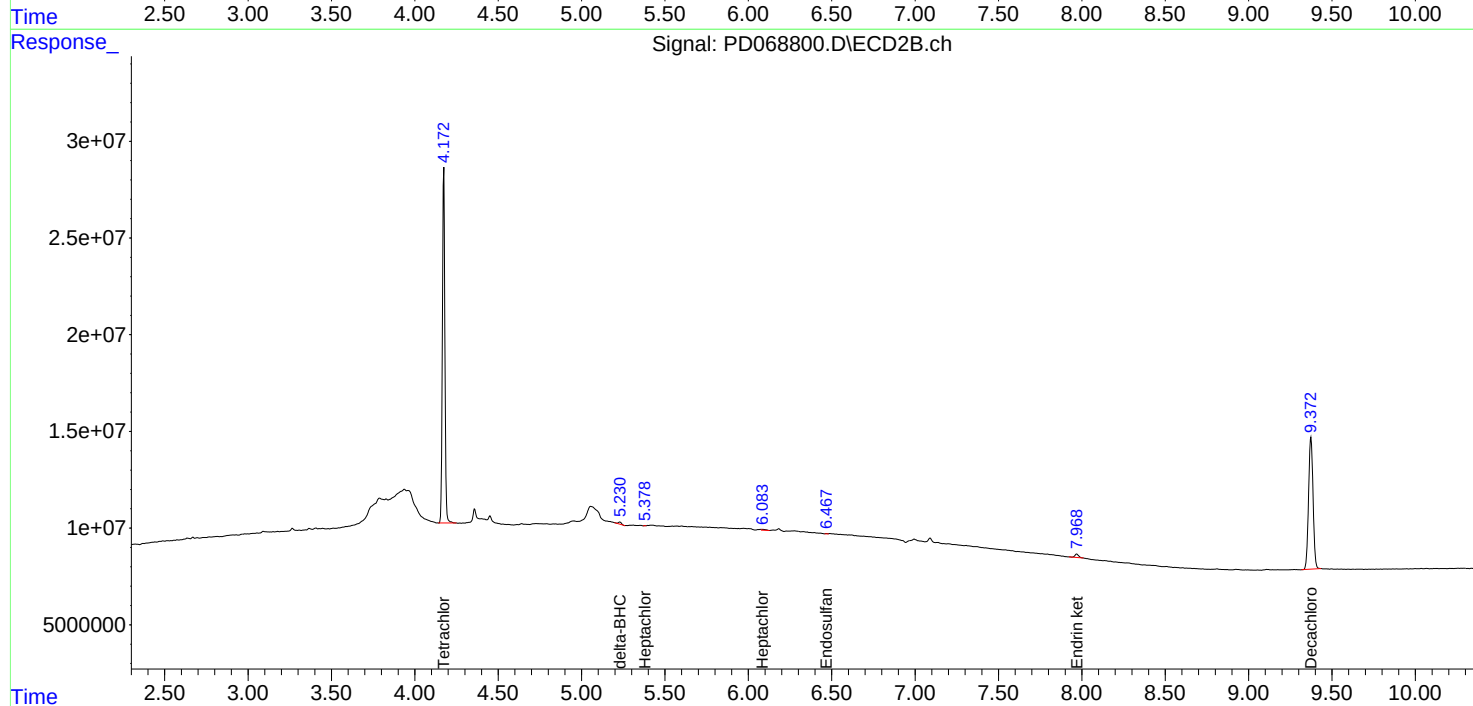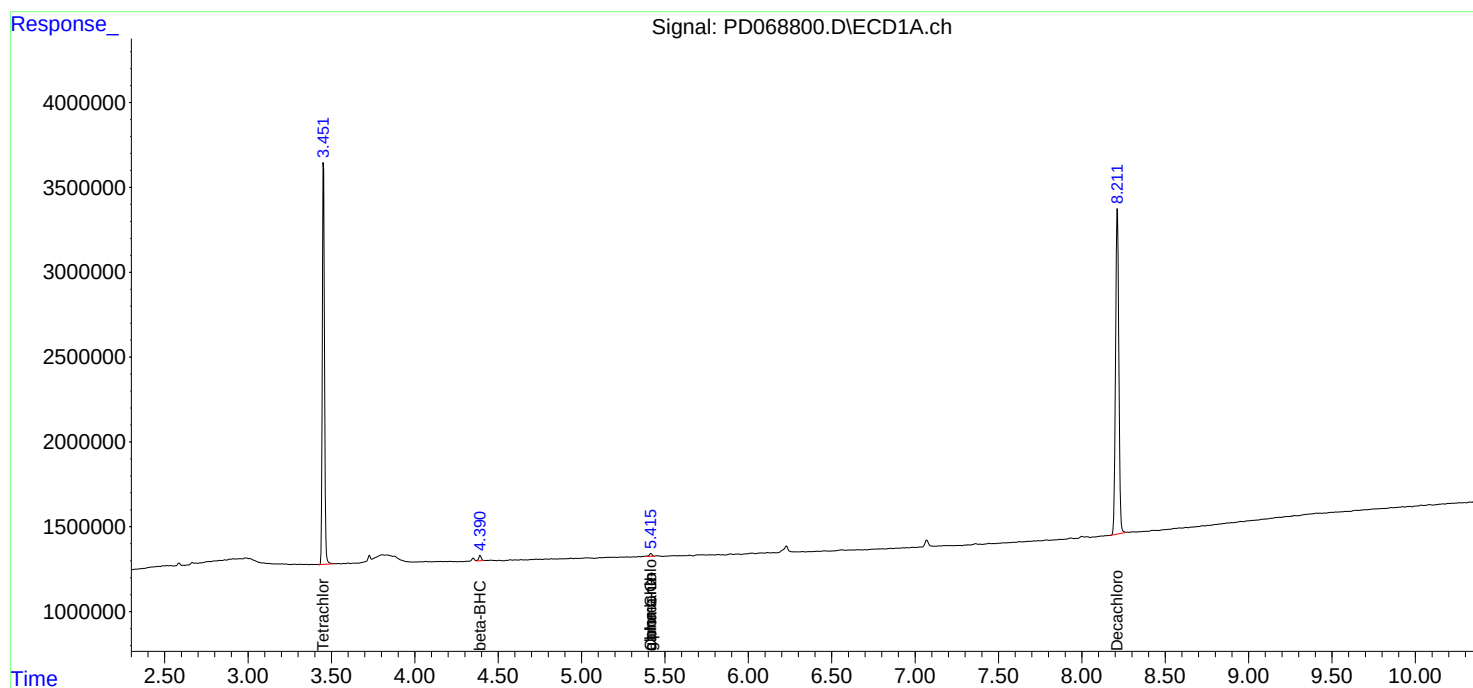


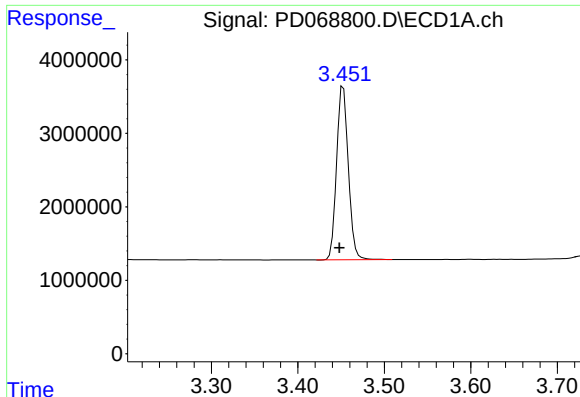

#1 Tetrachloro-m-xylene


R.T.: 3.453 min
Delta R.T.: 0.005 min
Response: 22200592
Conc: 18.28 ng/ml

Instrument :
ECD_D
ClientSampleId :

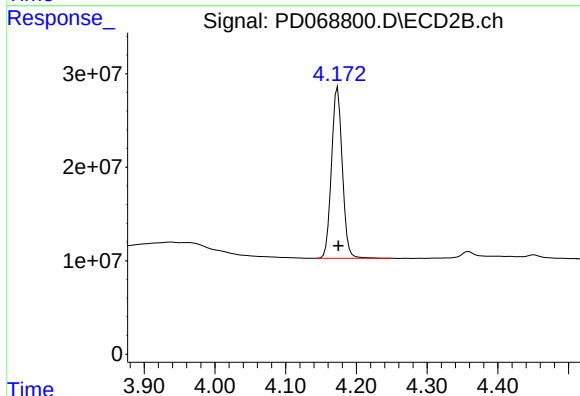


#1 Tetrachloro-m-xylene

R.T.: 4.174 min
Delta R.T.: -0.001 min
Response: 194361988
Conc: 20.33 ng/ml

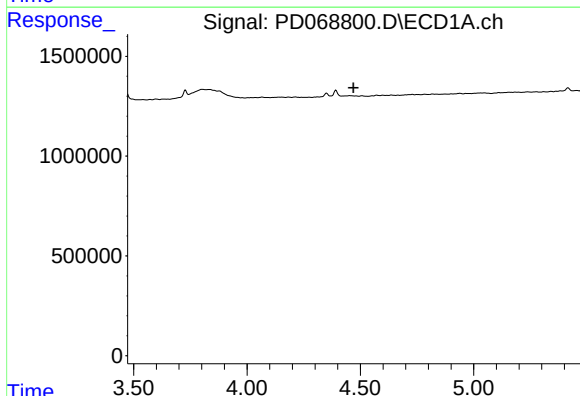


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.470 min
Response: 0
Conc: N.D.

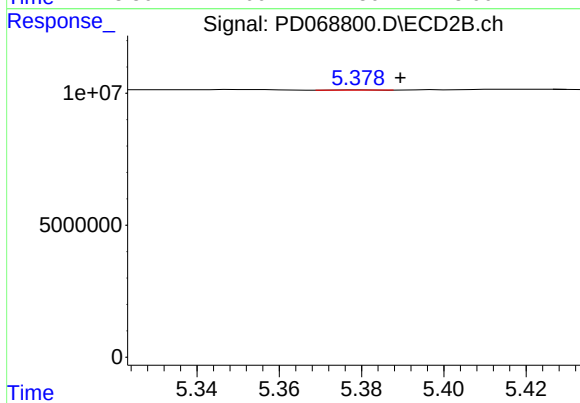

#4 Heptachlor


R.T.: 5.380 min
Delta R.T.: -0.010 min
Response: 56734
Conc: 0.00 ng/ml

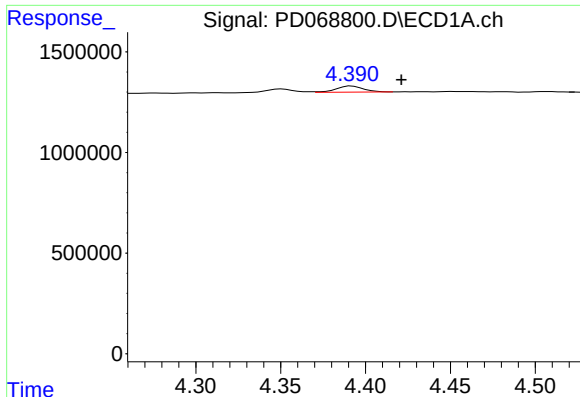

#6 beta-BHC


R.T.: 4.392 min
Delta R.T.: -0.029 min
Response: 336639
Conc: 0.45 ng/ml

Instrument :
ECD_D
ClientSampleId :

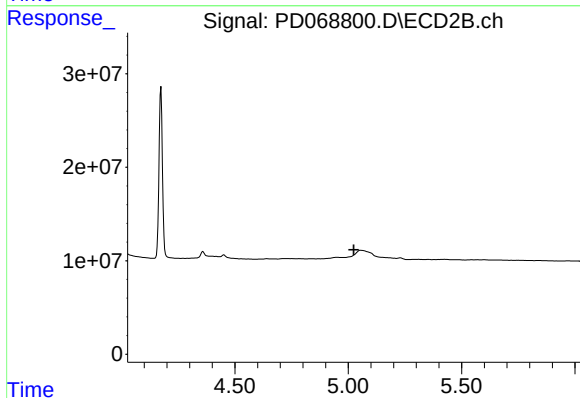


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 5.024 min
Response: 0
Conc: N.D.

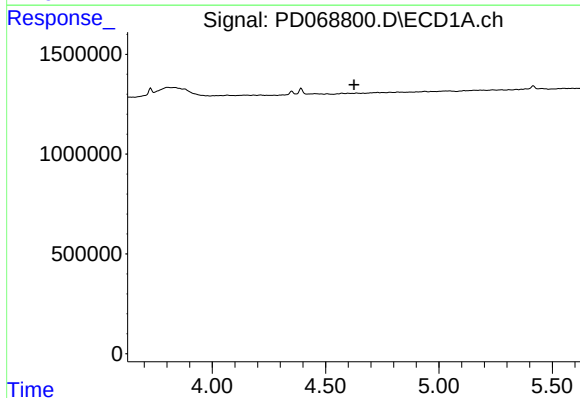


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.626 min
Response: 0
Conc: N.D.

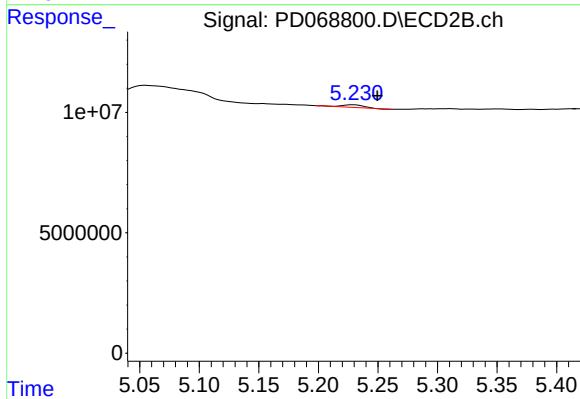

#7 delta-BHC


R.T.: 5.230 min
Delta R.T.: -0.020 min
Response: 1452366
Conc: 0.12 ng/ml

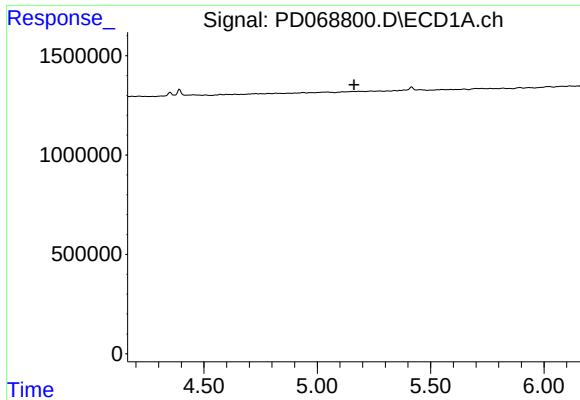

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.162 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

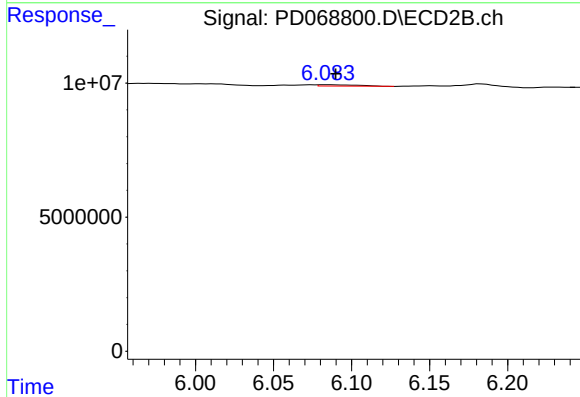


#8 Heptachlor epoxide

R.T.: 6.084 min
Delta R.T.: -0.006 min
Response: 906346
Conc: 0.09 ng/ml

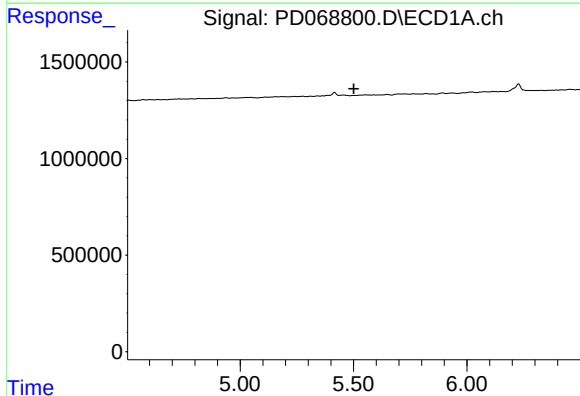


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.501 min
Response: 0
Conc: N.D.

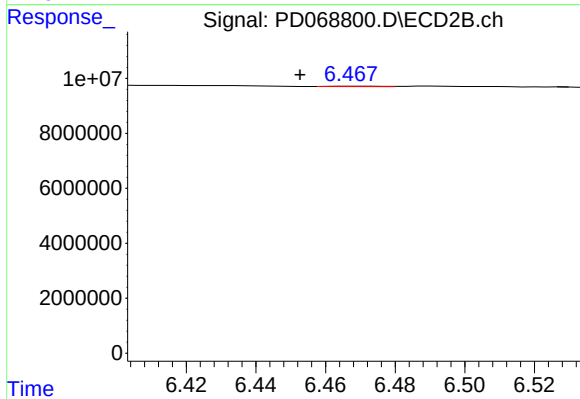

#9 Endosulfan I


R.T.: 6.468 min
Delta R.T.: 0.015 min
Response: 147374
Conc: 0.02 ng/ml

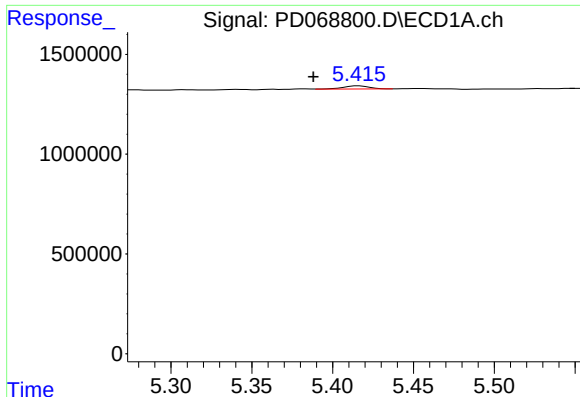

#10 gamma-Chlordane


R.T.: 5.416 min
Delta R.T.: 0.028 min
Response: 184807
Conc: 0.12 ng/ml

Instrument :
ECD_D
ClientSampleId :

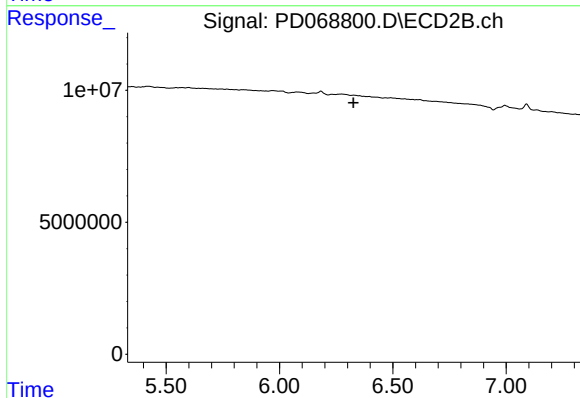


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.327 min
Response: 0
Conc: N.D.

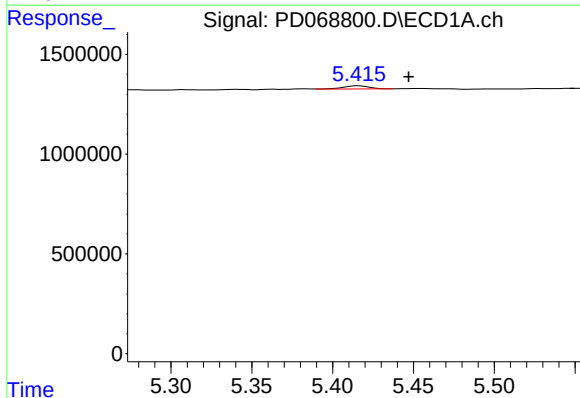


#11 alpha-Chlordane

R.T.: 5.416 min
Delta R.T.: -0.031 min
Response: 184807
Conc: 0.12 ng/ml

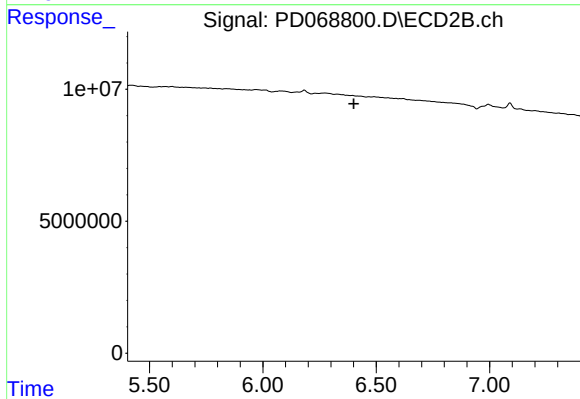

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.401 min
Response: 0
Conc: N.D.

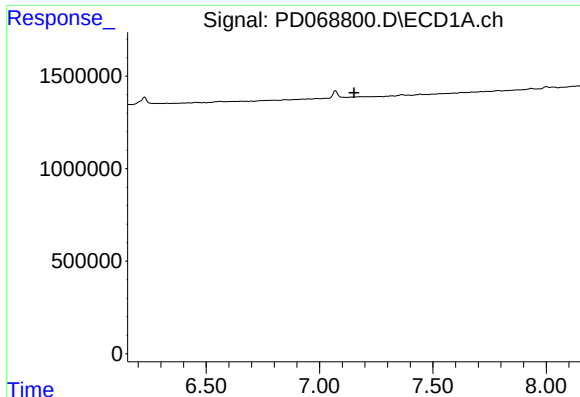

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.153 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

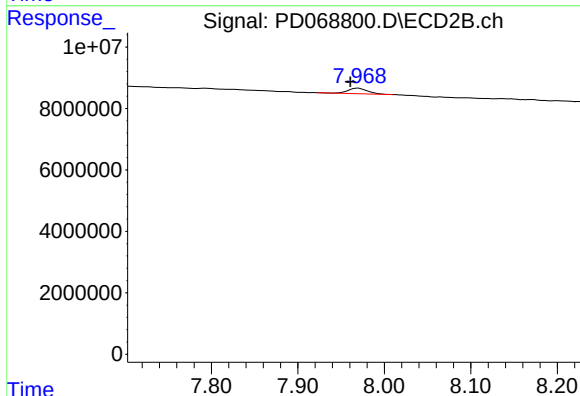


#21 Endrin ketone

R.T.: 7.969 min
Delta R.T.: 0.009 min
Response: 2726398
Conc: 0.35 ng/ml

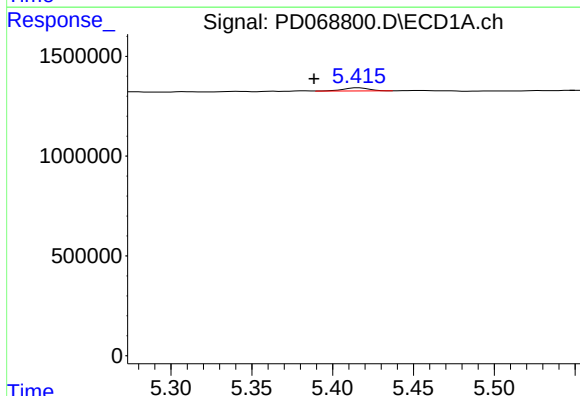


#25 Chlordane-3

R.T.: 5.416 min
Delta R.T.: 0.028 min
Response: 184807
Conc: 1.33 ng/ml

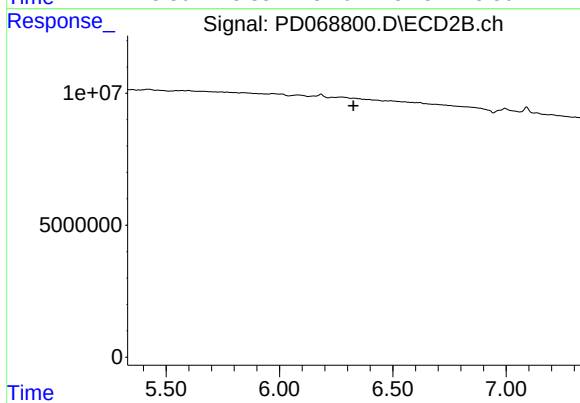

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 6.327 min
Response: 0
Conc: N.D.

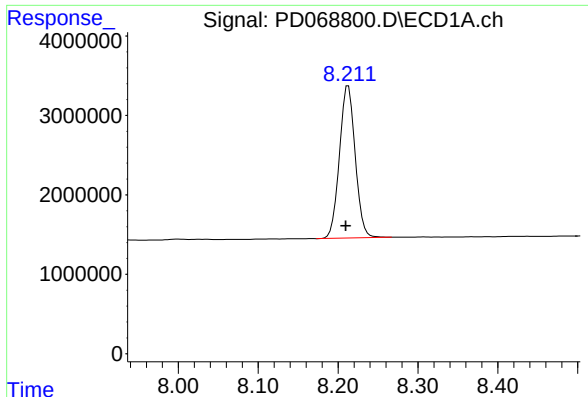

#28 Decachlorobiphenyl

R.T.: 8.213 min
Delta R.T.: 0.003 min
Response: 26216779
Conc: 20.75 ng/ml

Instrument :
ECD_D
ClientSampleId :

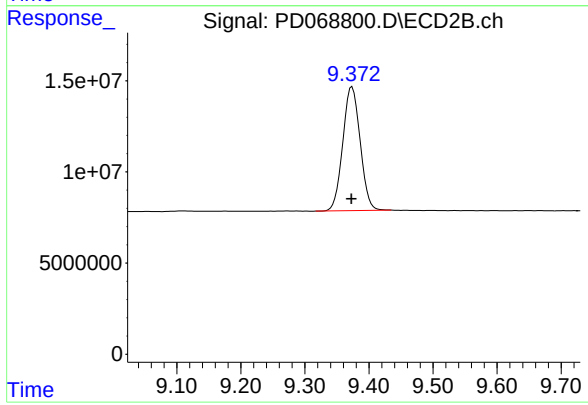

#28 Decachlorobiphenyl

R.T.: 9.374 min
Delta R.T.: 0.001 min
Response: 127814392
Conc: 22.56 ng/ml