

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032822\
 Data File : PD068796.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Mar 2022 12:51
 Operator : AR\AJ
 Sample : N2085-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 GW-3-23-2022

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 03/29/2022
 Supervised By : mohammad ahmed 03/29/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 28 15:45:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 03:30:32 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.448	4.172	23222798	138.2E6	19.126	14.455m
28) SA Decachlor...	8.208	9.371	26227818	127.4E6	20.760	22.488

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032822\
Data File : PD068796.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Mar 2022 12:51
Operator : AR\AJ
Sample : N2085-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampled :
GW-3-23-2022


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 03/29/2022
Supervised By : mohammad ahmed 03/29/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 28 15:45:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 03:30:32 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

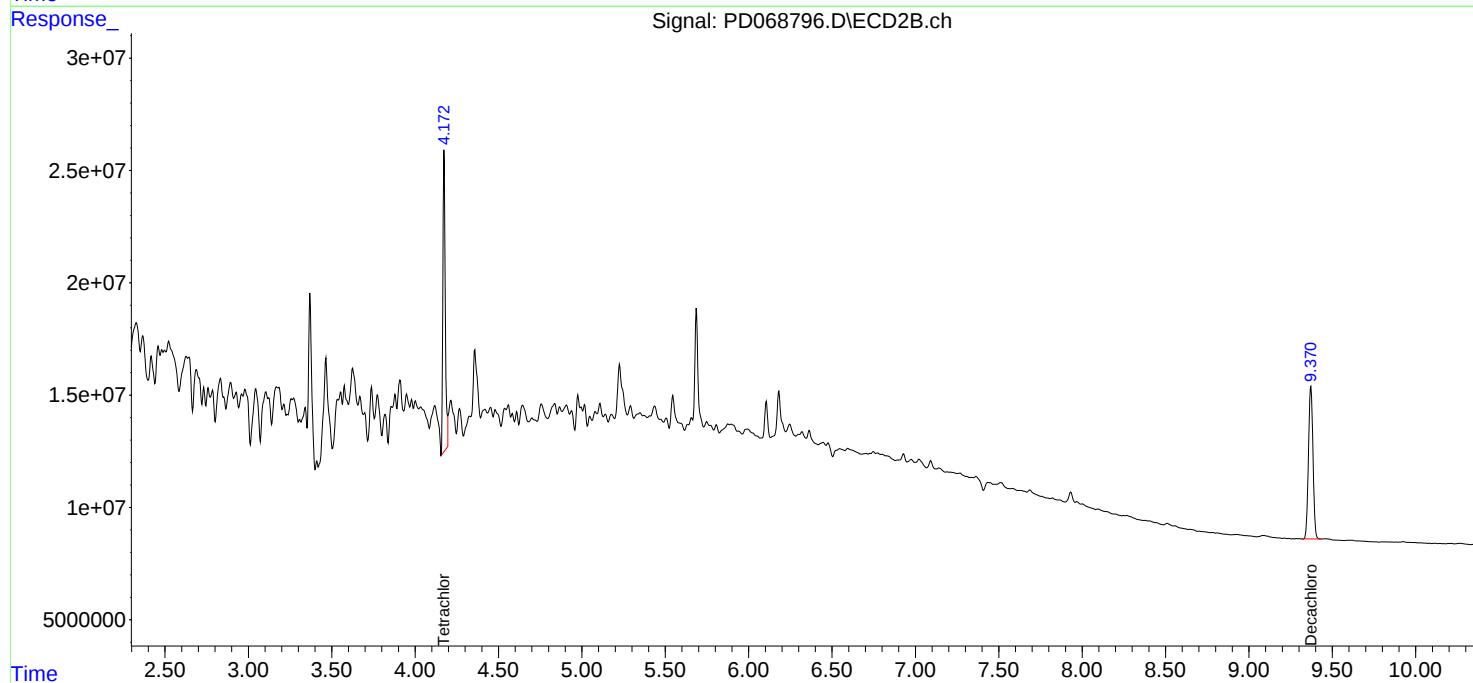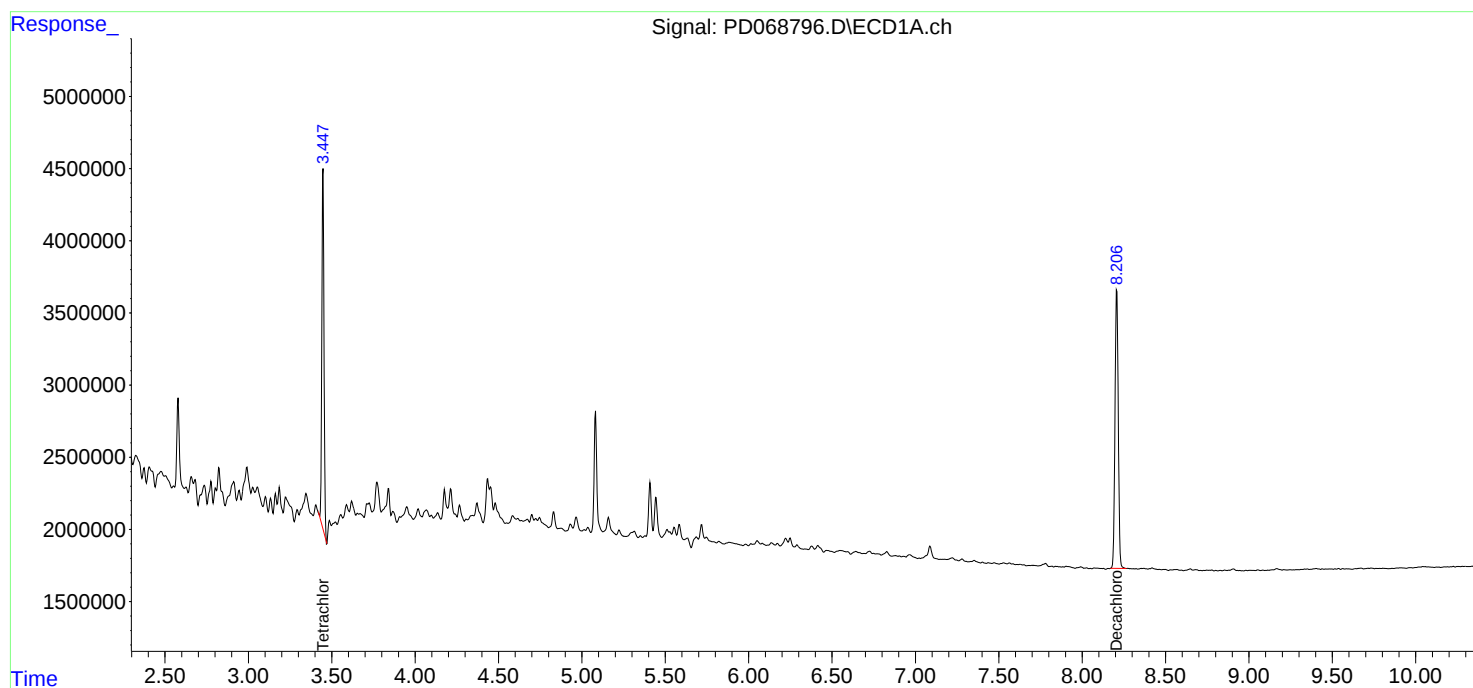

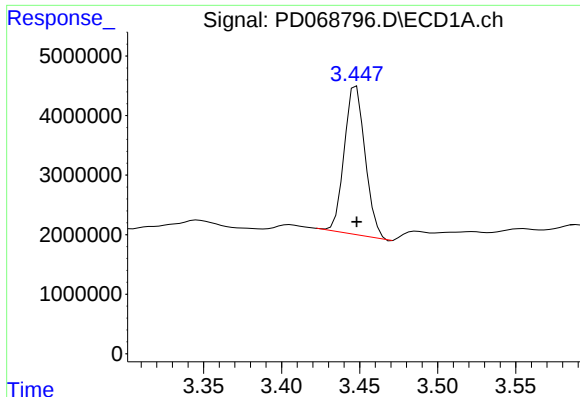


#1 Tetrachloro-m-xylene

R.T.: 3.448 min
Delta R.T.: 0.000 min
Response: 23222798
Conc: 19.13 ng/ml

Instrument :
ECD_D
ClientSampleId :
GW-3-23-2022


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/29/2022
Supervised By :mohammad ahmed 03/29/2022

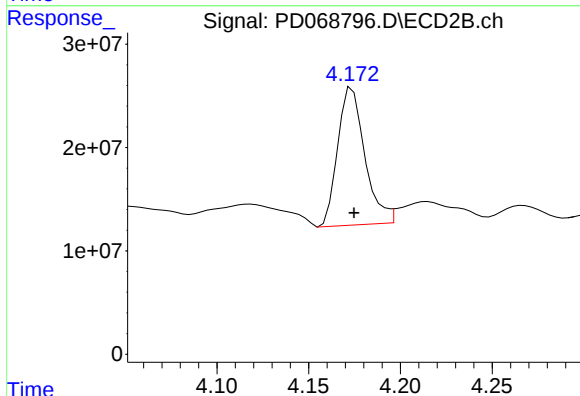


#1 Tetrachloro-m-xylene

R.T.: 4.172 min
Delta R.T.: -0.002 min
Response: 138199122
Conc: 14.45 ng/ml m

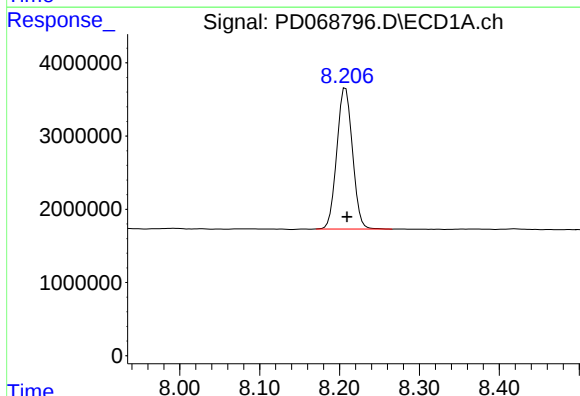

#28 Decachlorobiphenyl

R.T.: 8.208 min
Delta R.T.: -0.002 min
Response: 26227818
Conc: 20.76 ng/ml

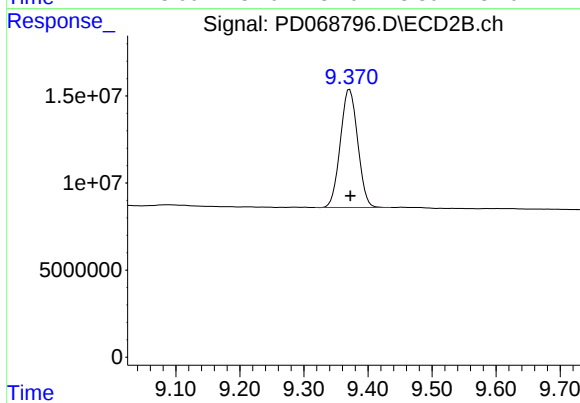

#28 Decachlorobiphenyl

R.T.: 9.371 min
Delta R.T.: -0.001 min
Response: 127431755
Conc: 22.49 ng/ml