

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032822\
 Data File : PD068804.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Mar 2022 14:49
 Operator : AR\AJ
 Sample : N2123-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 Lab Filtration

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 03/29/2022
 Supervised By : mohammad ahmed 03/29/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 01:47:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 03:30:32 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.447	4.173	15152049	121.9E6	12.479	12.749
2)	SA Decachlor...	8.206	9.370	9705857	44795114	7.682	7.905
Target Compounds							
12)	B 4,4'-DDE	5.615	6.548	3278730	2795810	2.397	0.302m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032822\
Data File : PD068804.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Mar 2022 14:49
Operator : AR\AJ
Sample : N2123-06
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
Lab Filtration


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 03/29/2022
Supervised By : mohammad ahmed 03/29/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 01:47:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 03:30:32 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

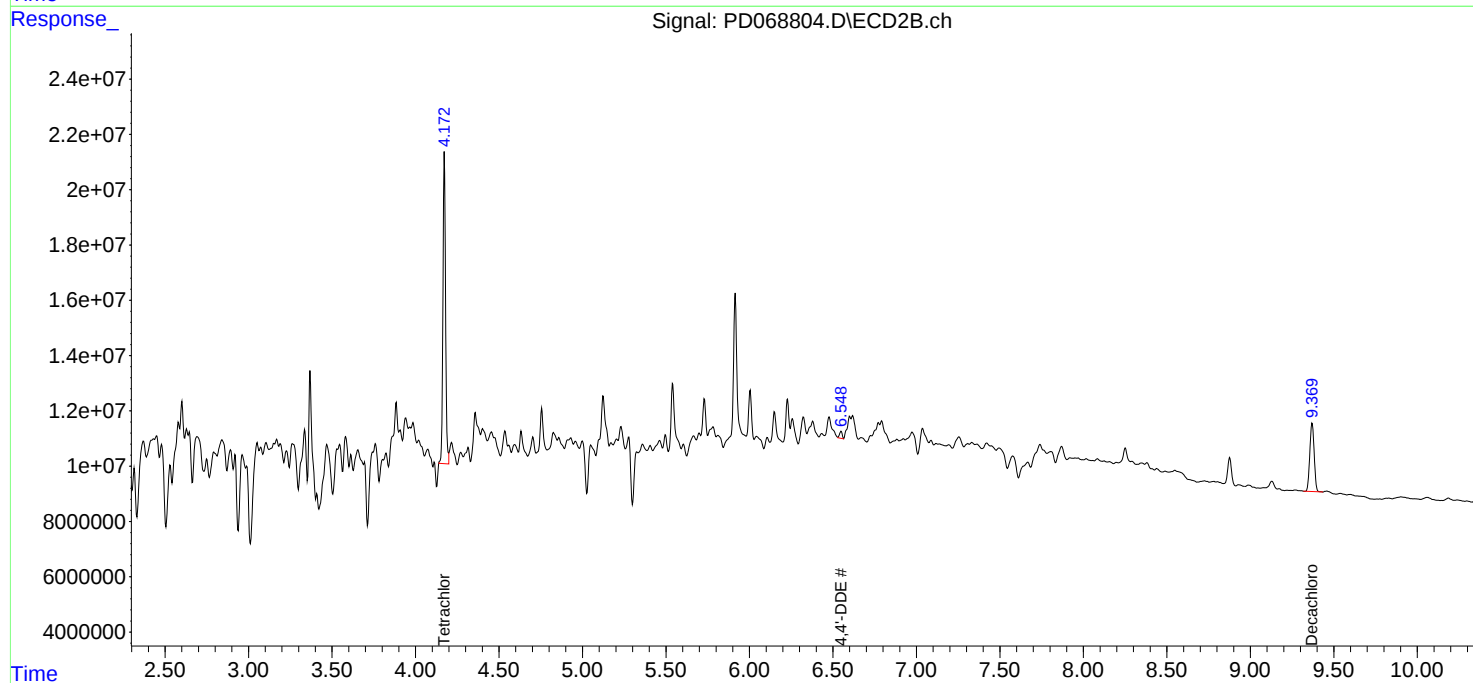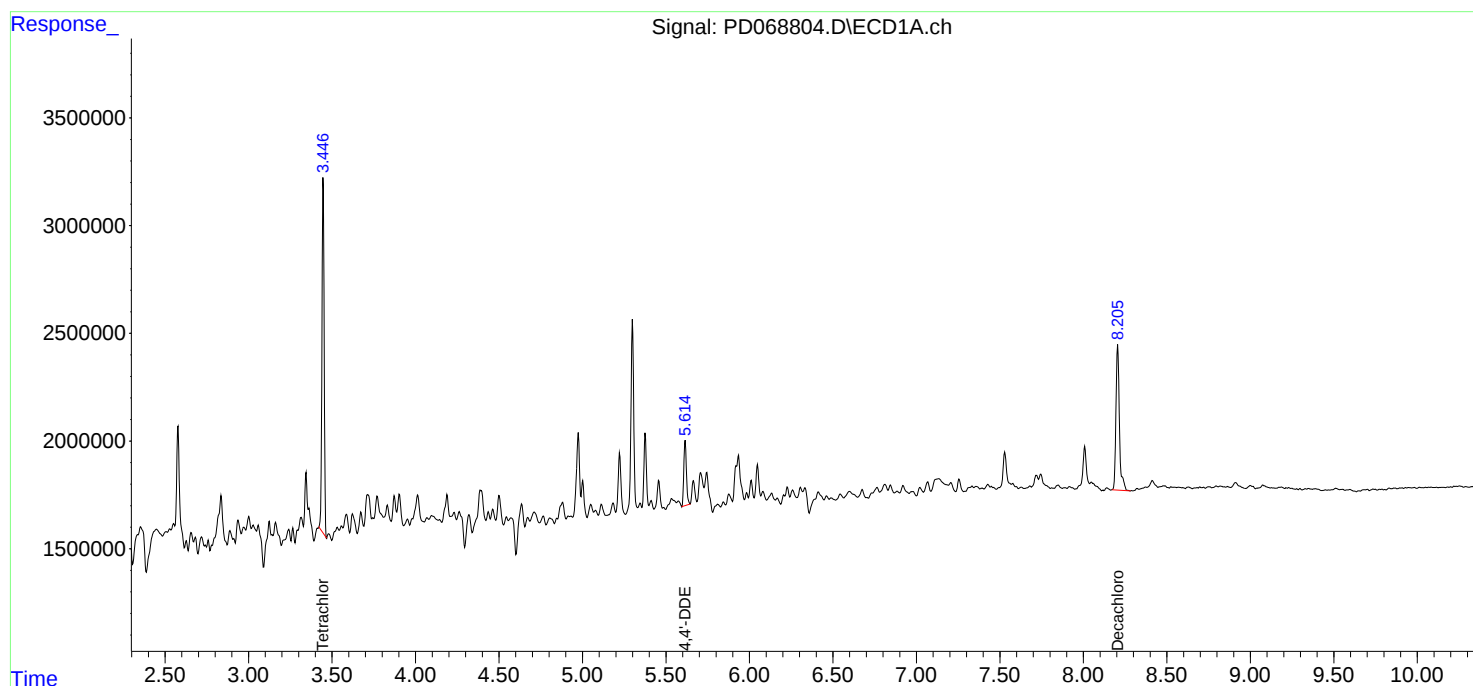

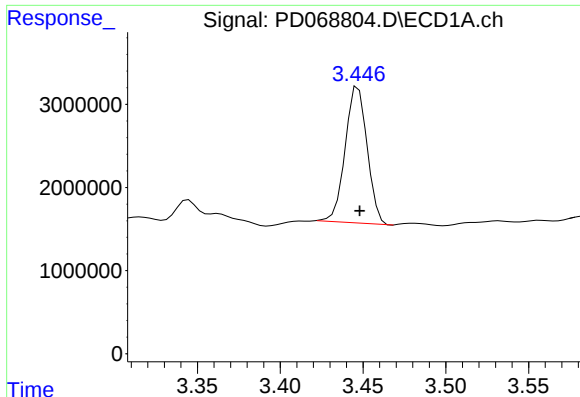


#1 Tetrachloro-m-xylene

R.T.: 3.447 min
Delta R.T.: 0.000 min
Response: 15152049
Conc: 12.48 ng/ml

Instrument :
ECD_D
ClientSampleId :
Lab Filtration


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/29/2022
Supervised By :mohammad ahmed 03/29/2022

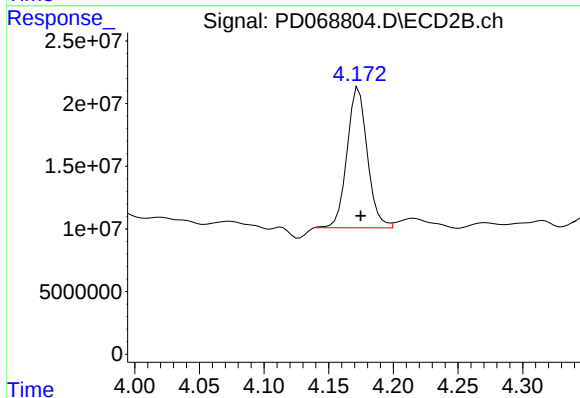


#1 Tetrachloro-m-xylene

R.T.: 4.173 min
Delta R.T.: -0.001 min
Response: 121886783
Conc: 12.75 ng/ml

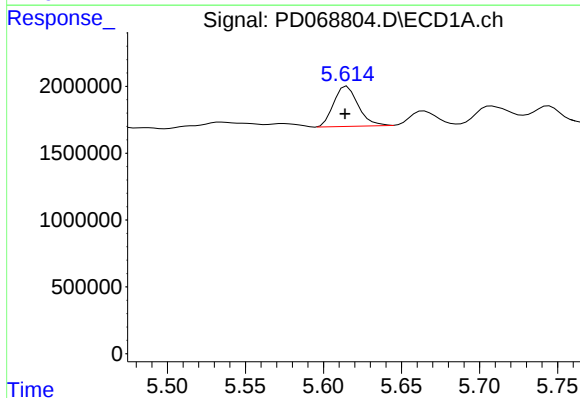


#12 4,4'-DDE

R.T.: 5.615 min
Delta R.T.: 0.001 min
Response: 3278730
Conc: 2.40 ng/ml

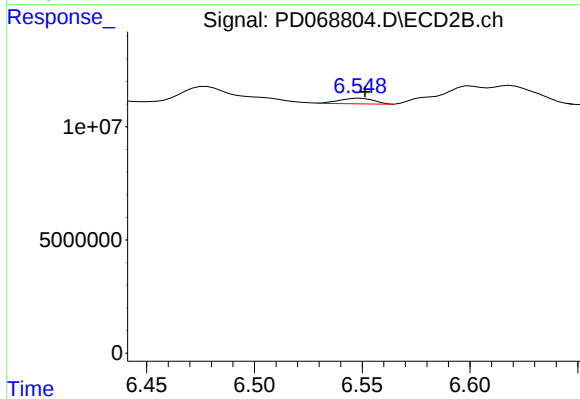

#12 4,4'-DDE

R.T.: 6.548 min
Delta R.T.: -0.003 min
Response: 2795810
Conc: 0.30 ng/ml m

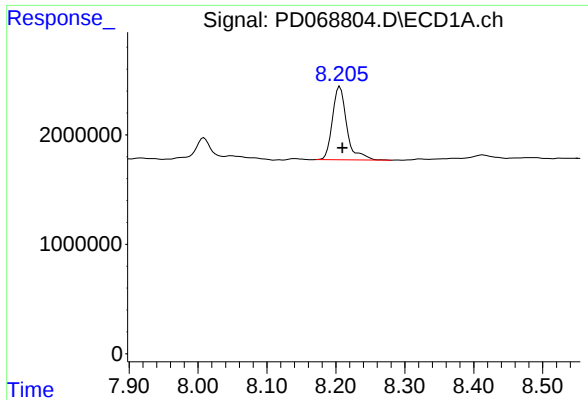


#28 Decachlorobiphenyl

R.T.: 8.206 min
Delta R.T.: -0.004 min
Response: 9705857
Conc: 7.68 ng/ml

Instrument :
ECD_D
ClientSampleId :
Lab Filtration

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/29/2022
Supervised By :mohammad ahmed 03/29/2022

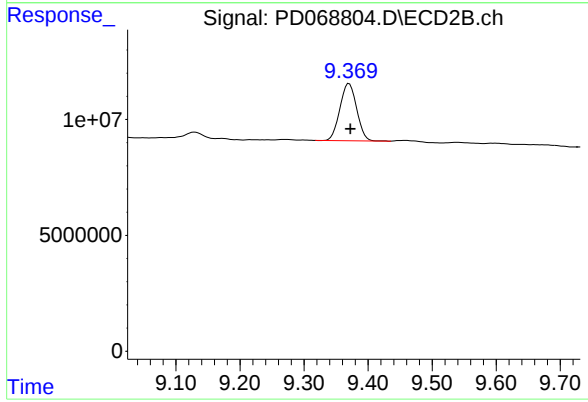

#28 Decachlorobiphenyl

R.T.: 9.370 min
Delta R.T.: -0.002 min
Response: 44795114
Conc: 7.90 ng/ml