

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032822\
 Data File : PD068808.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Mar 2022 15:45
 Operator : AR\AJ
 Sample : N2123-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SPLP-LEACHATE-AMENDED-COMP-CS-1

Manual Integrations APPROVED

Reviewed By : Abdul Mirza 03/29/2022
 Supervised By : mohammad ahmed 03/29/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 01:49:10 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 03:30:32 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.447	4.172	19419791	162.7E6	15.994	17.020m
28) SA Decachlor...	8.206	9.371	25172525	110.4E6	19.925	19.483

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032822\
Data File : PD068808.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Mar 2022 15:45
Operator : AR\AJ
Sample : N2123-03
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
SPLP-LEACHATE-AMENDED-COMP-CS-1


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 03/29/2022
Supervised By : mohammad ahmed 03/29/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 01:49:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 03:30:32 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

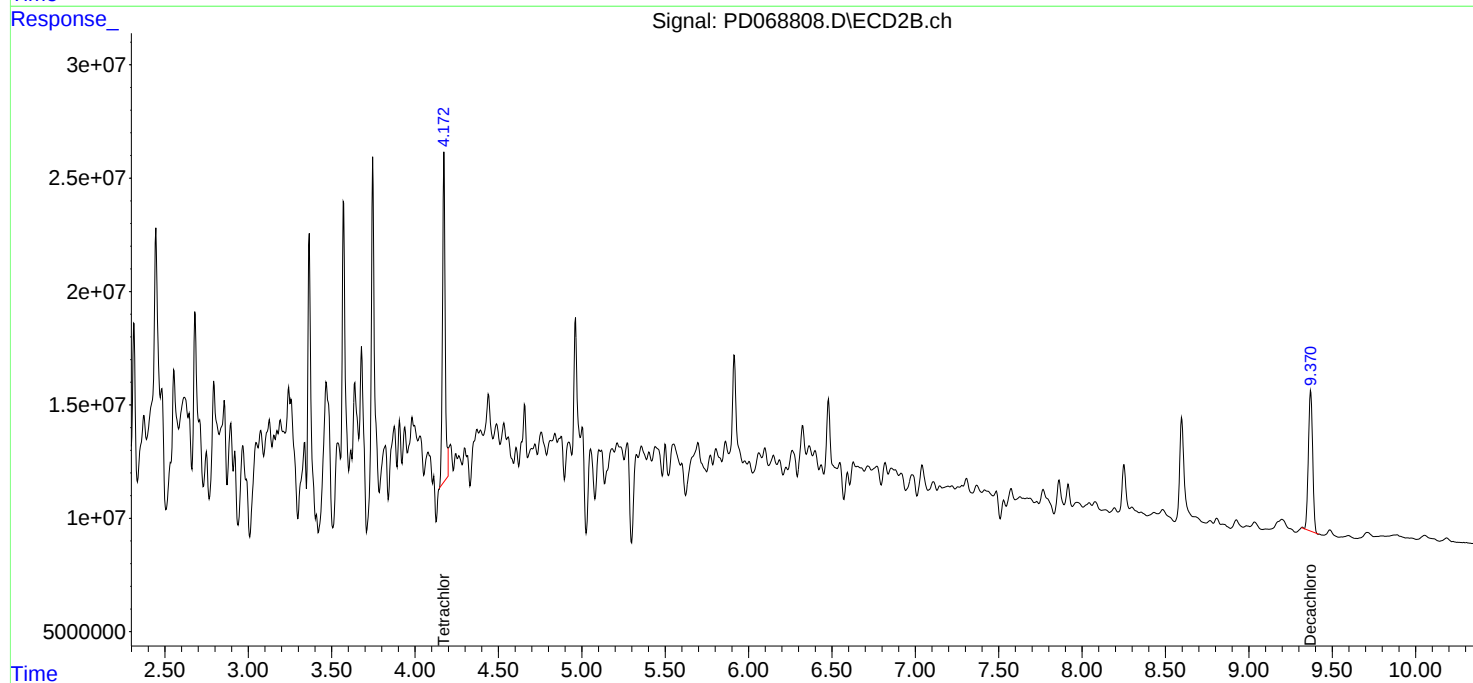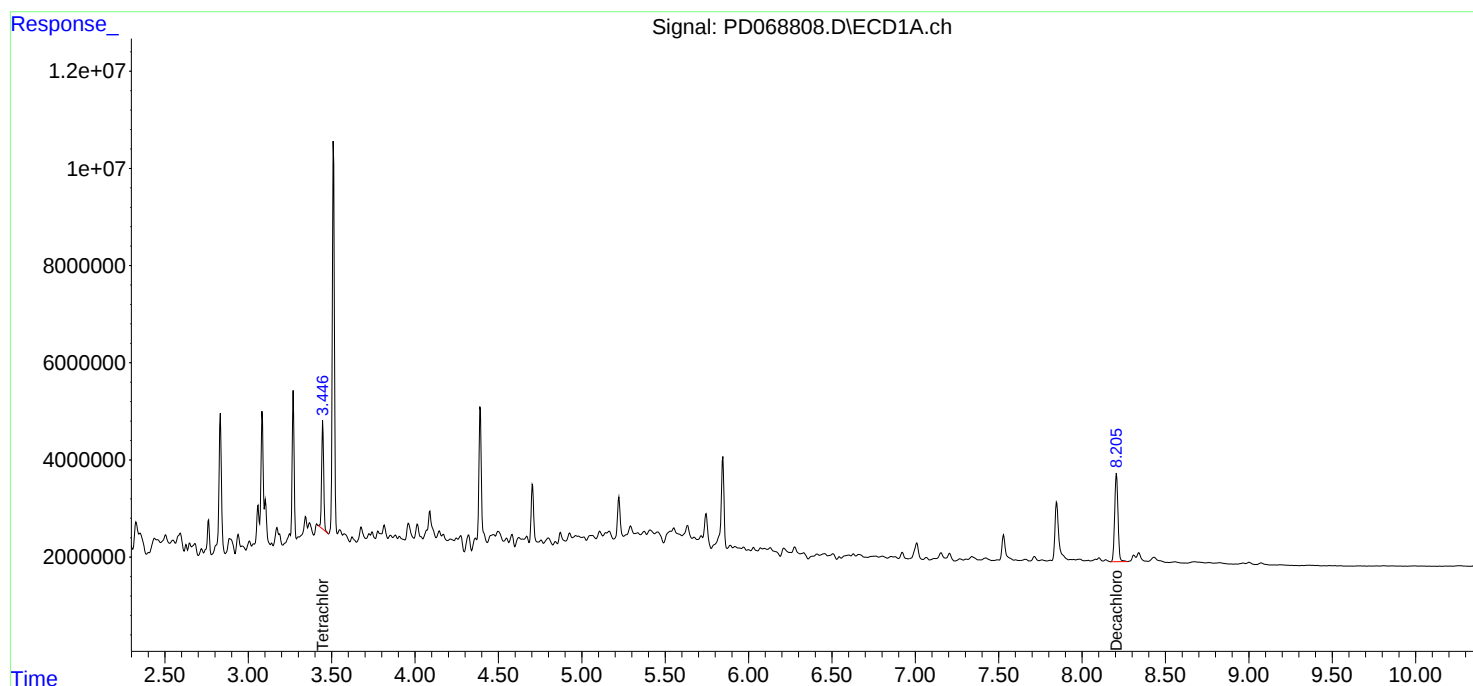

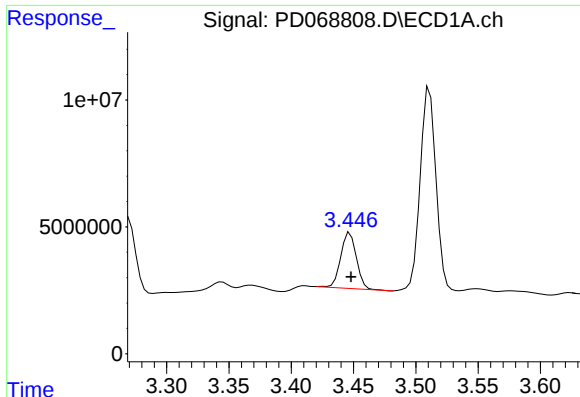


#1 Tetrachloro-m-xylene

R.T.: 3.447 min
Delta R.T.: 0.000 min
Response: 19419791
Conc: 15.99 ng/ml

Instrument :
ECD_D
ClientSampleId :
SPLP-LEACHATE-AMENDED-COMP-CS-1


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/29/2022
Supervised By :mohammad ahmed 03/29/2022

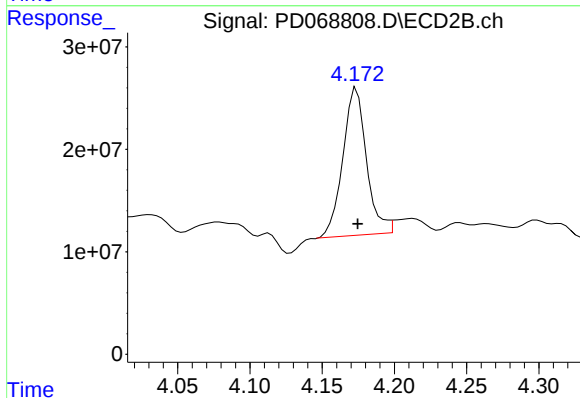


#1 Tetrachloro-m-xylene

R.T.: 4.172 min
Delta R.T.: -0.002 min
Response: 162722265
Conc: 17.02 ng/ml m

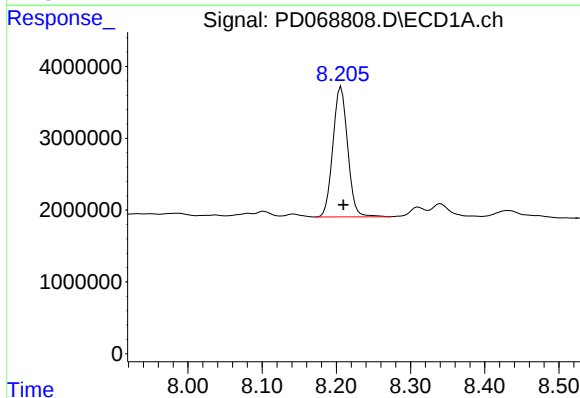

#28 Decachlorobiphenyl

R.T.: 8.206 min
Delta R.T.: -0.003 min
Response: 25172525
Conc: 19.92 ng/ml

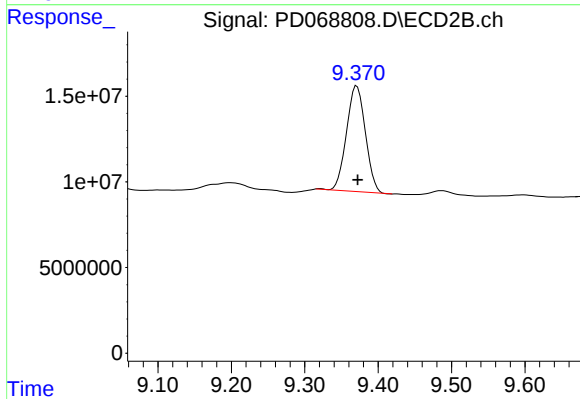

#28 Decachlorobiphenyl

R.T.: 9.371 min
Delta R.T.: -0.001 min
Response: 110406212
Conc: 19.48 ng/ml