

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032823\
 Data File : PD074531.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Mar 2023 00:11
 Operator : AR\AJ
 Sample : PB151725BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 04:08:53 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 14 03:05:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.550	2.771	49436902	24817659	19.899	19.726
27)	SA Decachlor...	9.093	7.922	109.7E6	45900792	40.092	38.334
Target Compounds							
2)	A alpha-BHC	3.964f	0.000	197670	0	<MDL	N.D. #
4)	MA Heptachlor	4.948	0.000	227819	0	<MDL	N.D. #
6)	B beta-BHC	4.560	3.862f	127398	283585	<MDL	0.350 #
7)	B delta-BHC	4.776	0.000	2189120	0	0.602	N.D. #
8)	B Heptachlo...	5.693	0.000	1564317	0	0.476	N.D. #
9)	A Endosulfan I	0.000	5.161f	0	281101	N.D.	0.200
12)	B 4,4'-DDE	6.274f	0.000	97557	0	<MDL	N.D. #
14)	MA Endrin	6.584	5.657	736421	99646	0.279	<MDL #
15)	B Endosulfa...	6.785	5.941	512929	231097	0.186	0.172
16)	A 4,4'-DDD	6.785f	0.000	512929	0	0.217	N.D. #
20)	A Methoxychlor	7.462f	0.000	1422837	0	1.036	N.D. #
21)	B Endrin ke...	7.695	0.000	39673	0	<MDL	N.D. #
22)	Toxaphene-1	6.274	0.000	97557	0	4.157	N.D. #
23)	Toxaphene-2	6.495	5.657f	237839	99646	8.020	10.610 #
24)	Toxaphene-3	6.629	5.941	131287	231097	6.239	21.770 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032823\
Data File : PD074531.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Mar 2023 00:11
Operator : AR\AJ
Sample : PB151725BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 04:08:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 14 03:05:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

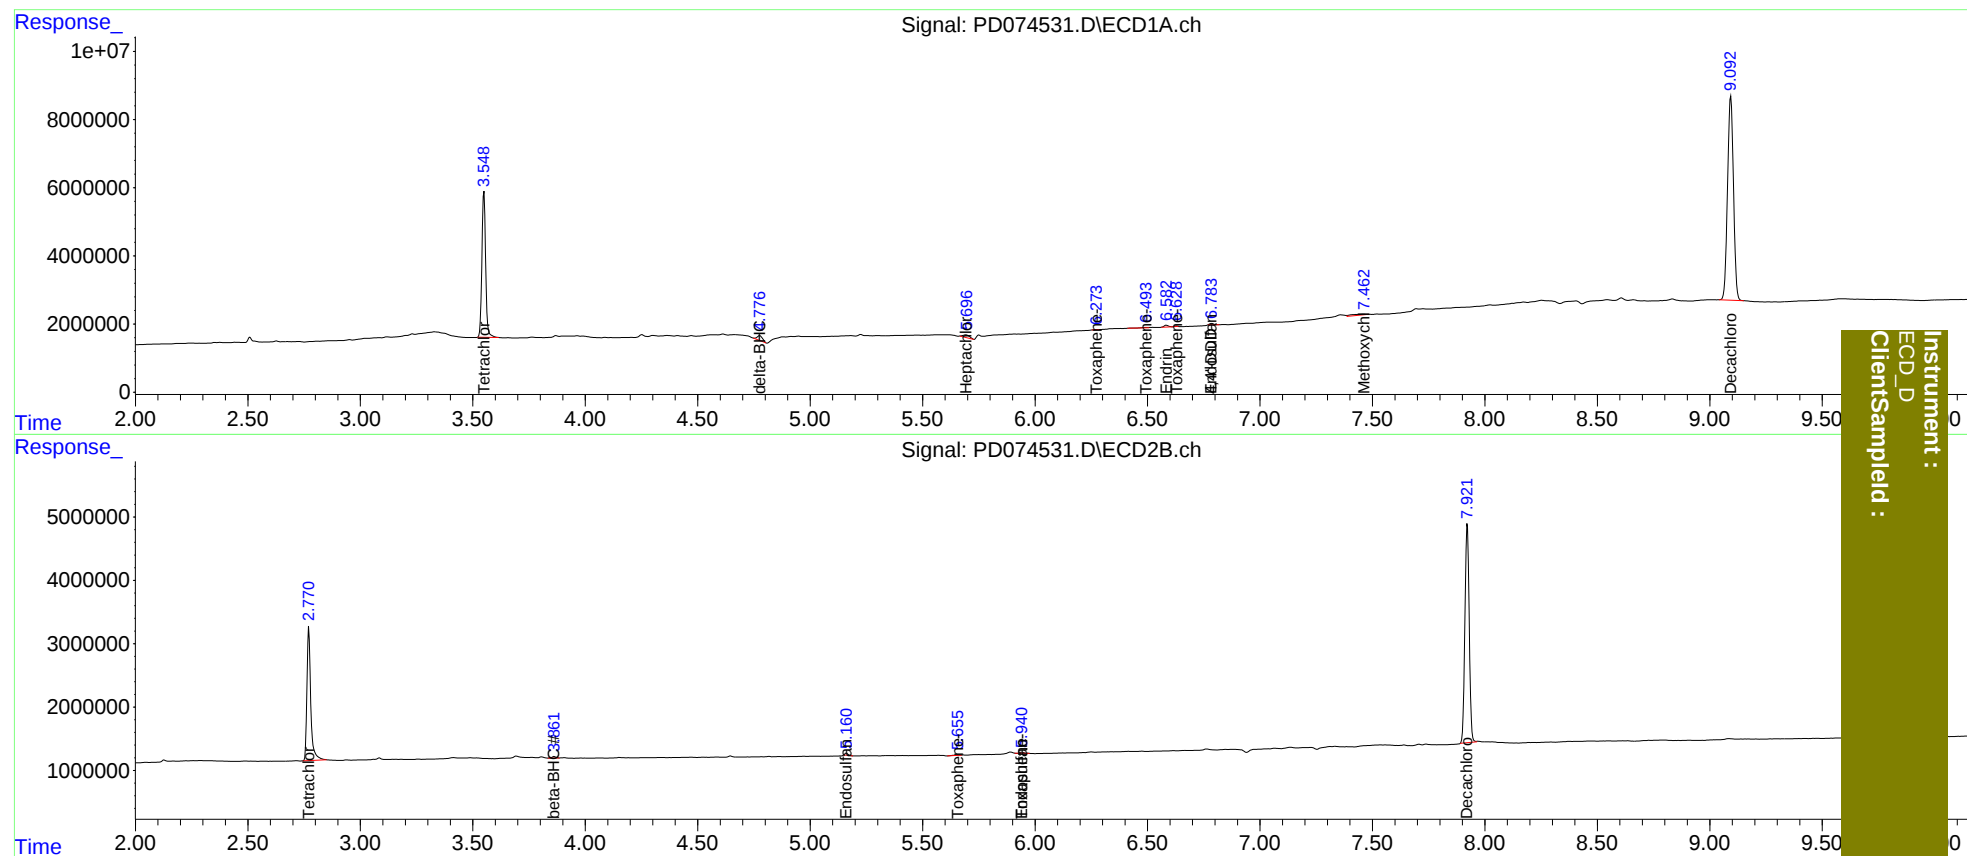


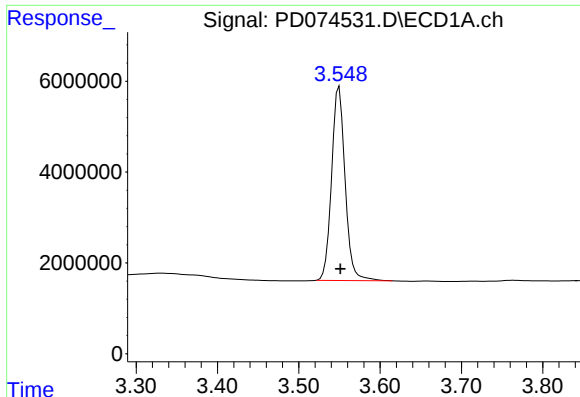

#1 Tetrachloro-m-xylene


R.T.: 3.550 min
Delta R.T.: -0.001 min
Response: 49436902
Conc: 19.90 ng/ml

Instrument :
ECD_D
ClientSampleId :

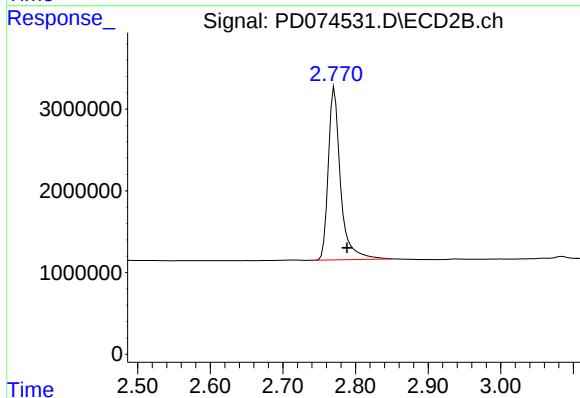


#1 Tetrachloro-m-xylene

R.T.: 2.771 min
Delta R.T.: -0.018 min
Response: 24817659
Conc: 19.73 ng/ml

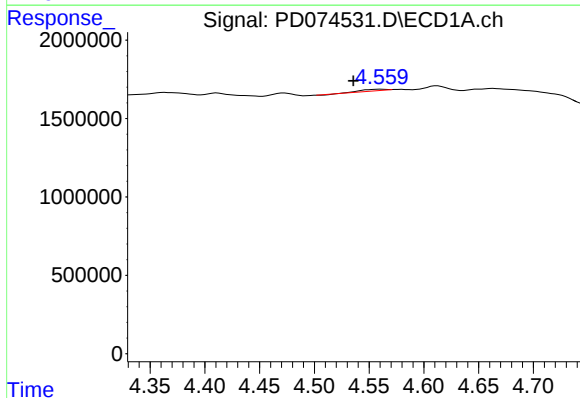


#6 beta-BHC

R.T.: 4.560 min
Delta R.T.: 0.025 min
Response: 127398
Conc: N.D.

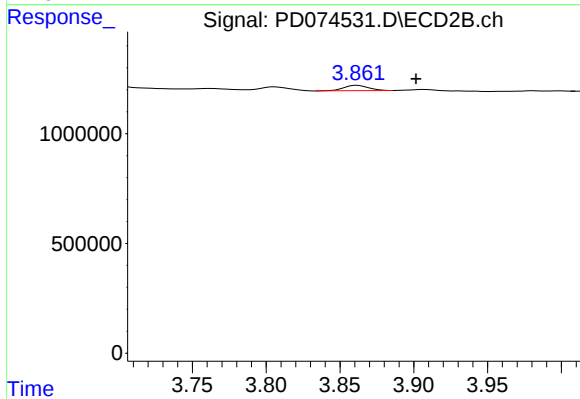

#6 beta-BHC


R.T.: 3.862 min
Delta R.T.: -0.039 min
Response: 283585
Conc: 0.35 ng/ml

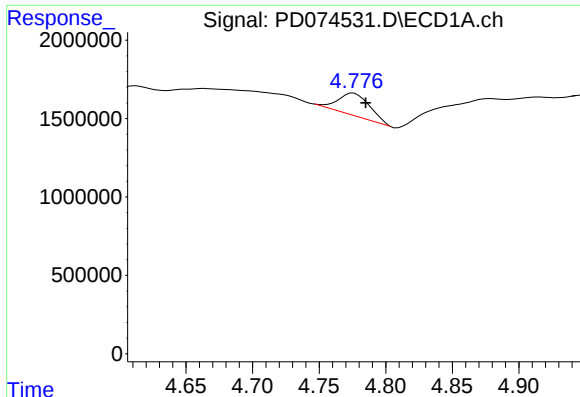

#7 delta-BHC


R.T.: 4.776 min
Delta R.T.: -0.009 min
Response: 2189120
Conc: 0.60 ng/ml

Instrument :
ECD_D
ClientSampleId :

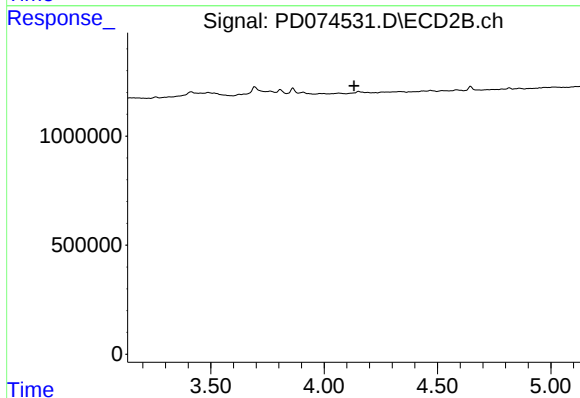


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.133 min
Response: 0
Conc: N.D.

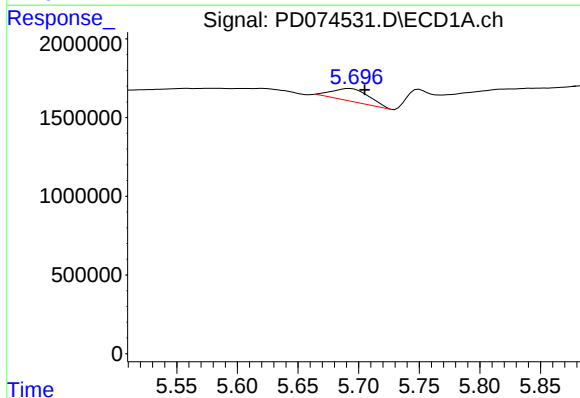


#8 Heptachlor epoxide

R.T.: 5.693 min
Delta R.T.: -0.012 min
Response: 1564317
Conc: 0.48 ng/ml

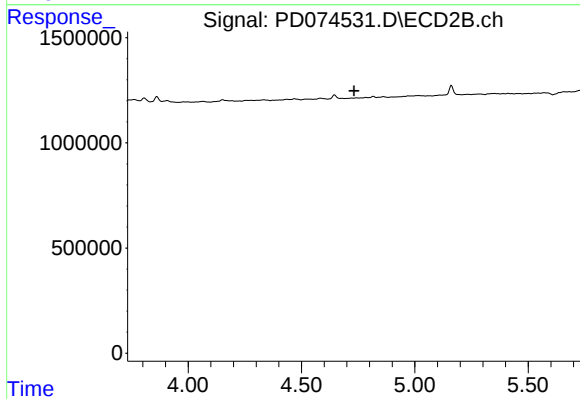

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.732 min
Response: 0
Conc: N.D.

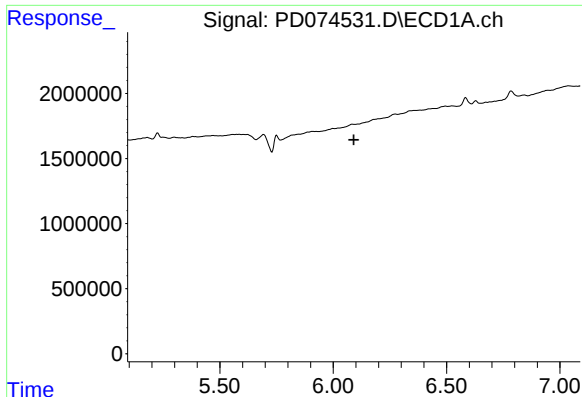

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.091 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

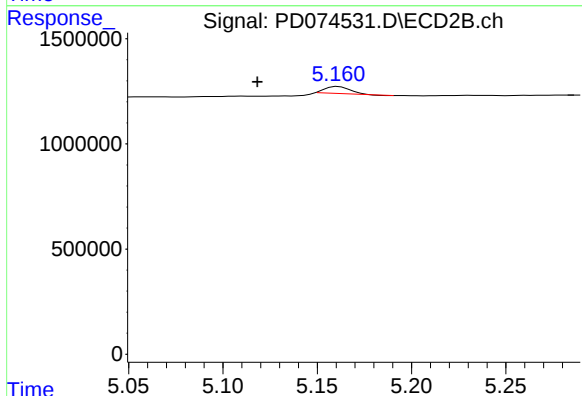


#9 Endosulfan I

R.T.: 5.161 min
Delta R.T.: 0.043 min
Response: 281101
Conc: 0.20 ng/ml

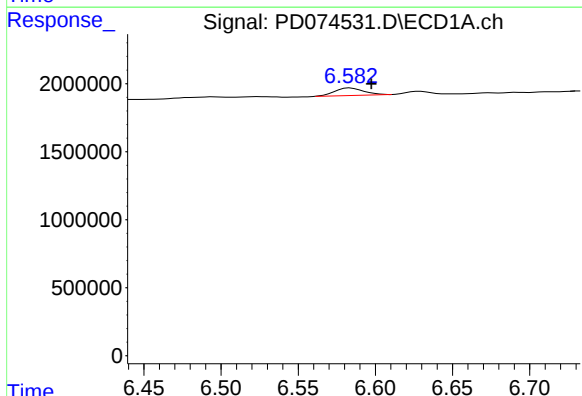


#14 Endrin

R.T.: 6.584 min
Delta R.T.: -0.014 min
Response: 736421
Conc: 0.28 ng/ml

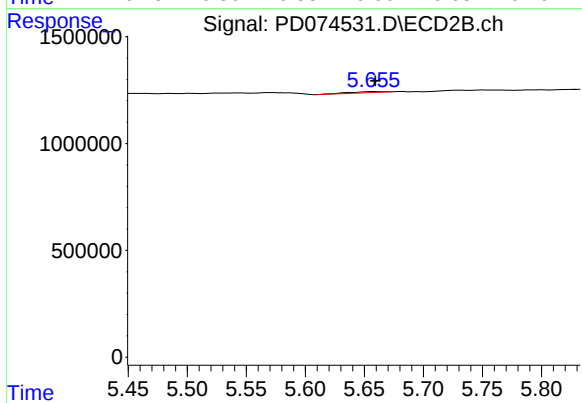

#14 Endrin


R.T.: 5.657 min
Delta R.T.: -0.003 min
Response: 99646
Conc: N.D.

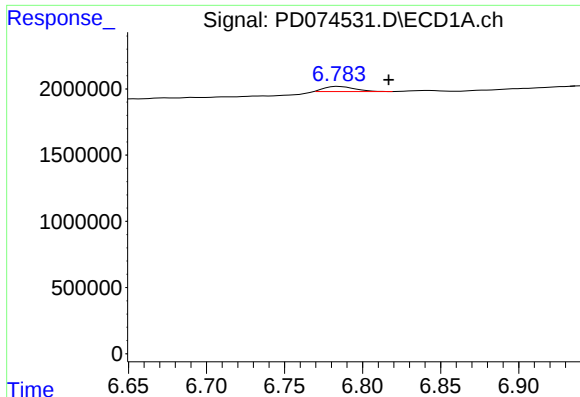

#15 Endosulfan II


R.T.: 6.785 min
Delta R.T.: -0.032 min
Response: 512929
Conc: 0.19 ng/ml

Instrument :
ECD_D
ClientSampleId :

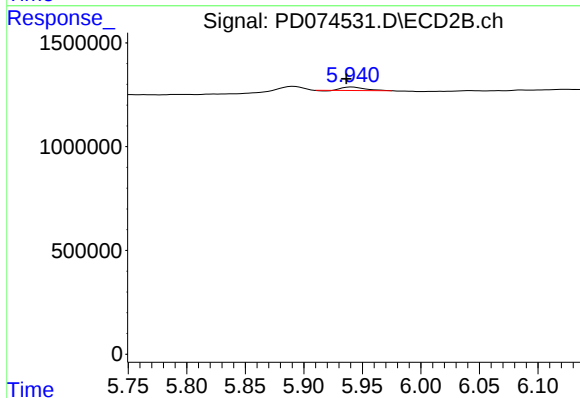


#15 Endosulfan II

R.T.: 5.941 min
Delta R.T.: 0.005 min
Response: 231097
Conc: 0.17 ng/ml

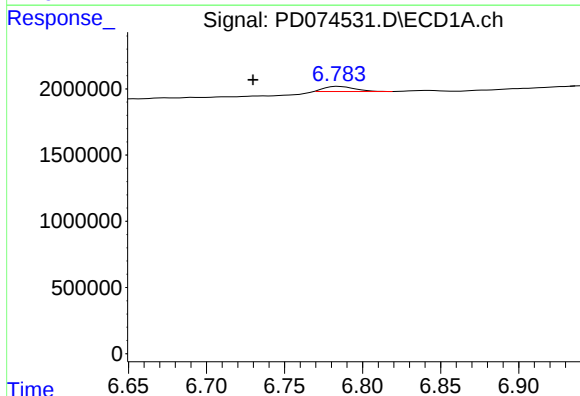


#16 4,4'-DDD

R.T.: 6.785 min
Delta R.T.: 0.055 min
Response: 512929
Conc: 0.22 ng/ml

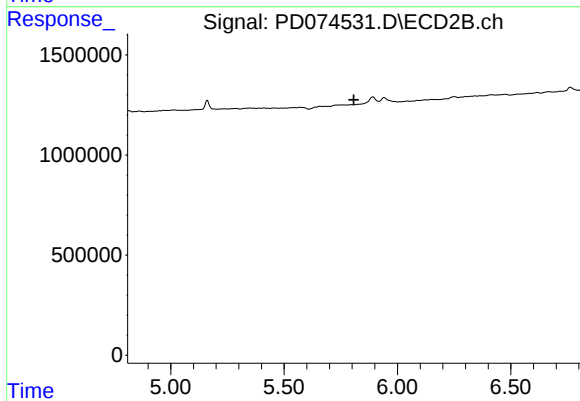

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 5.808 min
Response: 0
Conc: N.D.

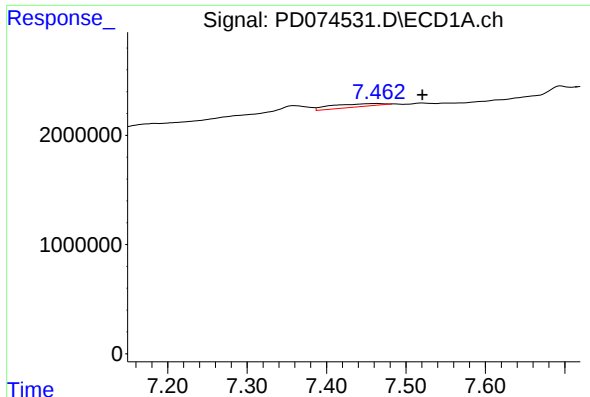

#20 Methoxychlor


R.T.: 7.462 min
Delta R.T.: -0.058 min
Response: 1422837
Conc: 1.04 ng/ml

Instrument :
ECD_D
ClientSampleId :

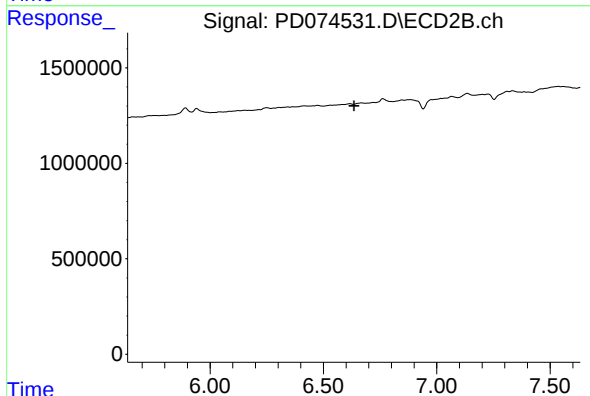


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.636 min
Response: 0
Conc: N.D.

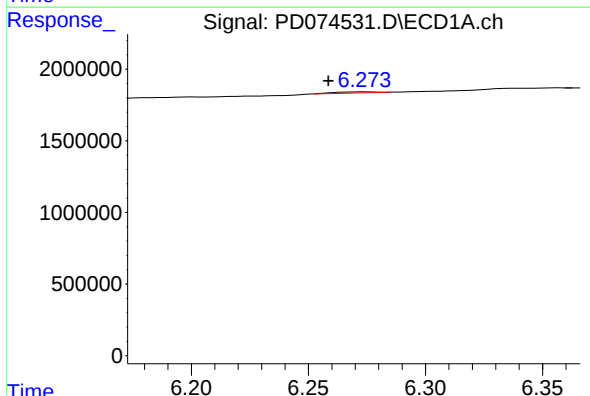


#22 Toxaphene-1

R.T.: 6.274 min
Delta R.T.: 0.016 min
Response: 97557
Conc: 4.16 ng/ml

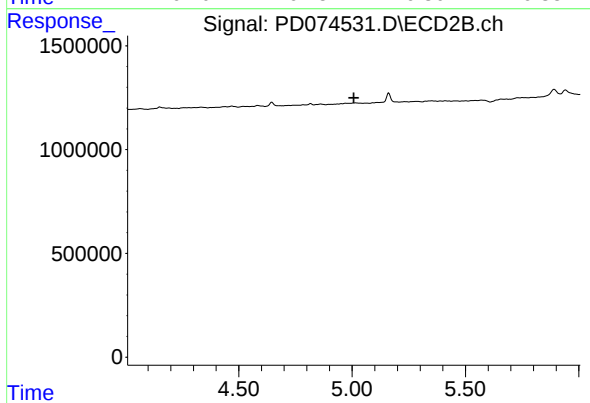

#22 Toxaphene-1


R.T.: 0.000 min
Exp R.T. : 5.007 min
Response: 0
Conc: N.D.

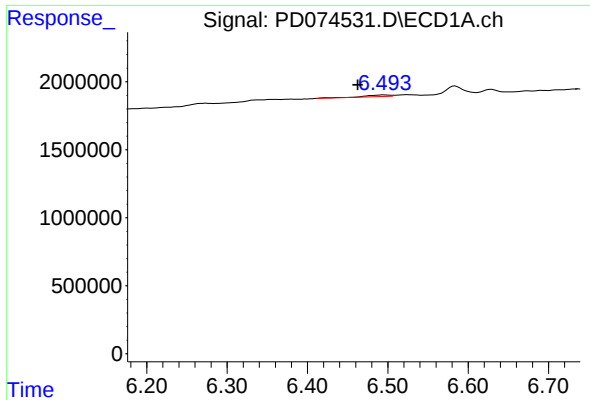

#23 Toxaphene-2


R.T.: 6.495 min
Delta R.T.: 0.032 min
Response: 237839
Conc: 8.02 ng/ml

Instrument :
ECD_D
ClientSampleId :

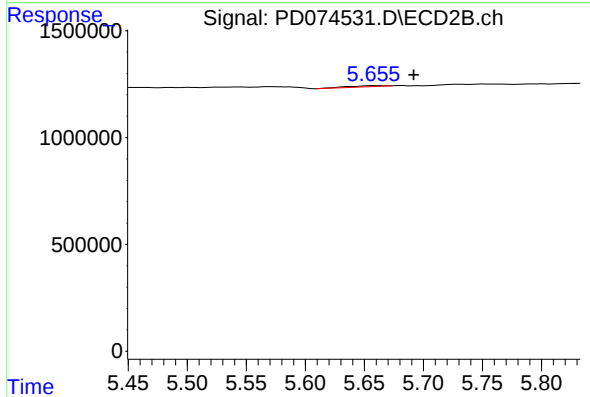


#23 Toxaphene-2

R.T.: 5.657 min
Delta R.T.: -0.035 min
Response: 99646
Conc: 10.61 ng/ml

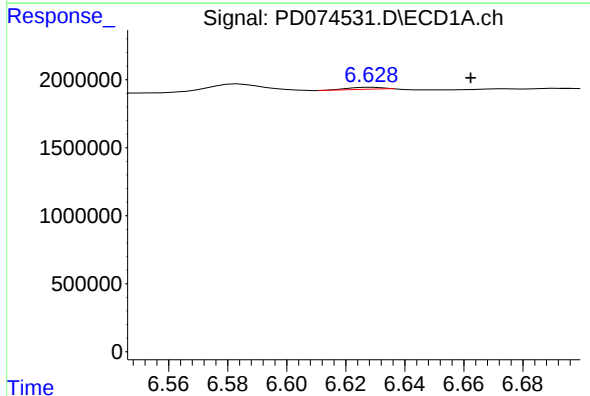


#24 Toxaphene-3

R.T.: 6.629 min
Delta R.T.: -0.033 min
Response: 131287
Conc: 6.24 ng/ml

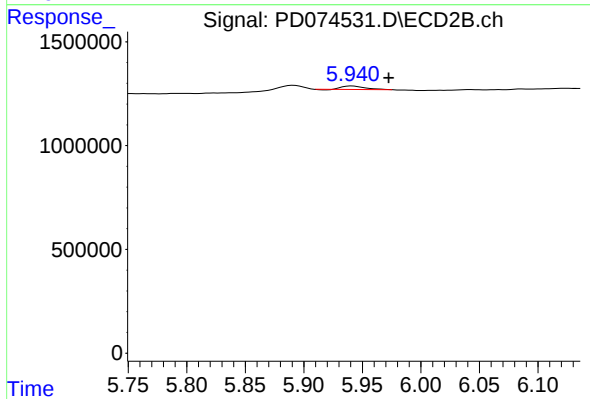

#24 Toxaphene-3


R.T.: 5.941 min
Delta R.T.: -0.032 min
Response: 231097
Conc: 21.77 ng/ml

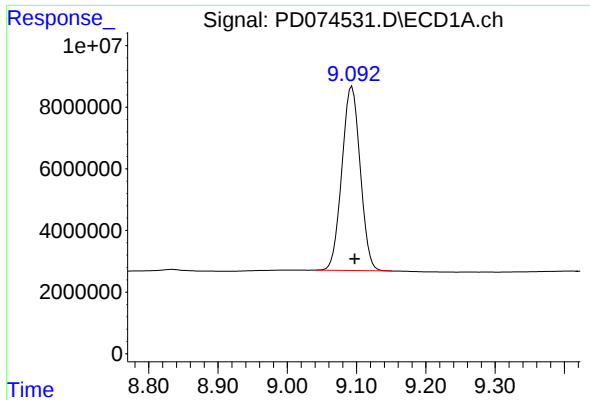

#27 Decachlorobiphenyl

R.T.: 9.093 min
Delta R.T.: -0.004 min
Response: 109729464
Conc: 40.09 ng/ml

Instrument :
ECD_D
ClientSampleId :

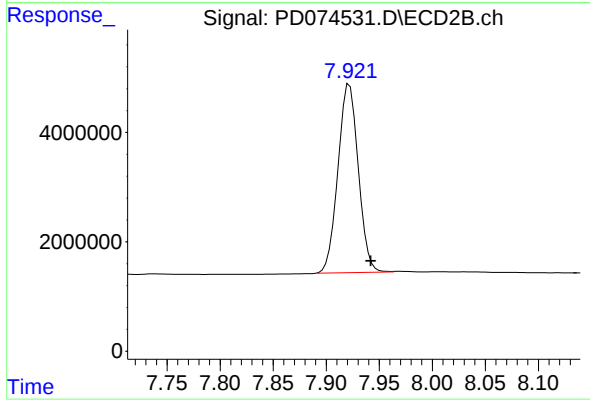

#27 Decachlorobiphenyl

R.T.: 7.922 min
Delta R.T.: -0.020 min
Response: 45900792
Conc: 38.33 ng/ml