

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032823\
 Data File : PD074517.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Mar 2023 21:02
 Operator : AR\AJ
 Sample : PB151708BS
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS708

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 04:06:53 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 14 03:05:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.549	2.771	45434867	23286163	18.288	18.509
2)	SA Decachlor...	9.092	7.922	100.7E6	42696257	36.795	35.658
Target Compounds							
2)	A alpha-BHC	4.005	3.274	15733587	7244824	4.032	4.054
3)	MA gamma-BHC...	4.339	3.604	14673424	6821660	3.975	3.994
4)	MA Heptachlor	4.931	3.946	16021232	7208904	4.232	4.348
5)	MB Aldrin	5.274	4.226	16065128	7484652	4.396	4.372
6)	B beta-BHC	4.534	3.900	7827655	3763868	4.630	4.646
7)	B delta-BHC	4.782	4.131	14522328	6220667	3.991	3.517
8)	B Heptachlo...	5.701	4.729	15375963	6644668	4.683	4.194
9)	A Endosulfan I	6.088	5.099	13559159	6066782	4.545	4.327
10)	B trans-Chl...	5.957	4.980	13868916	6723720	4.323	4.346
11)	B cis-Chlor...	6.038	5.044	14701200	6886561	4.486	4.353
12)	B 4,4'-DDE	6.210	5.233	25383629	12080634	8.474	8.317
13)	MA Dieldrin	6.364	5.364	28297477	13439499	8.920	8.669
14)	MA Endrin	6.594	5.640	23585962	12318162	8.950	9.157
15)	B Endosulfa...	6.813	5.934	25003938	11243686	9.059	8.363
16)	A 4,4'-DDD	6.727	5.788	21067183	10486174	8.914	8.906
17)	MA 4,4'-DDT	7.042	6.040	21486118	10013568	8.562	7.993
18)	B Endrin al...	6.944	6.113	17749139	8855014	7.880	8.055
19)	B Endosulfa...	7.178	6.336	22806679	10950181	8.756	8.699
20)	A Methoxychlor	7.518	6.616	65300258	30710132	47.565	49.929
21)	B Endrin ke...	7.665	6.843	26439350	13616683	8.917	8.949

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032823\
Data File : PD074517.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Mar 2023 21:02
Operator : AR\AJ
Sample : PB151708BS
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 04:06:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 14 03:05:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

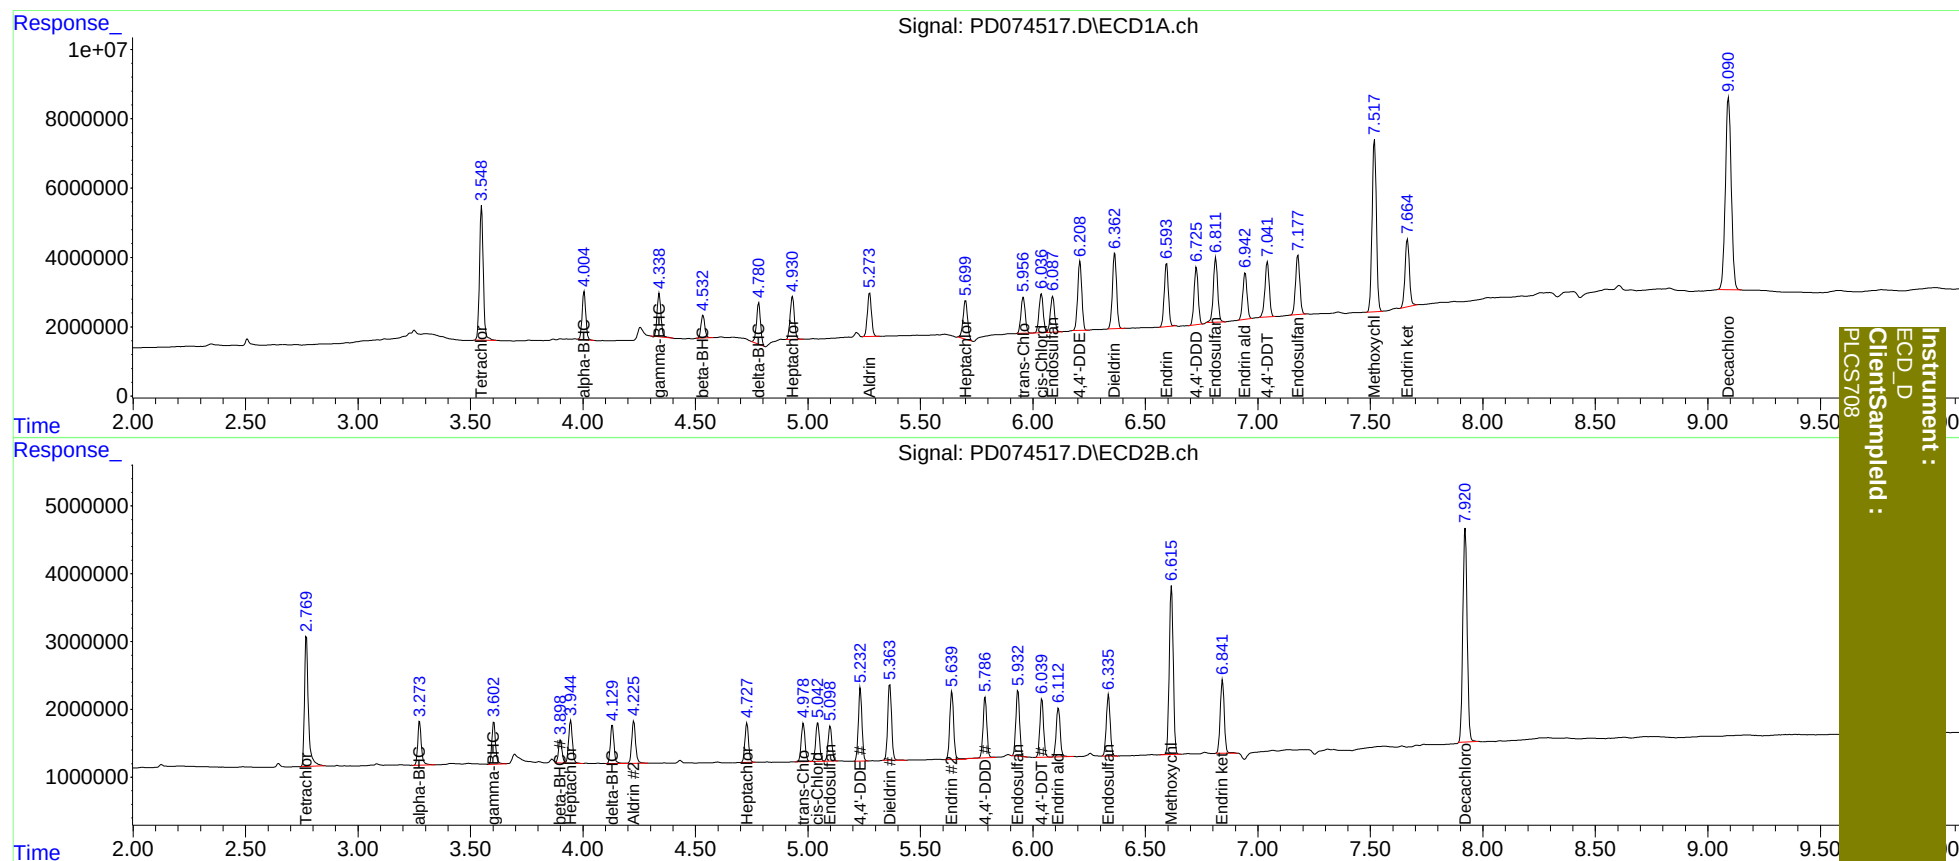

Instrument :
ECD_D
Client Sampled :
PLC5708