

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032823\
 Data File : PD074511.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Mar 2023 16:51
 Operator : AR\AJ
 Sample : 02006-04MS
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CB963MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 03/29/2023
 Supervised By :Ankita Jodhani 03/29/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 28 21:10:14 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 14 03:05:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.550	2.772	18035561	9573363	7.260	7.609
2)	SA Decachlor...	9.091	7.921	51045916	16268028	18.651	13.586 #
Target Compounds							
2)	A alpha-BHC	4.007	3.275	133.4E6	60863552	34.180	34.057
3)	MA gamma-BHC...	4.339	3.605	124.1E6	58260745	33.611m	34.110
4)	MA Heptachlor	4.932	3.946	120.6E6	54150999	31.861	32.659
5)	MB Aldrin	5.275	4.227	117.7E6	54301179	32.196	31.715
6)	B beta-BHC	4.534	3.898	38250822	21886486	22.626m	27.015m
7)	B delta-BHC	4.784	4.131	98760528	55984495	27.139	31.652
8)	B Heptachlo...	5.702	4.729	99079643	45803779	30.178	28.913
9)	A Endosulfan I	6.088	5.100	94128736	35128721	31.553m	25.053m
10)	B trans-Chl...	5.957	4.980	114.9E6	53662420	35.815m	34.688
11)	B cis-Chlor...	6.038	5.045	115.4E6	50767239	35.226	32.094
12)	B 4,4'-DDE	6.210	5.234	198.4E6	89427037	66.230	61.566
13)	MA Dieldrin	6.366	5.365	250.1E6	105.1E6	78.838	67.820
14)	MA Endrin	6.596	5.640	186.2E6	83209400	70.664	61.852m
15)	B Endosulfa...	6.814	5.934	191.9E6	78966827	69.526	58.734
16)	A 4,4'-DDD	6.728	5.788	187.7E6	73217506	79.440	62.185
17)	MA 4,4'-DDT	7.044	6.040	189.6E6	75980246	75.558	60.649
18)	B Endrin al...	6.945	6.114	135.7E6	58047753	60.240	52.805
19)	B Endosulfa...	7.180	6.337	167.8E6	67763702	64.439	53.832
20)	A Methoxychlor	7.519	6.616	493.5E6	212.6E6	359.465	345.617
21)	B Endrin ke...	7.666	6.843	183.7E6	78197675	61.955	51.391

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032823\
Data File : PD074511.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Mar 2023 16:51
Operator : AR\AJ
Sample : 02006-04MS
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 28 21:10:14 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 14 03:05:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

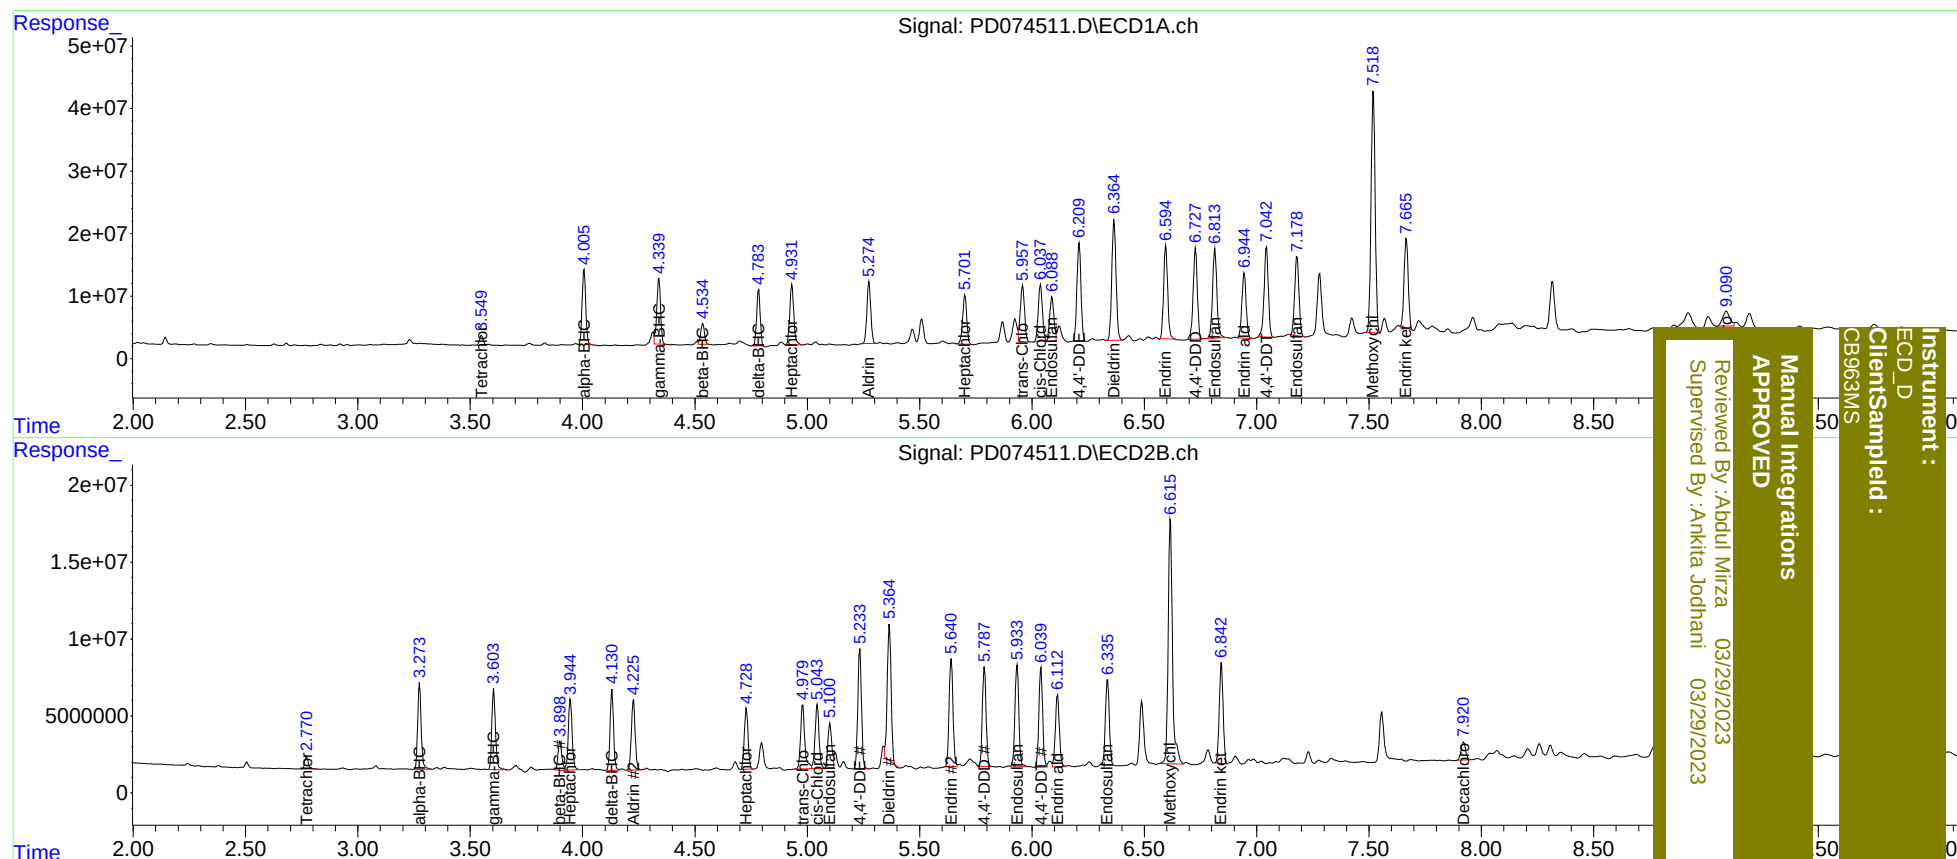

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 03/29/2023
Supervised By: Ankita Jodhani 03/29/2023

Instrument :
ECD_D
Client Sampled :
CB963MS