

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032824\
 Data File : PD082232.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Mar 2024 16:36
 Operator : AR\AJ
 Sample : P1830-07
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 VNJ-206

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 03/29/2024
 Supervised By :Ankita Jodhani 03/29/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 01:33:24 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032224.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 16:01:04 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.565	2.776	32179619	62222347	22.463m	25.318m
28) SA Decachlor...	9.120	7.910	42353697	54115831	22.314	24.860

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032824\
Data File : PD082232.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Mar 2024 16:36
Operator : AR\AJ
Sample : P1830-07
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
VNJ-206


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 03/29/2024
Supervised By : Ankita Jodhani 03/29/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 01:33:24 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032224.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 16:01:04 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

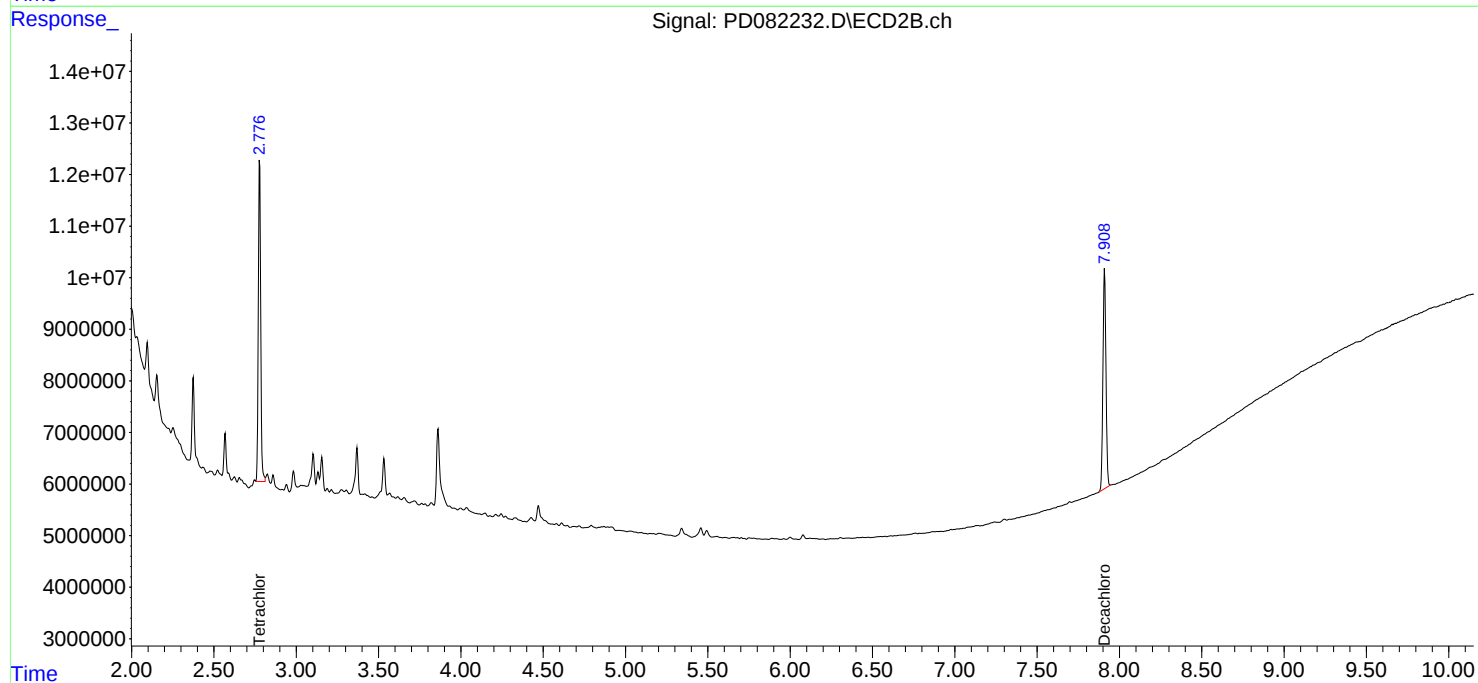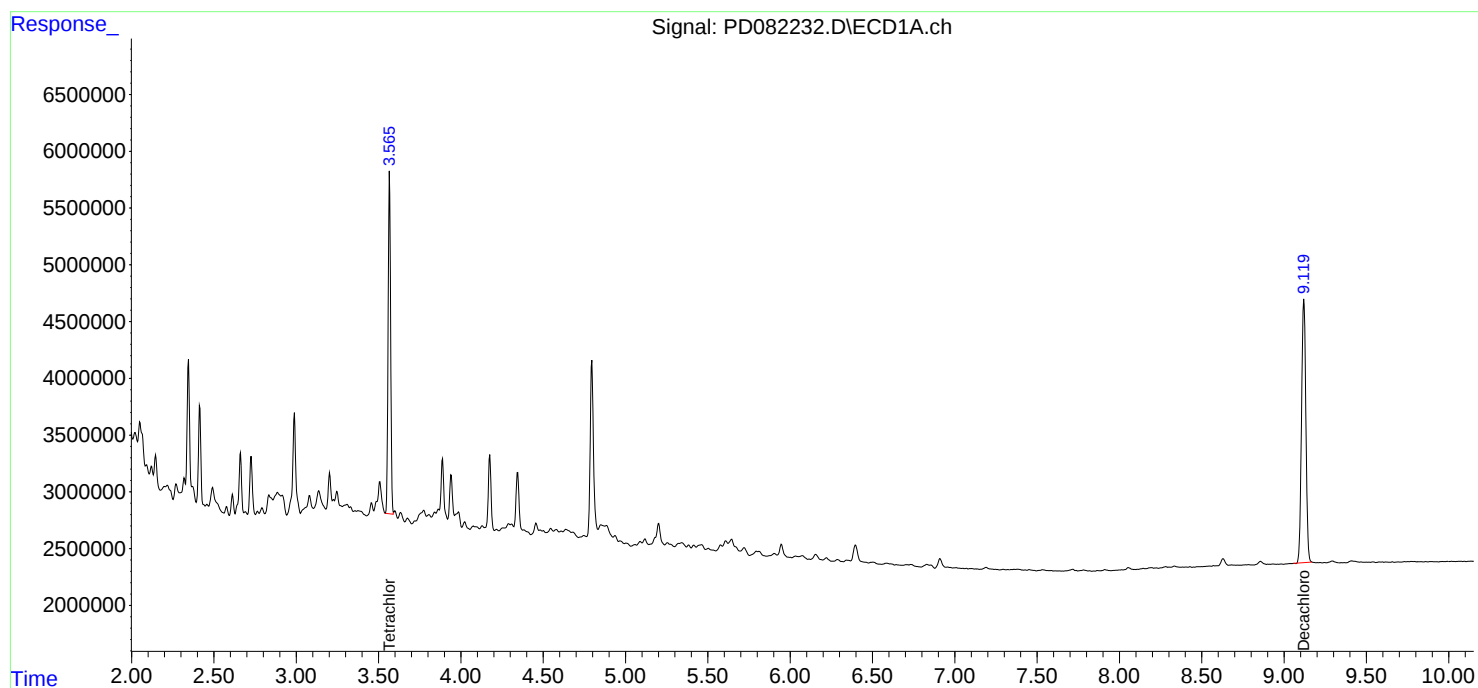

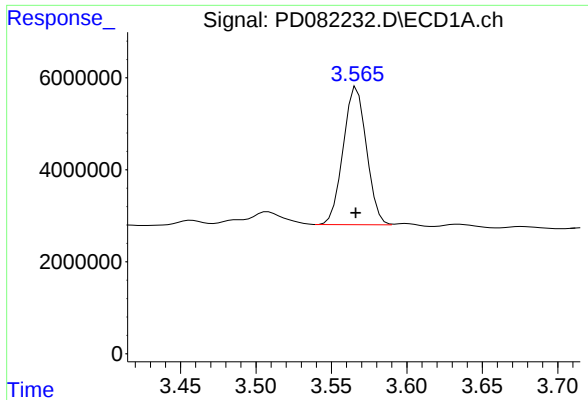


#1 Tetrachloro-m-xylene

R.T.: 3.565 min
Delta R.T.: 0.000 min
Response: 32179619
Conc: 22.46 ng/ml

Instrument :
ECD_D
ClientSampleId :
VNJ-206


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/29/2024
Supervised By :Ankita Jodhani 03/29/2024

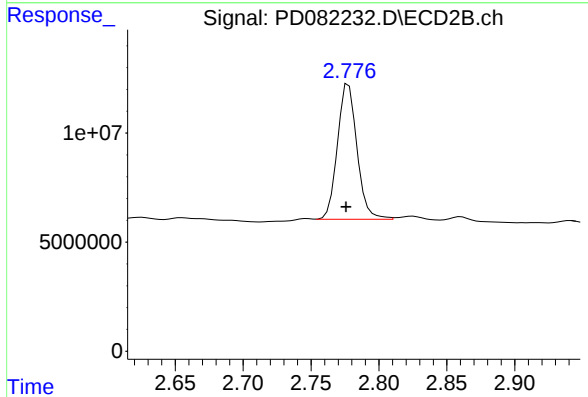


#1 Tetrachloro-m-xylene

R.T.: 2.776 min
Delta R.T.: 0.000 min
Response: 62222347
Conc: 25.32 ng/ml m

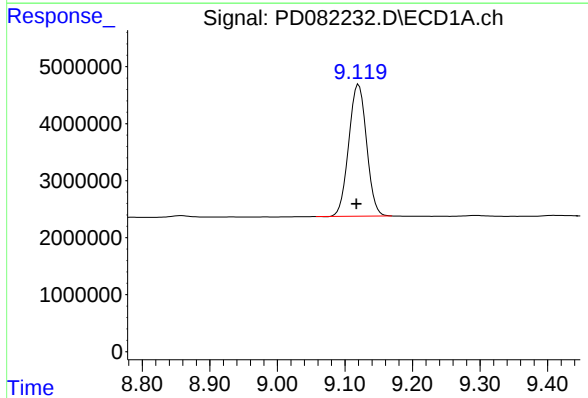

#28 Decachlorobiphenyl

R.T.: 9.120 min
Delta R.T.: 0.003 min
Response: 42353697
Conc: 22.31 ng/ml

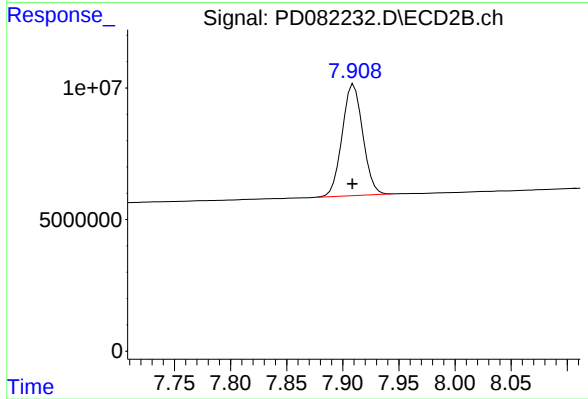

#28 Decachlorobiphenyl

R.T.: 7.910 min
Delta R.T.: 0.001 min
Response: 54115831
Conc: 24.86 ng/ml