

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032919\
 Data File : PD052281.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Mar 2019 9:38
 Operator : AJ\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 30 04:54:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 29 13:06:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
3) MA	gamma-BHC...	3.910	0.000	2380333	0	1.089 N.D. #
8) B	Heptachlo...	0.000	5.916	0	10134418	N.D. 0.314 #
9) A	Endosulfan I	0.000	6.264f	0	13295127	N.D. 0.455 #
11) B	alpha-Chl...	0.000	6.247	0	6982956	N.D. 0.222 #
15) B	Endosulfa...	5.890f	6.970	1063420	13842568	0.620 0.556
18) B	Endrin al...	0.000	7.091	0	20637439	N.D. 1.003 #
22)	Mirex	0.000	8.258	0	6991098	N.D. 0.542 #
26)	Chlordane-4	0.000	6.247	0	6982956	N.D. 1.373 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032919\
Data File : PD052281.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Mar 2019 9:38
Operator : AJ\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 30 04:54:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
Quant Title : GC Extractables
QLast Update : Fri Mar 29 13:06:45 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

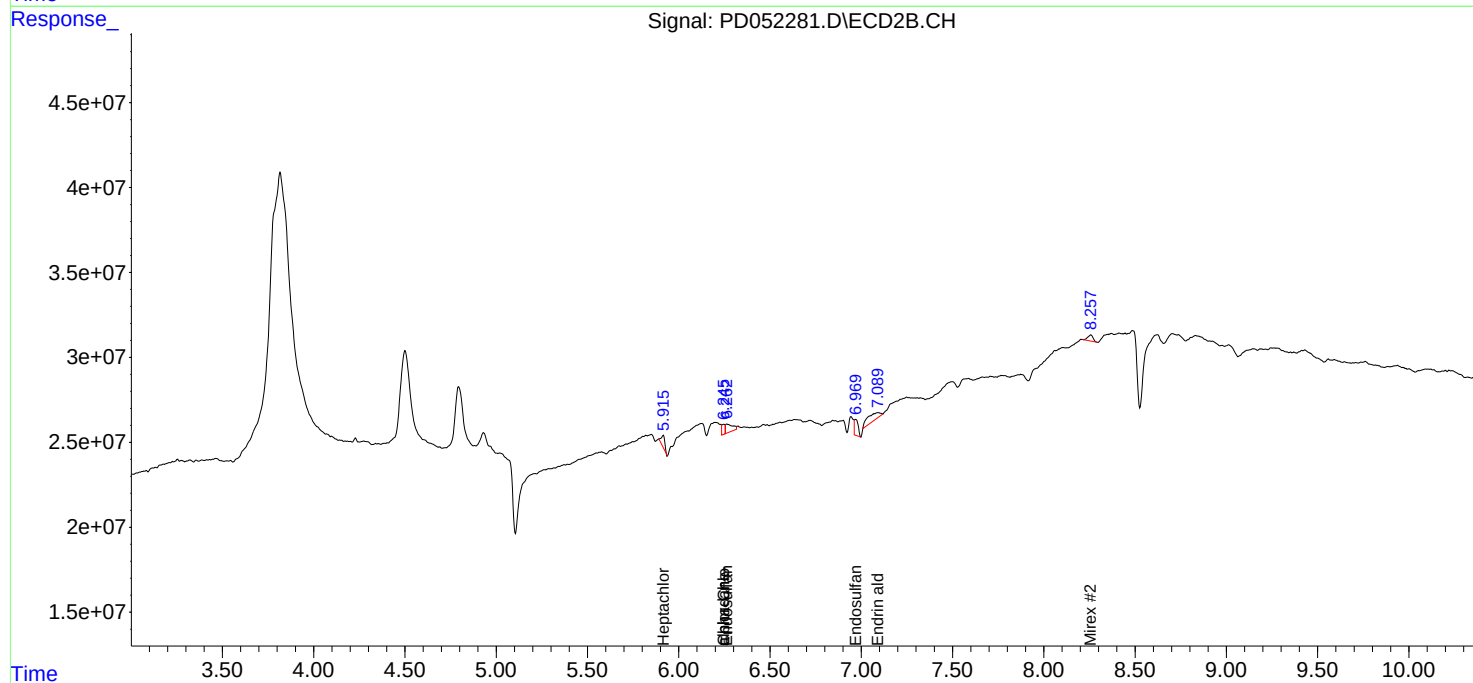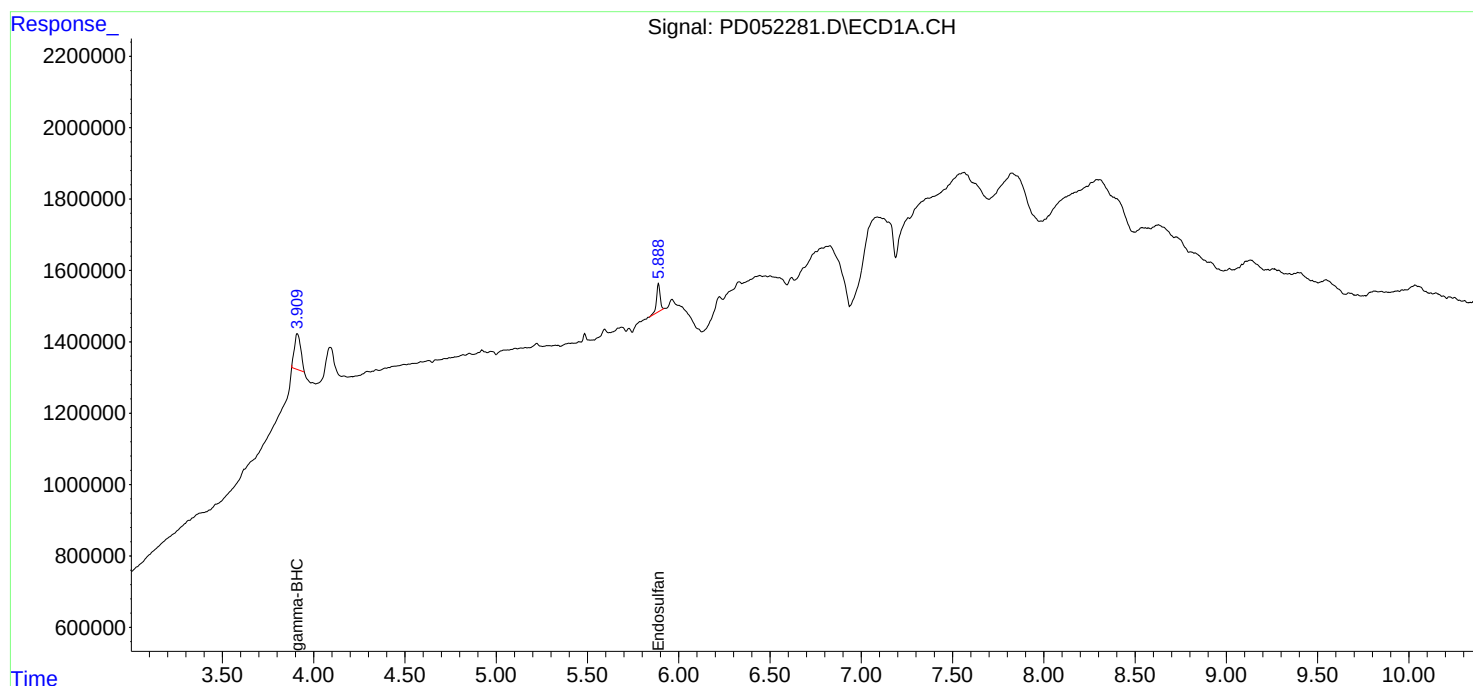


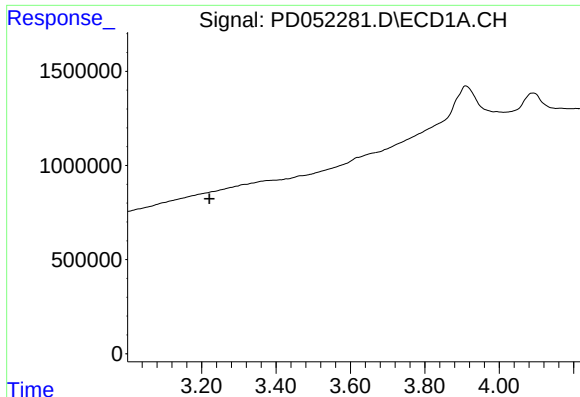

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.221 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

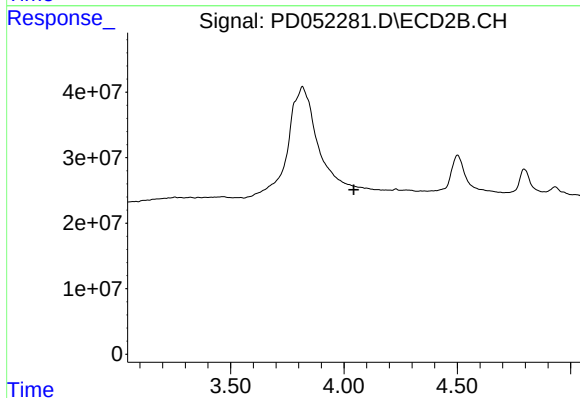


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 4.043 min
Response: 0
Conc: N.D.

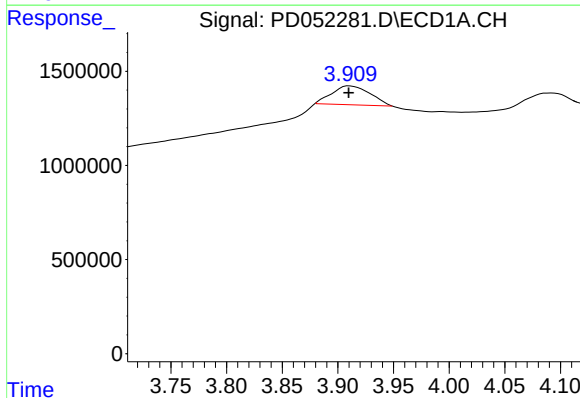


#3 gamma-BHC (Lindane)

R.T.: 3.910 min
Delta R.T.: 0.000 min
Response: 2380333
Conc: 1.09 ng/ml

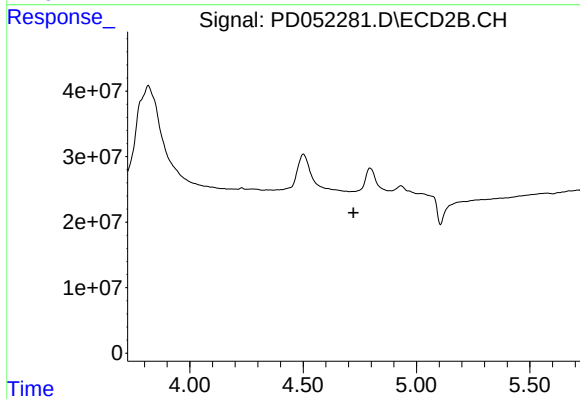

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.723 min
Response: 0
Conc: N.D.

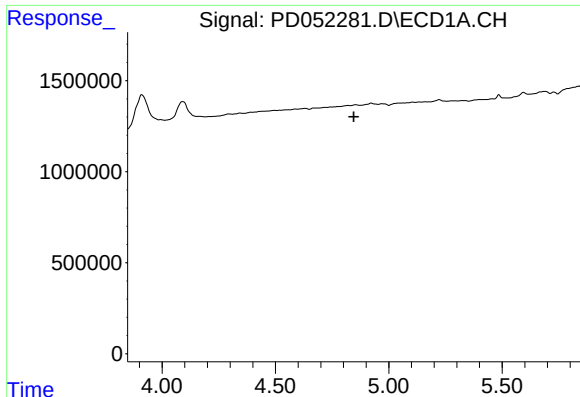

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.846 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

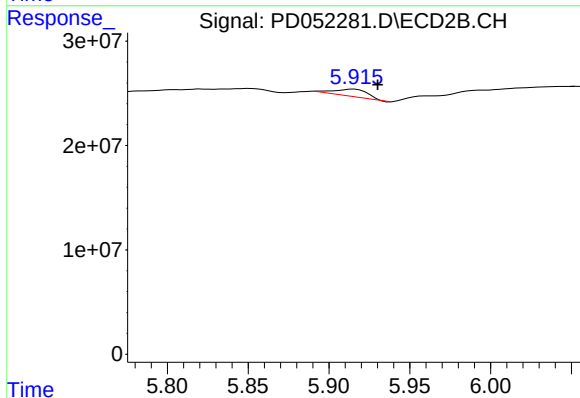


#8 Heptachlor epoxide

R.T.: 5.916 min
Delta R.T.: -0.015 min
Response: 10134418
Conc: 0.31 ng/ml

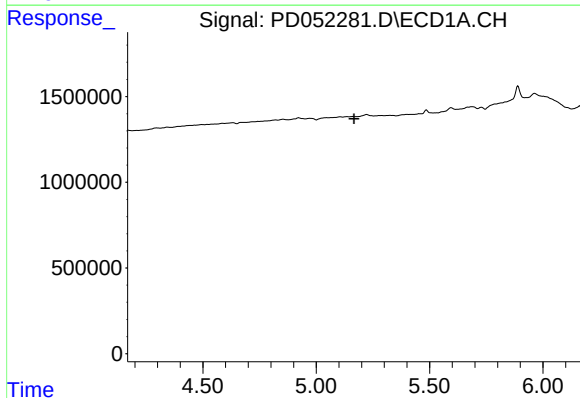


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.167 min
Response: 0
Conc: N.D.

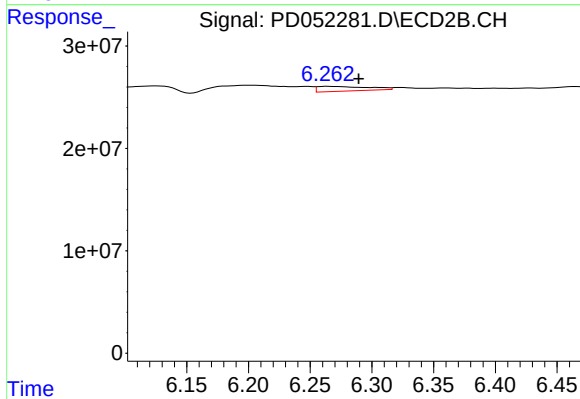

#9 Endosulfan I


R.T.: 6.264 min
Delta R.T.: -0.025 min
Response: 13295127
Conc: 0.46 ng/ml

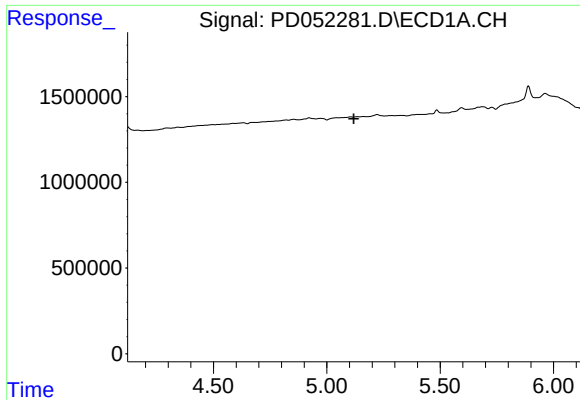

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.119 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

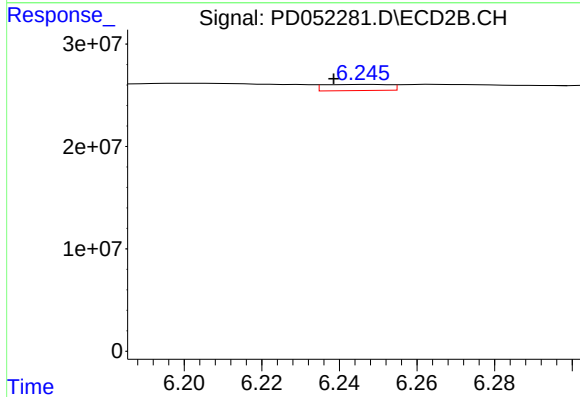


#11 alpha-Chlordane

R.T.: 6.247 min
Delta R.T.: 0.009 min
Response: 6982956
Conc: 0.22 ng/ml

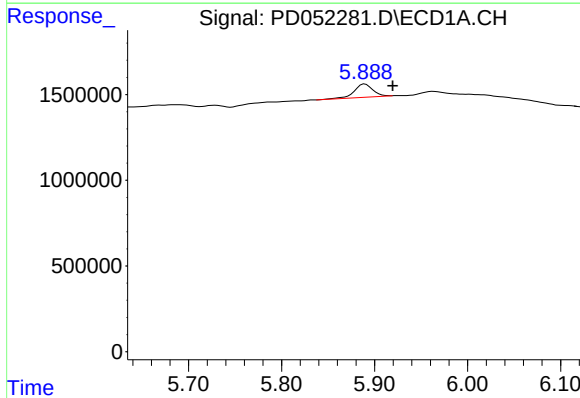


#15 Endosulfan II

R.T.: 5.890 min
Delta R.T.: -0.030 min
Response: 1063420
Conc: 0.62 ng/ml

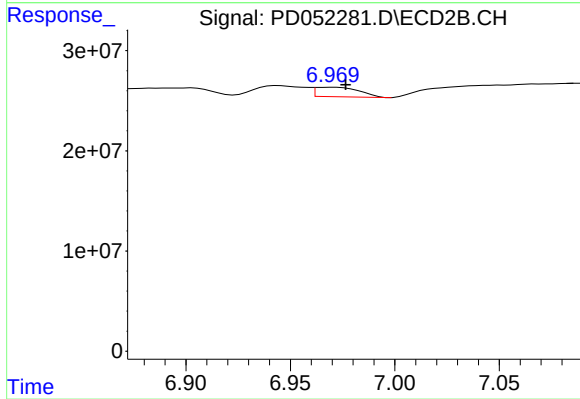

#15 Endosulfan II


R.T.: 6.970 min
Delta R.T.: -0.006 min
Response: 13842568
Conc: 0.56 ng/ml

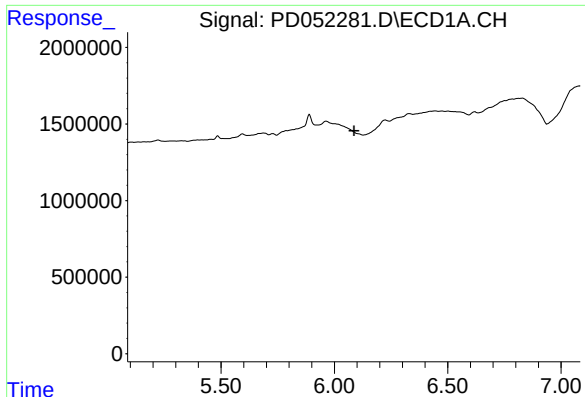

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.087 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

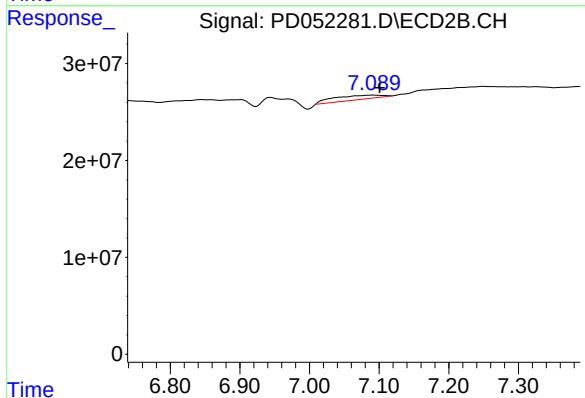


#18 Endrin aldehyde

R.T.: 7.091 min
Delta R.T.: -0.009 min
Response: 20637439
Conc: 1.00 ng/ml

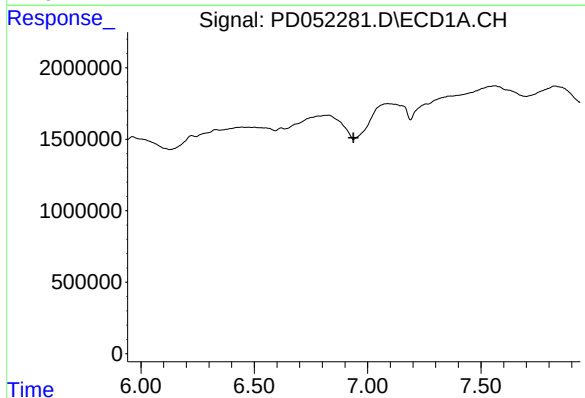


#22 Mirex

R.T.: 0.000 min
Exp R.T.: 6.938 min
Response: 0
Conc: N.D.

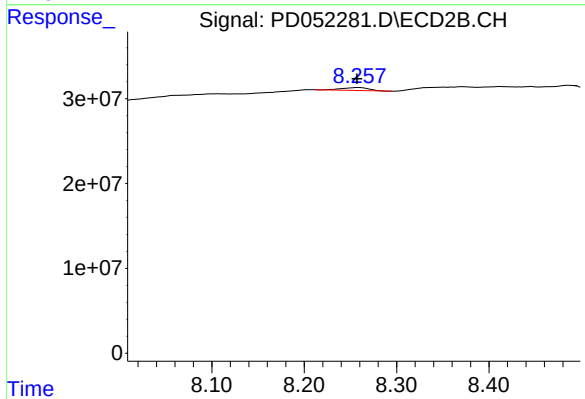

#22 Mirex


R.T.: 8.258 min
Delta R.T.: 0.001 min
Response: 6991098
Conc: 0.54 ng/ml

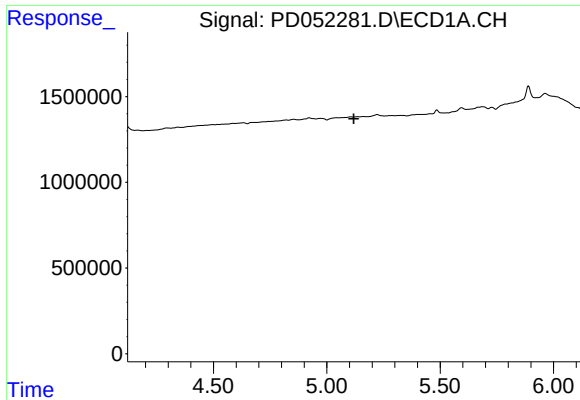

#26 Chlorodane-4


R.T.: 0.000 min
Exp R.T.: 5.118 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

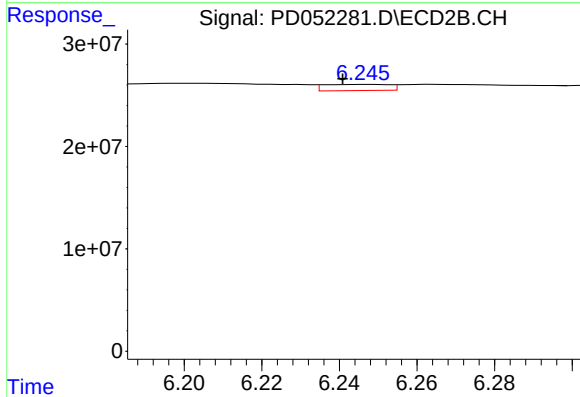


#26 Chlorodane-4

R.T.: 6.247 min
Delta R.T.: 0.006 min
Response: 6982956
Conc: 1.37 ng/ml

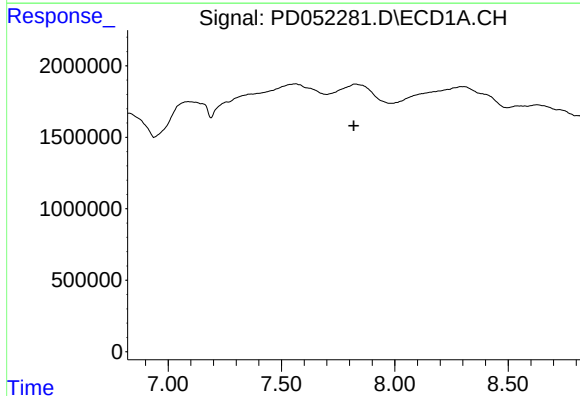

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 7.819 min
Response: 0
Conc: N.D.

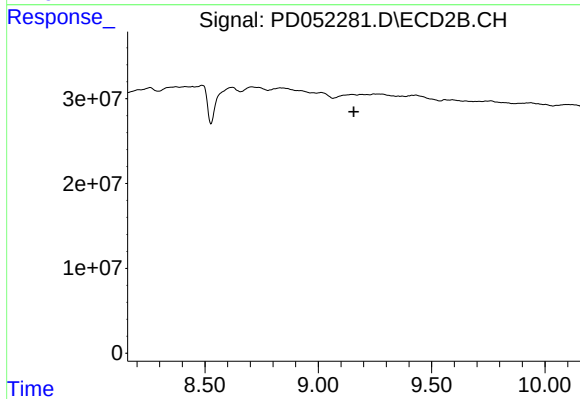

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 9.156 min
Response: 0
Conc: N.D.