

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032919\
 Data File : PD052290.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Mar 2019 11:44
 Operator : AJ\SJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 13:02:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 29 13:01:48 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.221	4.043	152.3E6	2736.9E6	103.581	95.484
28)	SA Decachlor...	7.818	9.156	132.3E6	1441.5E6	96.969	92.458
Target Compounds							
23)	Chlordane-1	4.043	5.045	65554293	1414.0E6	1031.917	949.283
24)	Chlordane-2	4.522	5.516	71907163	1244.5E6	975.555	923.214
25)	Chlordane-3	5.063	6.165	236.6E6	4080.5E6	1059.516	956.148
26)	Chlordane-4	5.118	6.240	222.3E6	4651.6E6	1038.578	950.357
27)	Chlordane-5	5.923	7.049	68965502	891.0E6	1019.955	952.226



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032919\
Data File : PD052290.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Mar 2019 11:44
Operator : AJ\SJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 13:02:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
Quant Title : GC Extractables
QLast Update : Fri Mar 29 13:01:48 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

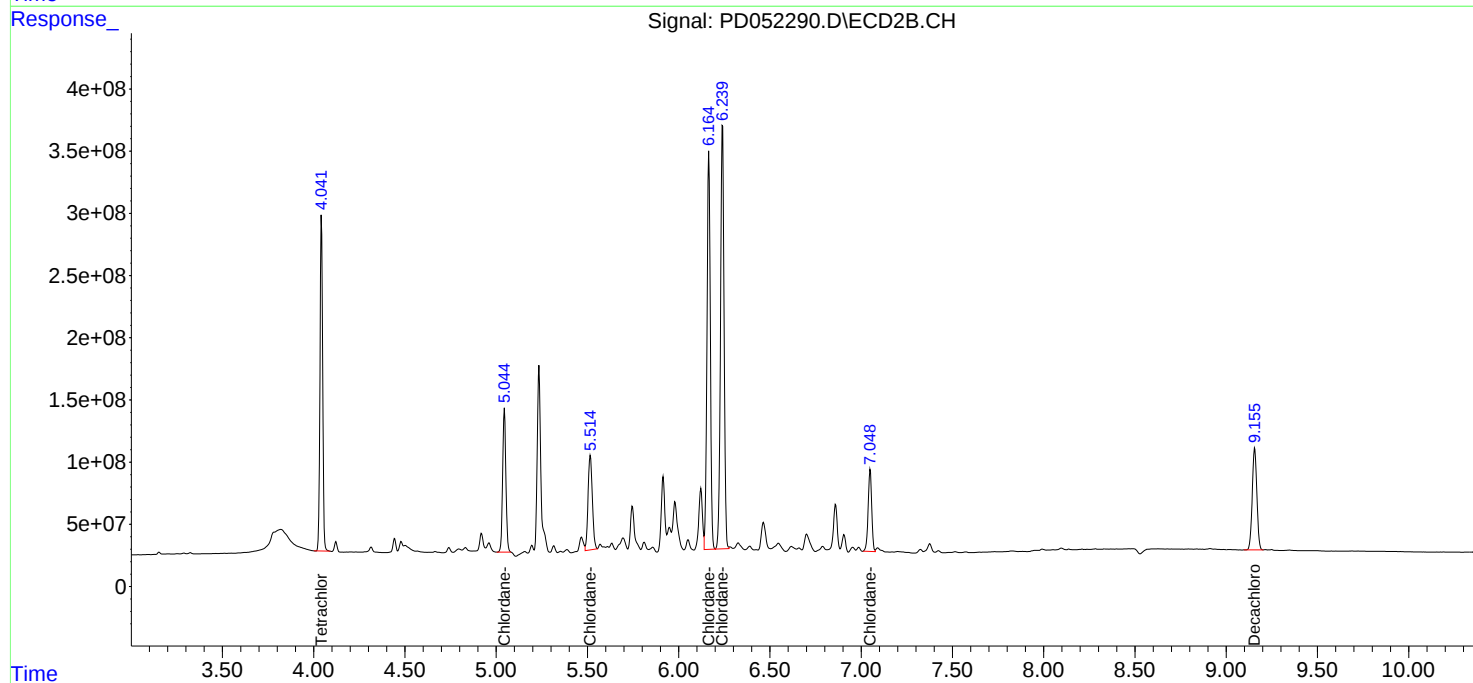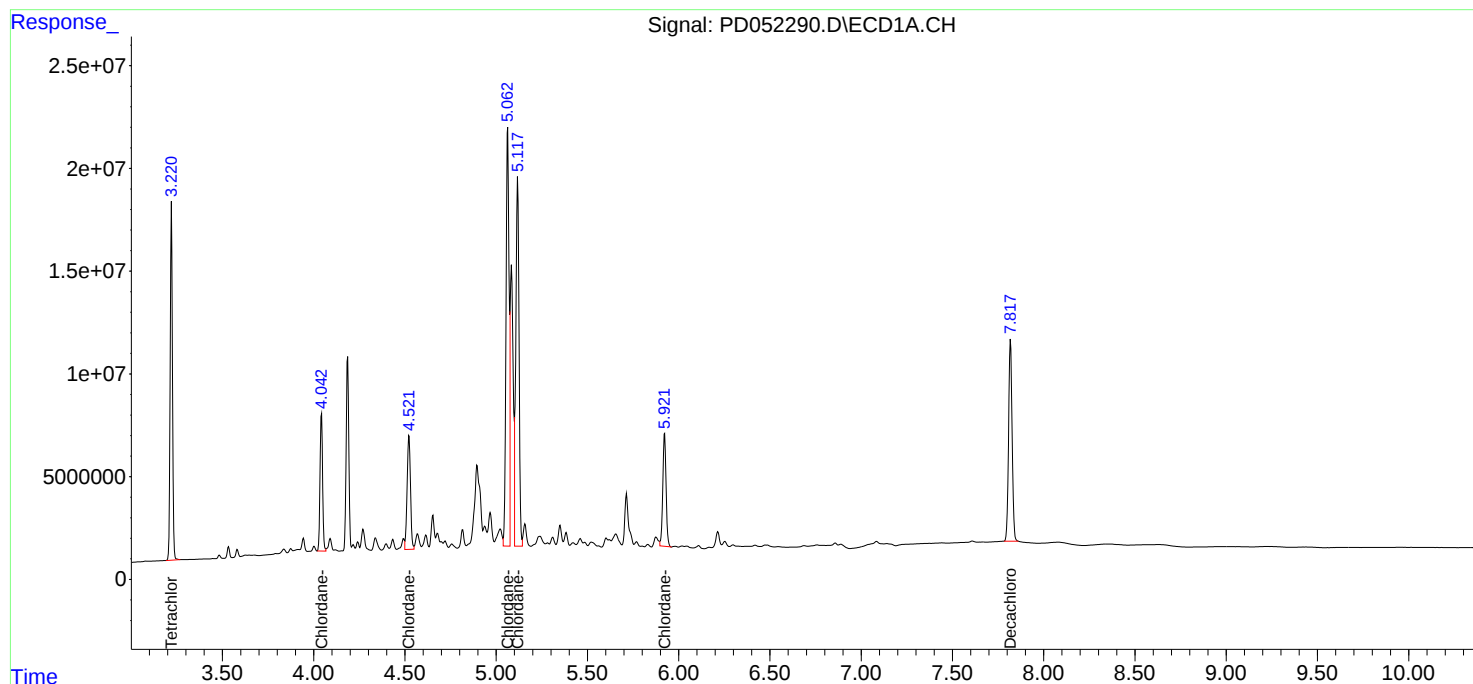


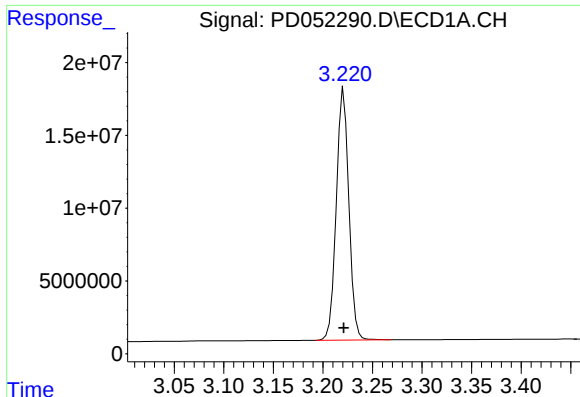

#1 Tetrachloro-m-xylene


R.T.: 3.221 min
Delta R.T.: 0.000 min
Response: 152255657
Conc: 103.58 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

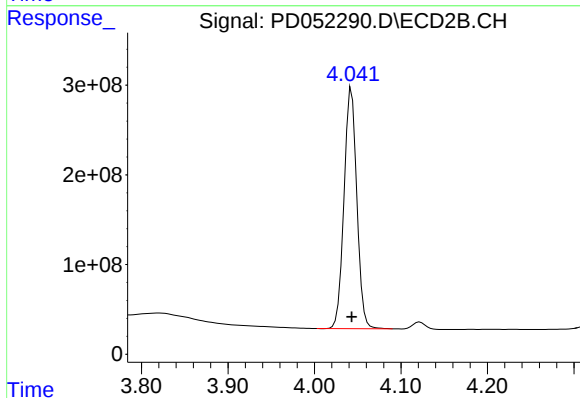


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 2736895979
Conc: 95.48 ng/ml

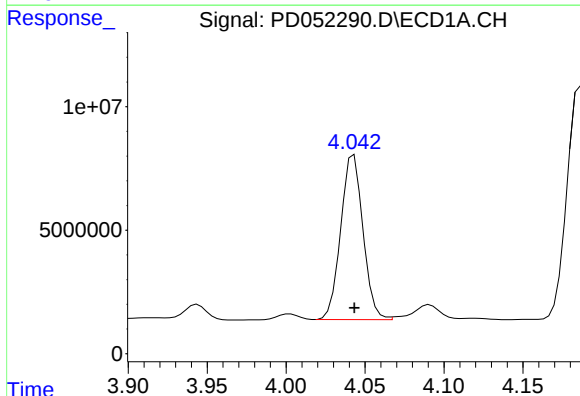


#23 Chlordane-1

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 65554293
Conc: 1031.92 ng/ml

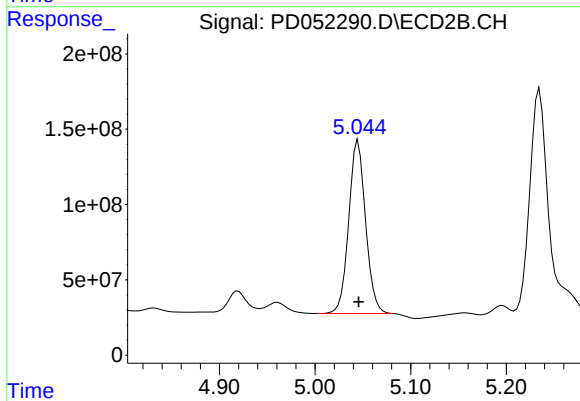

#23 Chlordane-1


R.T.: 5.045 min
Delta R.T.: 0.000 min
Response: 1413987495
Conc: 949.28 ng/ml

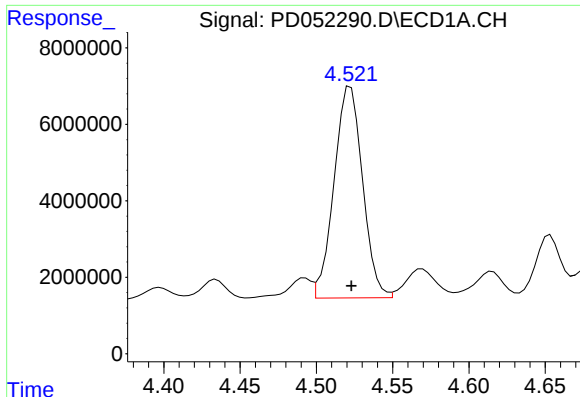

#24 Chlordane-2


R.T.: 4.522 min
Delta R.T.: 0.000 min
Response: 71907163
Conc: 975.55 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

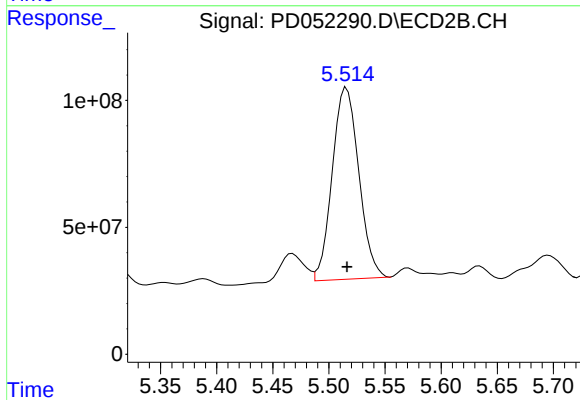


#24 Chlordane-2

R.T.: 5.516 min
Delta R.T.: 0.000 min
Response: 1244452046
Conc: 923.21 ng/ml

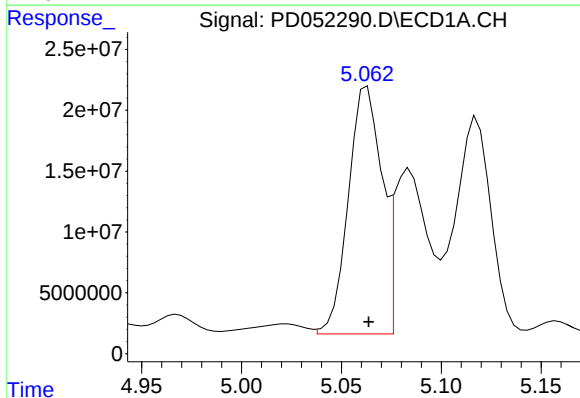


#25 Chlordane-3

R.T.: 5.063 min
Delta R.T.: 0.000 min
Response: 236642088
Conc: 1059.52 ng/ml

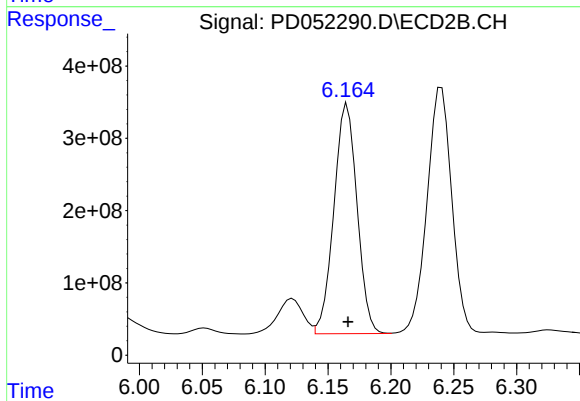

#25 Chlordane-3


R.T.: 6.165 min
Delta R.T.: 0.000 min
Response: 4080496522
Conc: 956.15 ng/ml

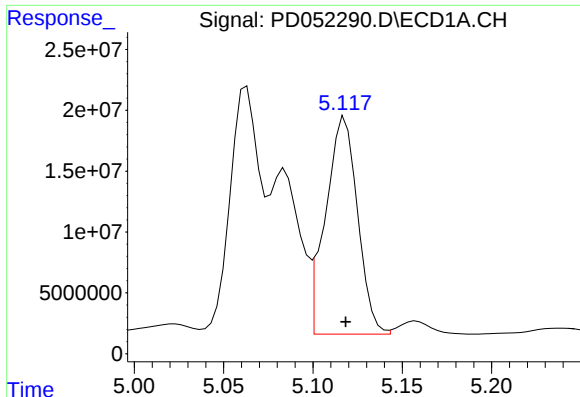

#26 Chlordane-4


R.T.: 5.118 min
Delta R.T.: 0.000 min
Response: 222293786
Conc: 1038.58 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

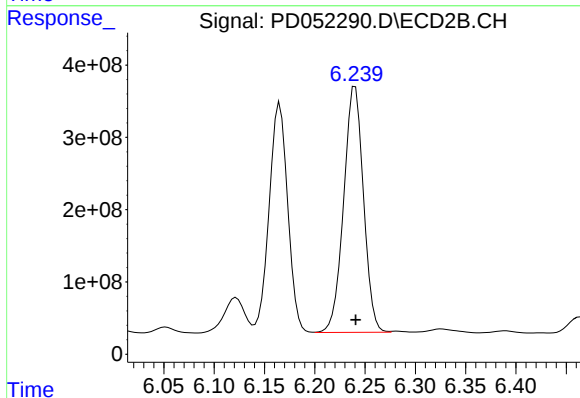


#26 Chlordane-4

R.T.: 6.240 min
Delta R.T.: 0.000 min
Response: 4651648108
Conc: 950.36 ng/ml

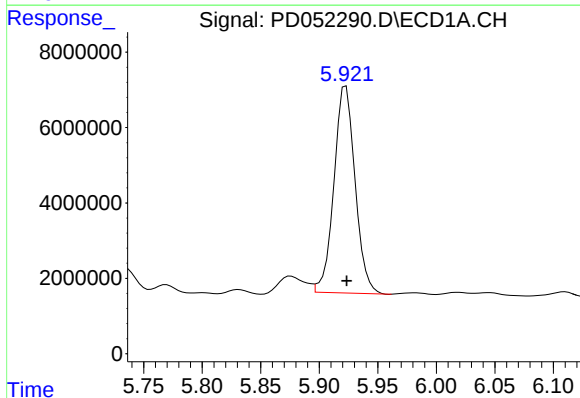


#27 Chlordane-5

R.T.: 5.923 min
Delta R.T.: 0.000 min
Response: 68965502
Conc: 1019.96 ng/ml

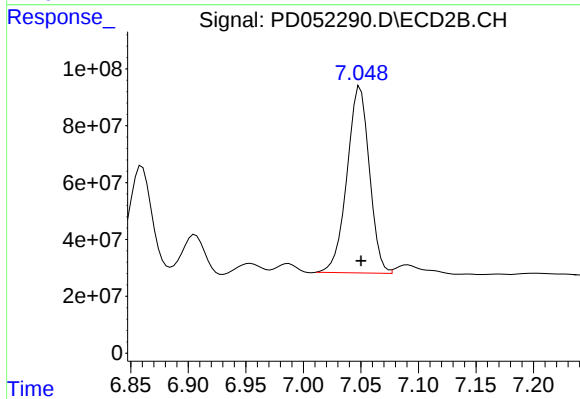

#27 Chlordane-5


R.T.: 7.049 min
Delta R.T.: 0.000 min
Response: 891016628
Conc: 952.23 ng/ml

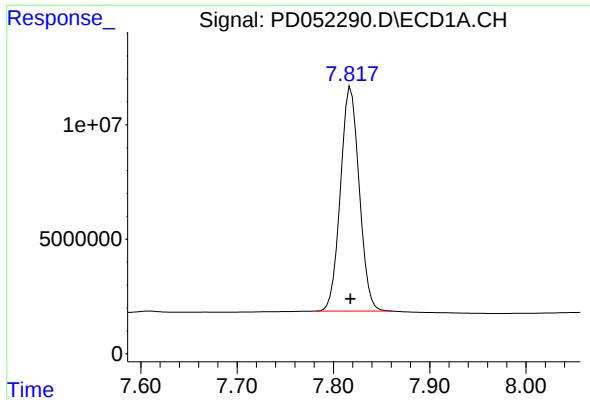

#28 Decachlorobiphenyl

R.T.: 7.818 min
Delta R.T.: 0.000 min
Response: 132335479
Conc: 96.97 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

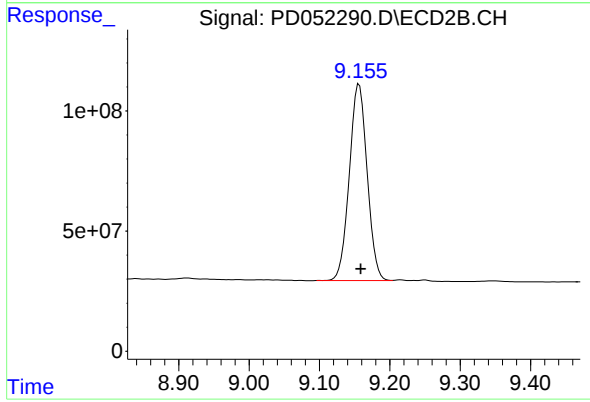

#28 Decachlorobiphenyl

R.T.: 9.156 min
Delta R.T.: -0.002 min
Response: 1441485199
Conc: 92.46 ng/ml