

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032919\
 Data File : PD052303.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Mar 2019 14:46
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 30 04:55:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 29 13:06:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.222	4.043	27432676	613.2E6	19.659	21.155
28)	SA Decachlor...	7.819	9.157	29912202	351.1E6	22.444	22.580
Target Compounds							
3)	MA gamma-BHC...	3.920	0.000	2639831	0	1.207	N.D. #
4)	MA Heptachlor	0.000	5.252f	0	794250	N.D.	0.020 #
8)	B Heptachlo...	0.000	5.923	0	59502714	N.D.	1.843 #
9)	A Endosulfan I	0.000	6.289	0	20923752	N.D.	0.716 #
10)	B gamma-Chl...	0.000	6.168	0	38711964	N.D.	1.210 #
11)	B alpha-Chl...	0.000	6.212f	0	13487778	N.D.	0.430 #
17)	MA 4,4'-DDT	0.000	7.193	0	4867633	N.D.	0.261 #
18)	B Endrin al...	0.000	7.090	0	1651124	N.D.	0.080 #
25)	Chlordane-3	0.000	6.168	0	38711964	N.D.	8.773 #
26)	Chlordane-4	0.000	6.212f	0	13487778	N.D.	2.652 #
27)	Chlordane-5	0.000	7.063	0	6211139	N.D.	6.732 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032919\
Data File : PD052303.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Mar 2019 14:46
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 30 04:55:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
Quant Title : GC Extractables
QLast Update : Fri Mar 29 13:06:45 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

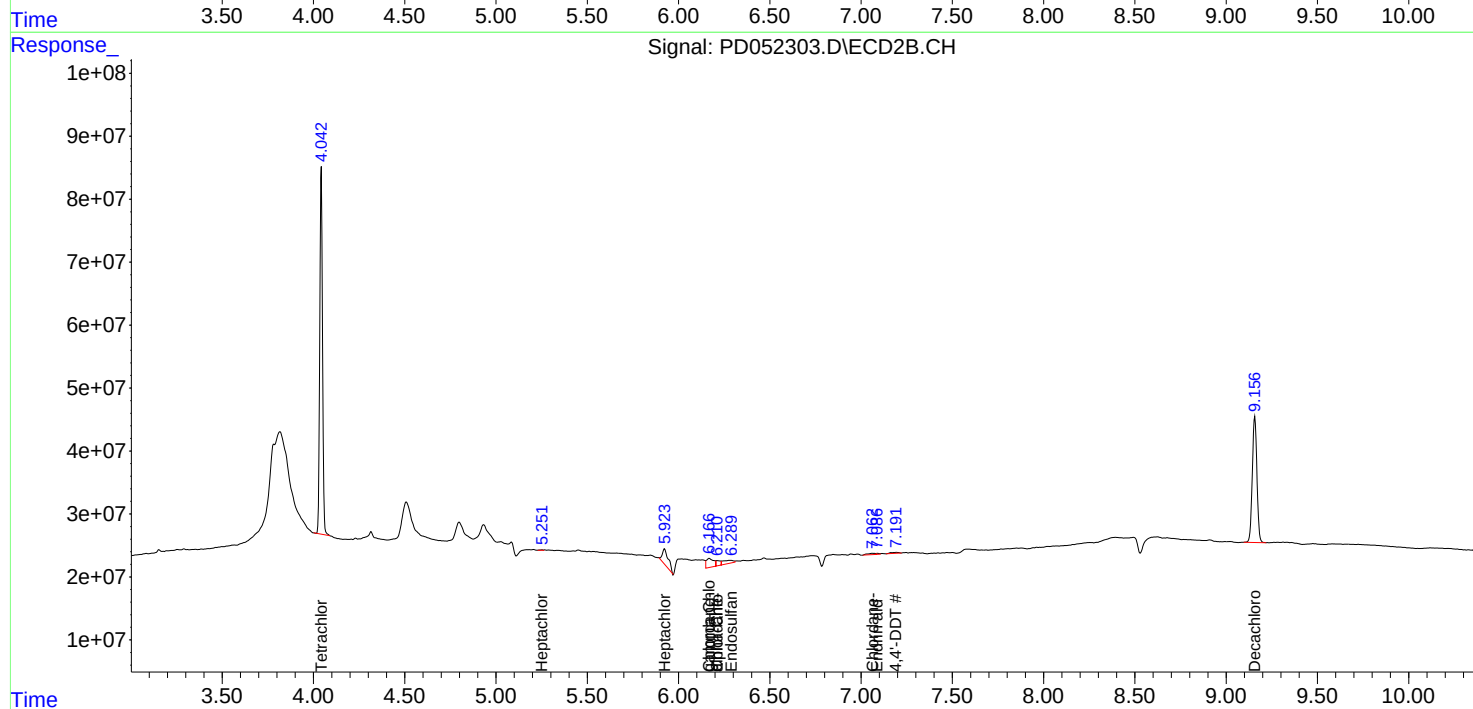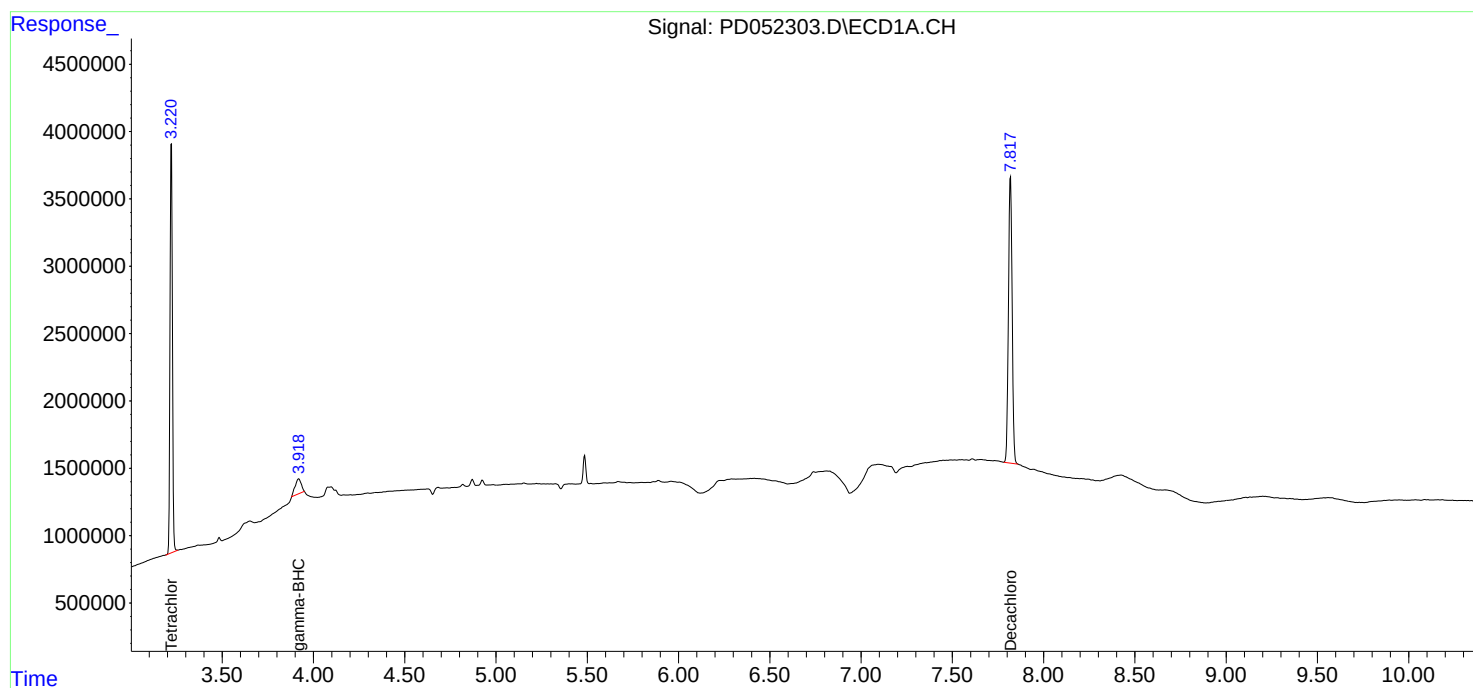


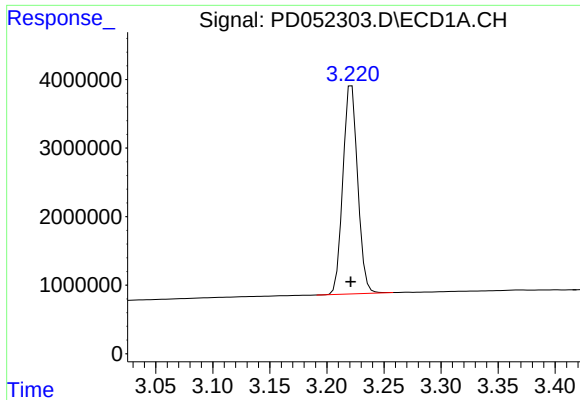

#1 Tetrachloro-m-xylene


R.T.: 3.222 min
Delta R.T.: 0.000 min
Response: 27432676
Conc: 19.66 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

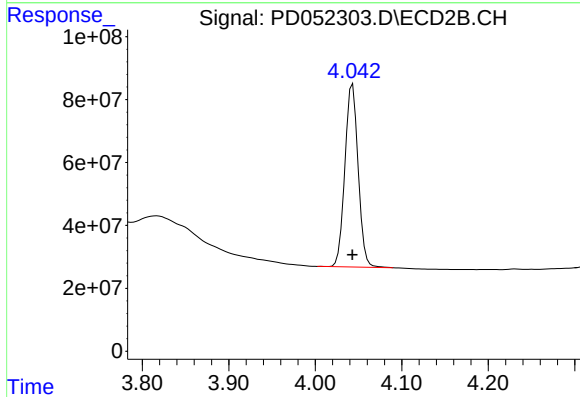


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 613164662
Conc: 21.16 ng/ml

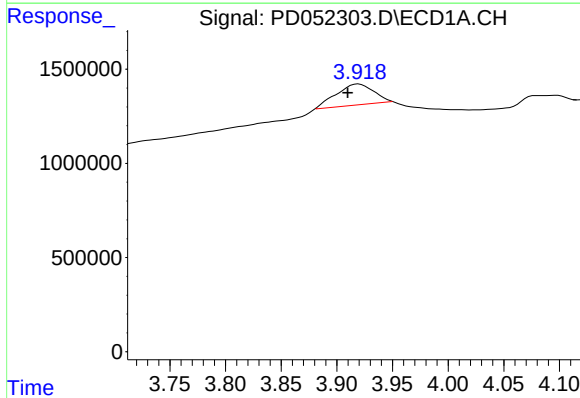


#3 gamma-BHC (Lindane)

R.T.: 3.920 min
Delta R.T.: 0.010 min
Response: 2639831
Conc: 1.21 ng/ml

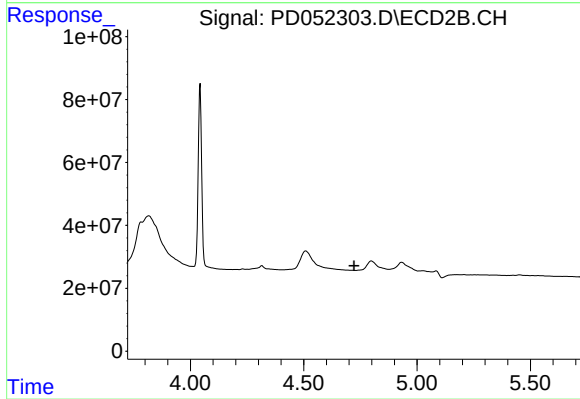

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.723 min
Response: 0
Conc: N.D.

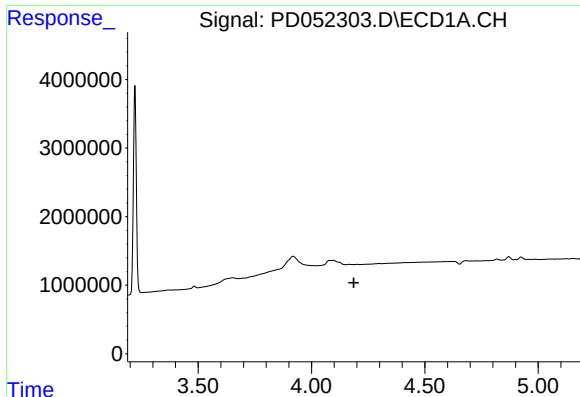

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.187 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

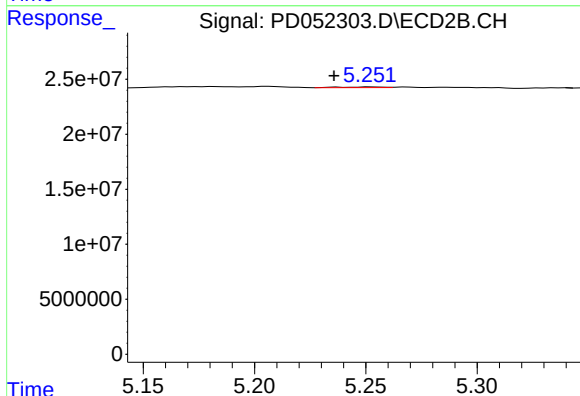


#4 Heptachlor

R.T.: 5.252 min
Delta R.T.: 0.017 min
Response: 794250
Conc: 0.02 ng/ml

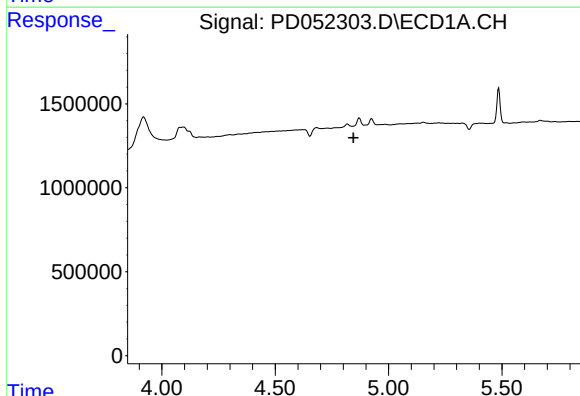


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 4.846 min
Response: 0
Conc: N.D.

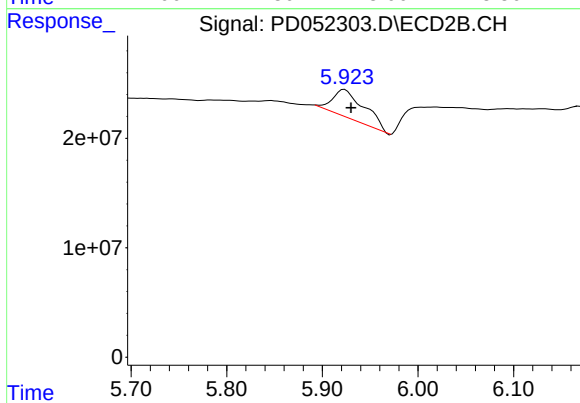

#8 Heptachlor epoxide


R.T.: 5.923 min
Delta R.T.: -0.007 min
Response: 59502714
Conc: 1.84 ng/ml

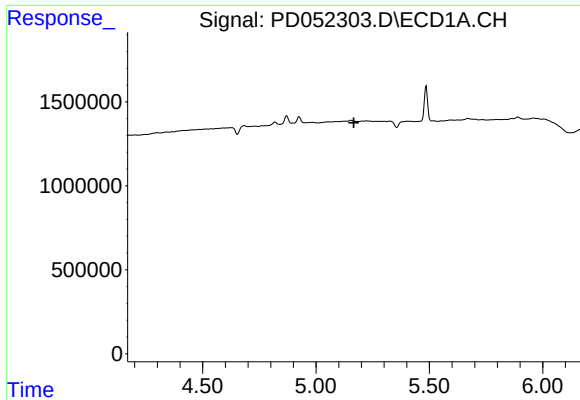

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.167 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

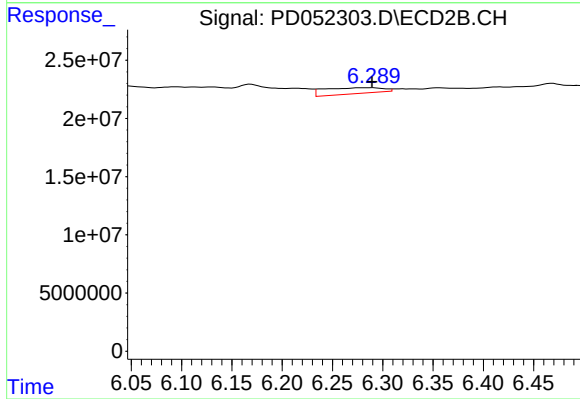


#9 Endosulfan I

R.T.: 6.289 min
Delta R.T.: 0.000 min
Response: 20923752
Conc: 0.72 ng/ml

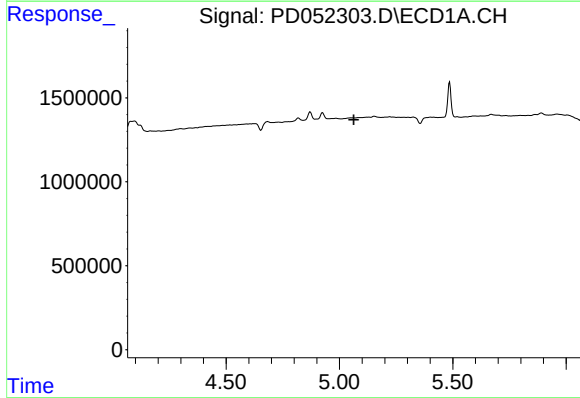


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.063 min
Response: 0
Conc: N.D.

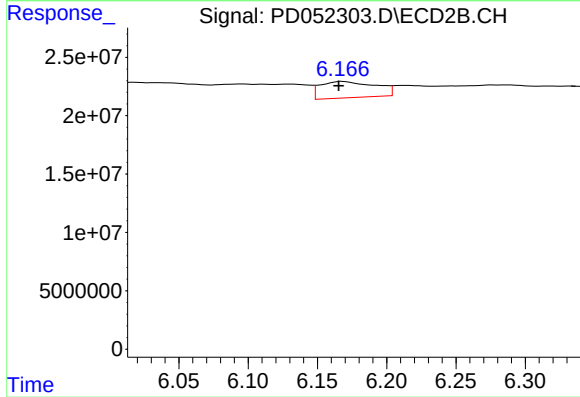

#10 gamma-Chlordane


R.T.: 6.168 min
Delta R.T.: 0.003 min
Response: 38711964
Conc: 1.21 ng/ml

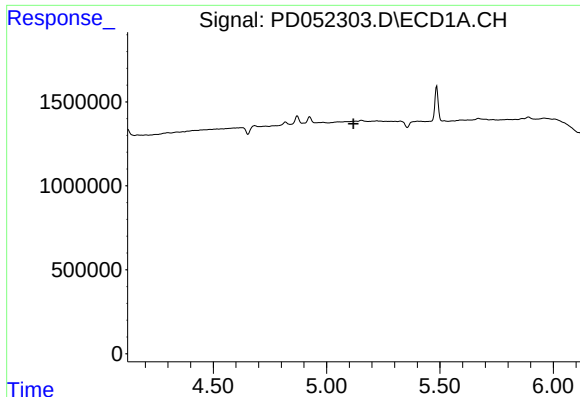

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.119 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

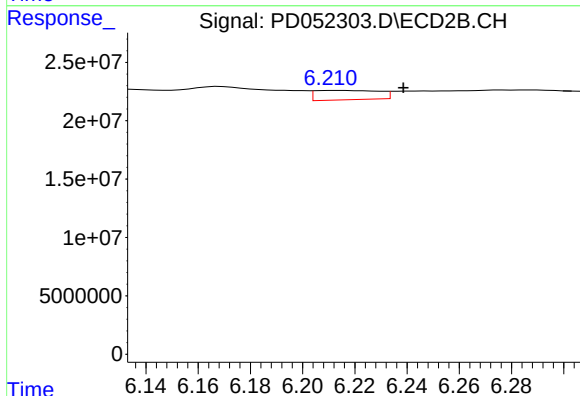


#11 alpha-Chlordane

R.T.: 6.212 min
Delta R.T.: -0.026 min
Response: 13487778
Conc: 0.43 ng/ml

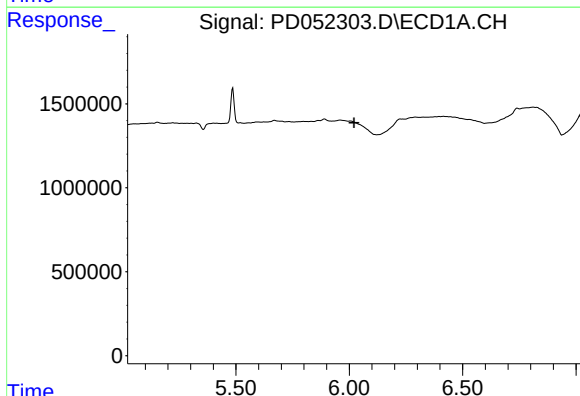


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 6.021 min
Response: 0
Conc: N.D.

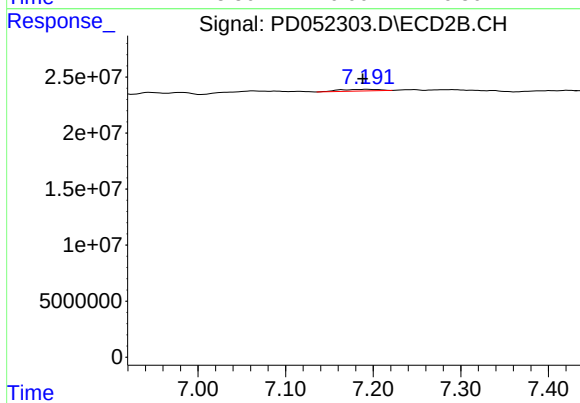

#17 4,4'-DDT


R.T.: 7.193 min
Delta R.T.: 0.005 min
Response: 4867633
Conc: 0.26 ng/ml

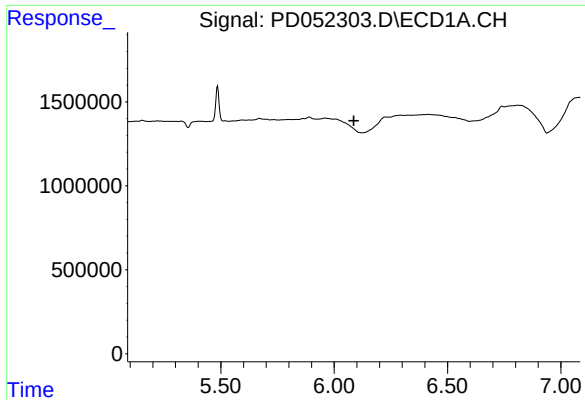

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.087 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

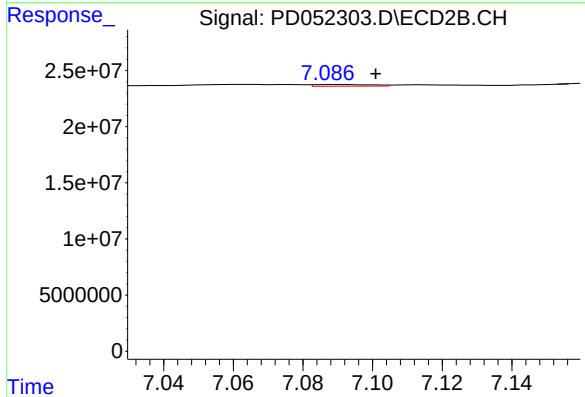


#18 Endrin aldehyde

R.T.: 7.090 min
Delta R.T.: -0.011 min
Response: 1651124
Conc: 0.08 ng/ml

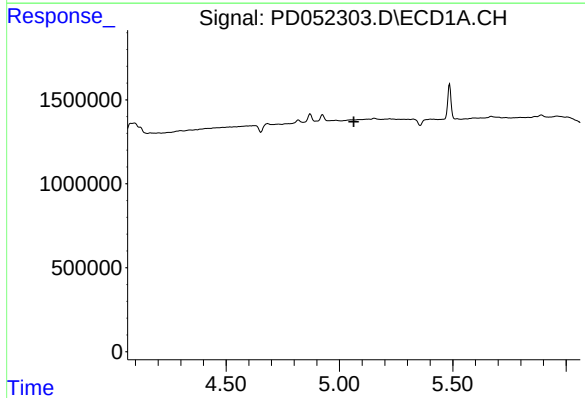


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.064 min
Response: 0
Conc: N.D.

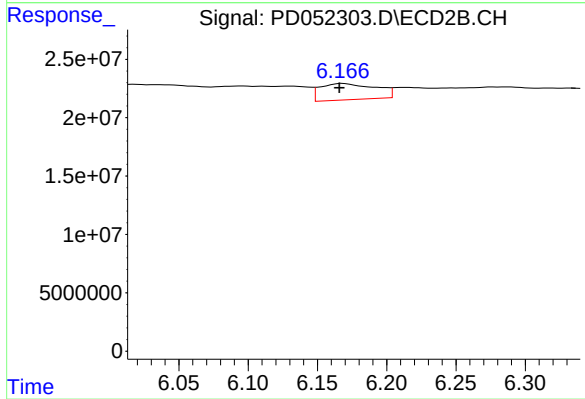

#25 Chlordane-3


R.T.: 6.168 min
Delta R.T.: 0.003 min
Response: 38711964
Conc: 8.77 ng/ml

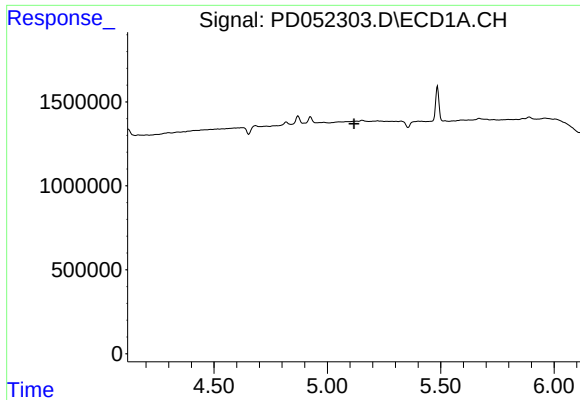

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.118 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

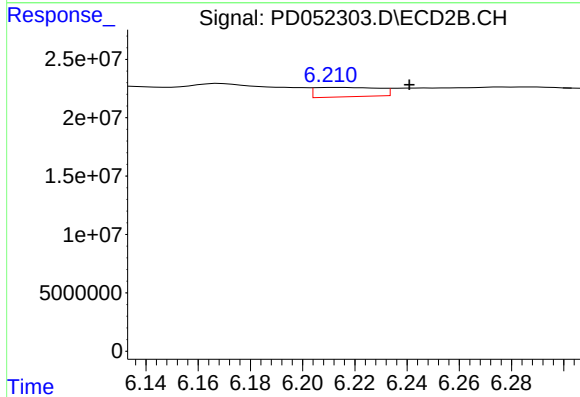


#26 Chlordane-4

R.T.: 6.212 min
Delta R.T.: -0.028 min
Response: 13487778
Conc: 2.65 ng/ml

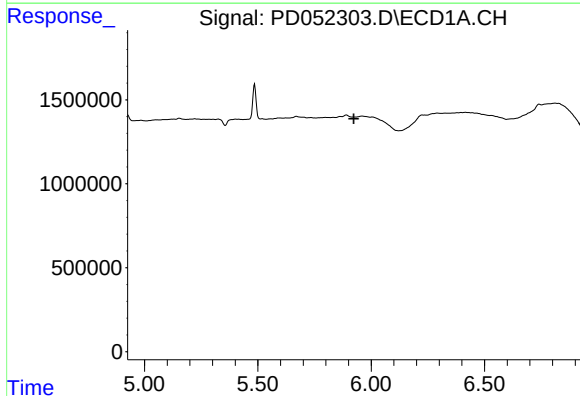


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 5.924 min
Response: 0
Conc: N.D.

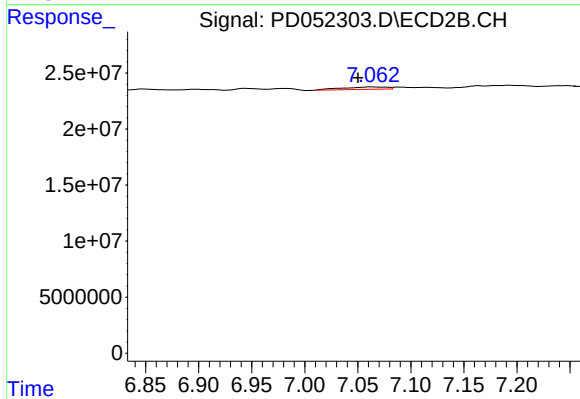

#27 Chlordane-5


R.T.: 7.063 min
Delta R.T.: 0.013 min
Response: 6211139
Conc: 6.73 ng/ml

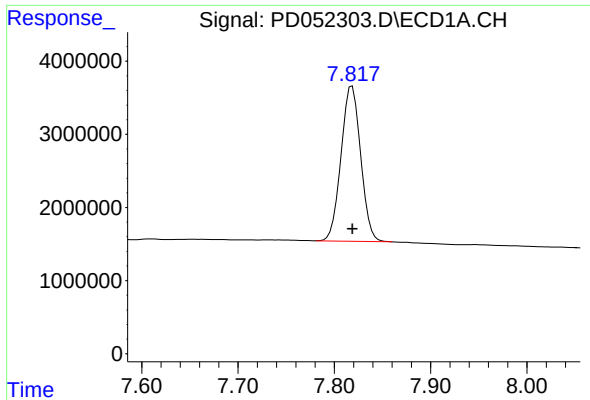

#28 Decachlorobiphenyl

R.T.: 7.819 min
Delta R.T.: 0.000 min
Response: 29912202
Conc: 22.44 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

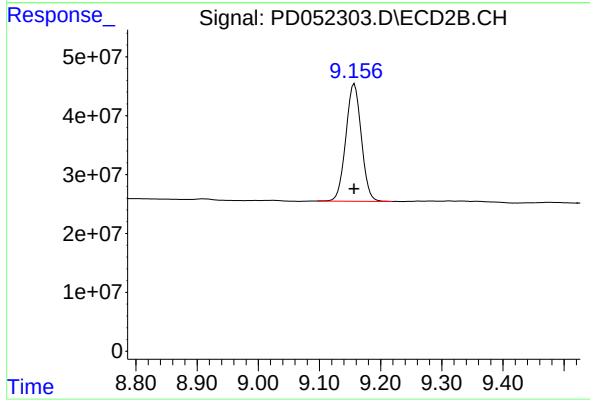

#28 Decachlorobiphenyl

R.T.: 9.157 min
Delta R.T.: 0.000 min
Response: 351146737
Conc: 22.58 ng/ml