

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032919\
 Data File : PD052321.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Mar 2019 18:59
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 30 04:58:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 29 13:06:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.221	4.043	27241427	576.8E6	19.522	19.899
28)	SA Decachlor...	7.818	9.156	30330549	371.3E6	22.758	23.878
Target Compounds							
3)	MA gamma-BHC...	3.920	0.000	3369392	0	1.541	N.D. #
4)	MA Heptachlor	0.000	5.243	0	1441359	N.D.	0.036 #
8)	B Heptachlo...	0.000	5.923	0	62278767	N.D.	1.929 #
9)	A Endosulfan I	0.000	6.283	0	31449301	N.D.	1.077 #
10)	B gamma-Chl...	0.000	6.166	0	65637402	N.D.	2.052 #
13)	MA Dieldrin	0.000	6.539	0	6740093	N.D.	0.225 #
15)	B Endosulfa...	0.000	6.977	0	4778327	N.D.	0.192 #
17)	MA 4,4'-DDT	0.000	7.198	0	18275313	N.D.	0.981 #
18)	B Endrin al...	0.000	7.091	0	18869922	N.D.	0.917 #
25)	Chlordane-3	0.000	6.166	0	65637402	N.D.	14.874 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032919\
Data File : PD052321.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Mar 2019 18:59
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 30 04:58:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
Quant Title : GC Extractables
QLast Update : Fri Mar 29 13:06:45 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

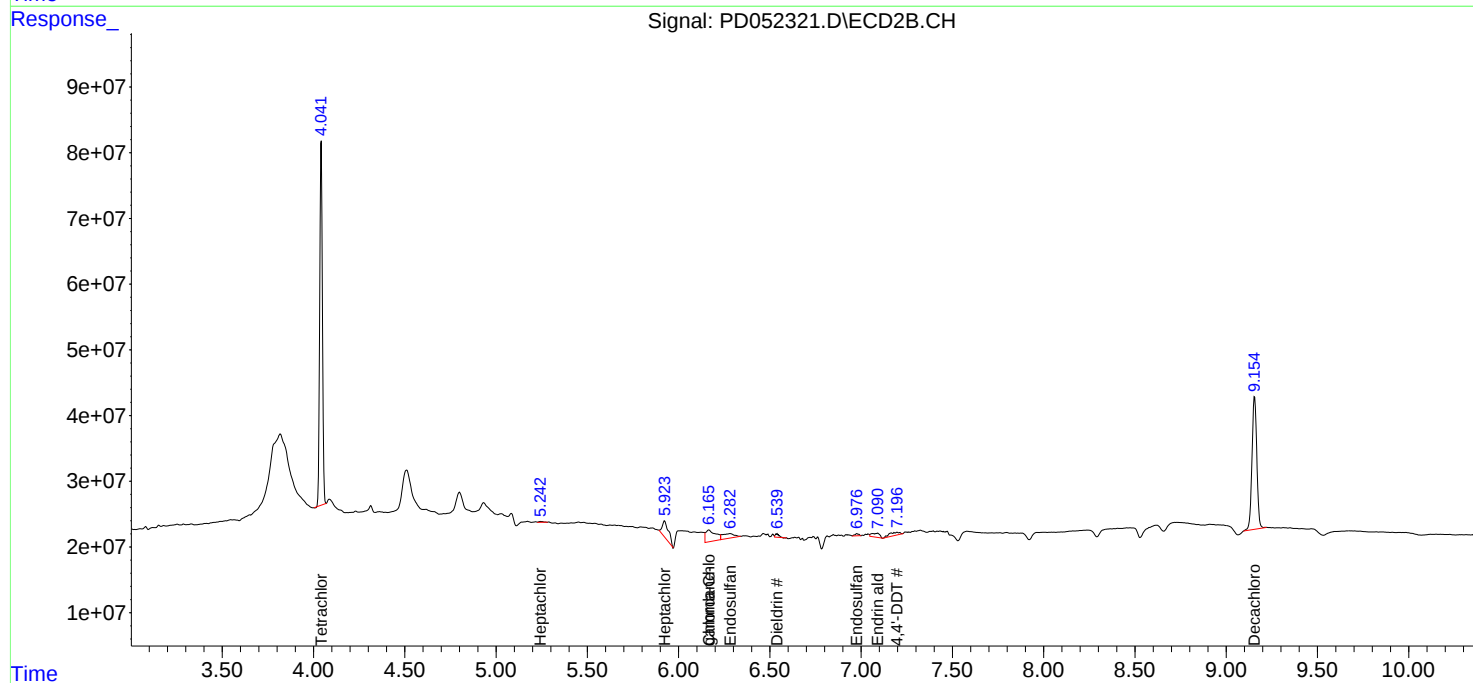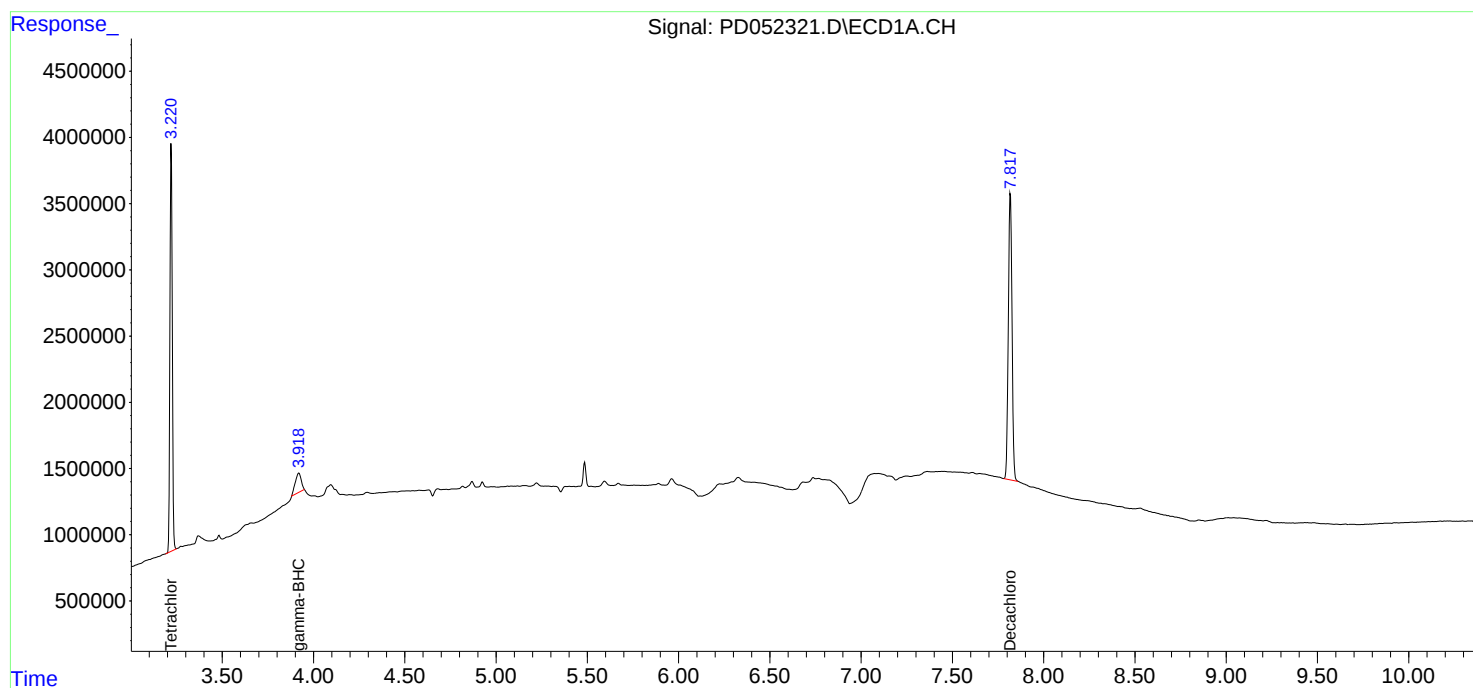


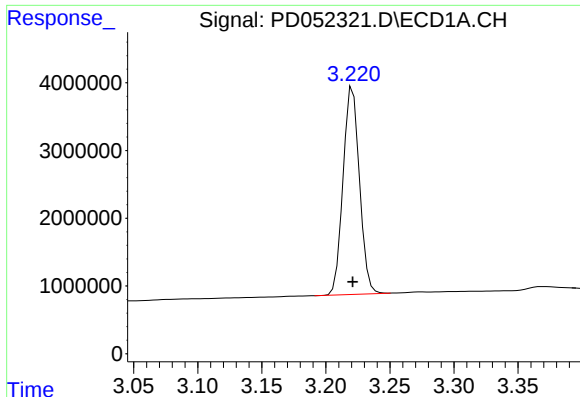

#1 Tetrachloro-m-xylene


R.T.: 3.221 min
Delta R.T.: 0.000 min
Response: 27241427
Conc: 19.52 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

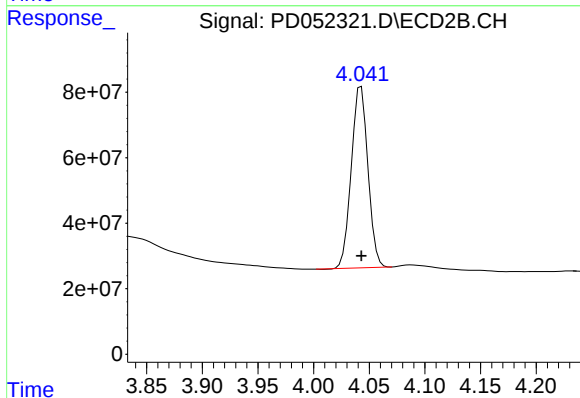


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 576751923
Conc: 19.90 ng/ml

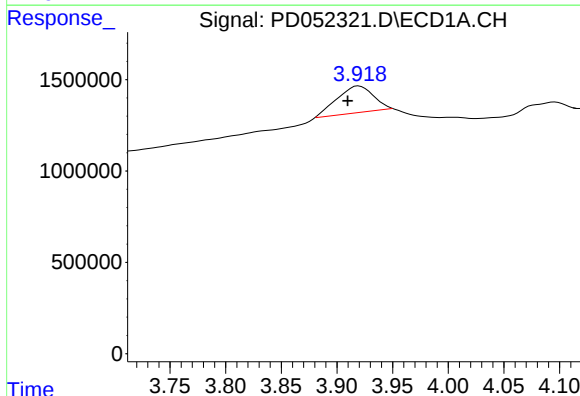


#3 gamma-BHC (Lindane)

R.T.: 3.920 min
Delta R.T.: 0.010 min
Response: 3369392
Conc: 1.54 ng/ml

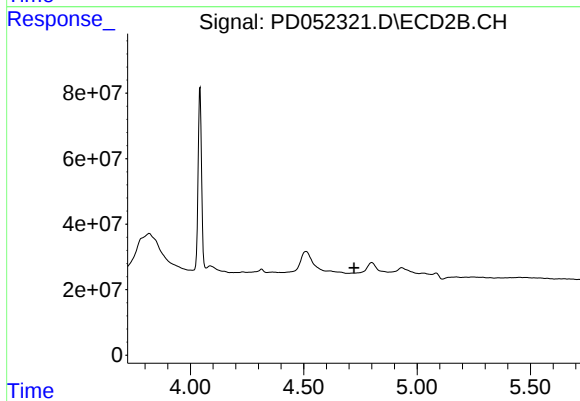

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.723 min
Response: 0
Conc: N.D.

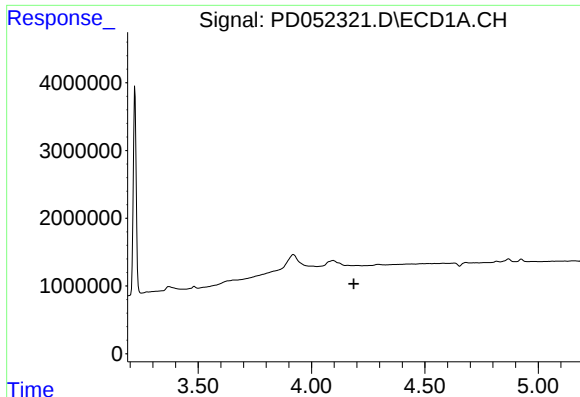

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.187 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

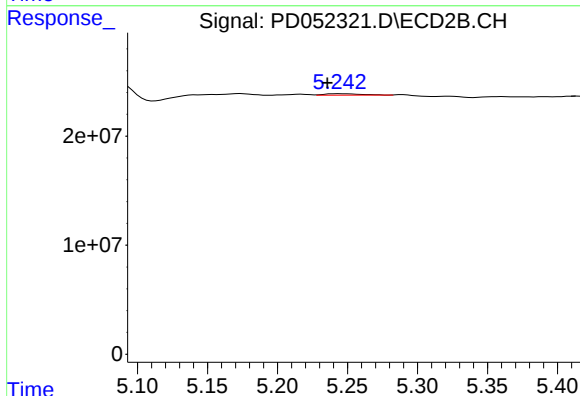


#4 Heptachlor

R.T.: 5.243 min
Delta R.T.: 0.008 min
Response: 1441359
Conc: 0.04 ng/ml

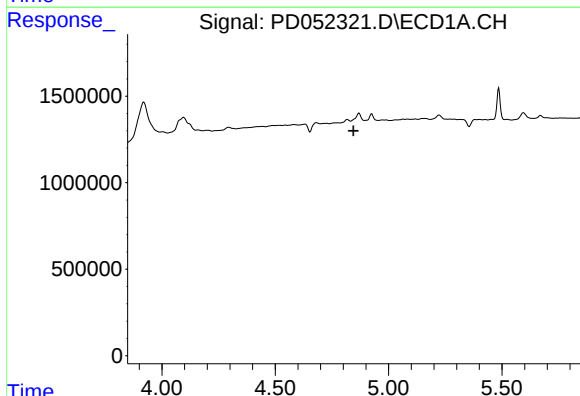


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 4.846 min
Response: 0
Conc: N.D.

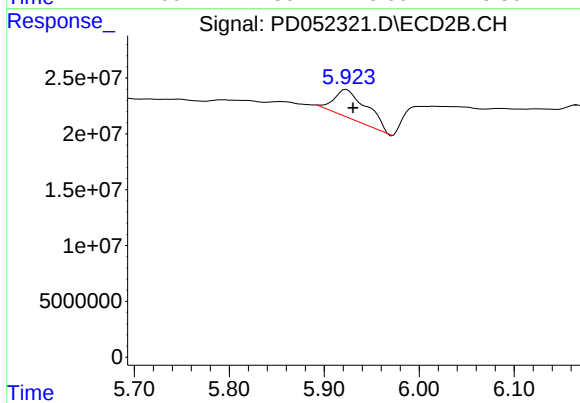

#8 Heptachlor epoxide


R.T.: 5.923 min
Delta R.T.: -0.007 min
Response: 62278767
Conc: 1.93 ng/ml

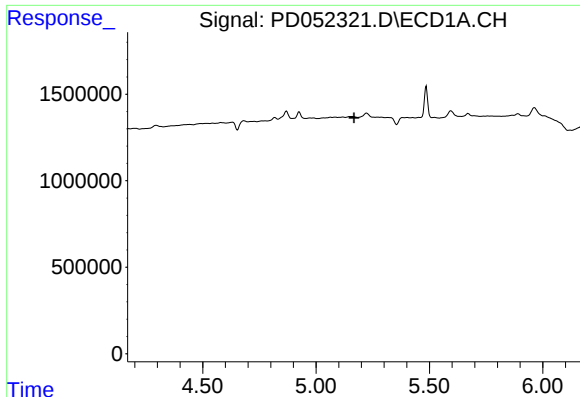

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.167 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

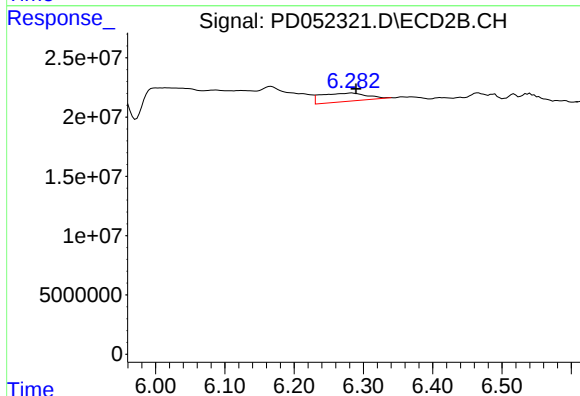


#9 Endosulfan I

R.T.: 6.283 min
Delta R.T.: -0.006 min
Response: 31449301
Conc: 1.08 ng/ml

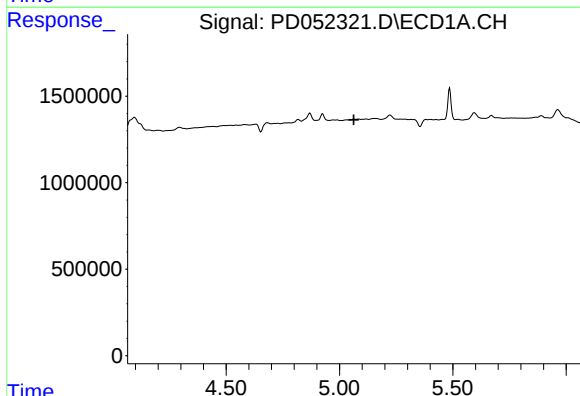


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.063 min
Response: 0
Conc: N.D.

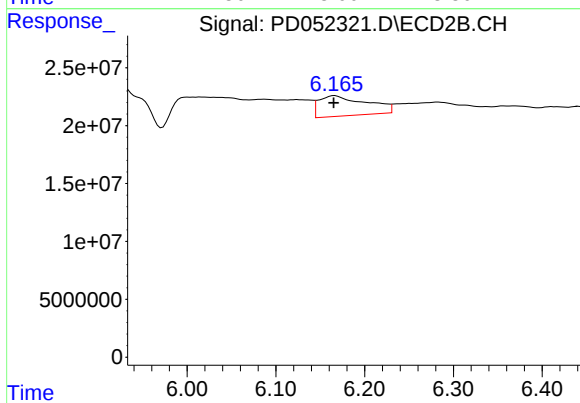

#10 gamma-Chlordane


R.T.: 6.166 min
Delta R.T.: 0.000 min
Response: 65637402
Conc: 2.05 ng/ml

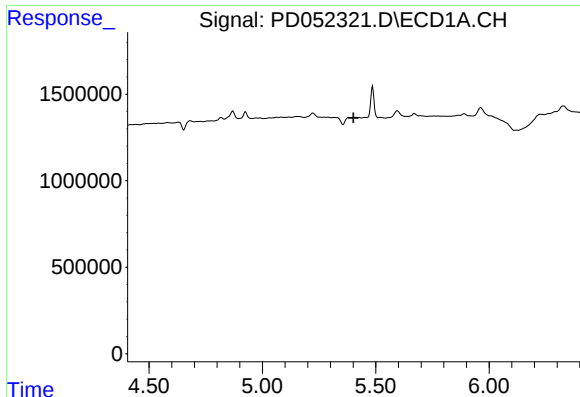

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 5.402 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

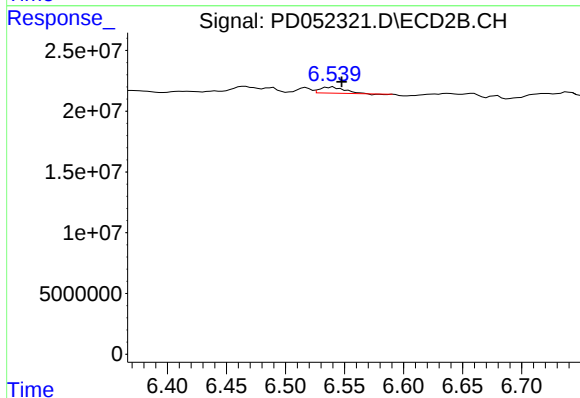


#13 Dieldrin

R.T.: 6.539 min
Delta R.T.: -0.008 min
Response: 6740093
Conc: 0.23 ng/ml

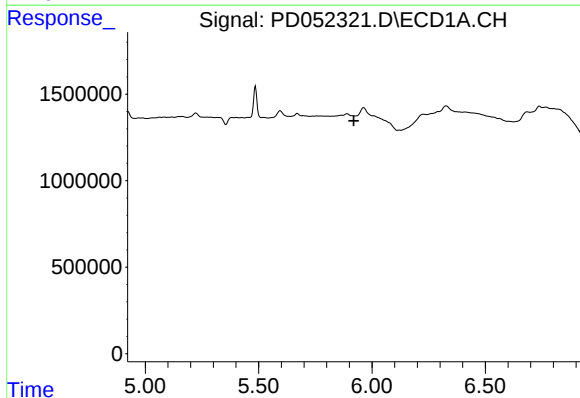


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.919 min
Response: 0
Conc: N.D.

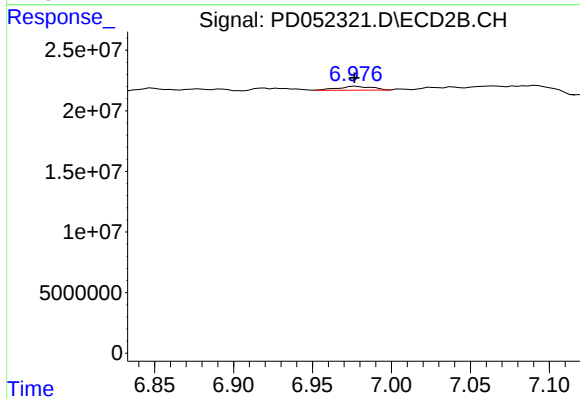

#15 Endosulfan II


R.T.: 6.977 min
Delta R.T.: 0.000 min
Response: 4778327
Conc: 0.19 ng/ml

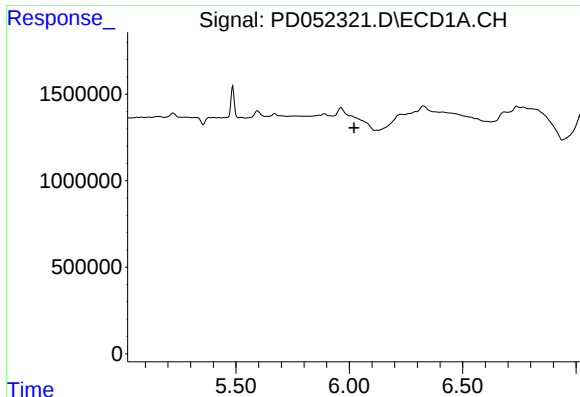

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.021 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

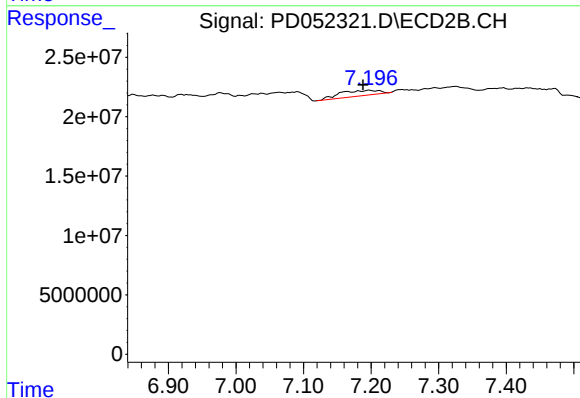


#17 4,4'-DDT

R.T.: 7.198 min
Delta R.T.: 0.010 min
Response: 18275313
Conc: 0.98 ng/ml

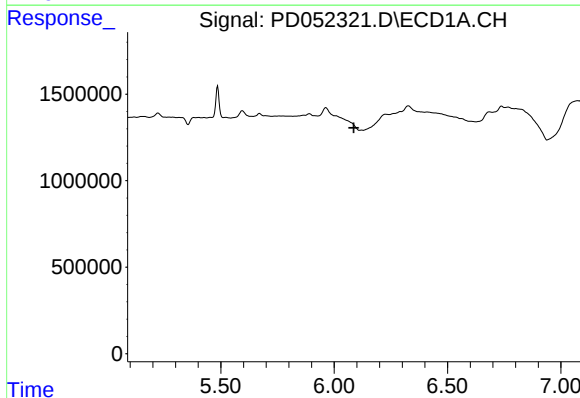


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.087 min
Response: 0
Conc: N.D.

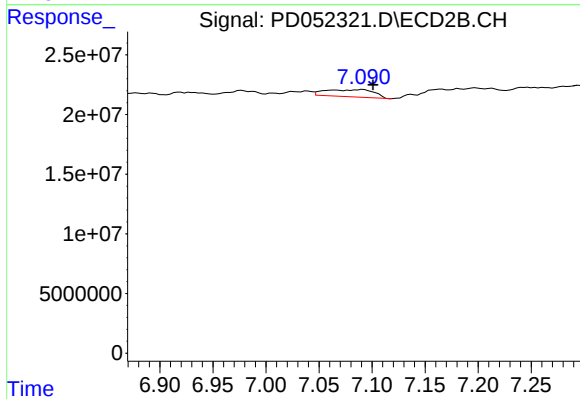

#18 Endrin aldehyde


R.T.: 7.091 min
Delta R.T.: -0.010 min
Response: 18869922
Conc: 0.92 ng/ml

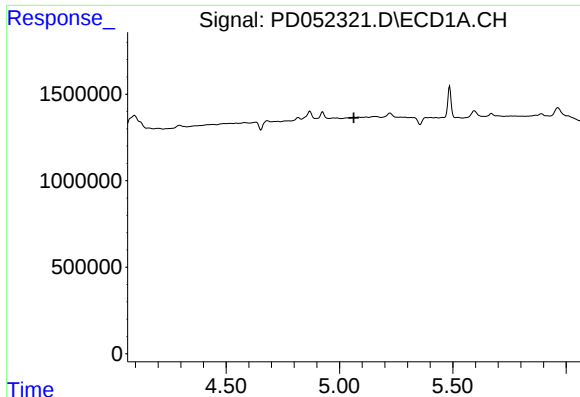

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.064 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

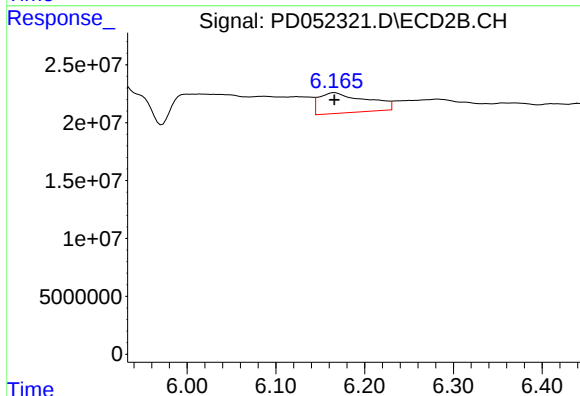


#25 Chlordane-3

R.T.: 6.166 min
Delta R.T.: 0.000 min
Response: 65637402
Conc: 14.87 ng/ml

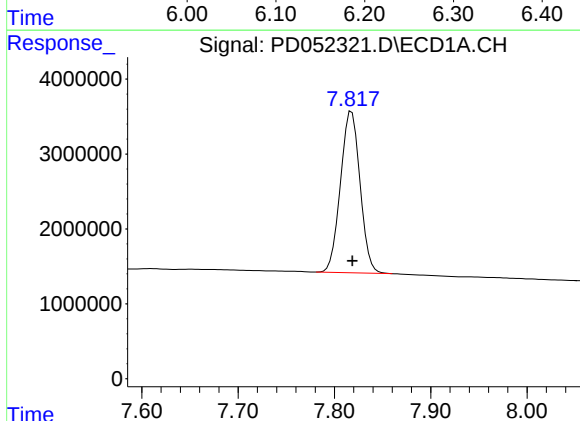

#28 Decachlorobiphenyl

R.T.: 7.818 min
Delta R.T.: 0.000 min
Response: 30330549
Conc: 22.76 ng/ml

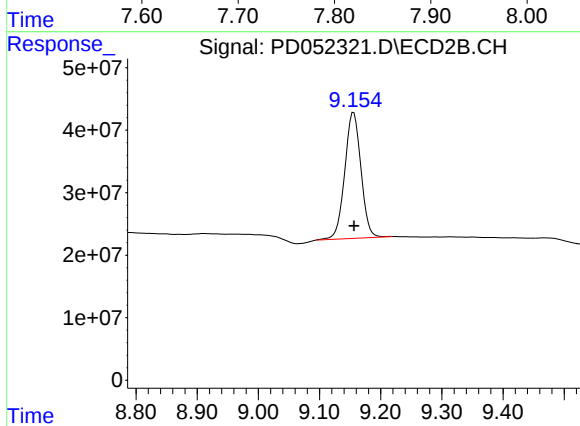

#28 Decachlorobiphenyl

R.T.: 9.156 min
Delta R.T.: 0.000 min
Response: 371327992
Conc: 23.88 ng/ml