

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032919\
 Data File : PD052329.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Mar 2019 20:52
 Operator : AJ\SJ
 Sample : MDL-BL-CHL-S-01
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 30 04:59:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 29 13:06:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.221	4.043	26478606	582.5E6	18.975	20.099
28)	SA Decachlor...	7.818	9.155	29025424	355.0E6	21.778	22.829
Target Compounds							
3)	MA gamma-BHC...	3.917	0.000	3600784	0	1.647	N.D. #
4)	MA Heptachlor	0.000	5.241	0	1009160	N.D.	0.025 #
10)	B gamma-Chl...	0.000	6.179	0	2771316	N.D.	0.087 #
17)	MA 4,4'-DDT	0.000	7.200	0	4859950	N.D.	0.261 #
18)	B Endrin al...	0.000	7.091	0	8051553	N.D.	0.391 #
21)	B Endrin ke...	0.000	7.817f	0	1295264	N.D.	0.063 #
25)	Chlordane-3	0.000	6.179	0	2771316	N.D.	0.628 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032919\
Data File : PD052329.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Mar 2019 20:52
Operator : AJ\SJ
Sample : MDL-BL-CHL-S-01
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 30 04:59:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
Quant Title : GC Extractables
QLast Update : Fri Mar 29 13:06:45 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

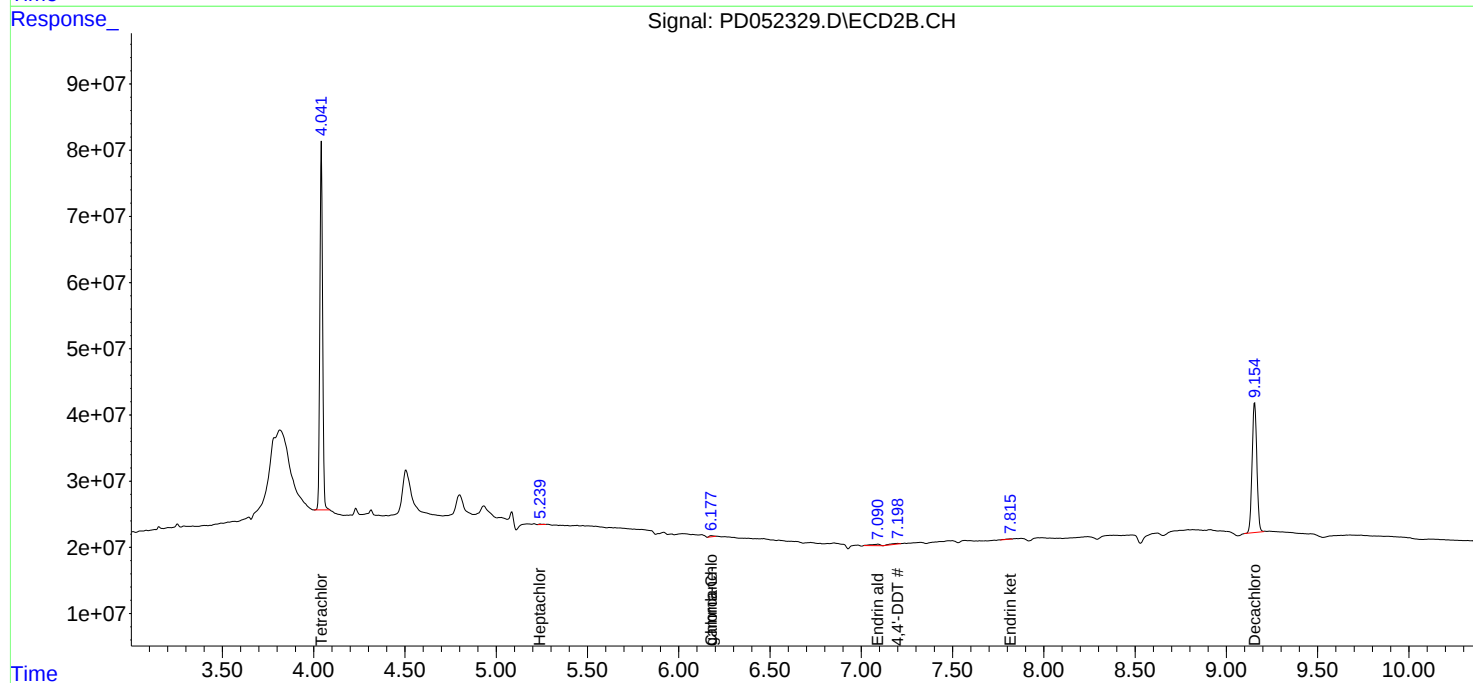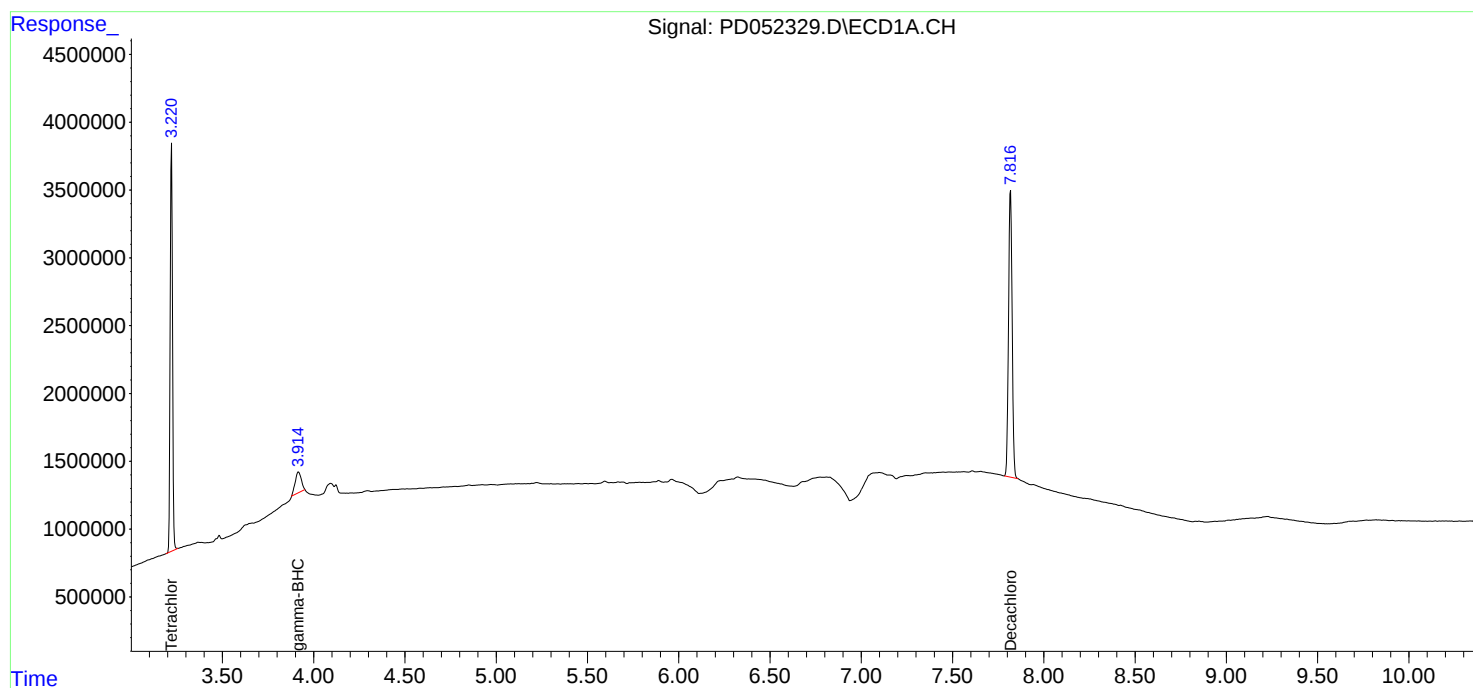


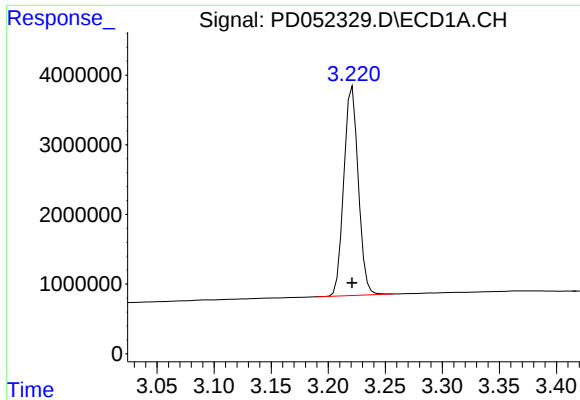

#1 Tetrachloro-m-xylene


R.T.: 3.221 min
Delta R.T.: 0.000 min
Response: 26478606
Conc: 18.98 ng/ml

Instrument :
ECD_D
ClientSampleId :

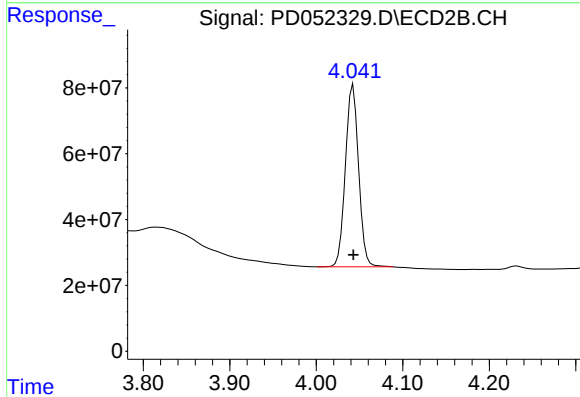


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 582544948
Conc: 20.10 ng/ml

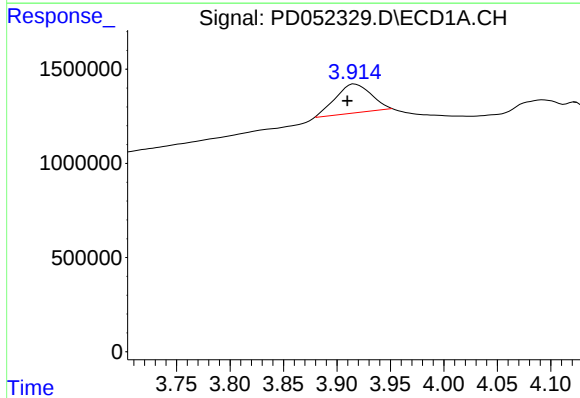


#3 gamma-BHC (Lindane)

R.T.: 3.917 min
Delta R.T.: 0.007 min
Response: 3600784
Conc: 1.65 ng/ml

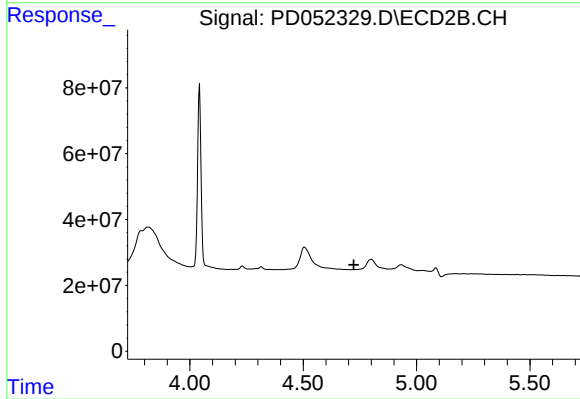

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.723 min
Response: 0
Conc: N.D.

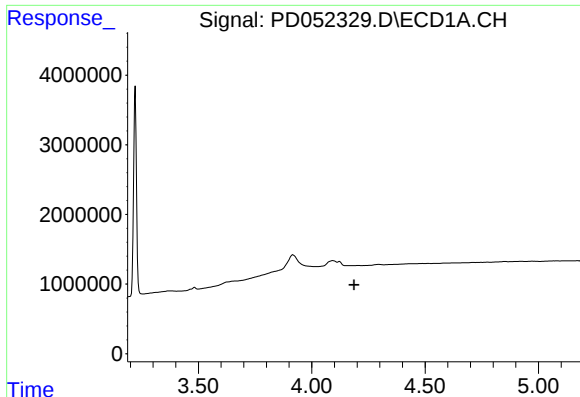

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.187 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

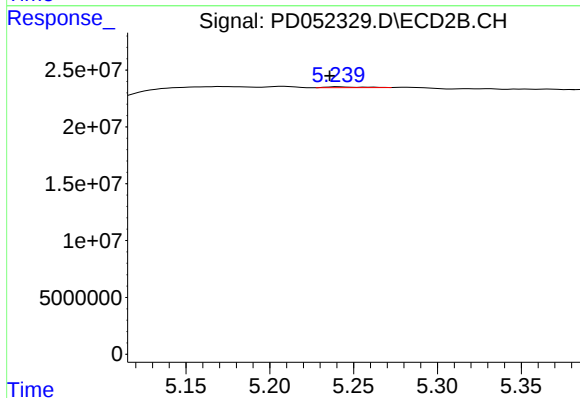


#4 Heptachlor

R.T.: 5.241 min
Delta R.T.: 0.005 min
Response: 1009160
Conc: 0.03 ng/ml

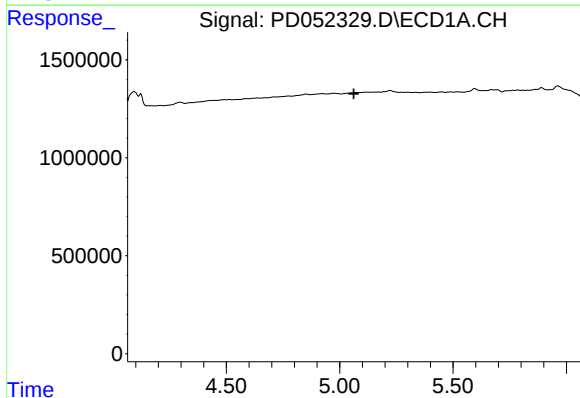


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.063 min
Response: 0
Conc: N.D.

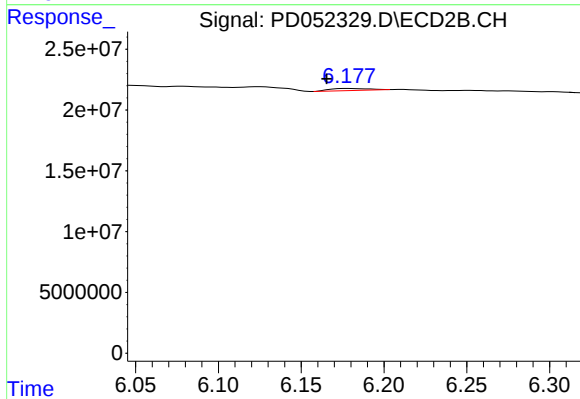

#10 gamma-Chlordane


R.T.: 6.179 min
Delta R.T.: 0.013 min
Response: 2771316
Conc: 0.09 ng/ml

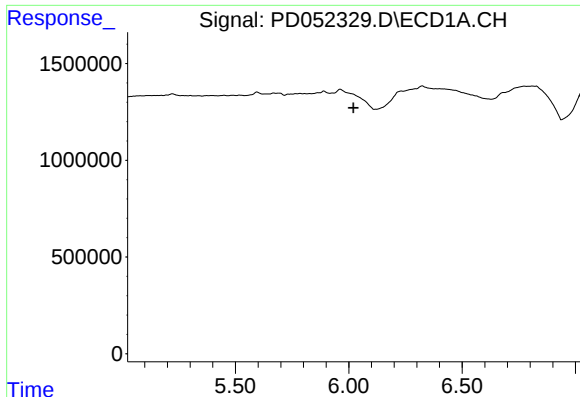

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.021 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

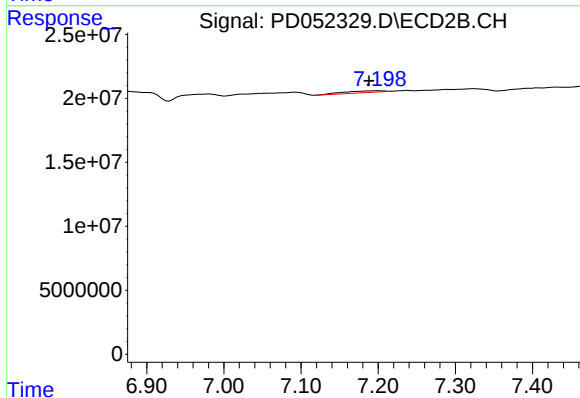


#17 4,4'-DDT

R.T.: 7.200 min
Delta R.T.: 0.011 min
Response: 4859950
Conc: 0.26 ng/ml

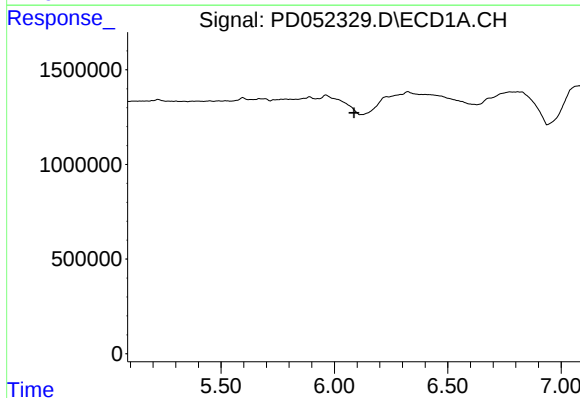


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.087 min
Response: 0
Conc: N.D.

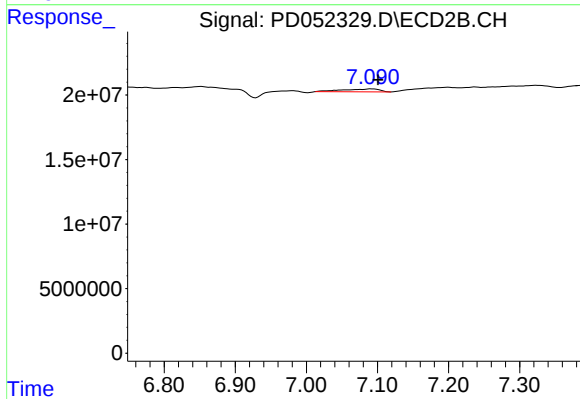

#18 Endrin aldehyde


R.T.: 7.091 min
Delta R.T.: -0.010 min
Response: 8051553
Conc: 0.39 ng/ml

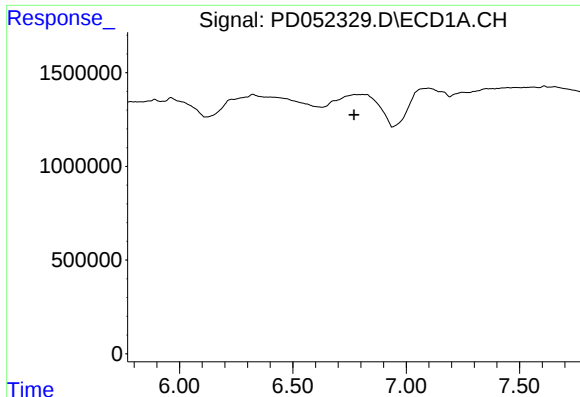

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 6.770 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

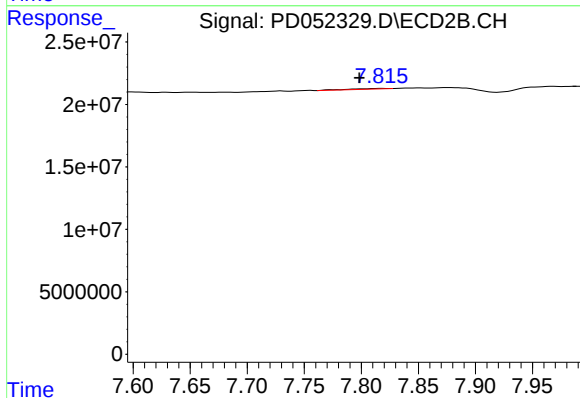


#21 Endrin ketone

R.T.: 7.817 min
Delta R.T.: 0.019 min
Response: 1295264
Conc: 0.06 ng/ml

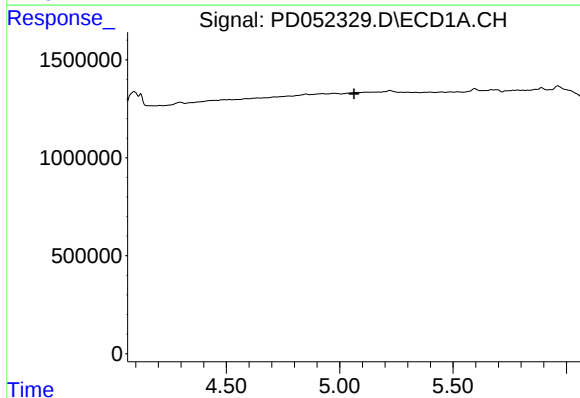


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.064 min
Response: 0
Conc: N.D.

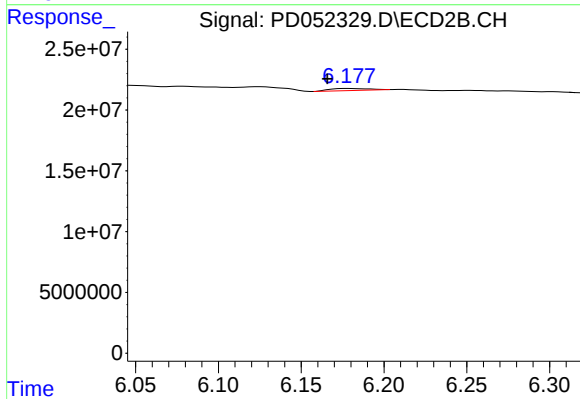

#25 Chlordane-3


R.T.: 6.179 min
Delta R.T.: 0.013 min
Response: 2771316
Conc: 0.63 ng/ml

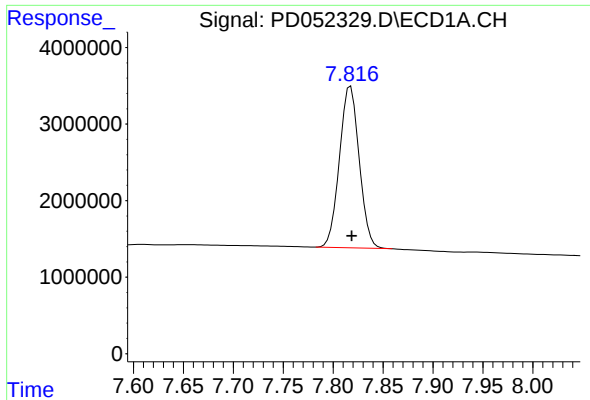

#28 Decachlorobiphenyl

R.T.: 7.818 min
Delta R.T.: -0.001 min
Response: 29025424
Conc: 21.78 ng/ml

Instrument :
ECD_D
ClientSampleId :

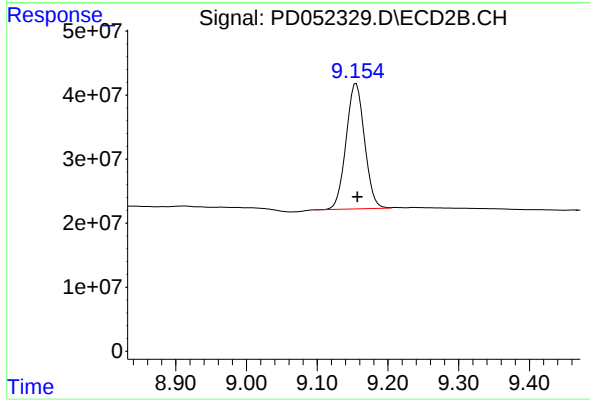

#28 Decachlorobiphenyl

R.T.: 9.155 min
Delta R.T.: -0.001 min
Response: 355025121
Conc: 22.83 ng/ml