

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032919\
 Data File : PD052330.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Mar 2019 21:06
 Operator : AJ\SJ
 Sample : MDL-BL-CHL-S-02
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MDL-BL-CHL-S-02

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 30 05:00:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 29 13:06:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.221	4.042	26766706	590.7E6	19.182	20.379
28)	SA Decachlor...	7.818	9.156	29267781	358.7E6	21.960	23.066
Target Compounds							
3)	MA gamma-BHC...	3.918	0.000	3400959	0	1.555	N.D. #
4)	MA Heptachlor	0.000	5.235	0	319817	N.D.	0.008 #
10)	B gamma-Chl...	0.000	6.176	0	1196136	N.D.	0.037 #
17)	MA 4,4'-DDT	0.000	7.203	0	1377706	N.D.	0.074 #
25)	Chlordane-3	0.000	6.176	0	1196136	N.D.	0.271 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032919\
Data File : PD052330.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Mar 2019 21:06
Operator : AJ\SJ
Sample : MDL-BL-CHL-S-02
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
MDL-BL-CHL-S-02

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 30 05:00:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
Quant Title : GC Extractables
QLast Update : Fri Mar 29 13:06:45 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

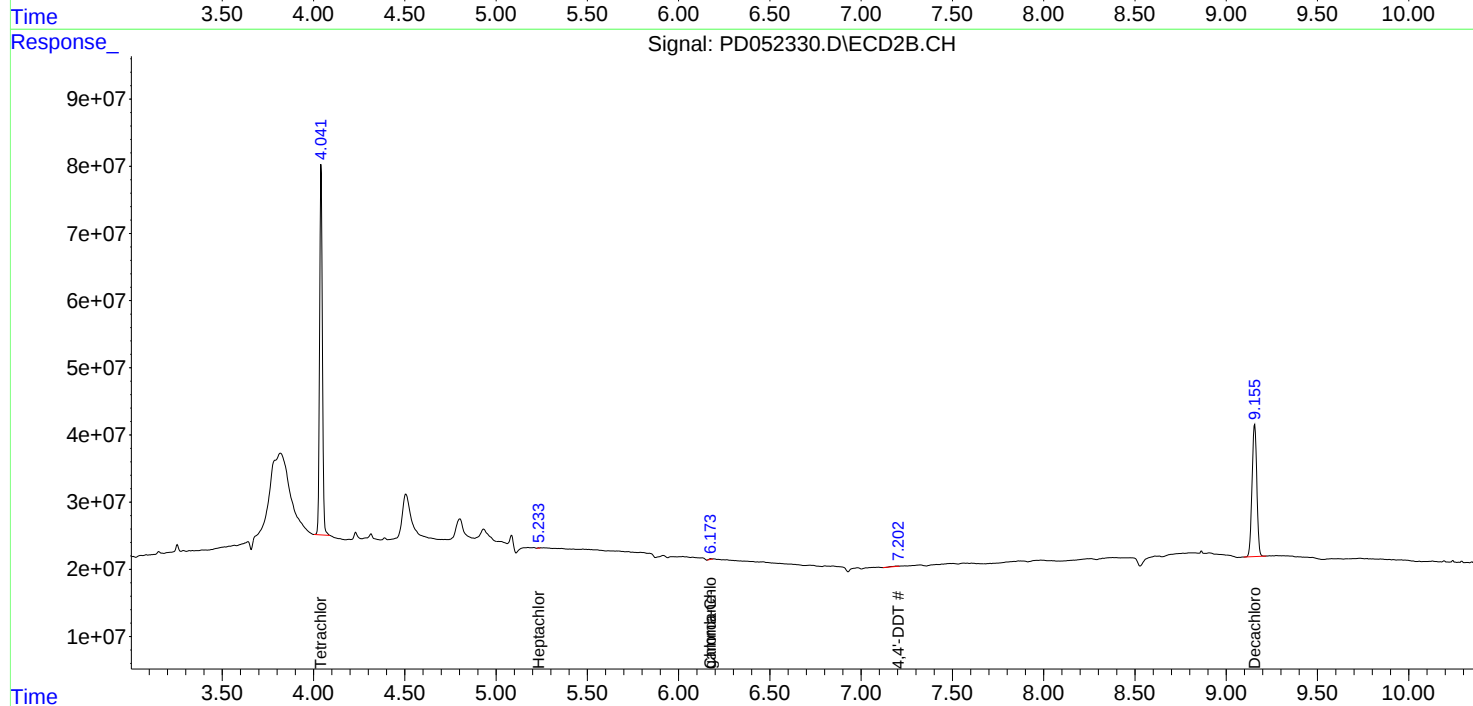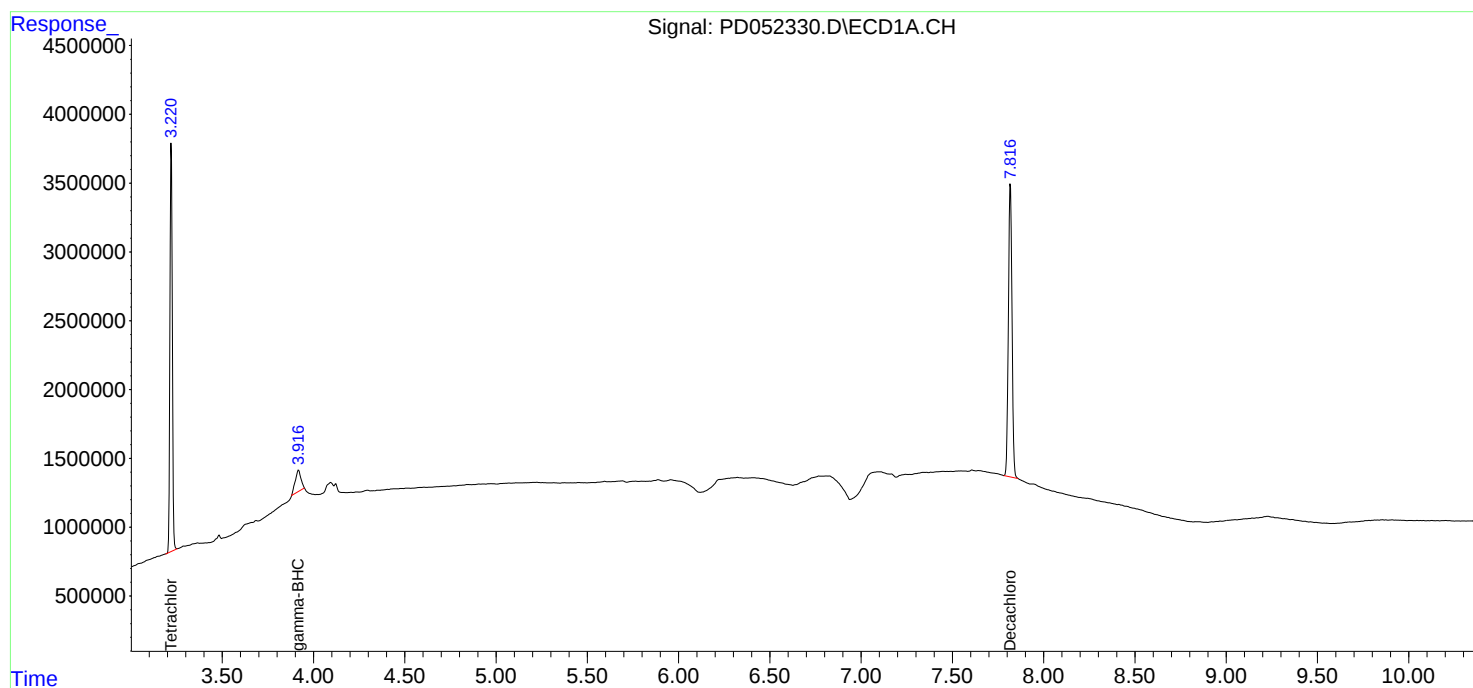


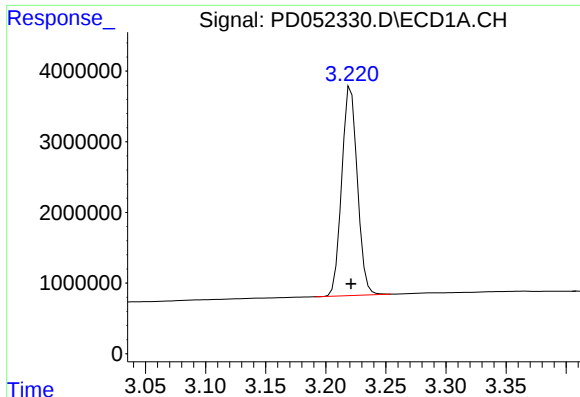

#1 Tetrachloro-m-xylene


R.T.: 3.221 min
Delta R.T.: 0.000 min
Response: 26766706
Conc: 19.18 ng/ml

Instrument :
ECD_D
ClientSampleId :
MDL-BL-CHL-S-02

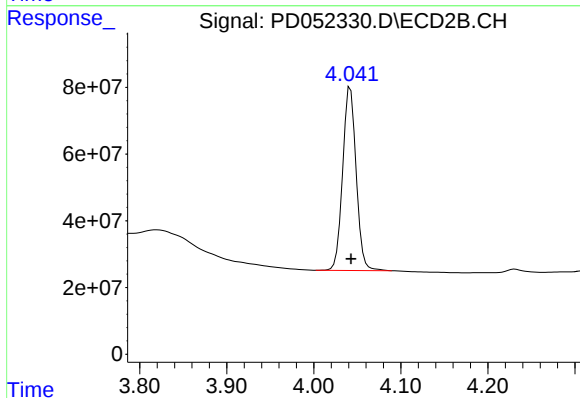


#1 Tetrachloro-m-xylene

R.T.: 4.042 min
Delta R.T.: 0.000 min
Response: 590672029
Conc: 20.38 ng/ml

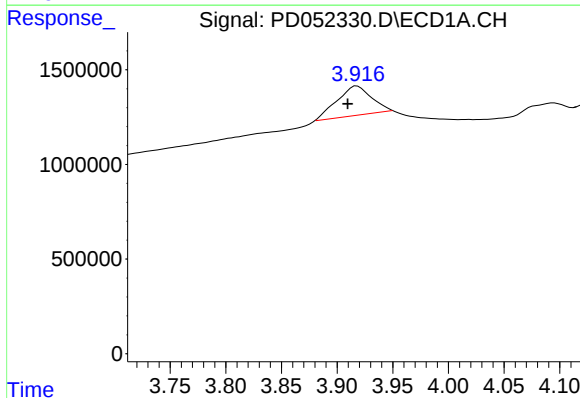


#3 gamma-BHC (Lindane)

R.T.: 3.918 min
Delta R.T.: 0.008 min
Response: 3400959
Conc: 1.56 ng/ml

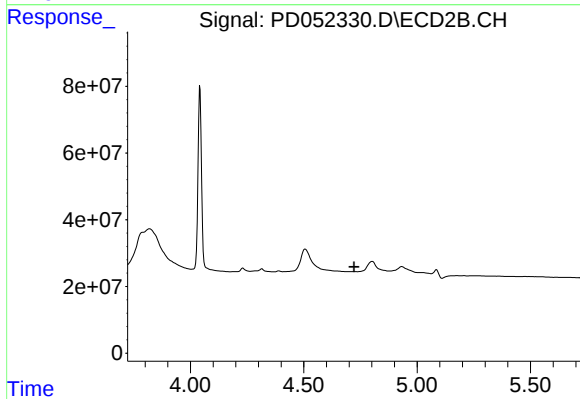

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.723 min
Response: 0
Conc: N.D.

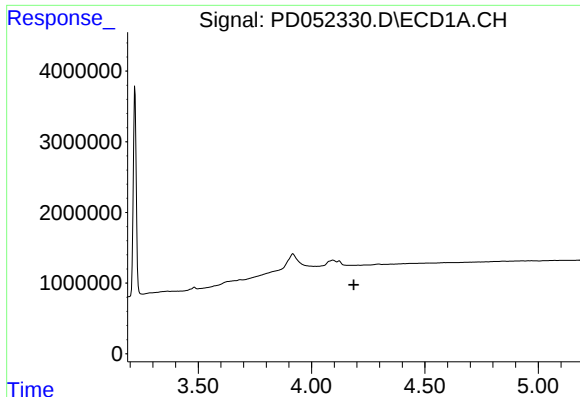

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.187 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
MDL-BL-CHL-S-02

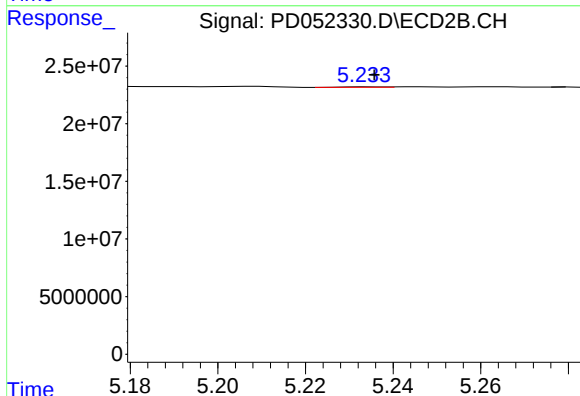


#4 Heptachlor

R.T.: 5.235 min
Delta R.T.: 0.000 min
Response: 319817
Conc: 0.01 ng/ml

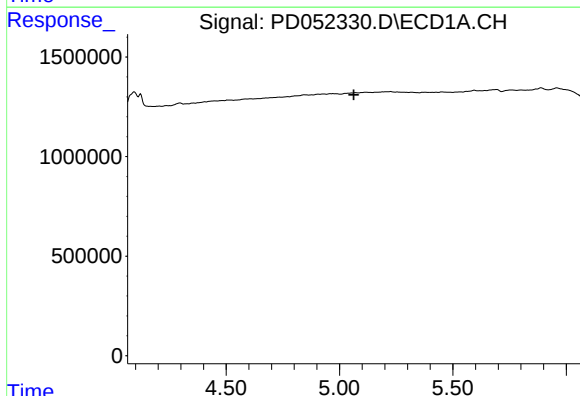


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.063 min
Response: 0
Conc: N.D.

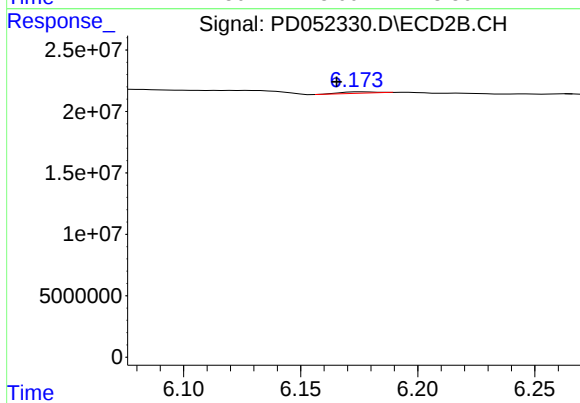

#10 gamma-Chlordane


R.T.: 6.176 min
Delta R.T.: 0.011 min
Response: 1196136
Conc: 0.04 ng/ml

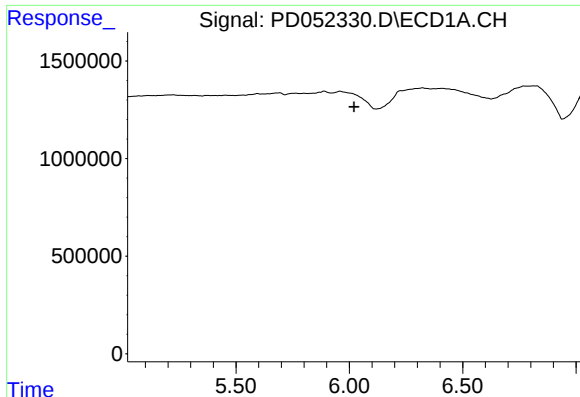

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.021 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
MDL-BL-CHL-S-02

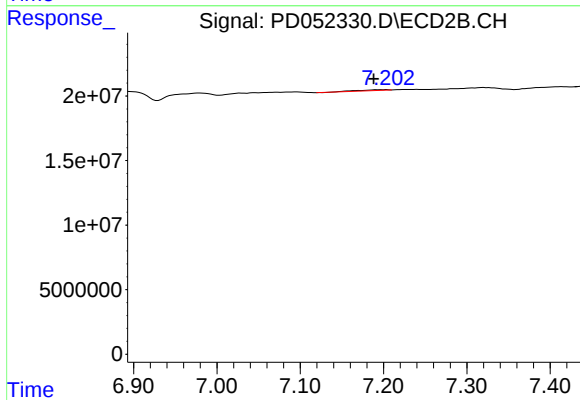


#17 4,4'-DDT

R.T.: 7.203 min
Delta R.T.: 0.015 min
Response: 1377706
Conc: 0.07 ng/ml

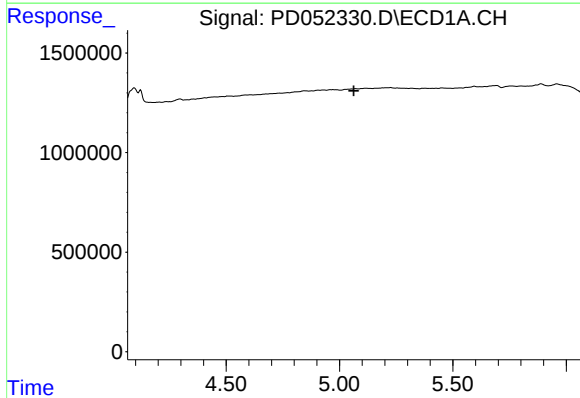


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.064 min
Response: 0
Conc: N.D.

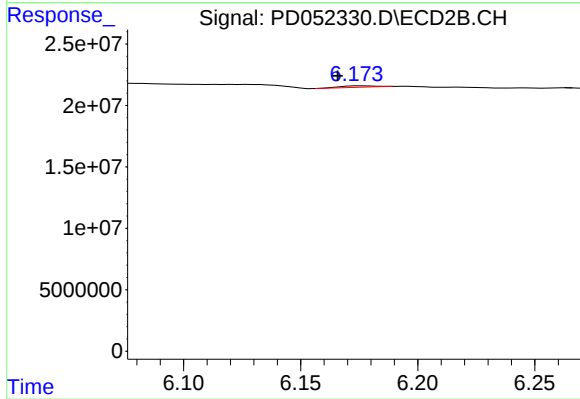

#25 Chlordane-3


R.T.: 6.176 min
Delta R.T.: 0.010 min
Response: 1196136
Conc: 0.27 ng/ml

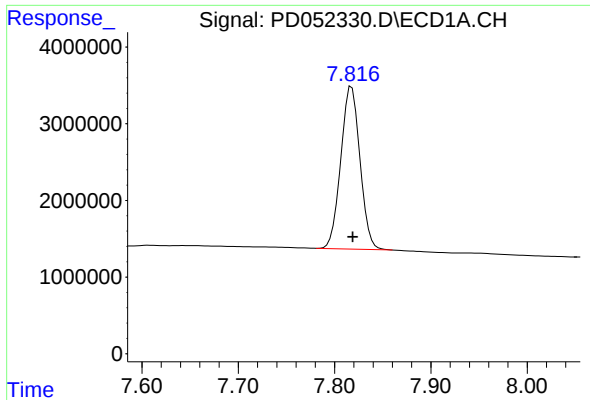

#28 Decachlorobiphenyl

R.T.: 7.818 min
Delta R.T.: 0.000 min
Response: 29267781
Conc: 21.96 ng/ml

Instrument :
ECD_D
ClientSampleId :
MDL-BL-CHL-S-02

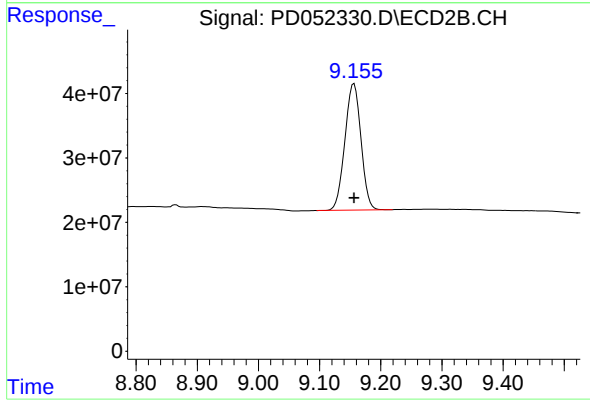

#28 Decachlorobiphenyl

R.T.: 9.156 min
Delta R.T.: 0.000 min
Response: 358702837
Conc: 23.07 ng/ml