

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032919\
 Data File : PD052337.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Mar 2019 22:45
 Operator : AJ\SJ
 Sample : MDL-BL-CHL-W-03
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MDL-BL-CHL-W-03

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 30 05:01:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 29 13:06:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.221	4.042	27400347	606.9E6	19.636	20.938
28)	SA Decachlor...	7.816	9.155	29694796	367.4E6	22.281	23.628
Target Compounds							
3)	MA gamma-BHC...	3.920	0.000	2918611	0	1.335	N.D. #
4)	MA Heptachlor	0.000	5.246	0	637843	N.D.	0.016 #
10)	B gamma-Chl...	0.000	6.183f	0	4772330	N.D.	0.149 #
17)	MA 4,4'-DDT	0.000	7.199	0	5173634	N.D.	0.278 #
25)	Chlordane-3	0.000	6.183f	0	4772330	N.D.	1.081 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032919\
Data File : PD052337.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Mar 2019 22:45
Operator : AJ\SJ
Sample : MDL-BL-CHL-W-03
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
MDL-BL-CHL-W-03

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 30 05:01:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
Quant Title : GC Extractables
QLast Update : Fri Mar 29 13:06:45 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

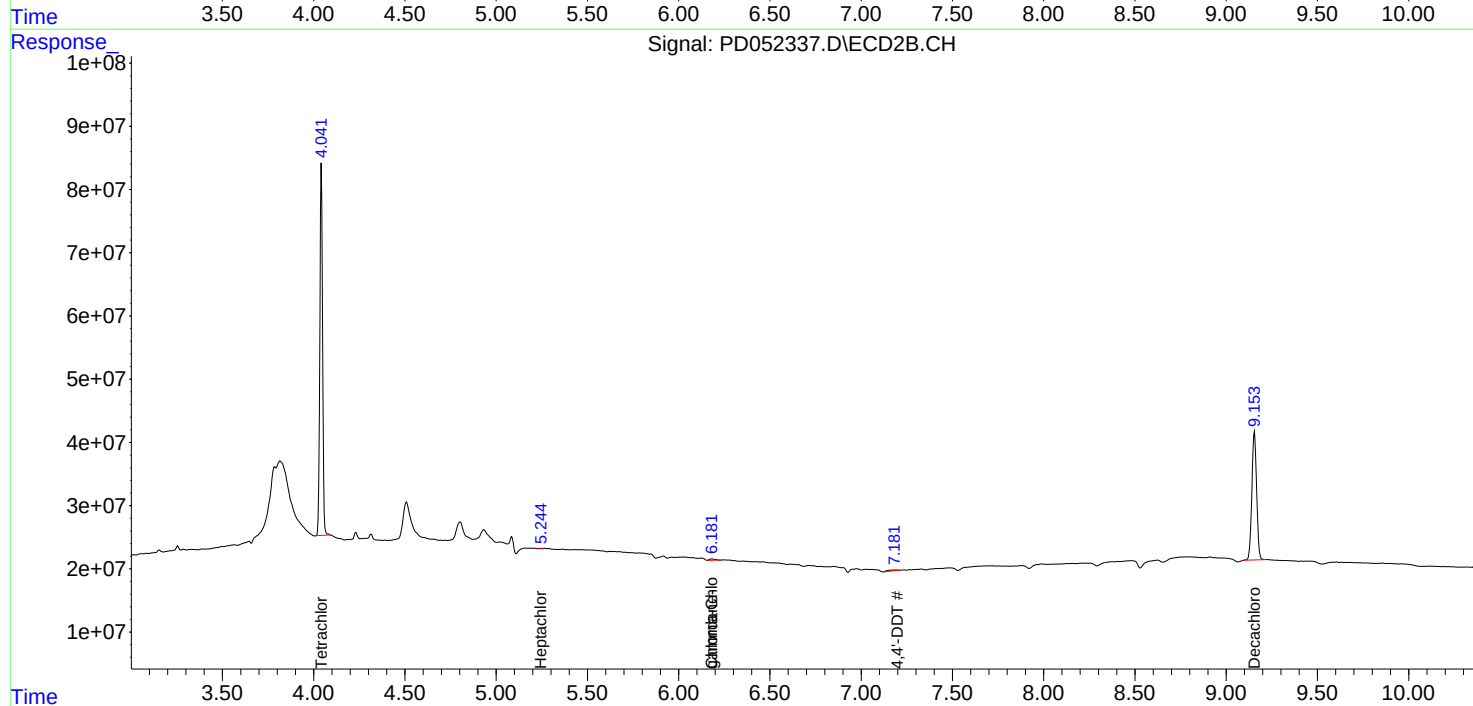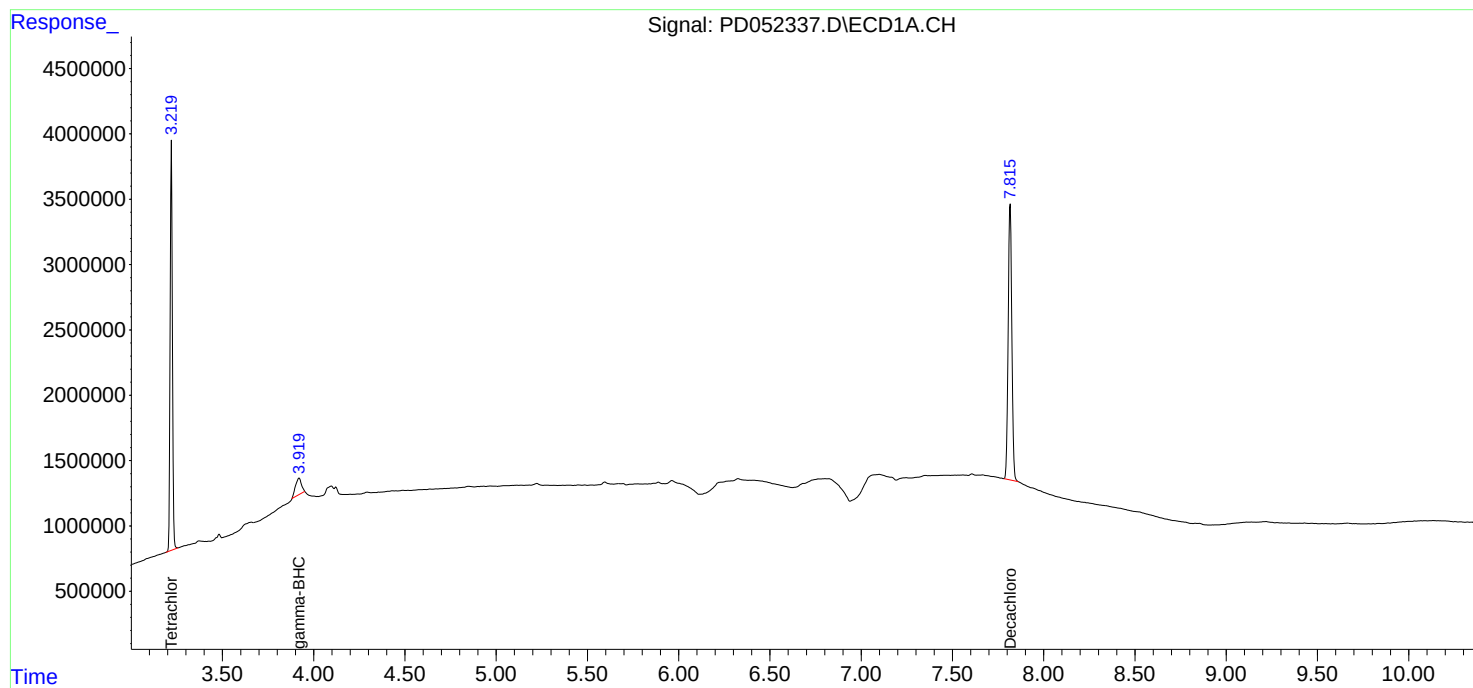


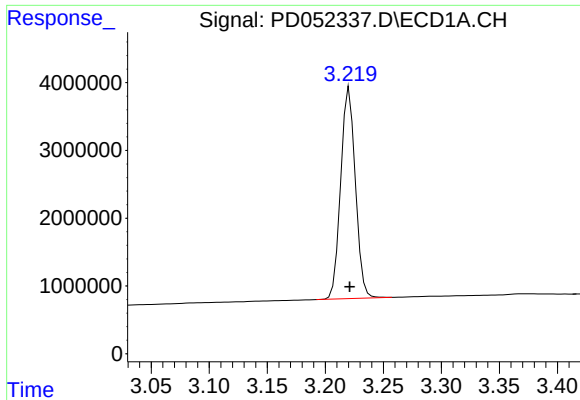

#1 Tetrachloro-m-xylene


R.T.: 3.221 min
Delta R.T.: 0.000 min
Response: 27400347
Conc: 19.64 ng/ml

Instrument :
ECD_D
ClientSampleId :
MDL-BL-CHL-W-03

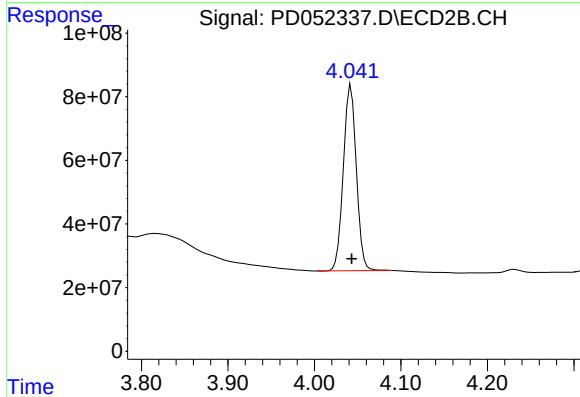


#1 Tetrachloro-m-xylene

R.T.: 4.042 min
Delta R.T.: 0.000 min
Response: 606865012
Conc: 20.94 ng/ml

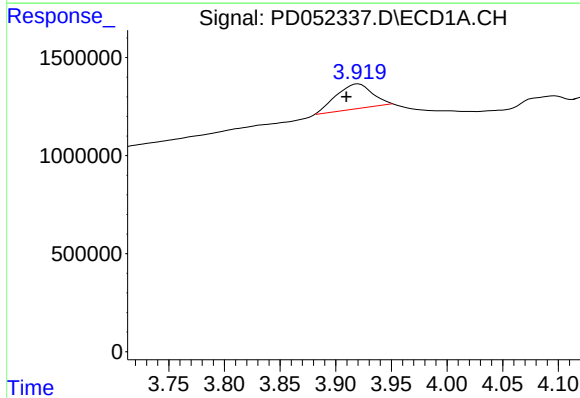


#3 gamma-BHC (Lindane)

R.T.: 3.920 min
Delta R.T.: 0.011 min
Response: 2918611
Conc: 1.33 ng/ml

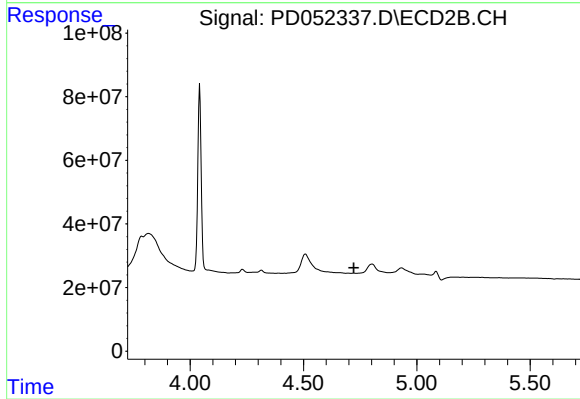

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.723 min
Response: 0
Conc: N.D.

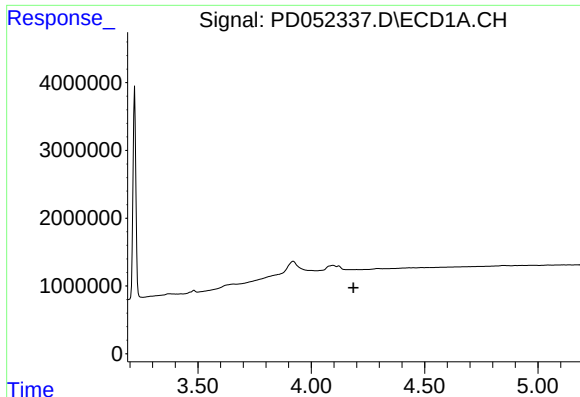

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.187 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
MDL-BL-CHL-W-03

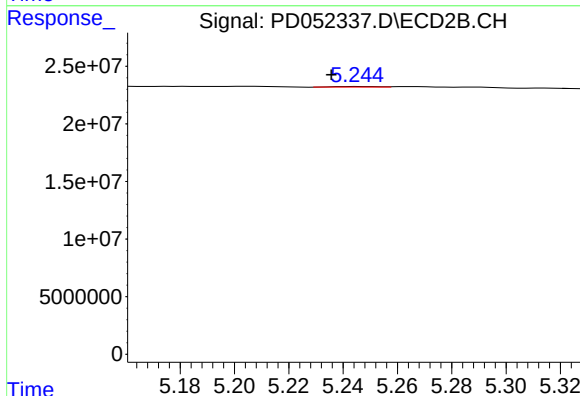


#4 Heptachlor

R.T.: 5.246 min
Delta R.T.: 0.010 min
Response: 637843
Conc: 0.02 ng/ml

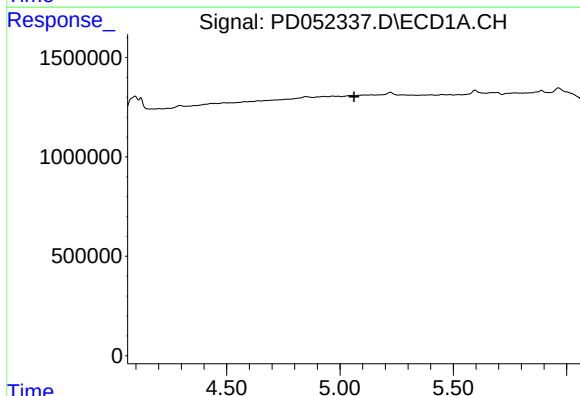


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.063 min
Response: 0
Conc: N.D.

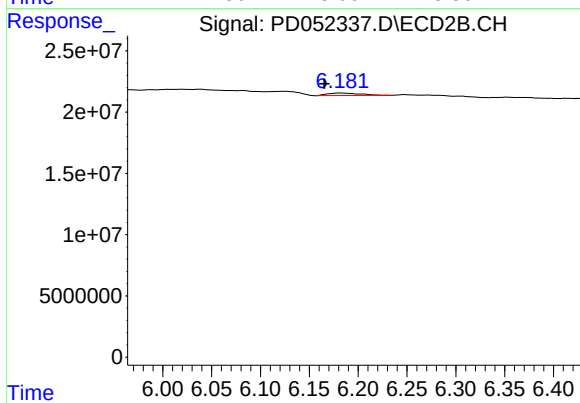

#10 gamma-Chlordane


R.T.: 6.183 min
Delta R.T.: 0.017 min
Response: 4772330
Conc: 0.15 ng/ml

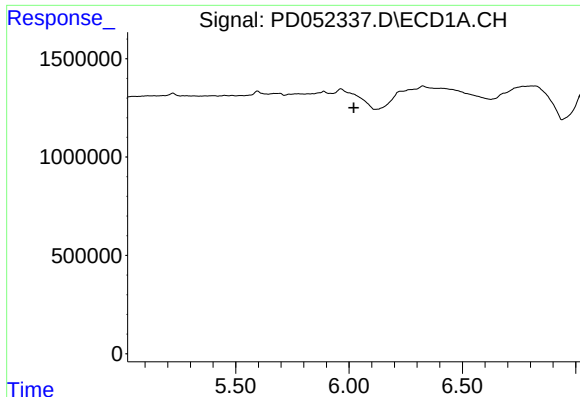

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.021 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
MDL-BL-CHL-W-03

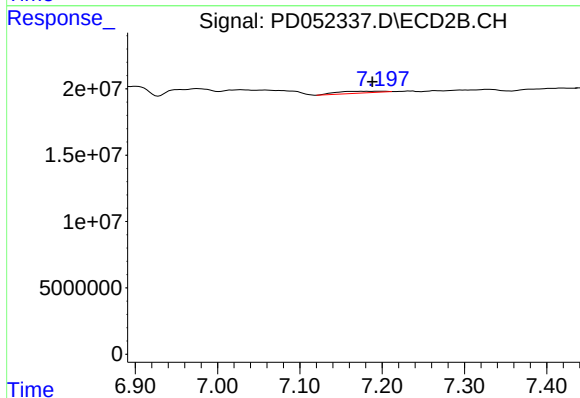


#17 4,4'-DDT

R.T.: 7.199 min
Delta R.T.: 0.011 min
Response: 5173634
Conc: 0.28 ng/ml

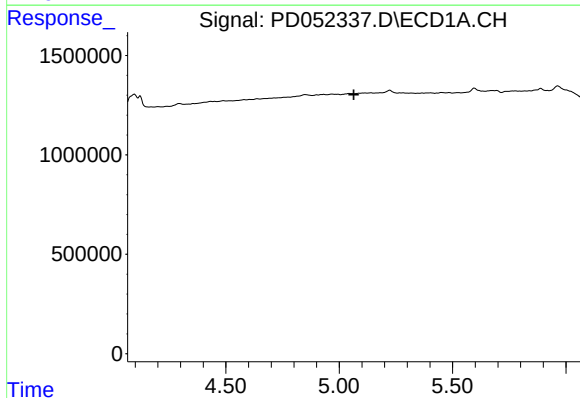


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.064 min
Response: 0
Conc: N.D.

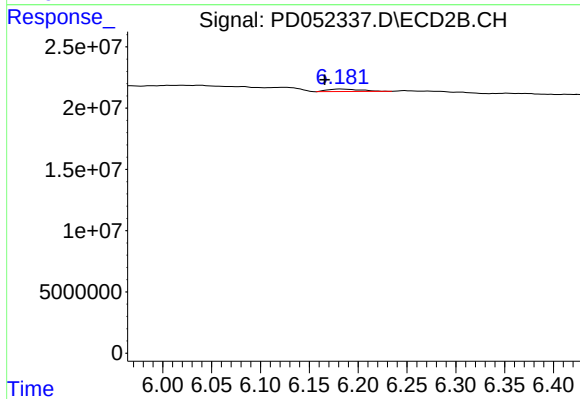

#25 Chlordane-3


R.T.: 6.183 min
Delta R.T.: 0.017 min
Response: 4772330
Conc: 1.08 ng/ml

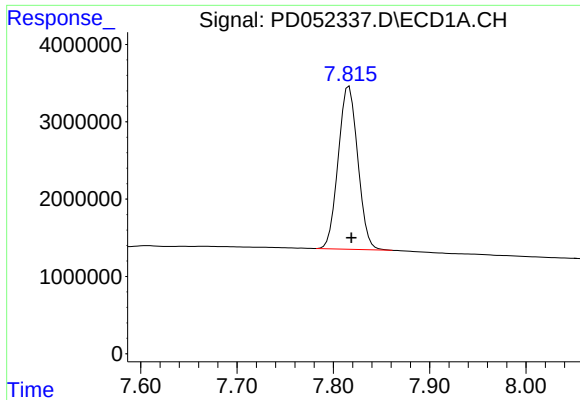

#28 Decachlorobiphenyl

R.T.: 7.816 min
Delta R.T.: -0.002 min
Response: 29694796
Conc: 22.28 ng/ml

Instrument :
ECD_D
ClientSampleId :
MDL-BL-CHL-W-03

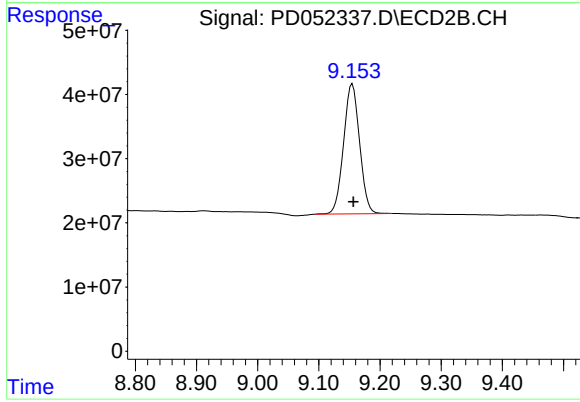

#28 Decachlorobiphenyl

R.T.: 9.155 min
Delta R.T.: -0.002 min
Response: 367443884
Conc: 23.63 ng/ml