

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032919\
 Data File : PD052338.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Mar 2019 23:00
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 30 05:01:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 29 13:06:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.221	4.042	28294047	636.3E6	20.276	21.952
28)	SA Decachlor...	7.816	9.155	30780161	378.1E6	23.095	24.315
Target Compounds							
3)	MA gamma-BHC...	3.924	0.000	2393428	0	1.095	N.D. #
8)	B Heptachlo...	0.000	5.923	0	79670004	N.D.	2.468 #
9)	A Endosulfan I	0.000	6.279	0	18839264	N.D.	0.645 #
10)	B gamma-Chl...	0.000	6.165	0	89326684	N.D.	2.792 #
11)	B alpha-Chl...	0.000	6.239	0	8527746	N.D.	0.272 #
25)	Chlordane-3	0.000	6.165	0	89326684	N.D.	20.243 #
26)	Chlordane-4	0.000	6.239	0	8527746	N.D.	1.677 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032919\
Data File : PD052338.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Mar 2019 23:00
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 30 05:01:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
Quant Title : GC Extractables
QLast Update : Fri Mar 29 13:06:45 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

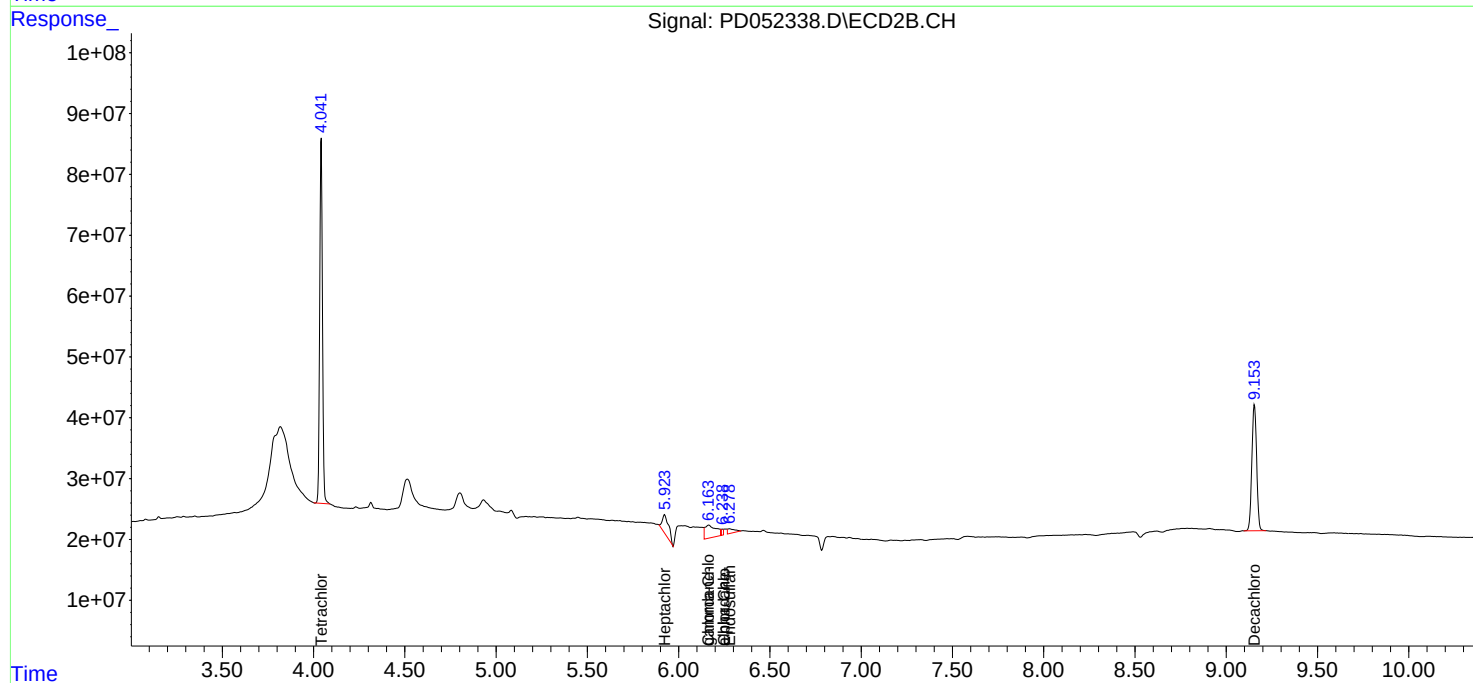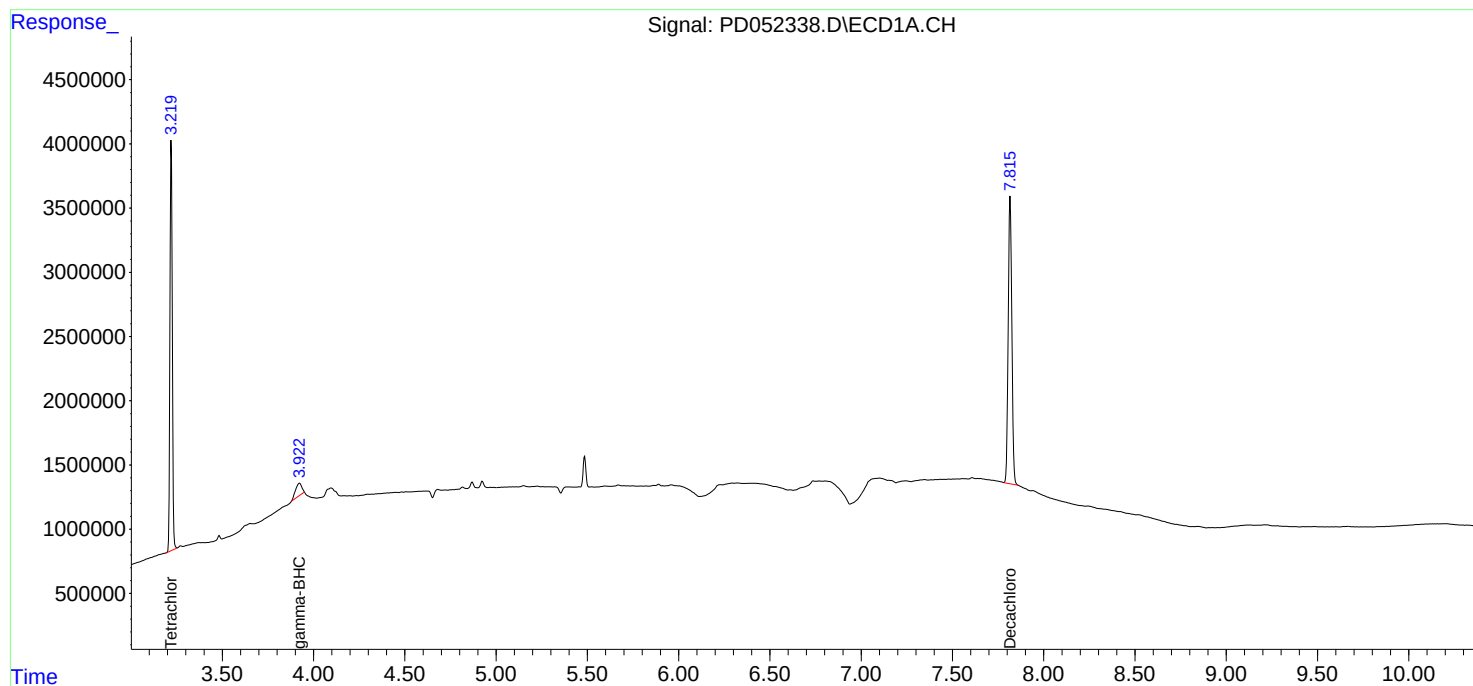


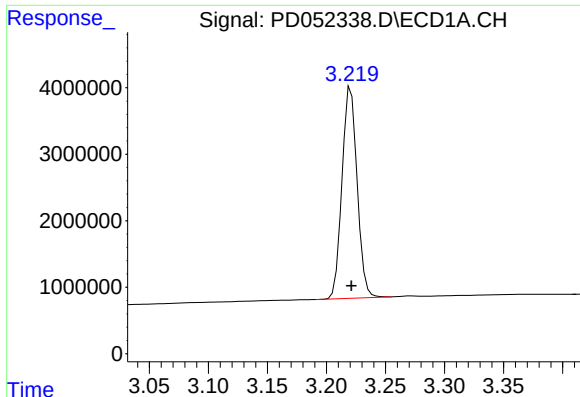

#1 Tetrachloro-m-xylene


R.T.: 3.221 min
Delta R.T.: 0.000 min
Response: 28294047
Conc: 20.28 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

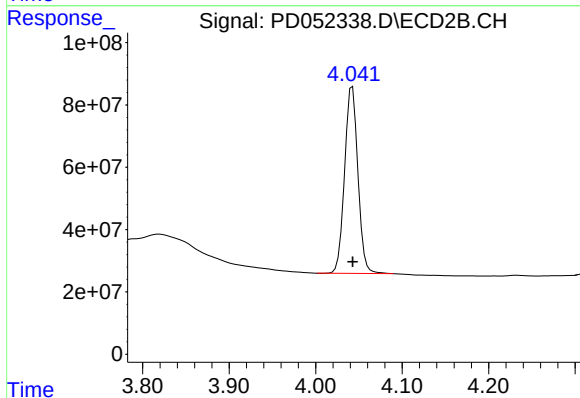


#1 Tetrachloro-m-xylene

R.T.: 4.042 min
Delta R.T.: 0.000 min
Response: 636259169
Conc: 21.95 ng/ml

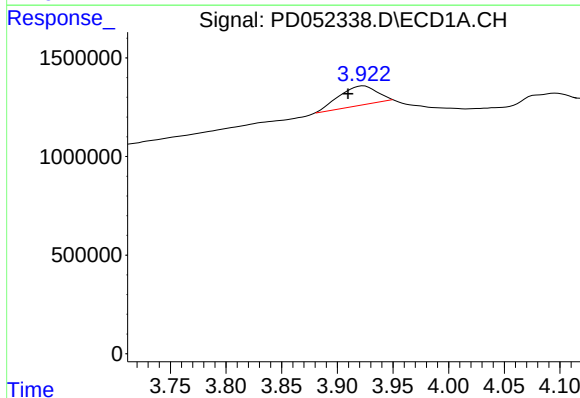


#3 gamma-BHC (Lindane)

R.T.: 3.924 min
Delta R.T.: 0.014 min
Response: 2393428
Conc: 1.09 ng/ml

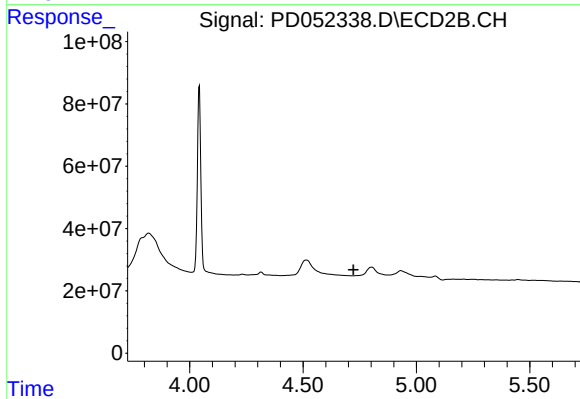

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.723 min
Response: 0
Conc: N.D.

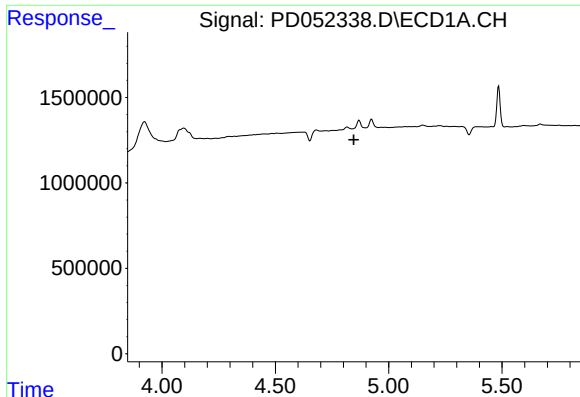

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.846 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

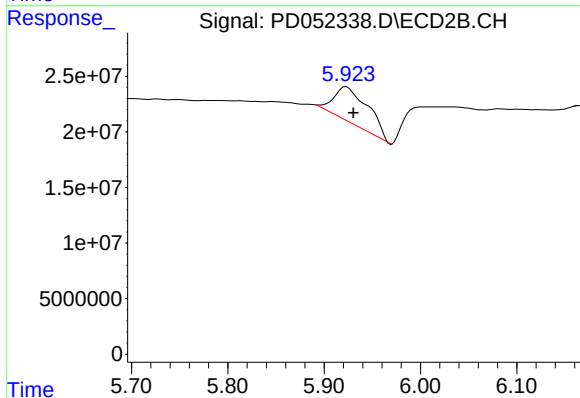


#8 Heptachlor epoxide

R.T.: 5.923 min
Delta R.T.: -0.007 min
Response: 79670004
Conc: 2.47 ng/ml

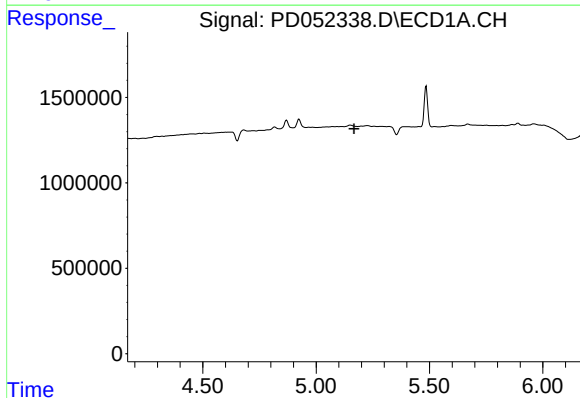


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.167 min
Response: 0
Conc: N.D.

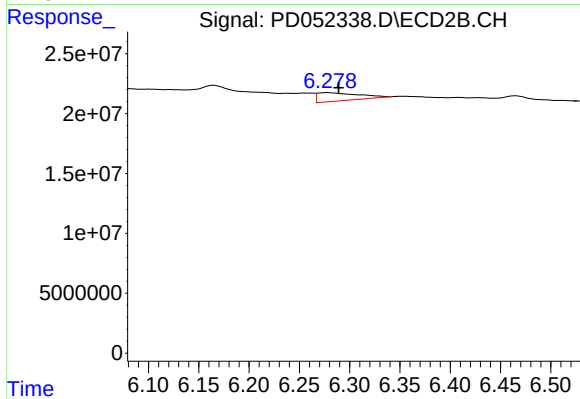

#9 Endosulfan I


R.T.: 6.279 min
Delta R.T.: -0.010 min
Response: 18839264
Conc: 0.64 ng/ml

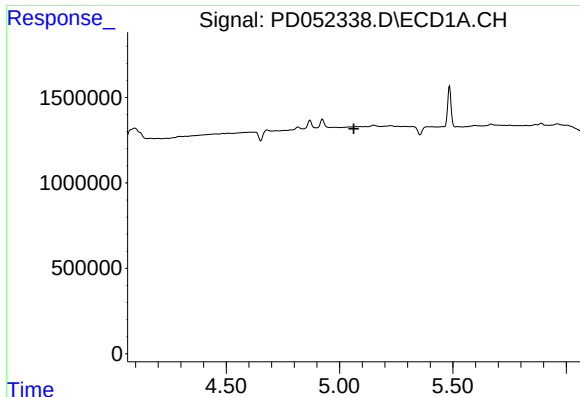

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.063 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

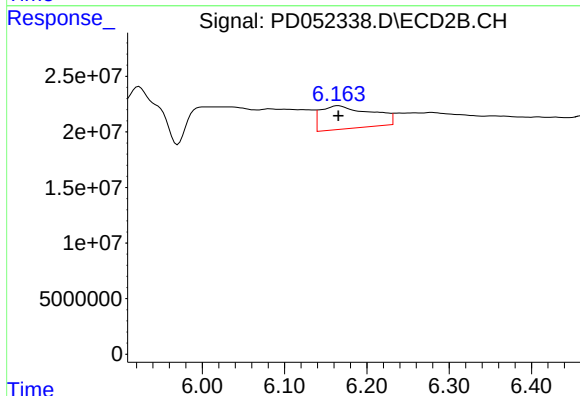


#10 gamma-Chlordane

R.T.: 6.165 min
Delta R.T.: 0.000 min
Response: 89326684
Conc: 2.79 ng/ml

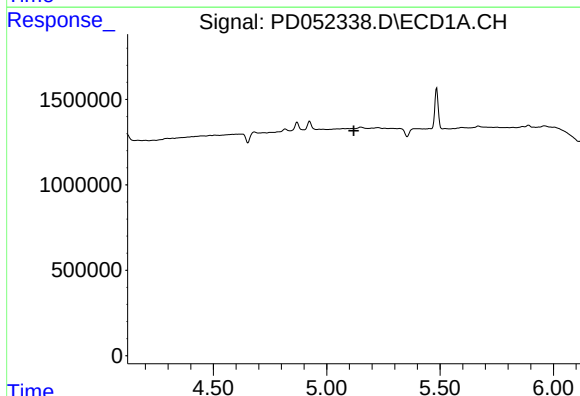


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.119 min
Response: 0
Conc: N.D.

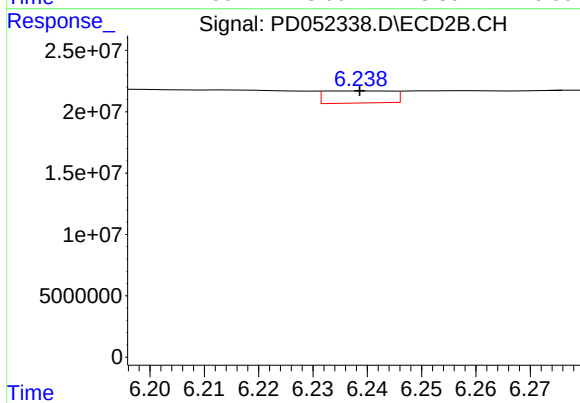

#11 alpha-Chlordane


R.T.: 6.239 min
Delta R.T.: 0.000 min
Response: 8527746
Conc: 0.27 ng/ml

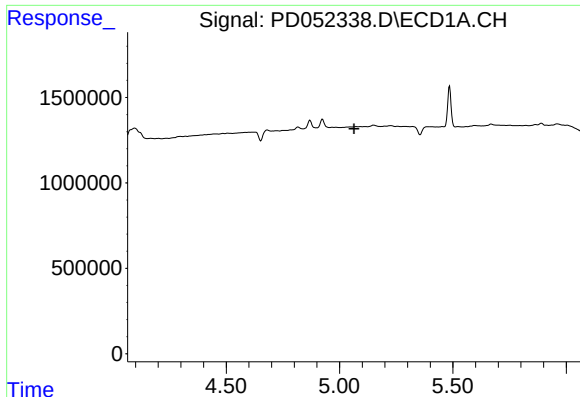

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.064 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

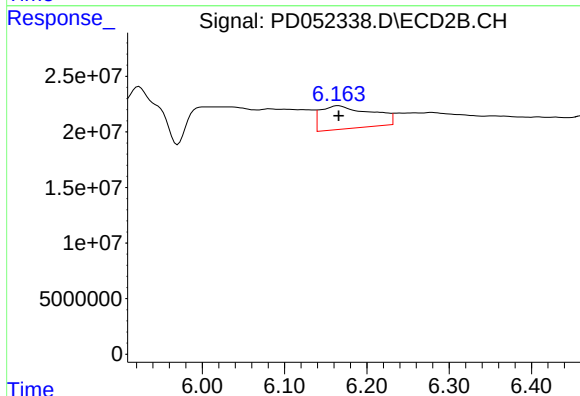


#25 Chlordane-3

R.T.: 6.165 min
Delta R.T.: 0.000 min
Response: 89326684
Conc: 20.24 ng/ml

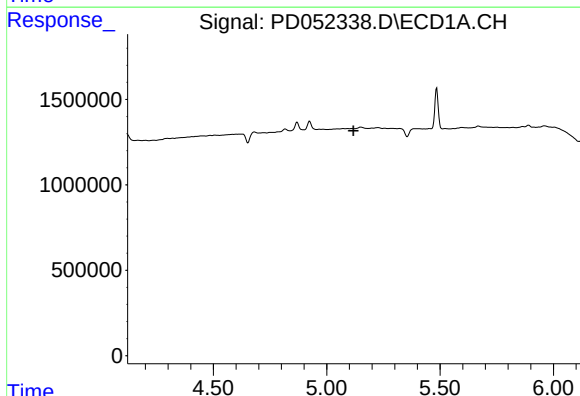


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.118 min
Response: 0
Conc: N.D.

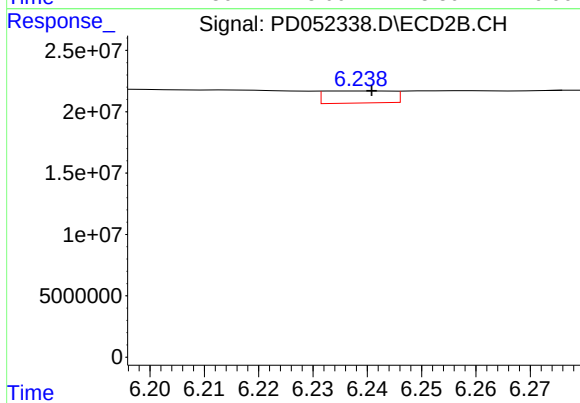

#26 Chlordane-4


R.T.: 6.239 min
Delta R.T.: -0.001 min
Response: 8527746
Conc: 1.68 ng/ml

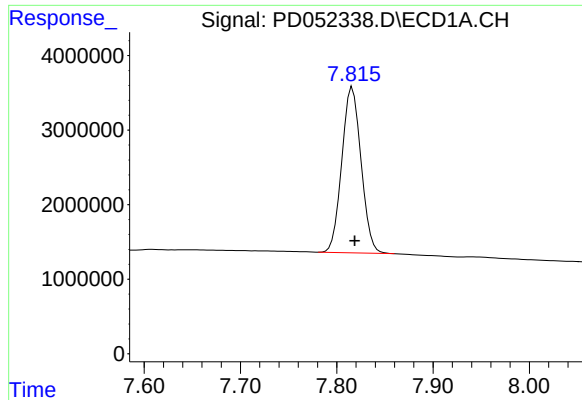

#28 Decachlorobiphenyl

R.T.: 7.816 min
Delta R.T.: -0.002 min
Response: 30780161
Conc: 23.10 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

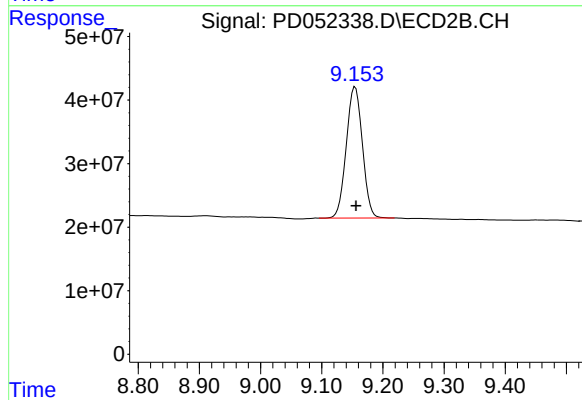

#28 Decachlorobiphenyl

R.T.: 9.155 min
Delta R.T.: -0.002 min
Response: 378130067
Conc: 24.31 ng/ml