

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032919\
 Data File : PD052293.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Mar 2019 12:26
 Operator : AJ\SJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 13:03:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 29 13:01:48 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.222	4.043	35132898	753.2E6	23.901	26.277
28)	SA Decachlor...	7.818	9.157	34816537	398.9E6	25.512	25.589
Target Compounds							
23)	Chlordane-1	4.043	5.046	15339614	389.3E6	241.467	261.365
24)	Chlordane-2	4.523	5.516	18326975	363.0E6	248.640	269.285
25)	Chlordane-3	5.064	6.166	52388479	1116.1E6	234.559	261.524
26)	Chlordane-4	5.118	6.240	50693218	1283.5E6	236.844	262.216
27)	Chlordane-5	5.923	7.050	16166274	231.1E6	239.089	246.934



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032919\
Data File : PD052293.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Mar 2019 12:26
Operator : AJ\SJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 13:03:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
Quant Title : GC Extractables
QLast Update : Fri Mar 29 13:01:48 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

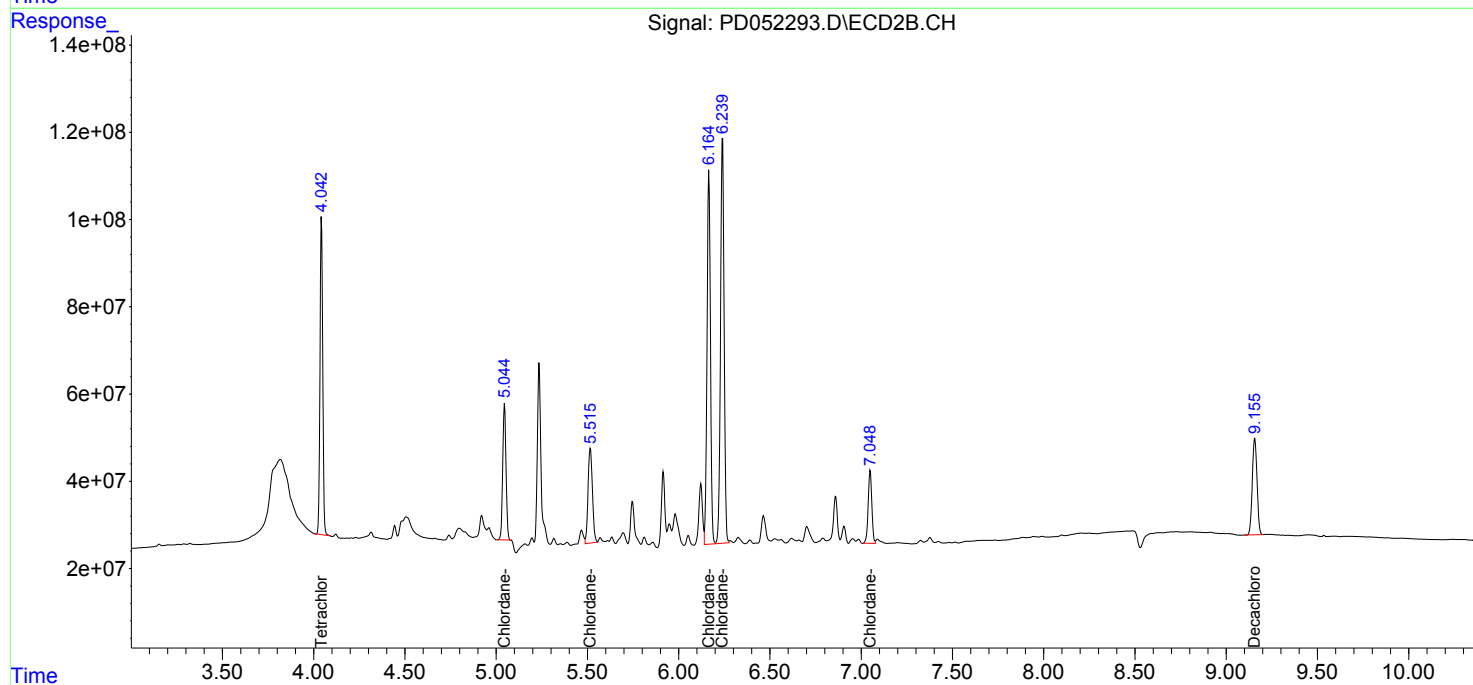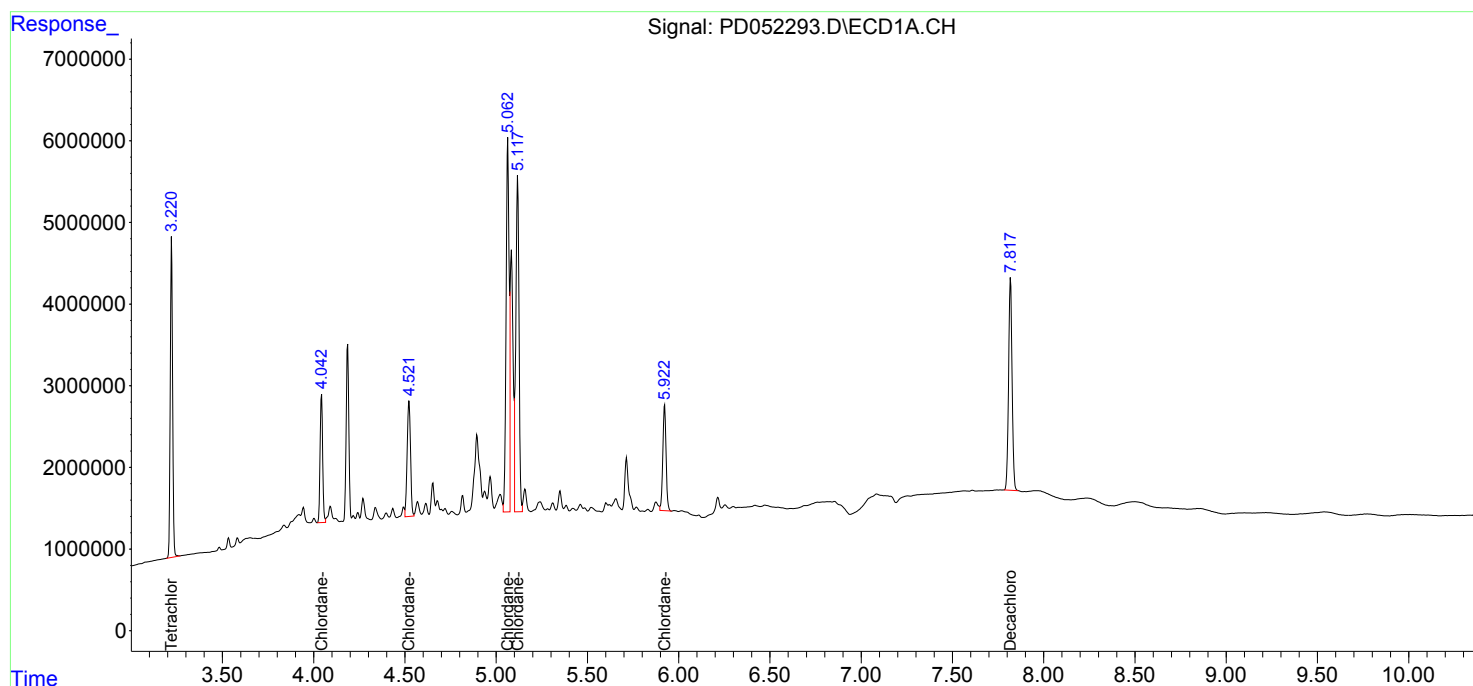


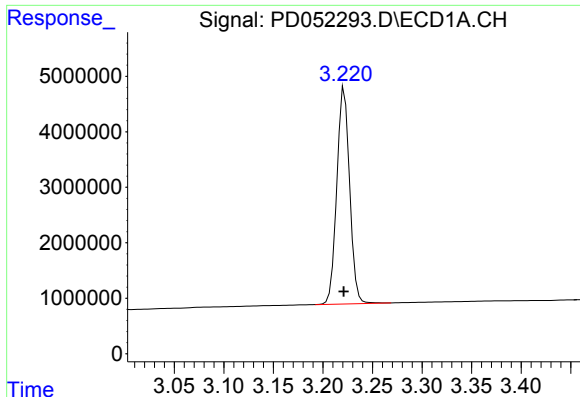

#1 Tetrachloro-m-xylene


R.T.: 3.222 min
Delta R.T.: 0.000 min
Response: 35132898
Conc: 23.90 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

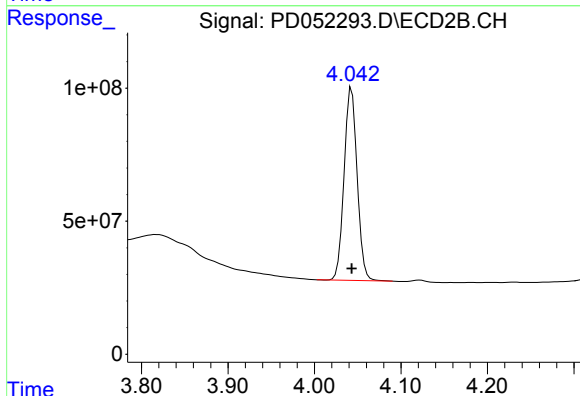


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 753187263
Conc: 26.28 ng/ml

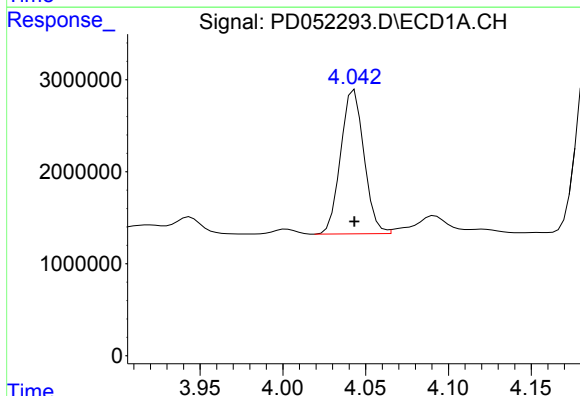


#23 Chlordane-1

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 15339614
Conc: 241.47 ng/ml

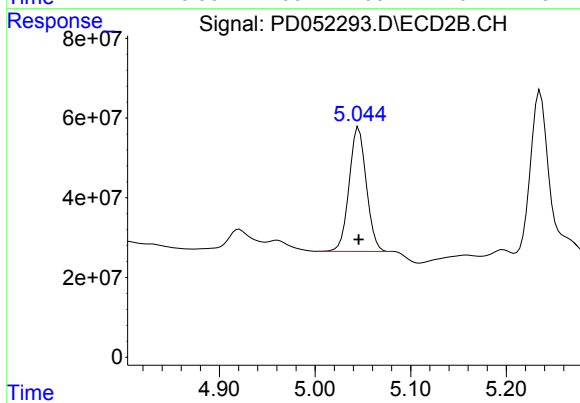

#23 Chlordane-1


R.T.: 5.046 min
Delta R.T.: 0.000 min
Response: 389311955
Conc: 261.37 ng/ml

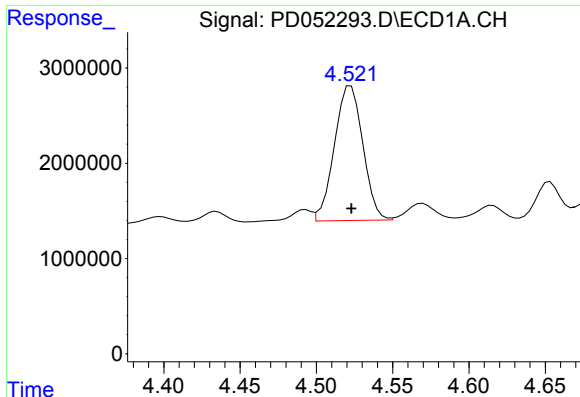

#24 Chlordane-2


R.T.: 4.523 min
Delta R.T.: 0.000 min
Response: 18326975
Conc: 248.64 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

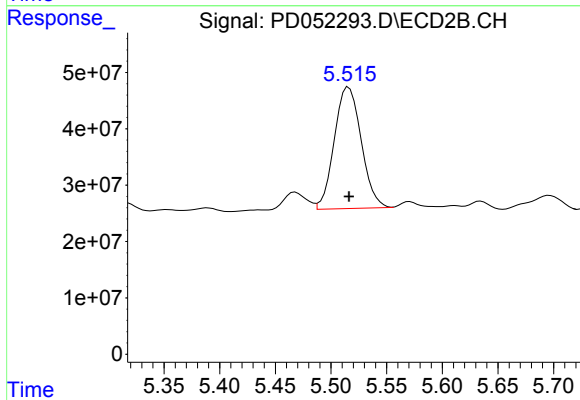


#24 Chlordane-2

R.T.: 5.516 min
Delta R.T.: 0.000 min
Response: 362984711
Conc: 269.29 ng/ml

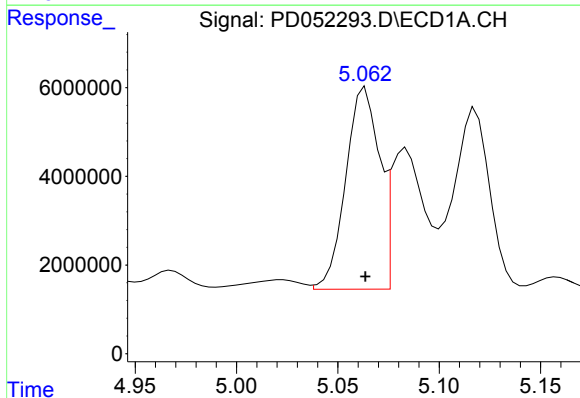


#25 Chlordane-3

R.T.: 5.064 min
Delta R.T.: 0.000 min
Response: 52388479
Conc: 234.56 ng/ml

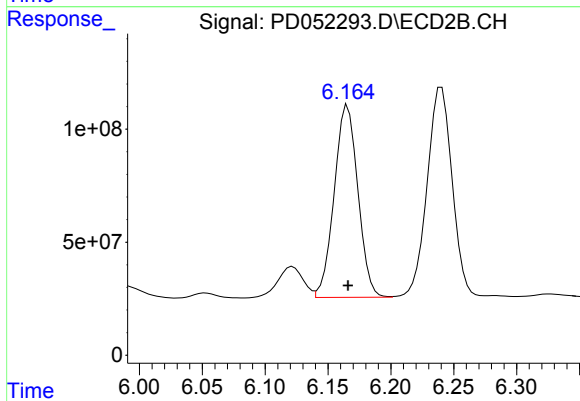

#25 Chlordane-3


R.T.: 6.166 min
Delta R.T.: 0.000 min
Response: 1116092251
Conc: 261.52 ng/ml

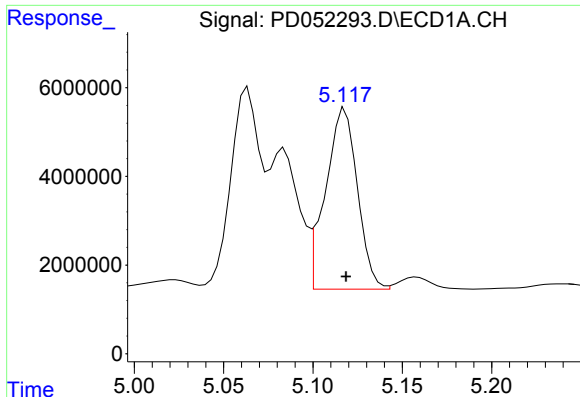

#26 Chlordane-4


R.T.: 5.118 min
Delta R.T.: 0.000 min
Response: 50693218
Conc: 236.84 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

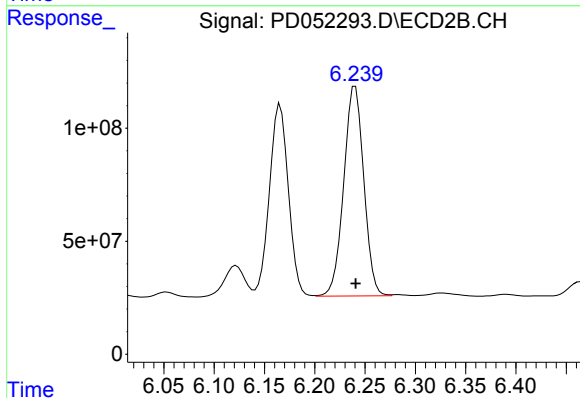


#26 Chlordane-4

R.T.: 6.240 min
Delta R.T.: 0.000 min
Response: 1283452566
Conc: 262.22 ng/ml

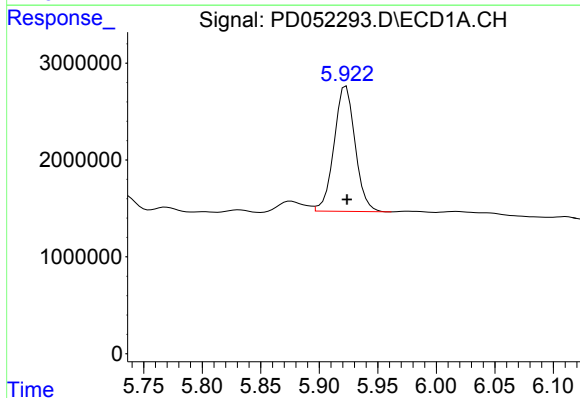


#27 Chlordane-5

R.T.: 5.923 min
Delta R.T.: 0.000 min
Response: 16166274
Conc: 239.09 ng/ml

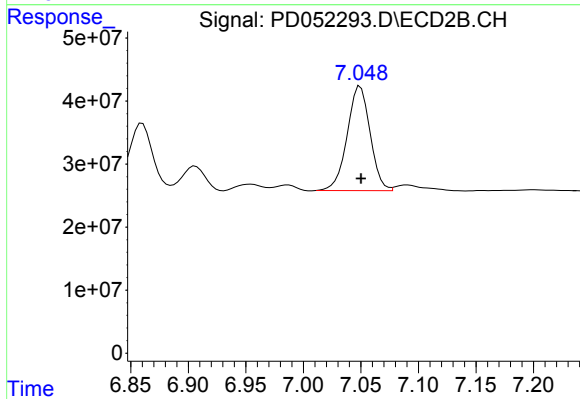

#27 Chlordane-5


R.T.: 7.050 min
Delta R.T.: 0.000 min
Response: 231060716
Conc: 246.93 ng/ml

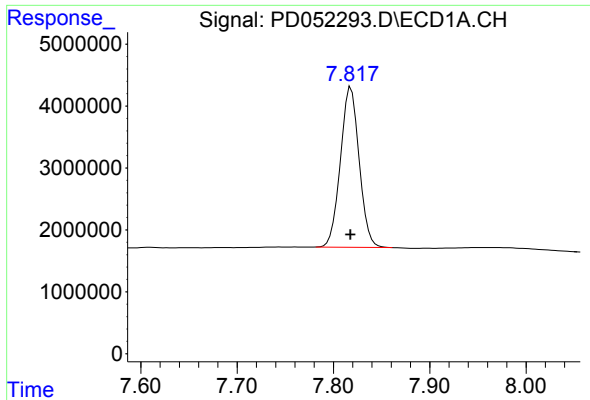

#28 Decachlorobiphenyl

R.T.: 7.818 min
Delta R.T.: 0.000 min
Response: 34816537
Conc: 25.51 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

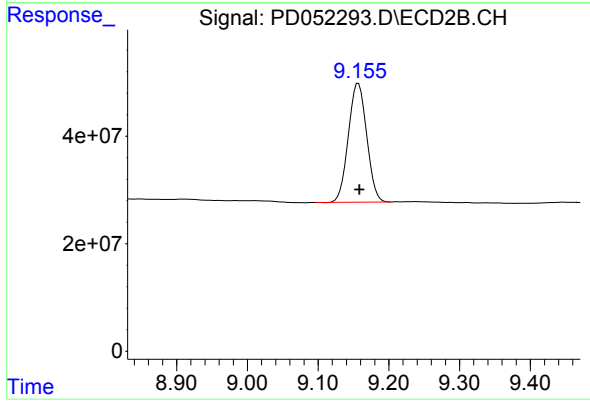

#28 Decachlorobiphenyl

R.T.: 9.157 min
Delta R.T.: -0.002 min
Response: 398943415
Conc: 25.59 ng/ml