

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032919\
 Data File : PD052301.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Mar 2019 14:18
 Operator : AJ\SJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD032919CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 14:59:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 29 13:06:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.221	4.043	70081287	1366.7E6	50.222	47.152
28)	SA Decachlor...	7.819	9.157	67001321	771.8E6	50.273	49.629
Target Compounds							
23)	Chlordane-1	4.044	5.046	30516596	716.8E6	485.980	467.268
24)	Chlordane-2	4.523	5.516	35643759	654.2E6	478.979	467.132
25)	Chlordane-3	5.064	6.166	109.0E6	2112.4E6	492.879	478.706
26)	Chlordane-4	5.119	6.240	104.2E6	2419.9E6	491.494	475.877
27)	Chlordane-5	5.923	7.050	32507531	462.6E6	499.862	501.376



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032919\
Data File : PD052301.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Mar 2019 14:18
Operator : AJ\SJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD032919CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 14:59:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
Quant Title : GC Extractables
QLast Update : Fri Mar 29 13:06:45 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

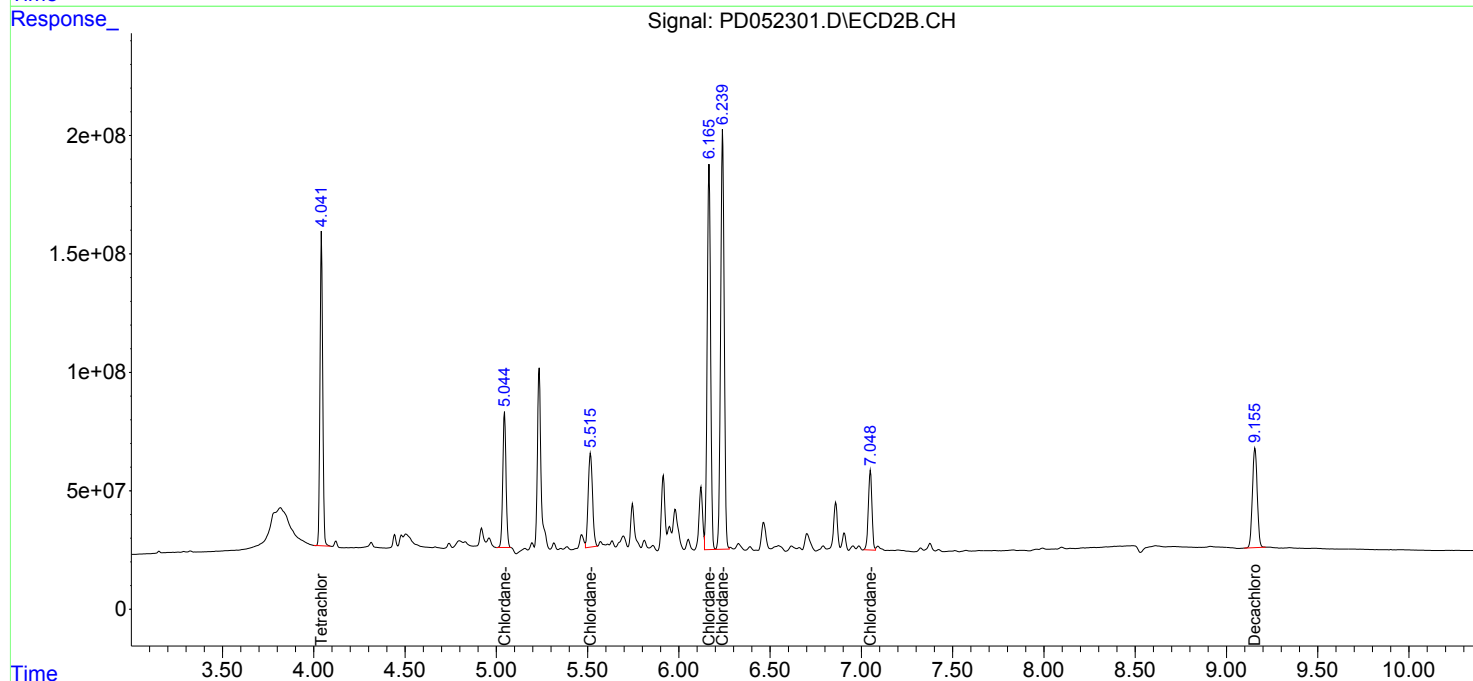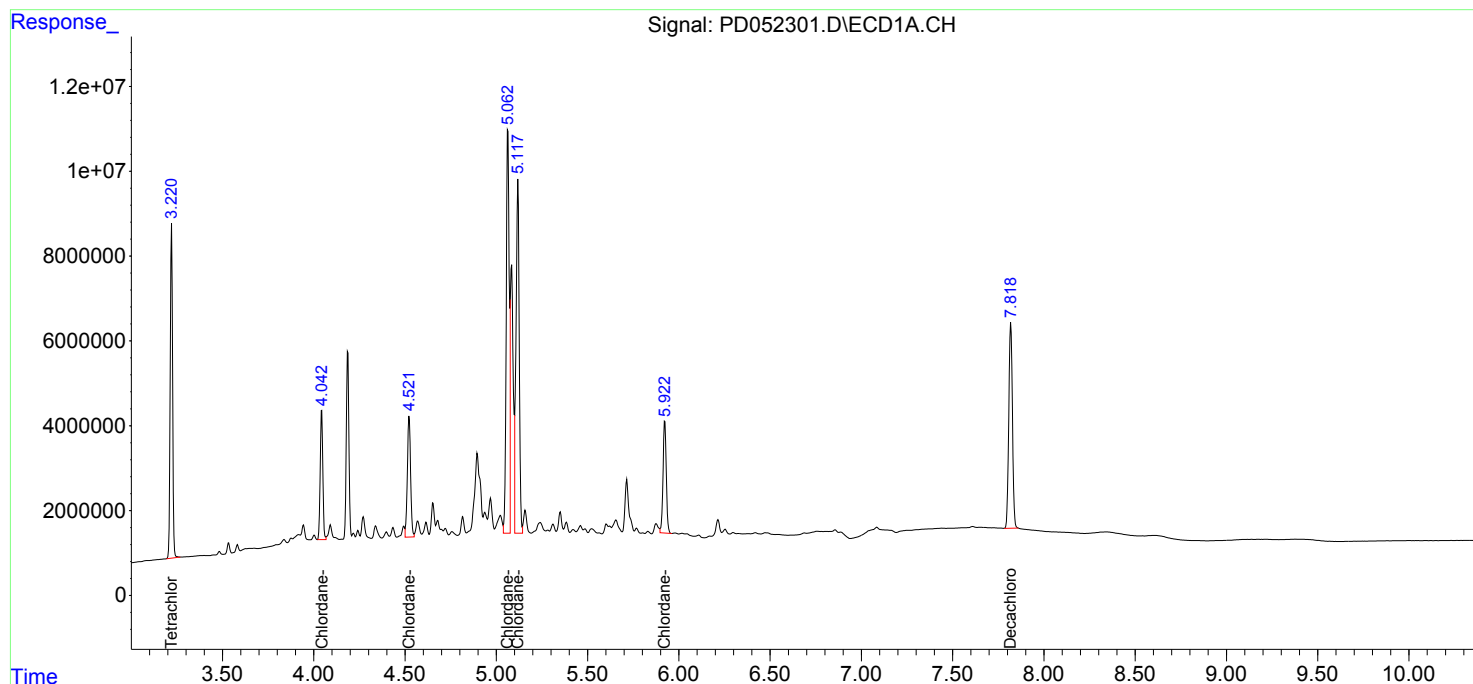


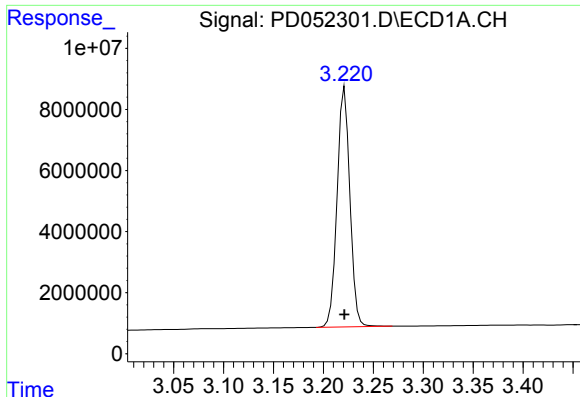

#1 Tetrachloro-m-xylene


R.T.: 3.221 min
Delta R.T.: 0.000 min
Response: 70081287
Conc: 50.22 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD032919CHLOR

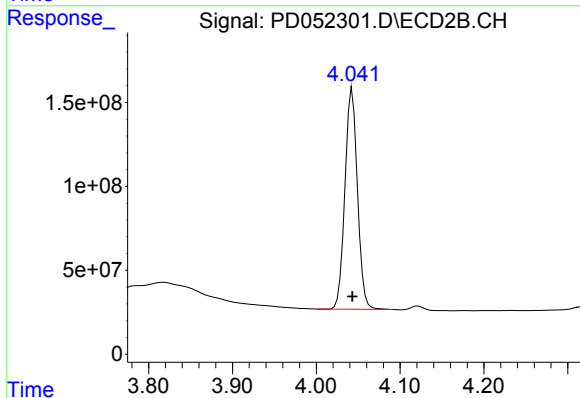


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 1366652202
Conc: 47.15 ng/ml

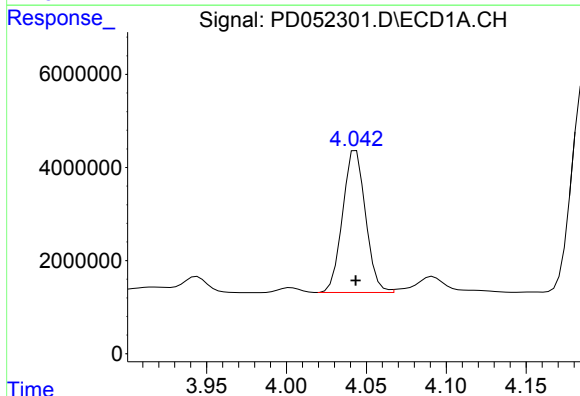


#23 Chlordane-1

R.T.: 4.044 min
Delta R.T.: 0.000 min
Response: 30516596
Conc: 485.98 ng/ml

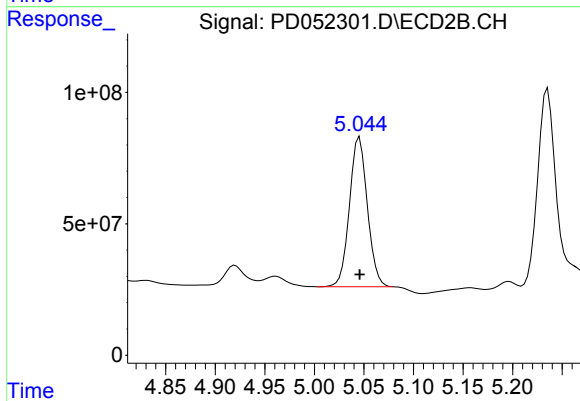

#23 Chlordane-1


R.T.: 5.046 min
Delta R.T.: 0.000 min
Response: 716834789
Conc: 467.27 ng/ml

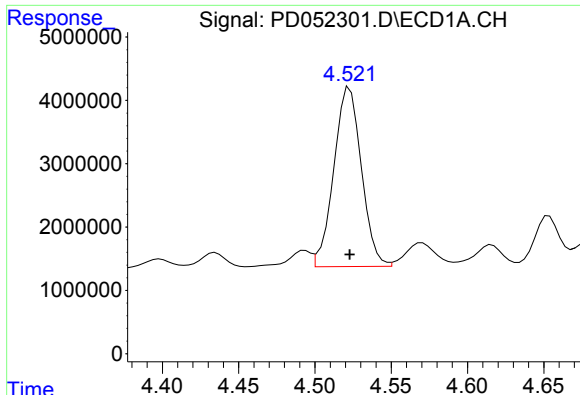

#24 Chlordane-2


R.T.: 4.523 min
Delta R.T.: 0.000 min
Response: 35643759
Conc: 478.98 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD032919CHLOR

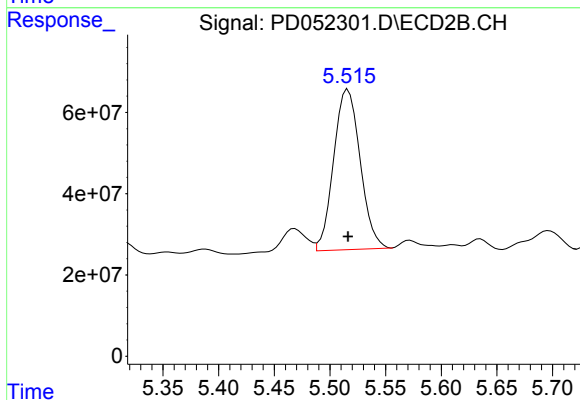


#24 Chlordane-2

R.T.: 5.516 min
Delta R.T.: 0.000 min
Response: 654203794
Conc: 467.13 ng/ml

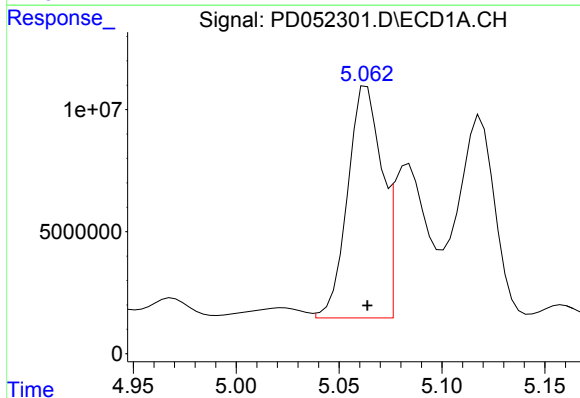


#25 Chlordane-3

R.T.: 5.064 min
Delta R.T.: 0.000 min
Response: 108993911
Conc: 492.88 ng/ml

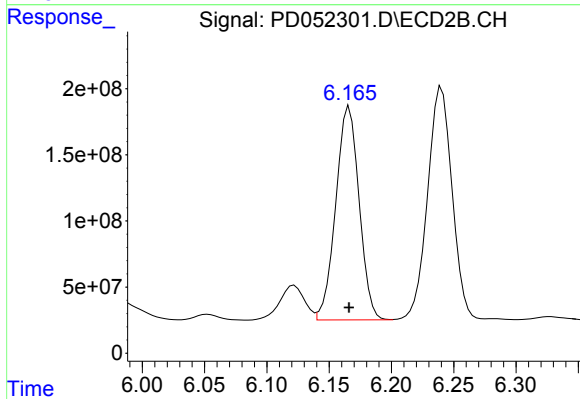

#25 Chlordane-3


R.T.: 6.166 min
Delta R.T.: 0.000 min
Response: 2112432048
Conc: 478.71 ng/ml

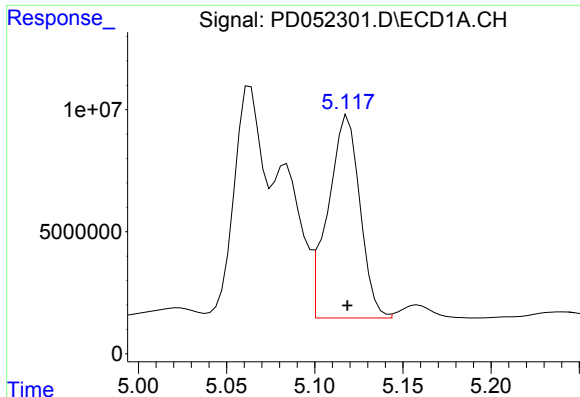

#26 Chlordane-4


R.T.: 5.119 min
Delta R.T.: 0.000 min
Response: 104242264
Conc: 491.49 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD032919CHLOR

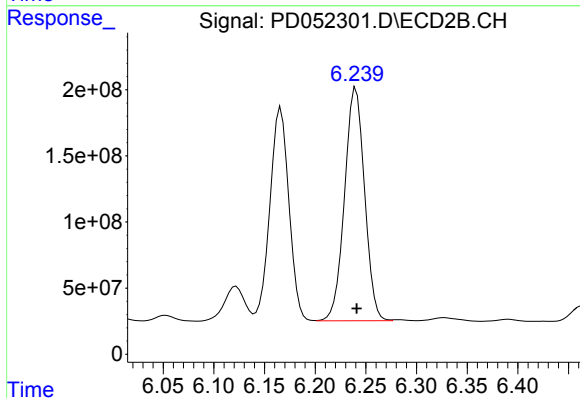


#26 Chlordane-4

R.T.: 6.240 min
Delta R.T.: 0.000 min
Response: 2419901062
Conc: 475.88 ng/ml

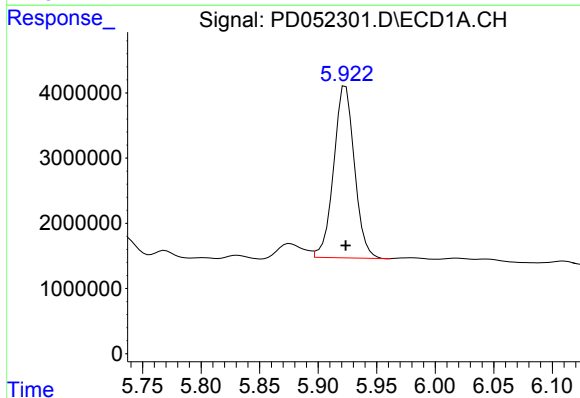


#27 Chlordane-5

R.T.: 5.923 min
Delta R.T.: 0.000 min
Response: 32507531
Conc: 499.86 ng/ml

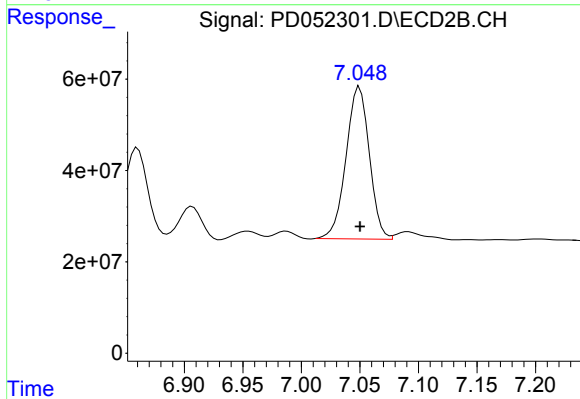

#27 Chlordane-5

R.T.: 7.050 min
Delta R.T.: 0.000 min
Response: 462573746
Conc: 501.38 ng/ml

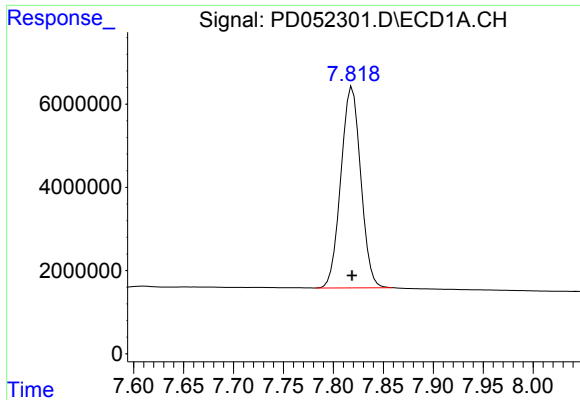

#28 Decachlorobiphenyl


R.T.: 7.819 min

Delta R.T.: 0.000 min

Response: 67001321

Conc: 50.27 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD032919CHLOR

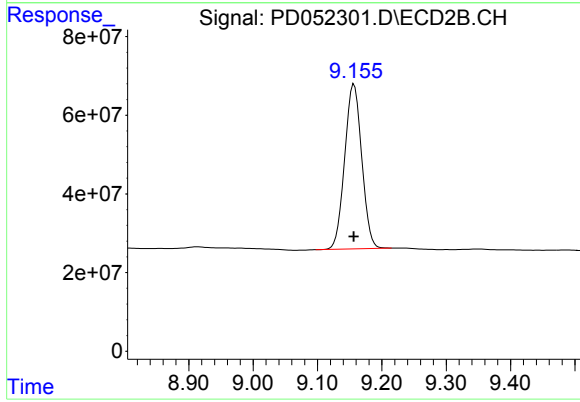

#28 Decachlorobiphenyl

R.T.: 9.157 min

Delta R.T.: 0.000 min

Response: 771803208

Conc: 49.63 ng/ml