

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032919\
 Data File : PD052324.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Mar 2019 19:41
 Operator : AJ\SJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 30 04:59:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 29 13:06:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.221	4.042	71386451	1408.5E6	51.158	48.597
28)	SA Decachlor...	7.818	9.156	68405113	799.0E6	51.326	51.376
Target Compounds							
23)	Chlordane-1	4.043	5.045	31209540	742.4E6	497.015	483.952
24)	Chlordane-2	4.522	5.515	36660729	678.1E6	492.645	484.165
25)	Chlordane-3	5.063	6.165	110.8E6	2199.9E6	501.033	498.526
26)	Chlordane-4	5.118	6.239	105.4E6	2519.7E6	497.075	495.501
27)	Chlordane-5	5.922	7.048	33536192	507.7E6	515.679	550.281


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032919\
Data File : PD052324.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Mar 2019 19:41
Operator : AJ\SJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 30 04:59:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
Quant Title : GC Extractables
QLast Update : Fri Mar 29 13:06:45 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

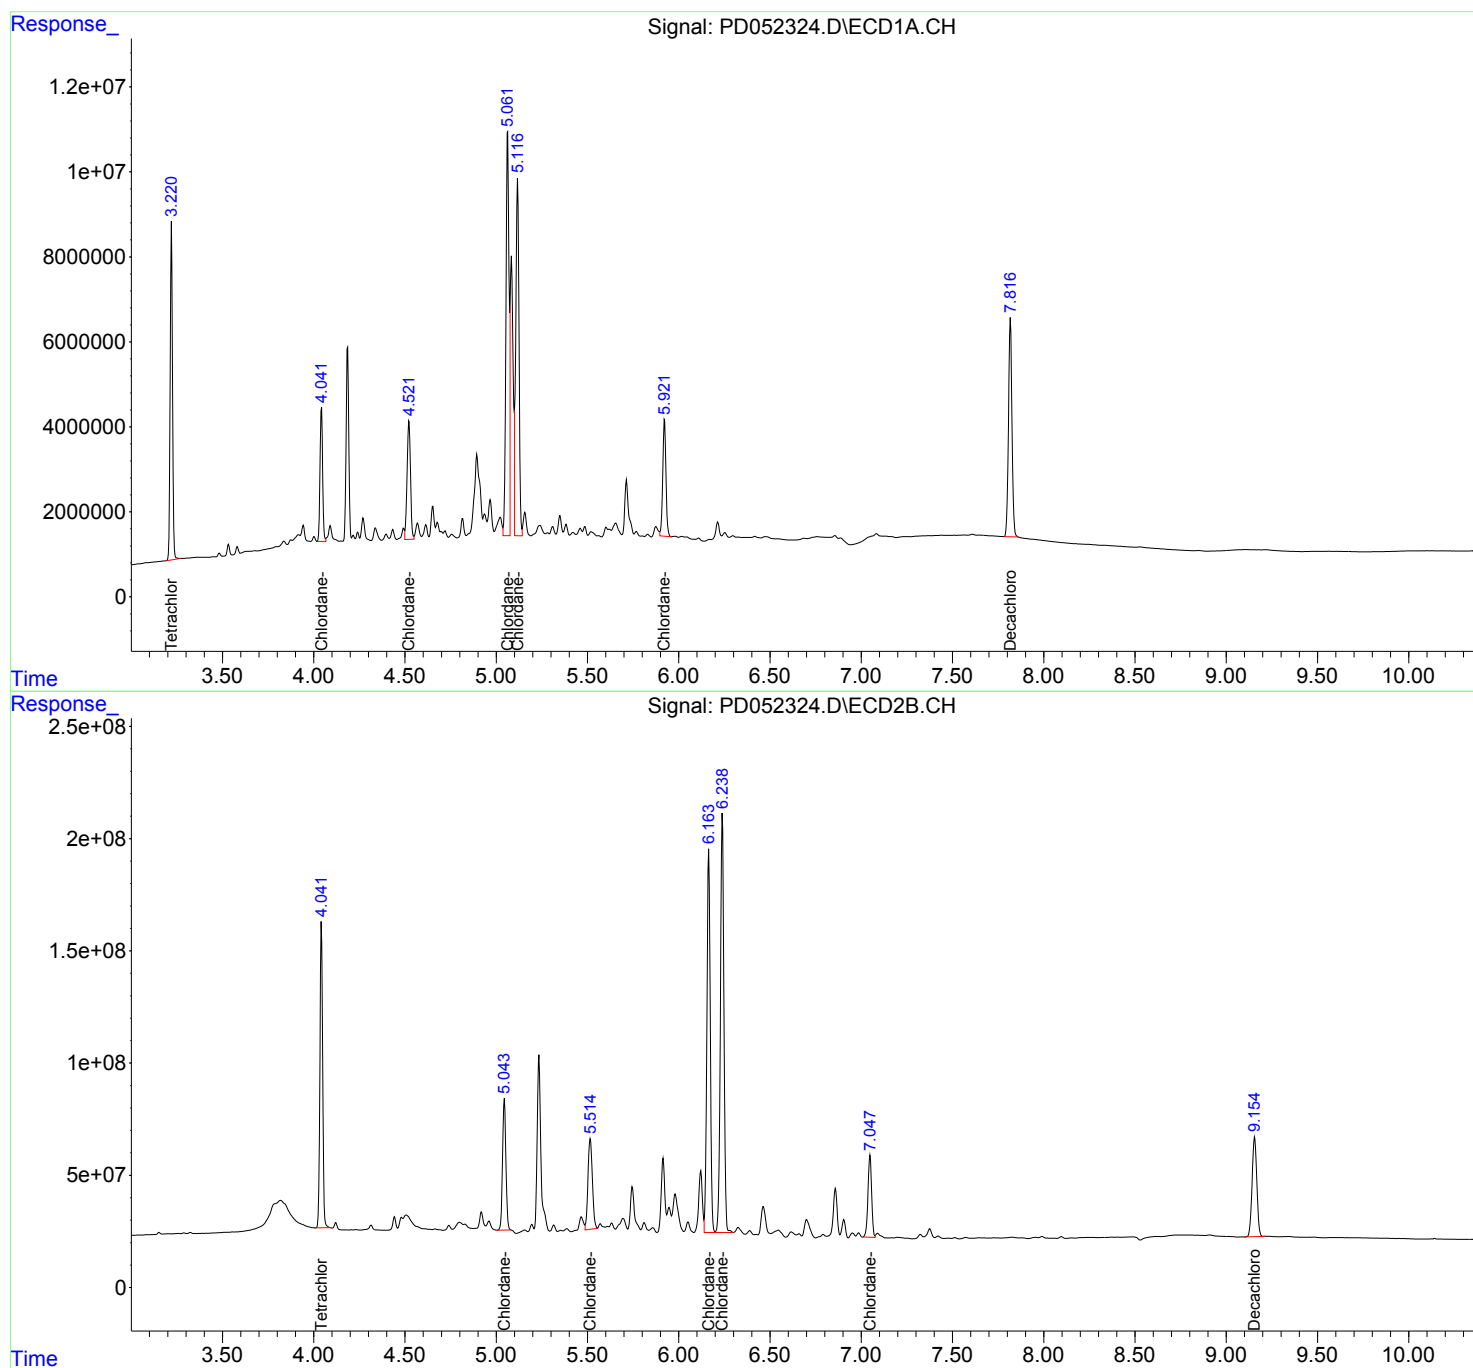


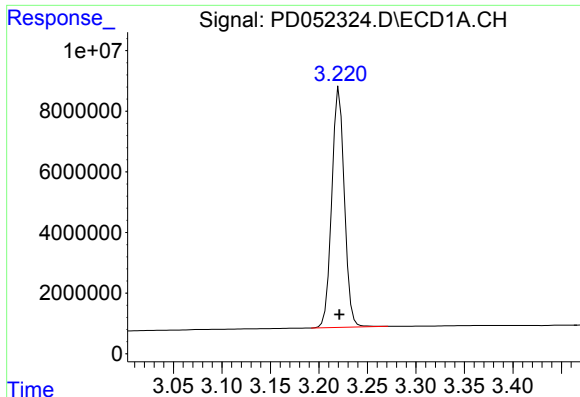

#1 Tetrachloro-m-xylene


R.T.: 3.221 min
Delta R.T.: 0.000 min
Response: 71386451
Conc: 51.16 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

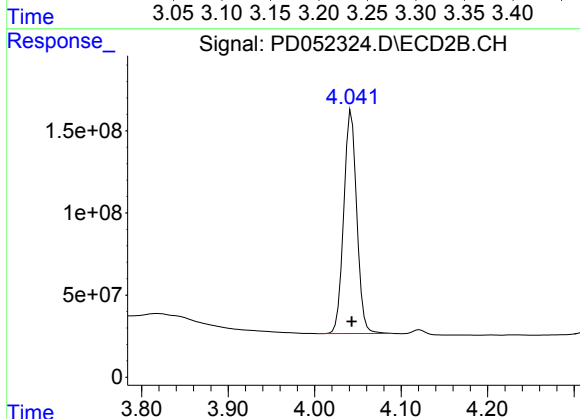


#1 Tetrachloro-m-xylene

R.T.: 4.042 min
Delta R.T.: 0.000 min
Response: 1408528036
Conc: 48.60 ng/ml

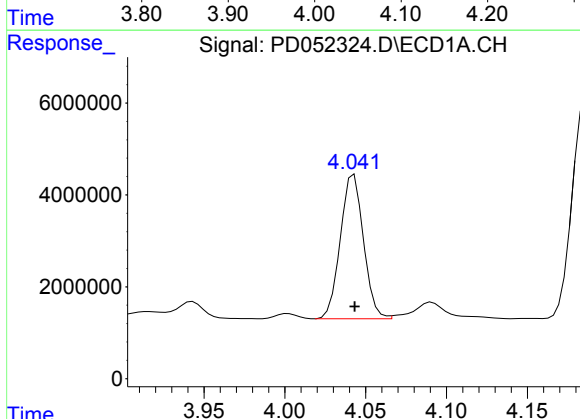


#23 Chlordane-1

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 31209540
Conc: 497.02 ng/ml

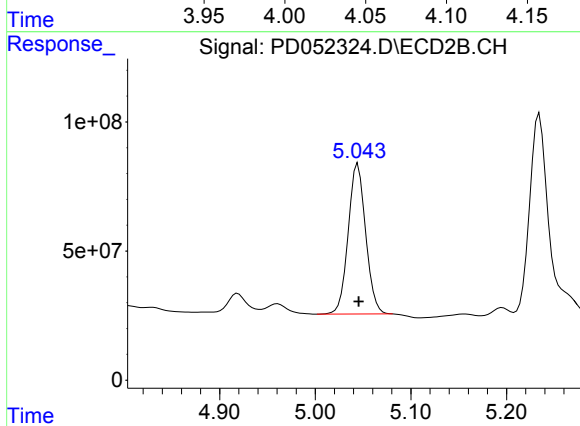

#23 Chlordane-1


R.T.: 5.045 min
Delta R.T.: 0.000 min
Response: 742430480
Conc: 483.95 ng/ml

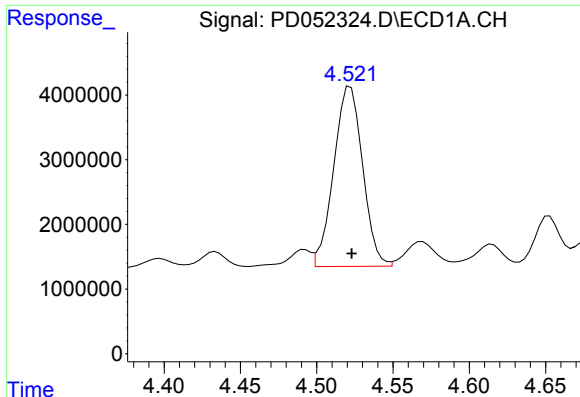

#24 Chlordane-2


R.T.: 4.522 min
Delta R.T.: 0.000 min
Response: 36660729
Conc: 492.64 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

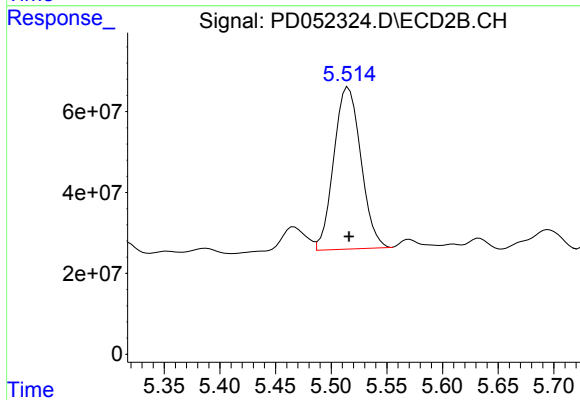


#24 Chlordane-2

R.T.: 5.515 min
Delta R.T.: 0.000 min
Response: 678058481
Conc: 484.16 ng/ml

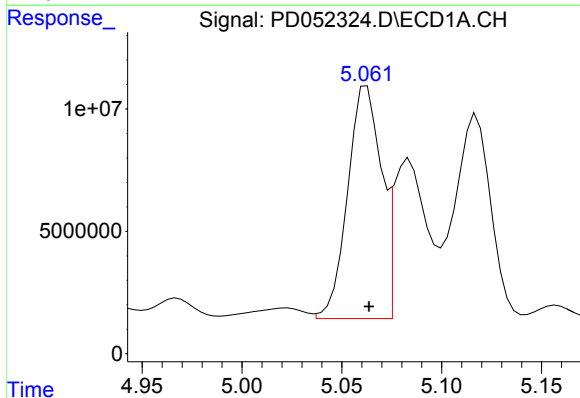


#25 Chlordane-3

R.T.: 5.063 min
Delta R.T.: -0.001 min
Response: 110797033
Conc: 501.03 ng/ml

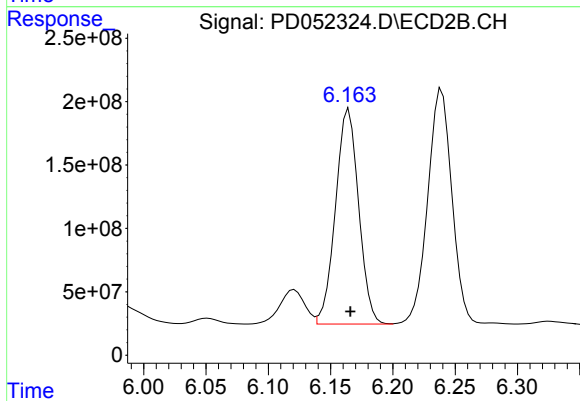

#25 Chlordane-3


R.T.: 6.165 min
Delta R.T.: -0.001 min
Response: 2199894567
Conc: 498.53 ng/ml

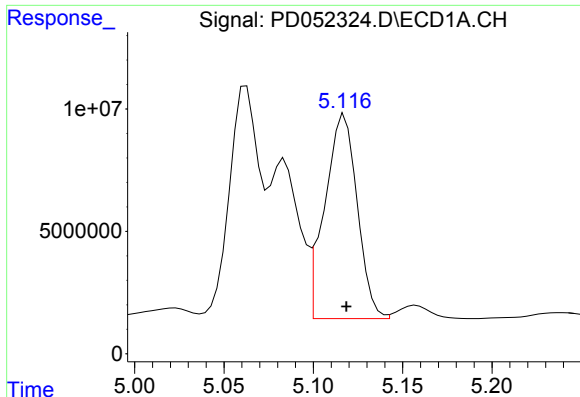

#26 Chlordane-4


R.T.: 5.118 min
Delta R.T.: 0.000 min
Response: 105425973
Conc: 497.07 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

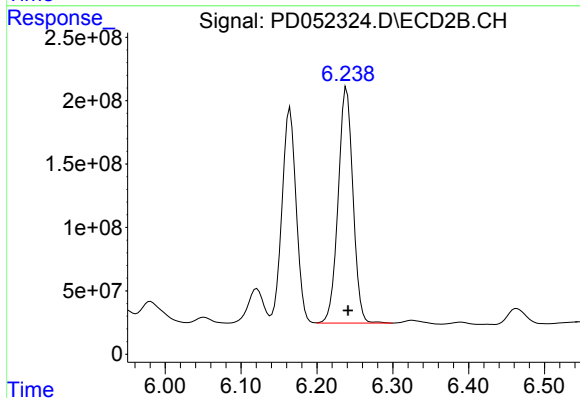


#26 Chlordane-4

R.T.: 6.239 min
Delta R.T.: -0.002 min
Response: 2519692529
Conc: 495.50 ng/ml

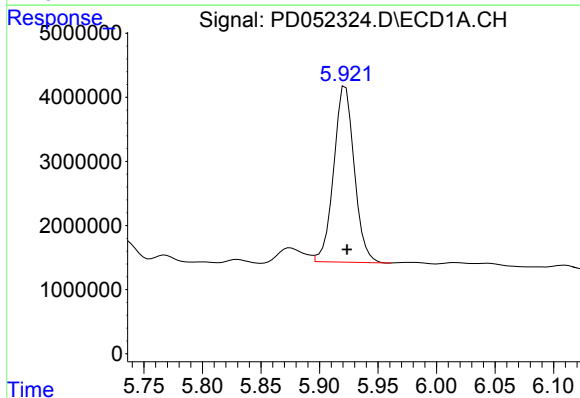


#27 Chlordane-5

R.T.: 5.922 min
Delta R.T.: -0.001 min
Response: 33536192
Conc: 515.68 ng/ml

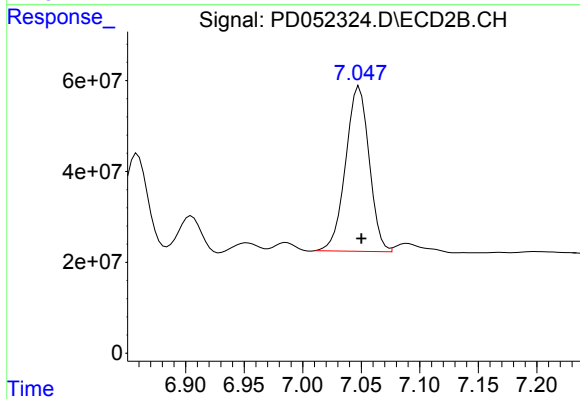

#27 Chlordane-5


R.T.: 7.048 min
Delta R.T.: -0.002 min
Response: 507694395
Conc: 550.28 ng/ml

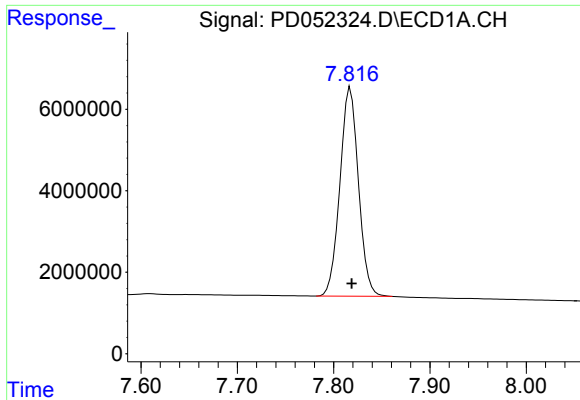

#28 Decachlorobiphenyl

R.T.: 7.818 min
Delta R.T.: -0.001 min
Response: 68405113
Conc: 51.33 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

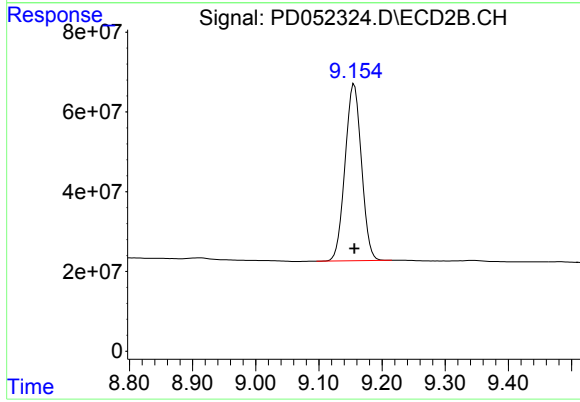

#28 Decachlorobiphenyl

R.T.: 9.156 min
Delta R.T.: 0.000 min
Response: 798969517
Conc: 51.38 ng/ml