

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032919\
 Data File : PD052327.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Mar 2019 20:24
 Operator : AJ\SJ
 Sample : MDL-CHL-S-02
 Misc : 25 PPB
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MDL-CHL-S-02

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 30 04:59:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 29 13:06:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.221	4.042	28167360	614.3E6	20.186	21.195
28)	SA Decachlor...	7.817	9.156	30785352	383.1E6	23.099	24.635
Target Compounds							
23)	Chlordane-1	4.043	5.044	1534010	43078698	24.429	28.081
24)	Chlordane-2	4.522	5.515	1897450	44710036	25.498	31.925 #
25)	Chlordane-3	5.062	6.165	4986541	139.3E6	22.550	31.562 #
26)	Chlordane-4	5.117	6.239	4960612	166.7E6	23.389	32.784 #
27)	Chlordane-5	5.921	7.049	1070710	33837437	16.464	36.676 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032919\
Data File : PD052327.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Mar 2019 20:24
Operator : AJ\SJ
Sample : MDL-CHL-S-02
Misc : 25 PPB
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
MDL-CHL-S-02

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 30 04:59:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
Quant Title : GC Extractables
QLast Update : Fri Mar 29 13:06:45 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

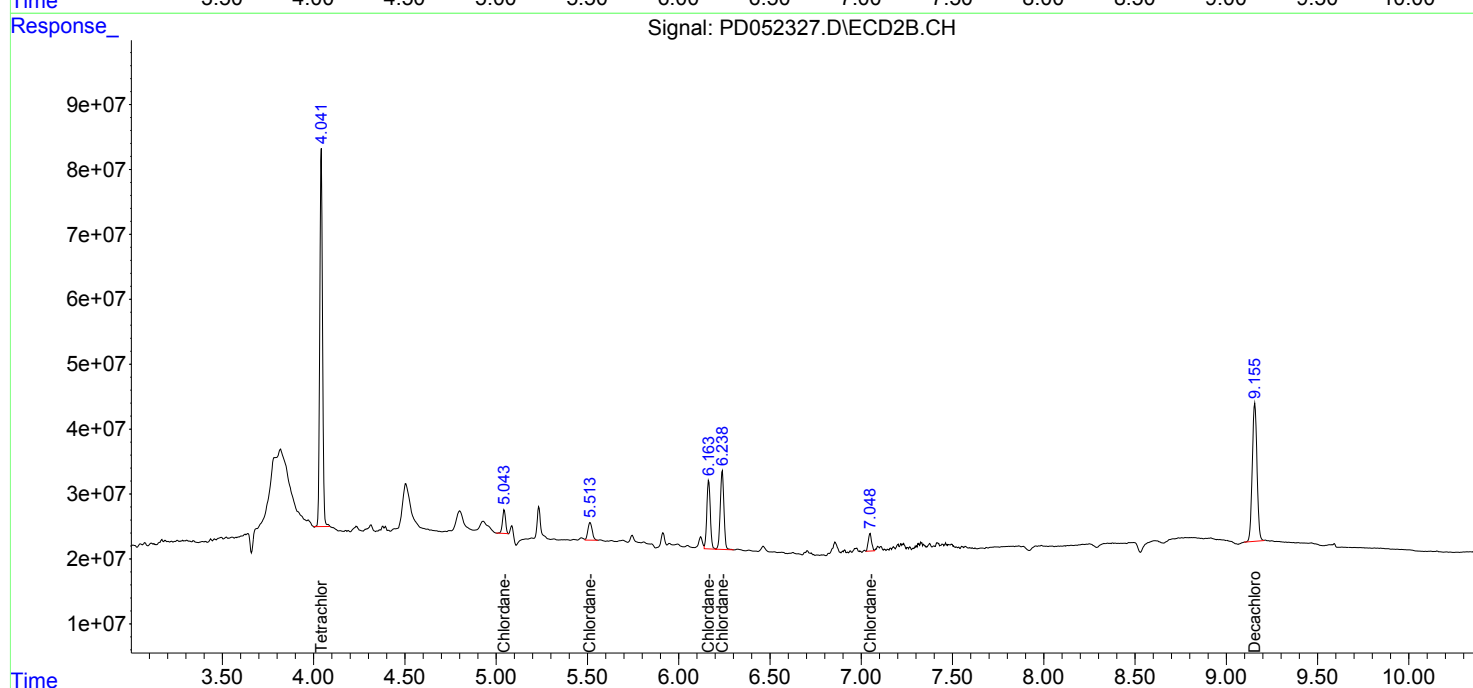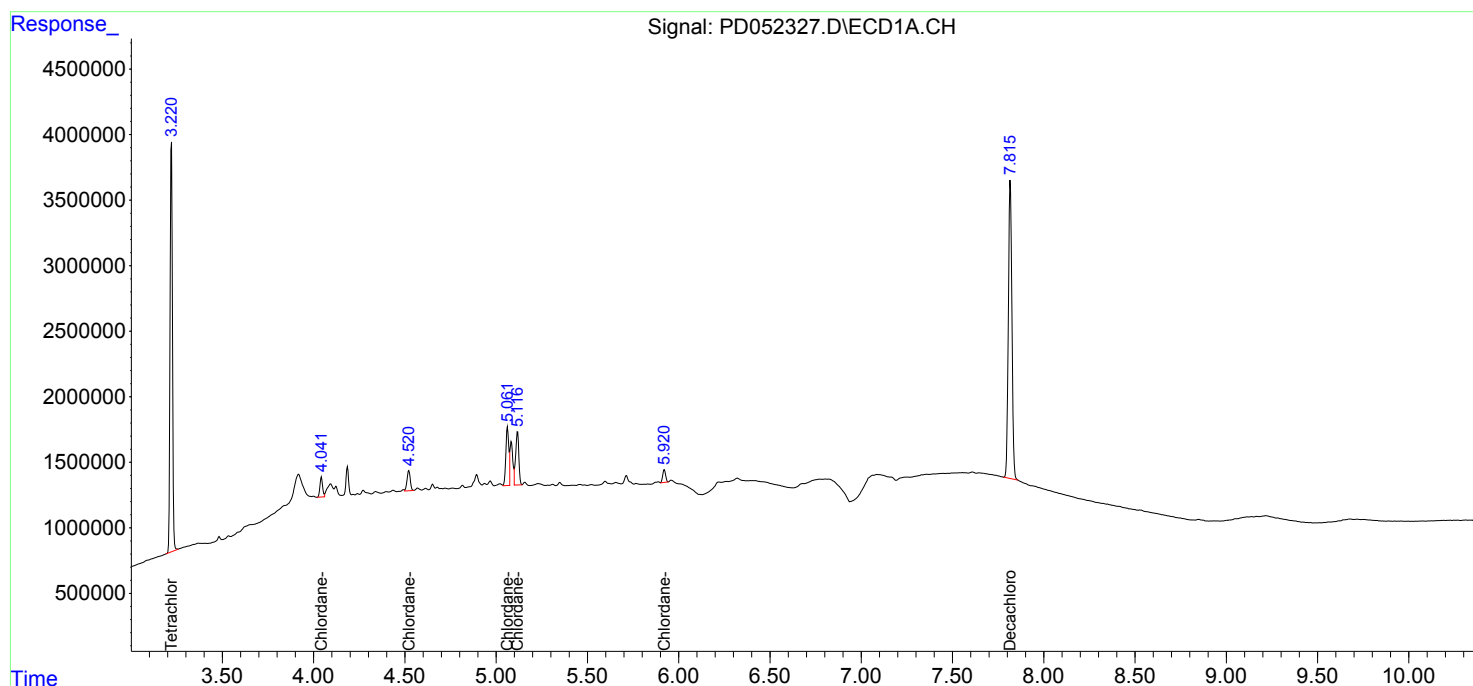


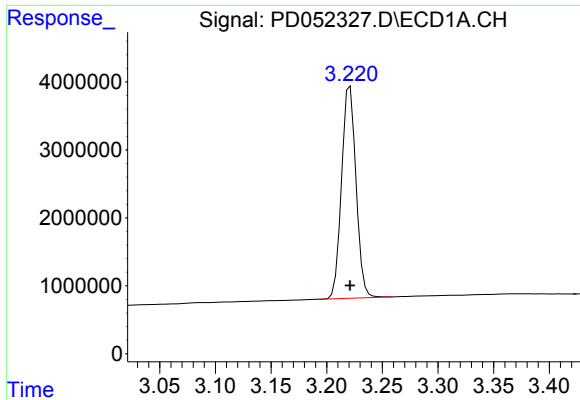

#1 Tetrachloro-m-xylene


R.T.: 3.221 min
Delta R.T.: 0.000 min
Response: 28167360
Conc: 20.19 ng/ml

Instrument :
ECD_D
ClientSampleId :
MDL-CHL-S-02

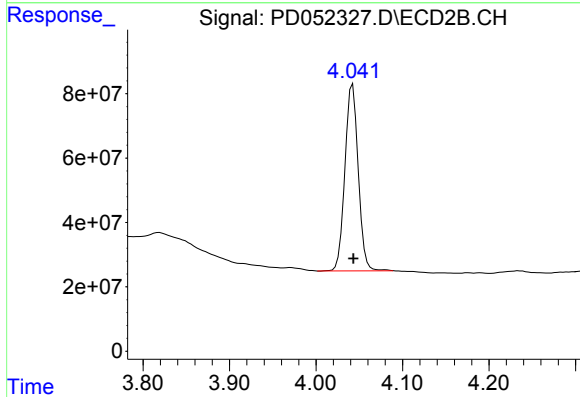


#1 Tetrachloro-m-xylene

R.T.: 4.042 min
Delta R.T.: 0.000 min
Response: 614320939
Conc: 21.20 ng/ml

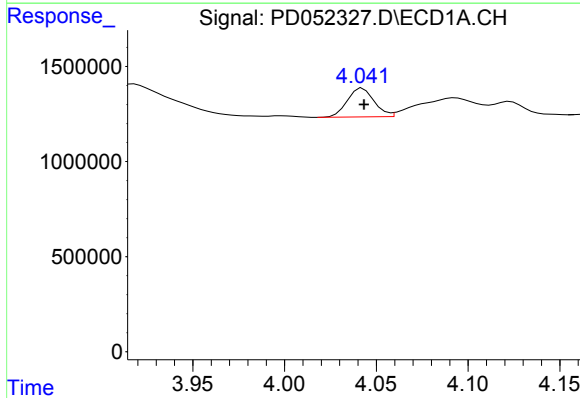


#23 Chlordane-1

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 1534010
Conc: 24.43 ng/ml

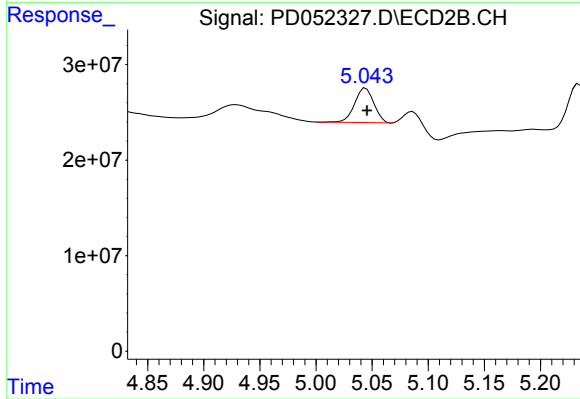

#23 Chlordane-1


R.T.: 5.044 min
Delta R.T.: -0.001 min
Response: 43078698
Conc: 28.08 ng/ml

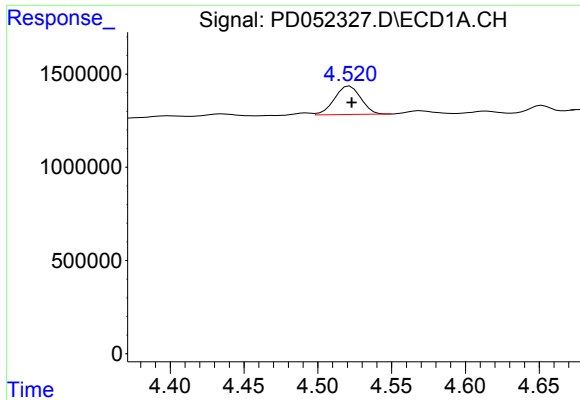

#24 Chlordane-2


R.T.: 4.522 min
Delta R.T.: -0.001 min
Response: 1897450
Conc: 25.50 ng/ml

Instrument :
ECD_D
ClientSampleId :
MDL-CHL-S-02

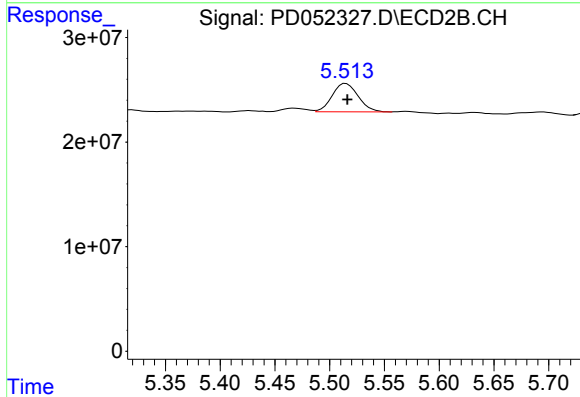


#24 Chlordane-2

R.T.: 5.515 min
Delta R.T.: -0.001 min
Response: 44710036
Conc: 31.93 ng/ml

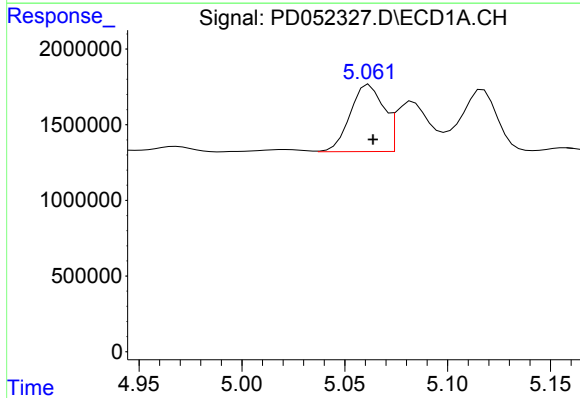


#25 Chlordane-3

R.T.: 5.062 min
Delta R.T.: -0.002 min
Response: 4986541
Conc: 22.55 ng/ml

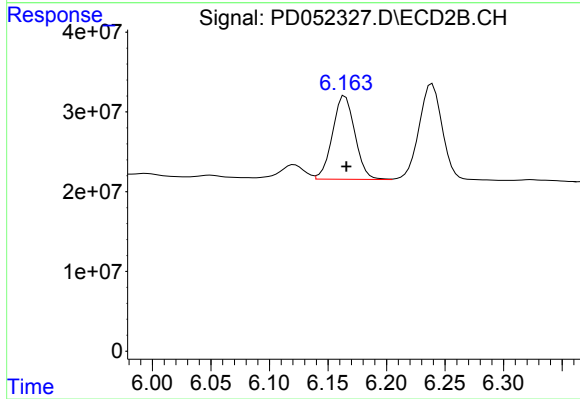

#25 Chlordane-3


R.T.: 6.165 min
Delta R.T.: -0.001 min
Response: 139278774
Conc: 31.56 ng/ml

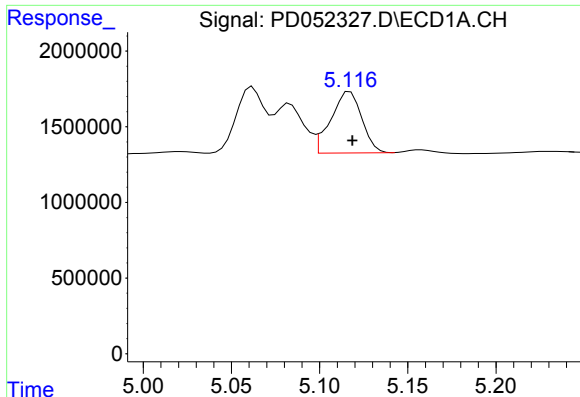

#26 Chlordane-4


R.T.: 5.117 min
Delta R.T.: -0.001 min
Response: 4960612
Conc: 23.39 ng/ml

Instrument :
ECD_D
ClientSampleId :
MDL-CHL-S-02

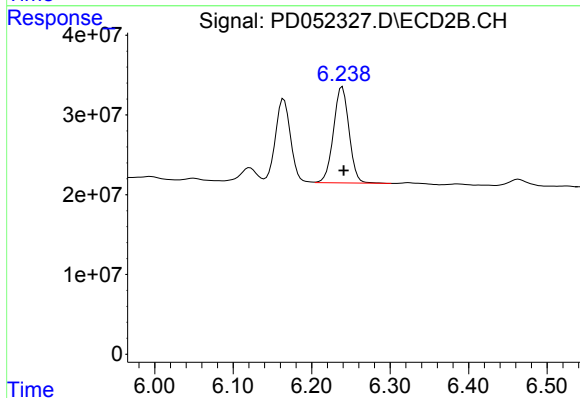


#26 Chlordane-4

R.T.: 6.239 min
Delta R.T.: -0.002 min
Response: 166709203
Conc: 32.78 ng/ml

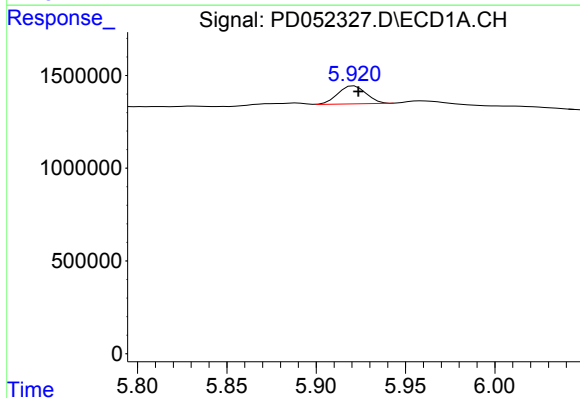


#27 Chlordane-5

R.T.: 5.921 min
Delta R.T.: -0.002 min
Response: 1070710
Conc: 16.46 ng/ml

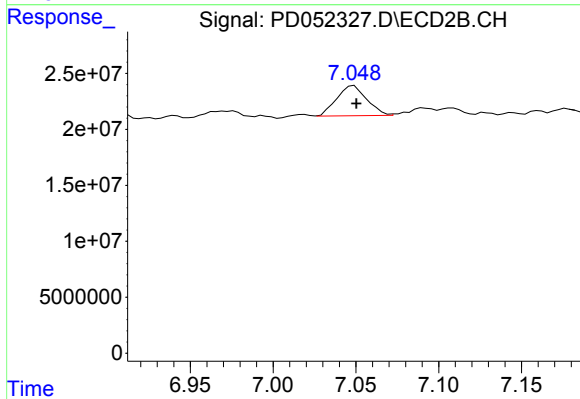

#27 Chlordane-5


R.T.: 7.049 min
Delta R.T.: -0.002 min
Response: 33837437
Conc: 36.68 ng/ml

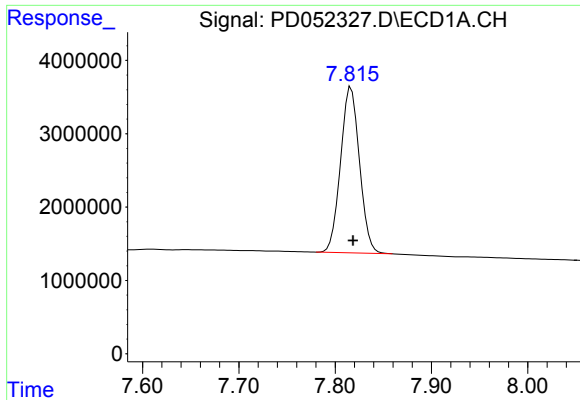

#28 Decachlorobiphenyl

R.T.: 7.817 min
Delta R.T.: -0.002 min
Response: 30785352
Conc: 23.10 ng/ml

Instrument :
ECD_D
ClientSampleId :
MDL-CHL-S-02

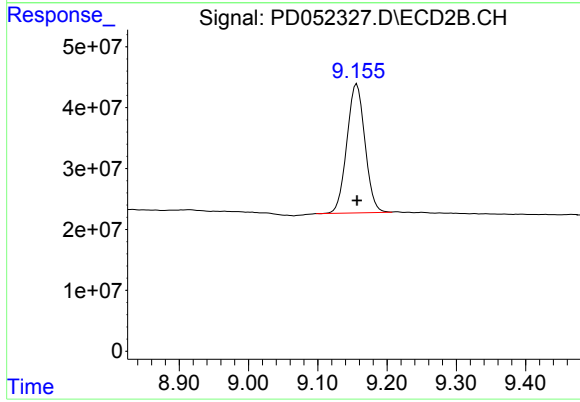

#28 Decachlorobiphenyl

R.T.: 9.156 min
Delta R.T.: 0.000 min
Response: 383110522
Conc: 24.64 ng/ml