Quantitation Report (QT Reviewed)

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032919\
Data File : PD052337.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Mar 2019 22:45
Operator : AJ\SJ
Sample : MDL-BL-CHL-W-03
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
MDL-BL-CHL-W-03

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 30 05:01:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
Quant Title : GC Extractables
QLast Update : Fri Mar 29 13:06:45 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
	System Monitoring Compounds						
1)	SA Tetrachlo...	3.221	4.042	27400347	606.9E6	19.636	20.938
28)	SA Decachlor...	7.816	9.155	29694796	367.4E6	22.281	23.628
	Target Compounds						

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Quantitation Report (QT Reviewed)

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032919\
Data File : PD052337.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Mar 2019 22:45
Operator : AJ\SJ
Sample : MDL-BL-CHL-W-03
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
MDL-BL-CHL-W-03

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 30 05:01:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
Quant Title : GC Extractables
QLast Update : Fri Mar 29 13:06:45 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

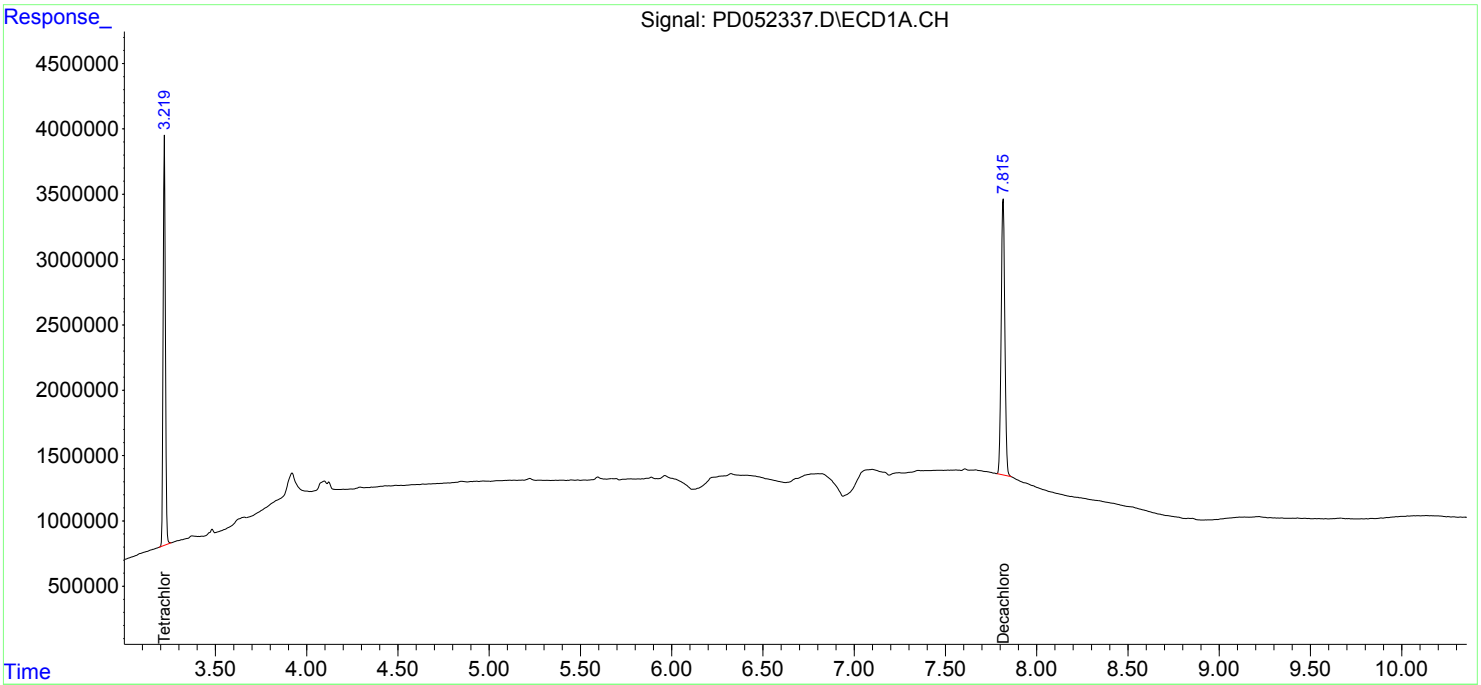

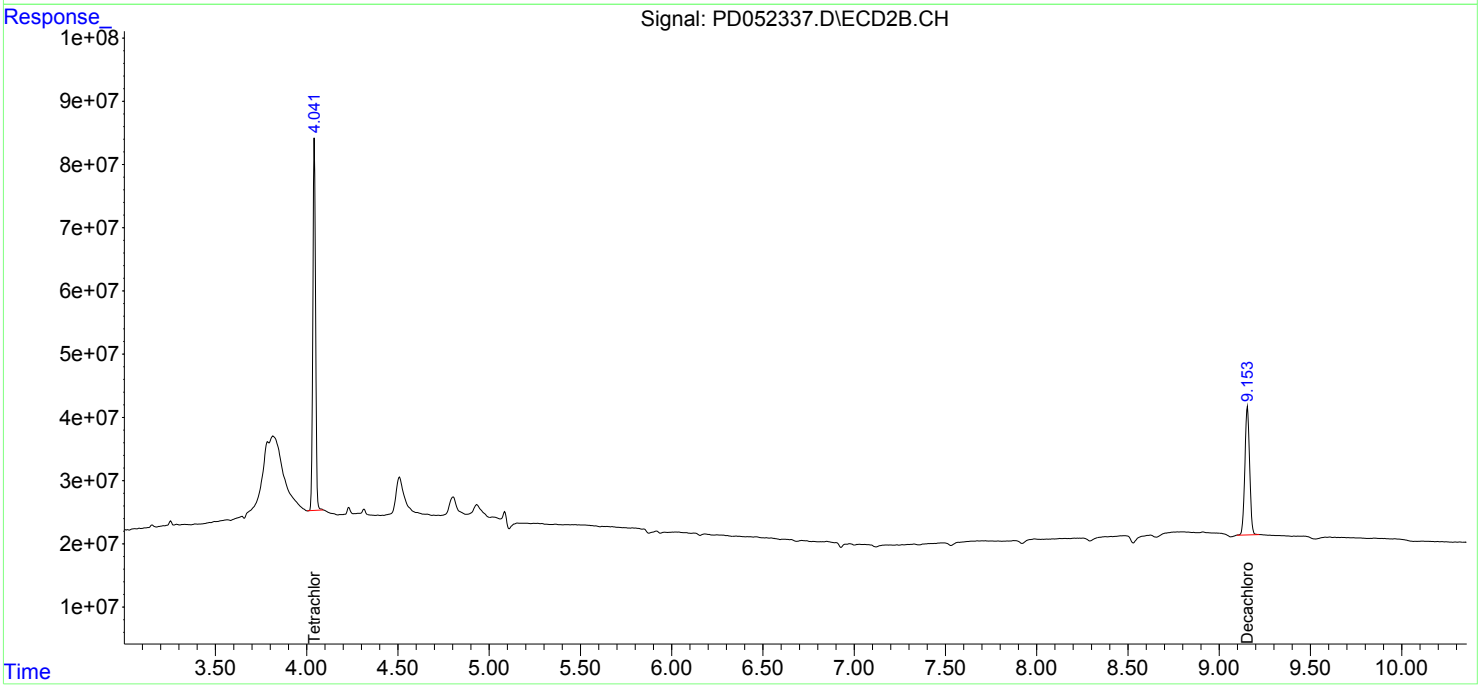

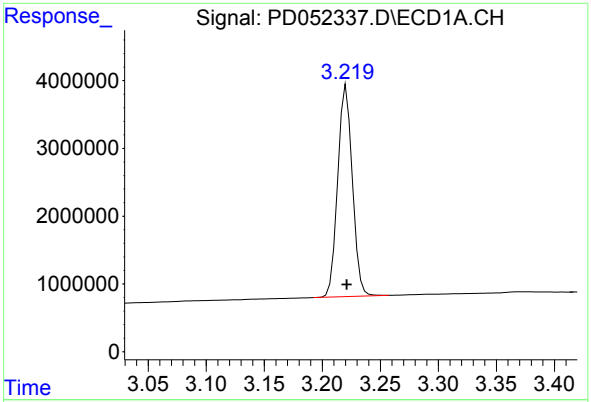

#1 Tetrachloro-m-xylene

R.T.: 3.221 min
Delta R.T.: 0.000 min
Response: 27400347
Conc: 19.64 ng/ml

Instrument :
ECD_D
ClientSampleId :
MDL-BL-CHL-W-03

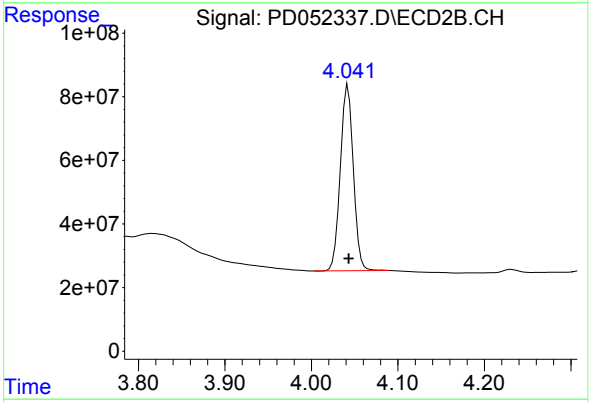

#1 Tetrachloro-m-xylene

R.T.: 4.042 min
Delta R.T.: 0.000 min
Response: 606865012
Conc: 20.94 ng/ml

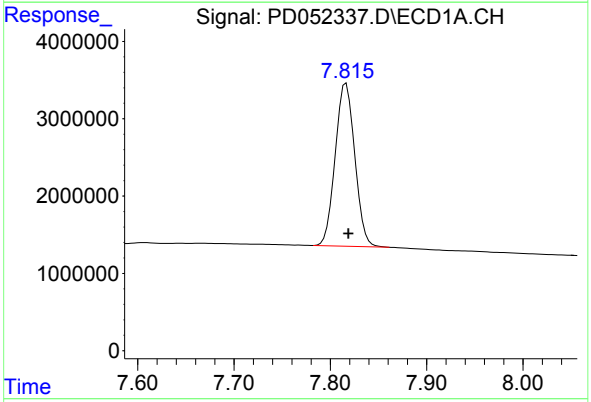

#28 Decachlorobiphenyl

R.T.: 7.816 min
Delta R.T.: -0.002 min
Response: 29694796
Conc: 22.28 ng/ml

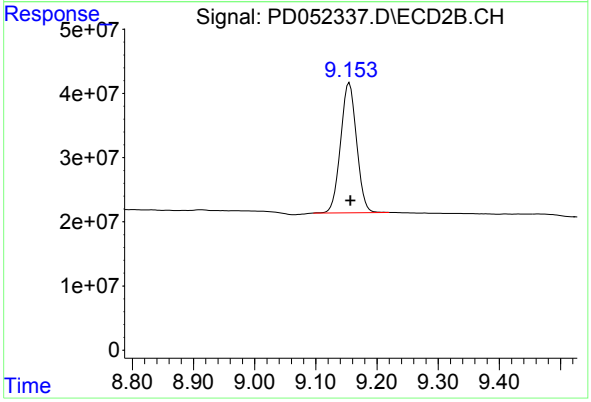

#28 Decachlorobiphenyl

R.T.: 9.155 min
Delta R.T.: -0.002 min
Response: 367443884
Conc: 23.63 ng/ml