

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032919\
 Data File : PD052352.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Mar 2019 2:18
 Operator : AJ\SJ
 Sample : MDL-BLTOX-W-02
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MDL-BLTOX-W-02

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 30 05:10:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX032919.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 29 14:07:32 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.221	4.042	27840961	614.1E6	20.492	22.012
7) SA Decachlor...	7.816	9.156	29409244	377.0E6	21.897	24.609


Target Compounds


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032919\
Data File : PD052352.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Mar 2019 2:18
Operator : AJ\SJ
Sample : MDL-BLTOX-W-02
Misc :
ALS Vial : 58 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 30 05:10:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX032919.M
Quant Title : GC Extractables
QLast Update : Fri Mar 29 14:07:32 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

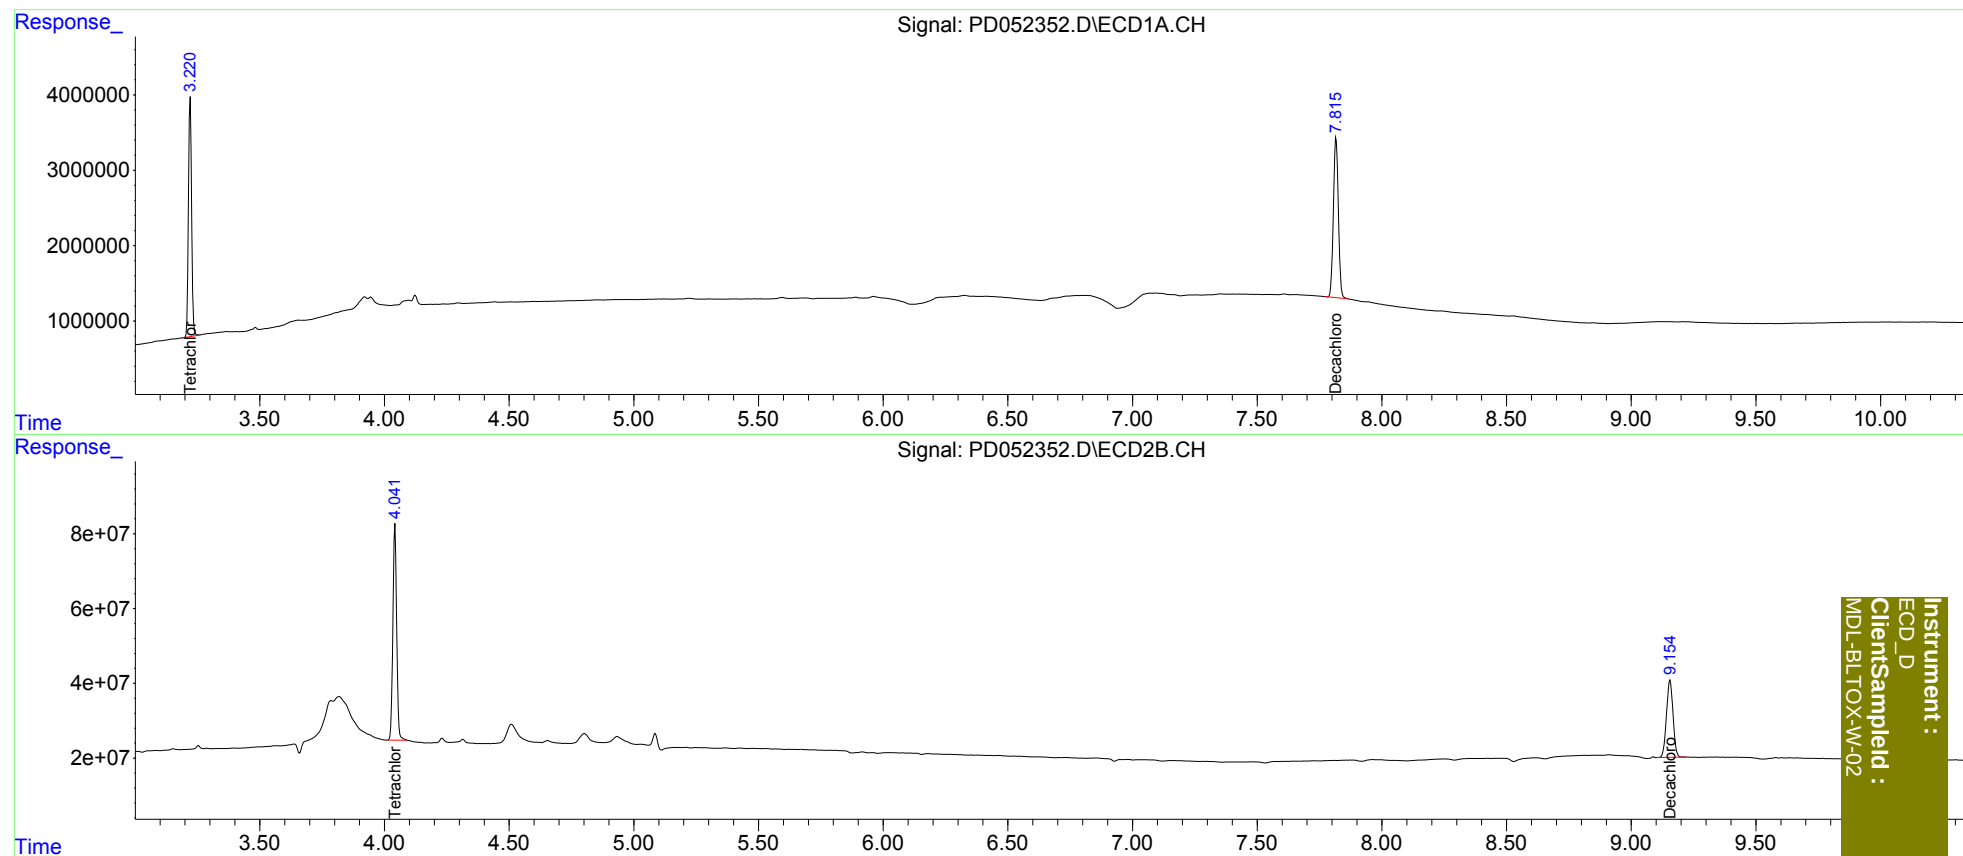


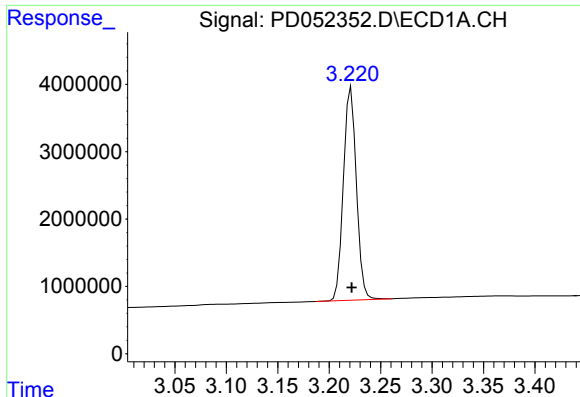

#1 Tetrachloro-m-xylene


R.T.: 3.221 min
Delta R.T.: 0.000 min
Response: 27840961
Conc: 20.49 ng/ml

Instrument :
ECD_D
ClientSampleId :
MDL-BLTOX-W-02

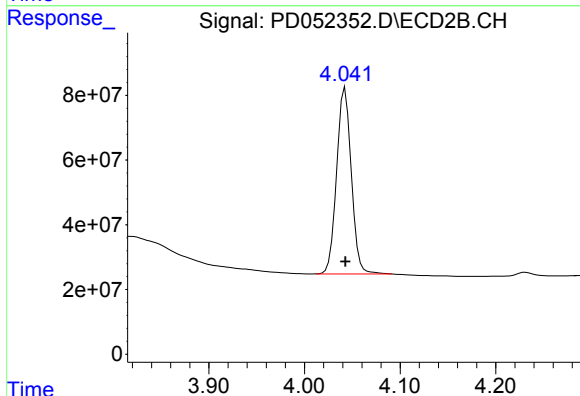


#1 Tetrachloro-m-xylene

R.T.: 4.042 min
Delta R.T.: 0.000 min
Response: 614073818
Conc: 22.01 ng/ml

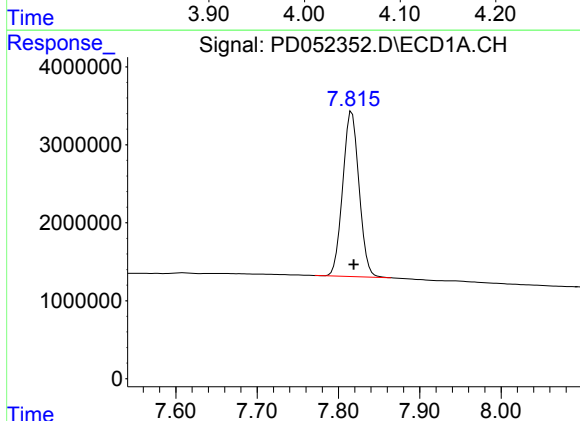

#7 Decachlorobiphenyl

R.T.: 7.816 min
Delta R.T.: -0.003 min
Response: 29409244
Conc: 21.90 ng/ml

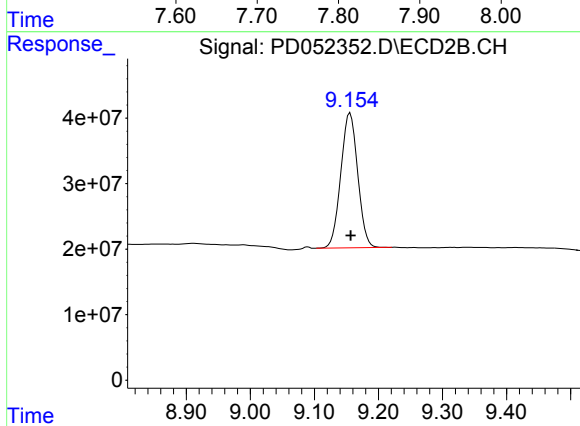

#7 Decachlorobiphenyl

R.T.: 9.156 min
Delta R.T.: -0.001 min
Response: 376986191
Conc: 24.61 ng/ml