

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032921\
 Data File : PD061838.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Mar 2021 02:04
 Operator : AR\AJ
 Sample : PB135412BL
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PB135412BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 30 05:57:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 30 04:47:56 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.486	3.981	15842305	166.2E6	18.921	19.131
28)	SA Decachlor...	8.257	9.038	24431608	180.6E6	19.856	19.134
Target Compounds							
3)	MA gamma-BHC...	0.000	4.652	0	1158425	N.D.	0.093 #
7)	B delta-BHC	0.000	5.035	0	13472923	N.D.	1.019 #
8)	B Heptachlo...	0.000	5.859	0	8039450	N.D.	0.679 #
10)	B gamma-Chl...	0.000	6.098	0	1249139	N.D.	0.105 #
13)	MA Dieldrin	0.000	6.479	0	333263	N.D.	0.029 #
18)	B Endrin al...	0.000	7.012	0	2342738	N.D.	0.298 #
19)	B Endosulfa...	0.000	7.242	0	2256445	N.D.	0.225 #
23)	Chlordane-1	0.000	4.963	0	1643843	N.D.	4.237 #
25)	Chlordane-3	0.000	6.098	0	1249139	N.D.	0.754 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032921\
Data File : PD061838.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Mar 2021 02:04
Operator : AR\AJ
Sample : PB135412BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PB135412BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 30 05:57:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
Quant Title : GC Extractables
QLast Update : Tue Mar 30 04:47:56 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

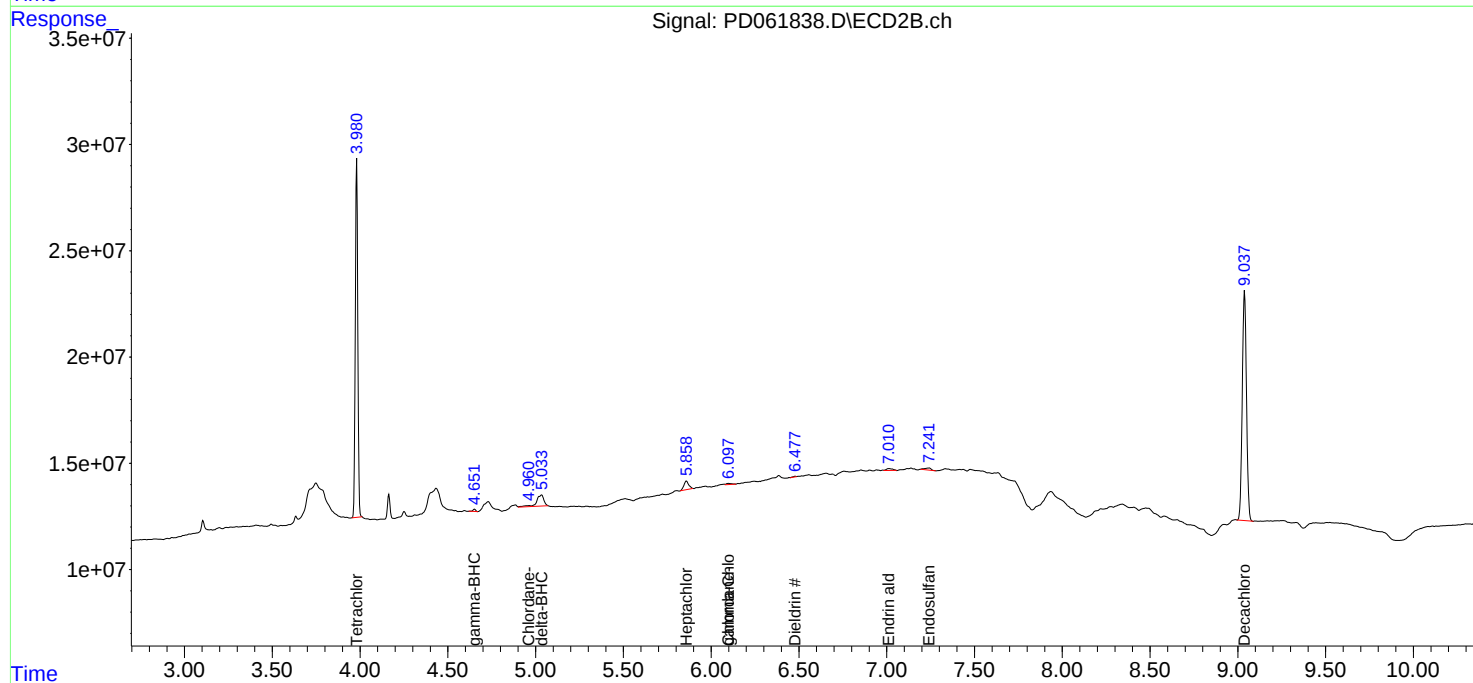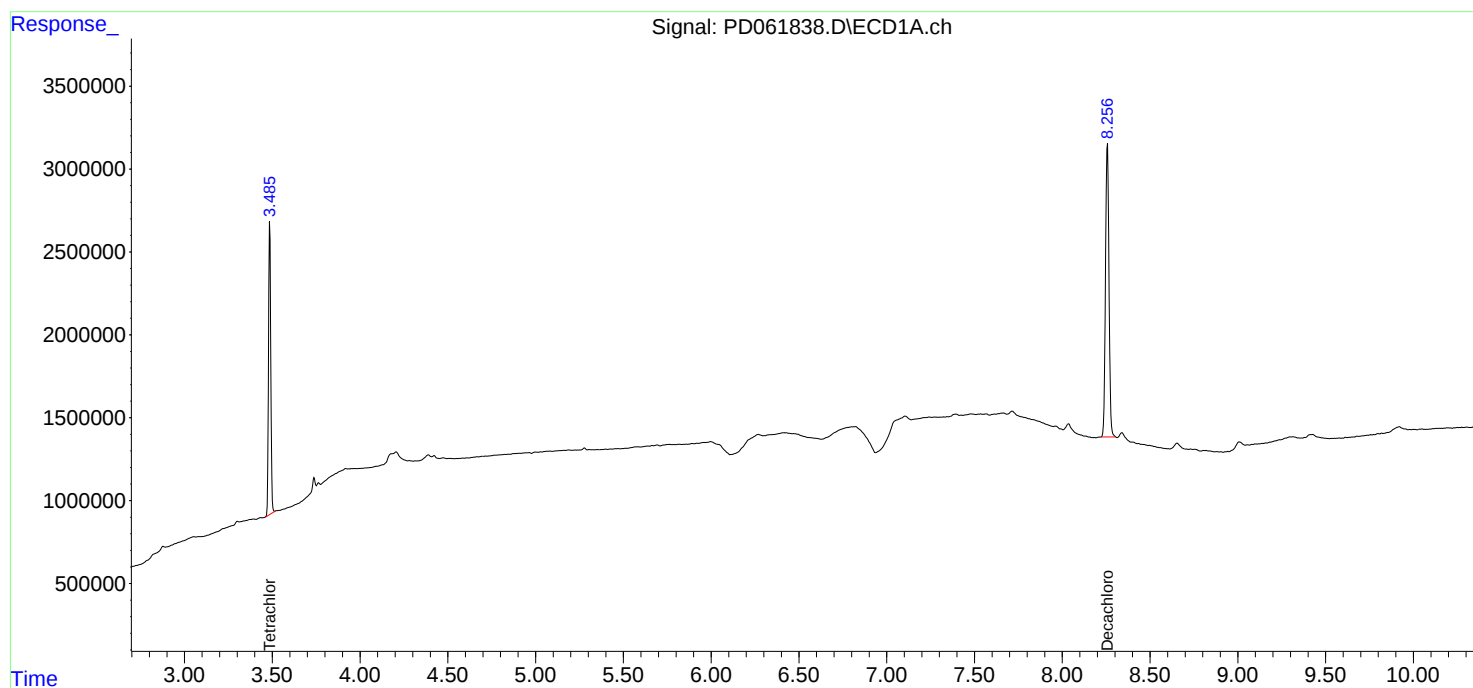


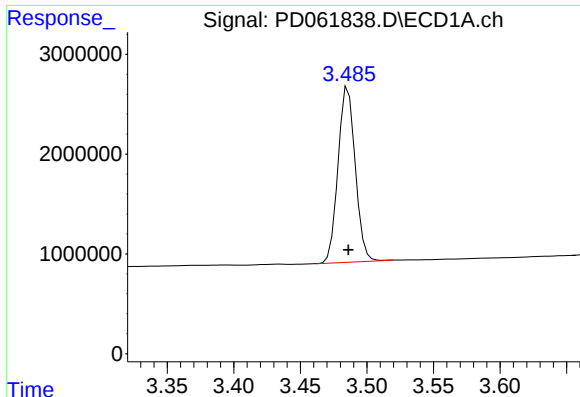

#1 Tetrachloro-m-xylene


R.T.: 3.486 min
Delta R.T.: 0.000 min
Response: 15842305
Conc: 18.92 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB135412BL

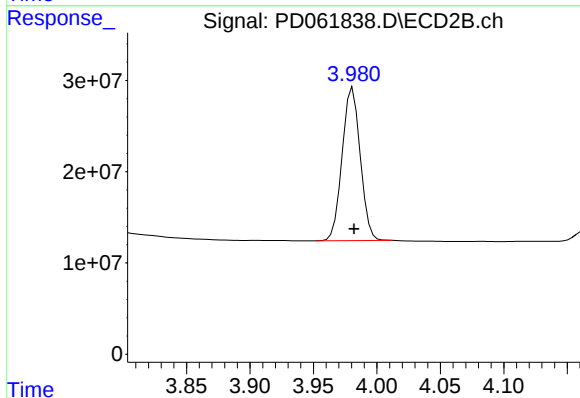


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 166230471
Conc: 19.13 ng/ml

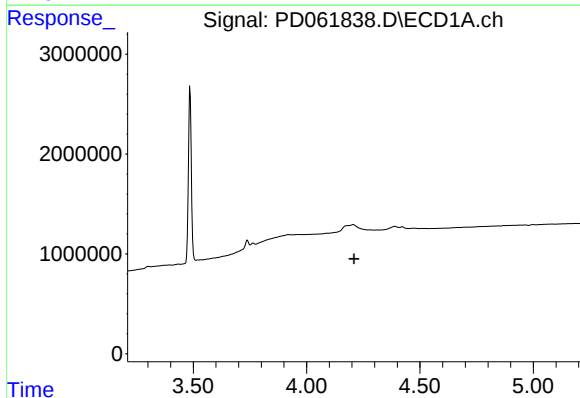


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.210 min
Response: 0
Conc: N.D.

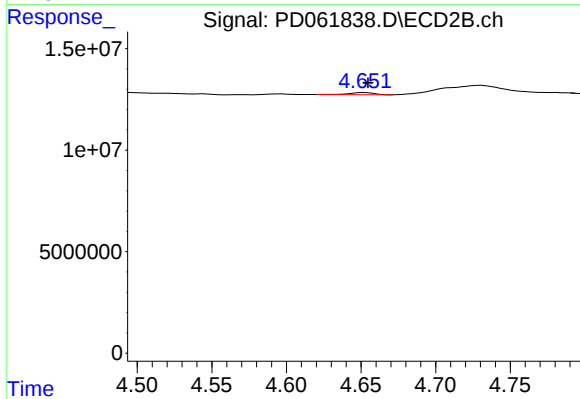

#3 gamma-BHC (Lindane)


R.T.: 4.652 min
Delta R.T.: -0.002 min
Response: 1158425
Conc: 0.09 ng/ml

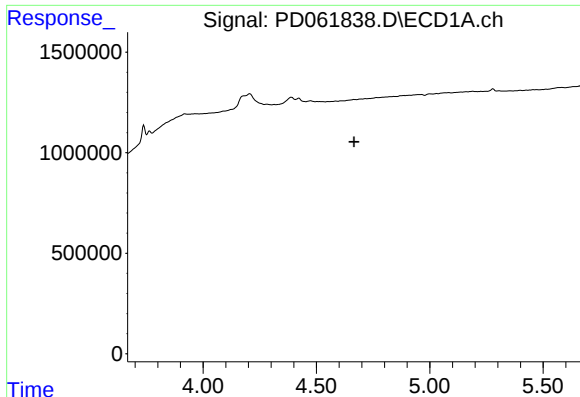

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.666 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB135412BL

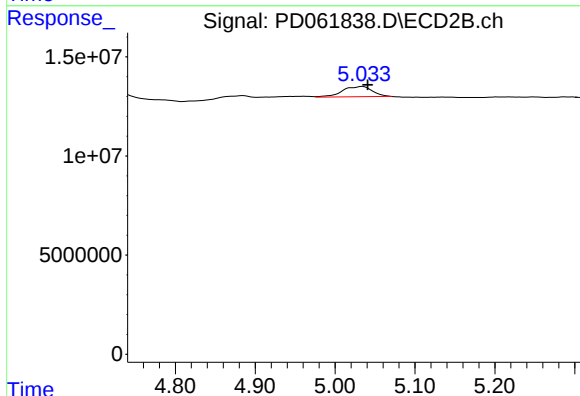


#7 delta-BHC

R.T.: 5.035 min
Delta R.T.: -0.006 min
Response: 13472923
Conc: 1.02 ng/ml

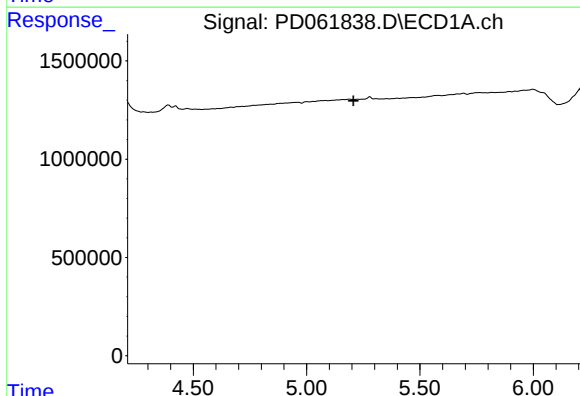


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.207 min
Response: 0
Conc: N.D.

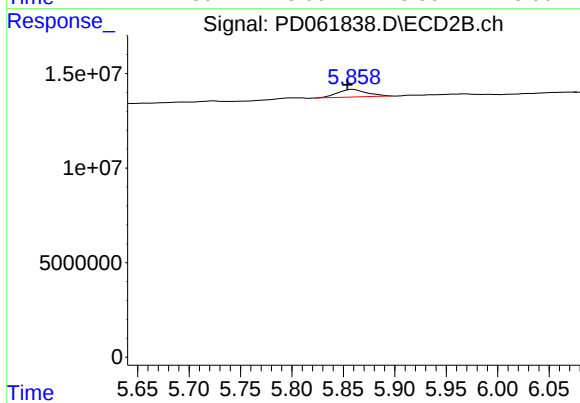

#8 Heptachlor epoxide


R.T.: 5.859 min
Delta R.T.: 0.006 min
Response: 8039450
Conc: 0.68 ng/ml

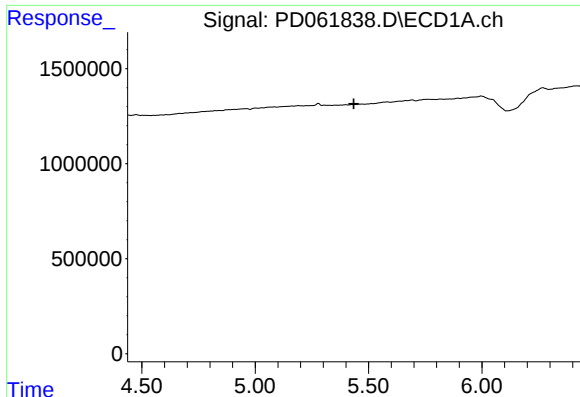

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.435 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB135412BL

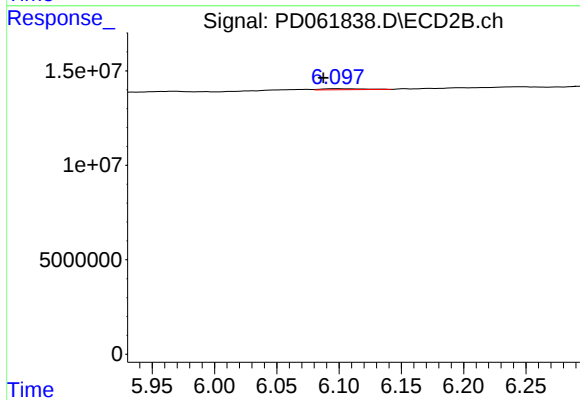


#10 gamma-Chlordane

R.T.: 6.098 min
Delta R.T.: 0.011 min
Response: 1249139
Conc: 0.11 ng/ml

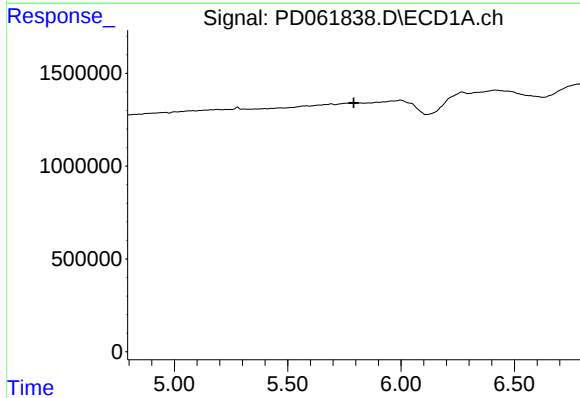


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 5.792 min
Response: 0
Conc: N.D.

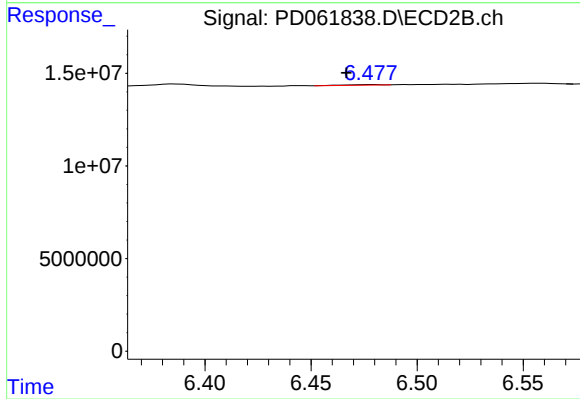

#13 Dieldrin


R.T.: 6.479 min
Delta R.T.: 0.012 min
Response: 333263
Conc: 0.03 ng/ml

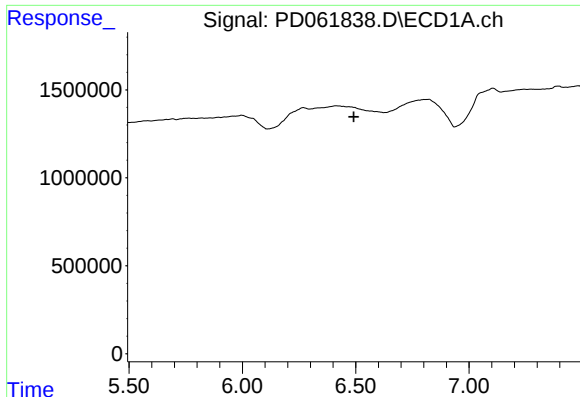

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.492 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB135412BL

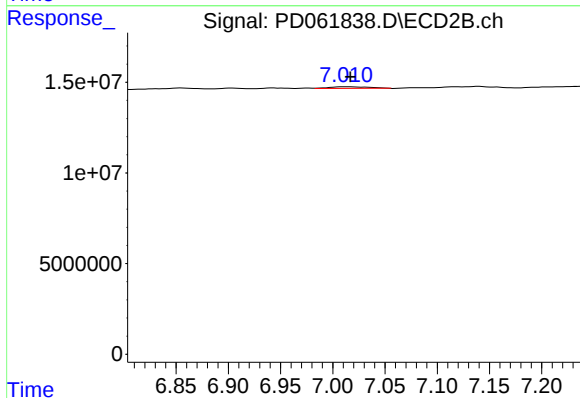


#18 Endrin aldehyde

R.T.: 7.012 min
Delta R.T.: -0.005 min
Response: 2342738
Conc: 0.30 ng/ml

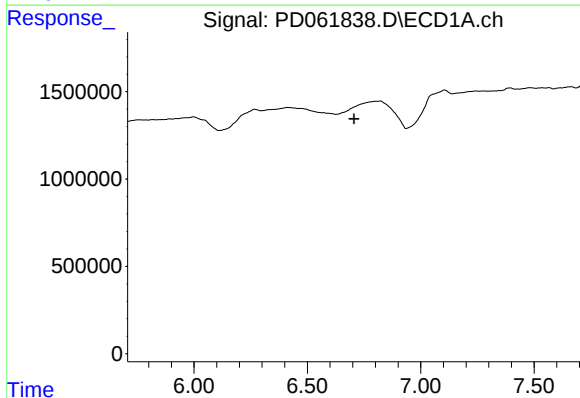


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 6.706 min
Response: 0
Conc: N.D.

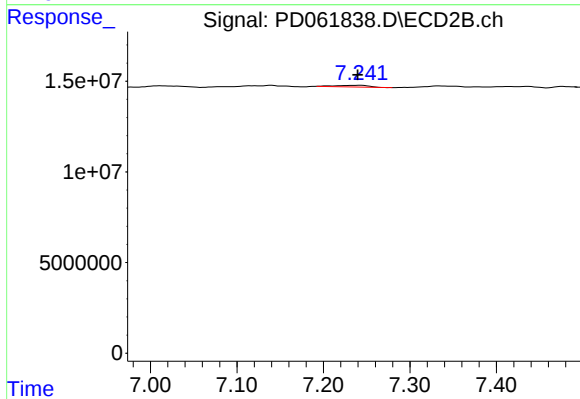

#19 Endosulfan Sulfate


R.T.: 7.242 min
Delta R.T.: 0.003 min
Response: 2256445
Conc: 0.23 ng/ml

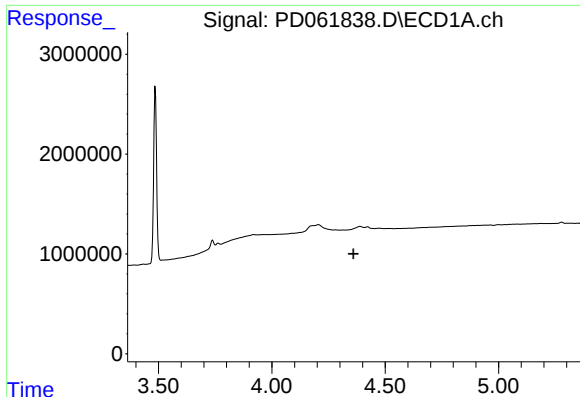

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.361 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB135412BL

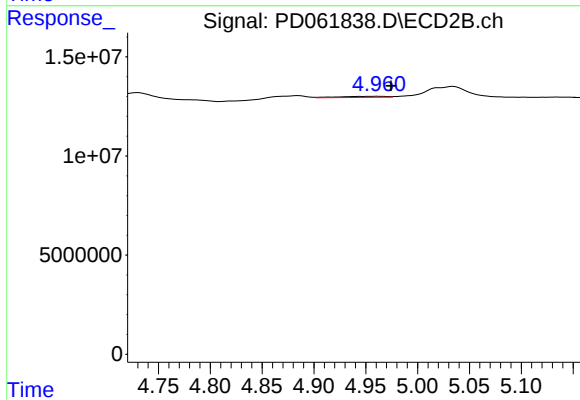


#23 Chlordane-1

R.T.: 4.963 min
Delta R.T.: -0.012 min
Response: 1643843
Conc: 4.24 ng/ml

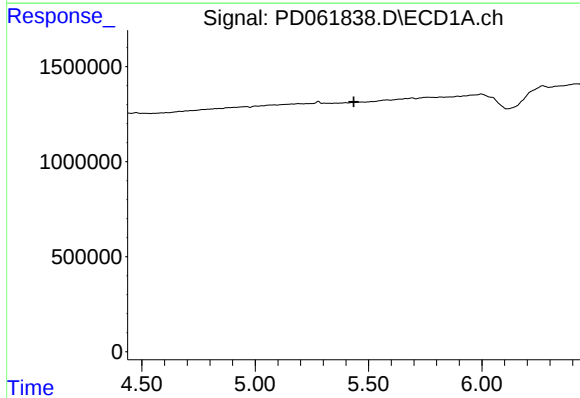


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.435 min
Response: 0
Conc: N.D.

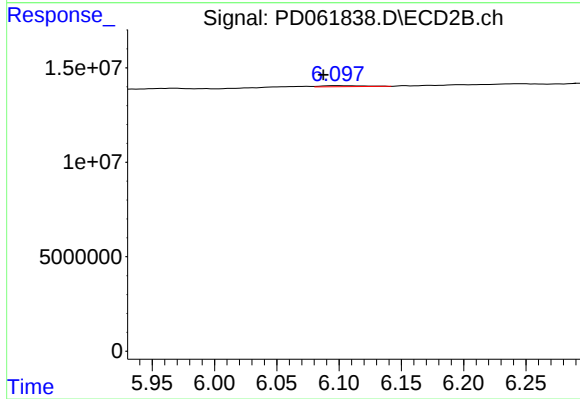

#25 Chlordane-3


R.T.: 6.098 min
Delta R.T.: 0.011 min
Response: 1249139
Conc: 0.75 ng/ml

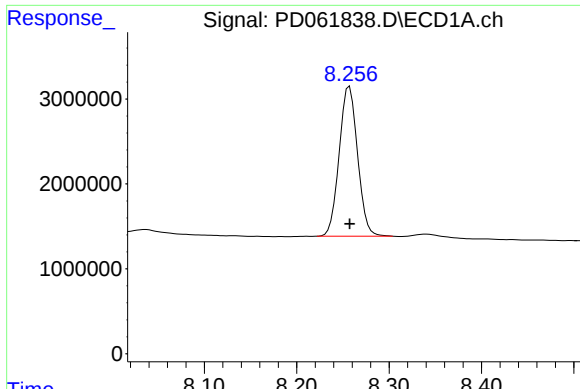

#28 Decachlorobiphenyl

R.T.: 8.257 min
Delta R.T.: 0.000 min
Response: 24431608
Conc: 19.86 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB135412BL

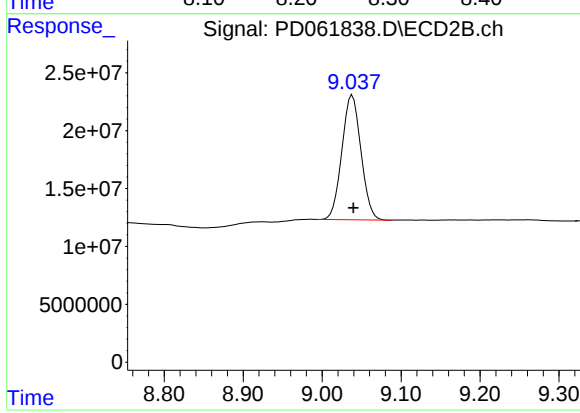

#28 Decachlorobiphenyl

R.T.: 9.038 min
Delta R.T.: -0.002 min
Response: 180635066
Conc: 19.13 ng/ml