

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032921\
 Data File : PD061833.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Mar 2021 21:18
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD032921

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 30 05:39:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 30 04:47:56 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	3.982	43881432	400.0E6	52.409	46.033
28)	SA Decachlor...	8.257	9.039	56079160	416.1E6	45.577	44.076
Target Compounds							
23)	Chlordane-1	4.360	4.975	14611990	174.2E6	459.851	449.144
24)	Chlordane-2	4.863	5.441	17420427	168.6E6	446.551	439.260
25)	Chlordane-3	5.435	6.087	51180913	726.7E6	441.173	438.386
26)	Chlordane-4	5.493	6.161	42193092	837.3E6	438.563	436.322
27)	Chlordane-5	6.333	6.965	18787009	158.9E6	426.650	440.899



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032921\
Data File : PD061833.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Mar 2021 21:18
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD032921

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 30 05:39:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
Quant Title : GC Extractables
QLast Update : Tue Mar 30 04:47:56 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

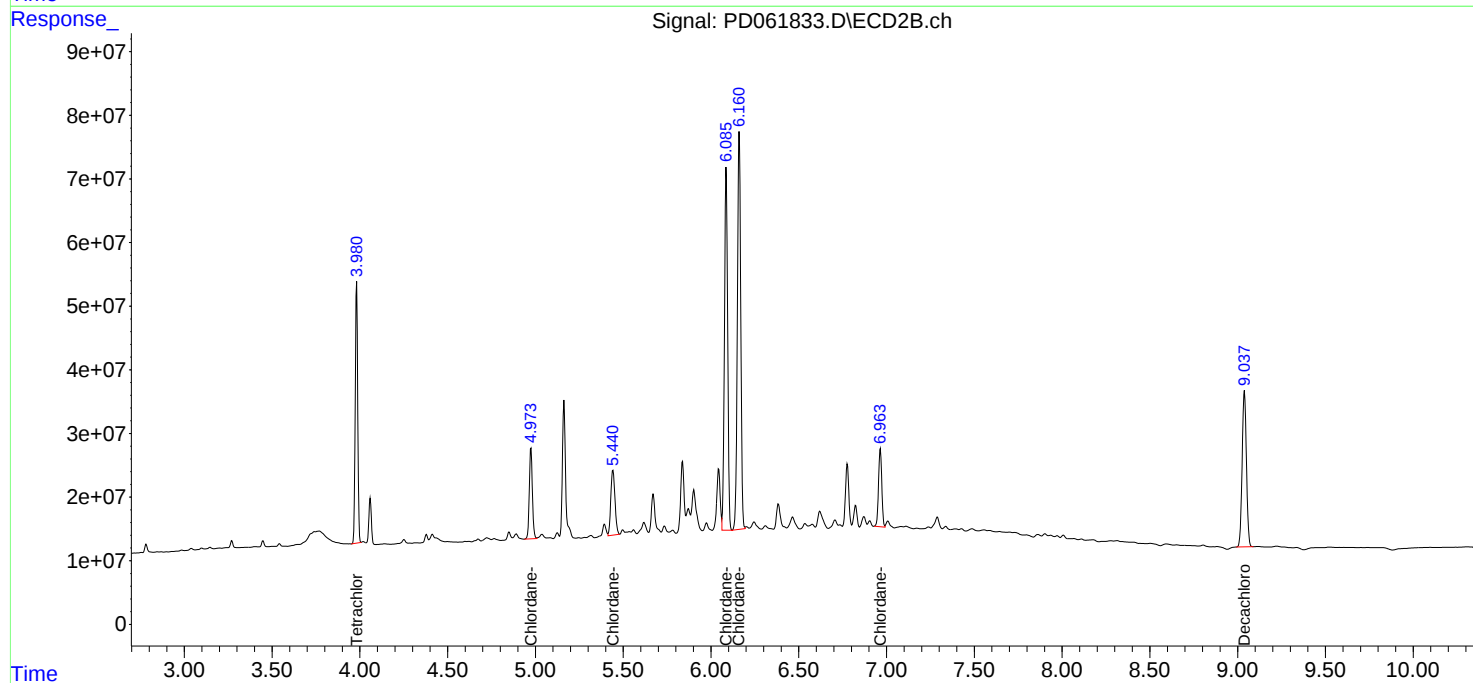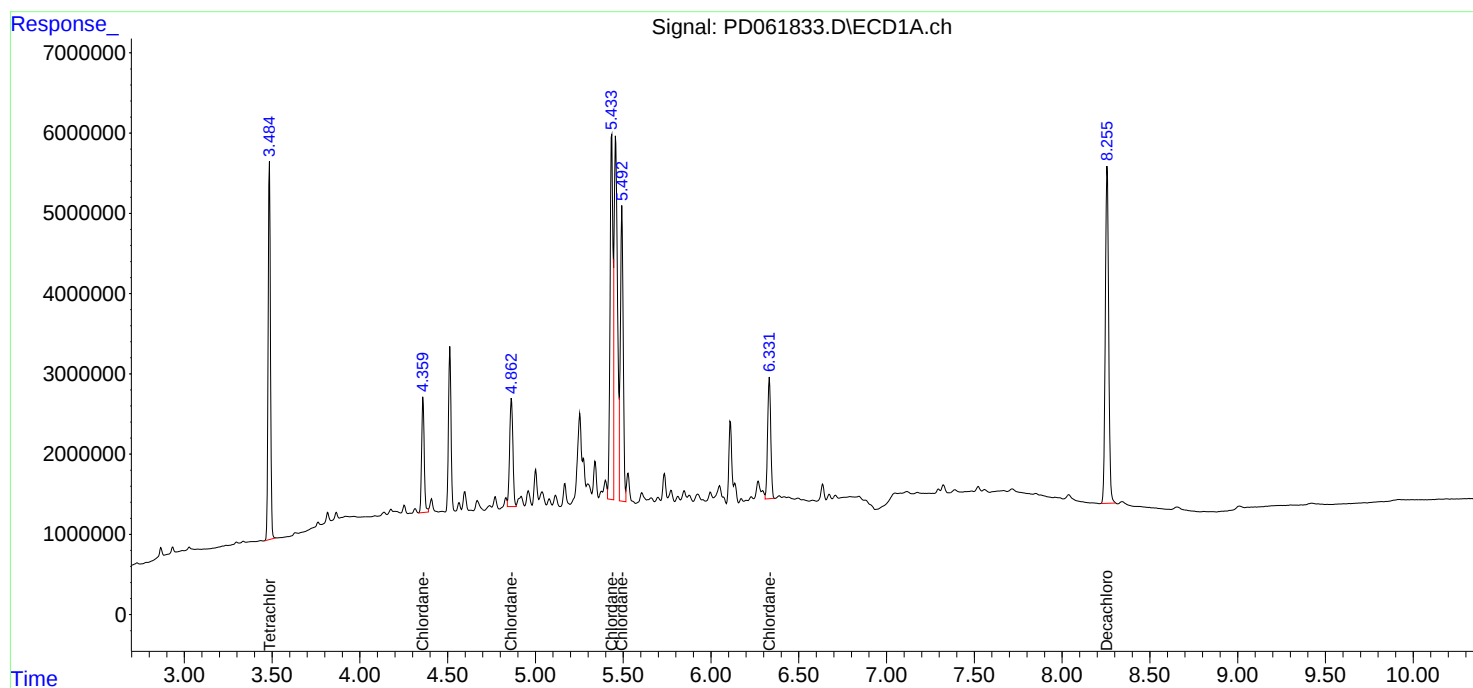


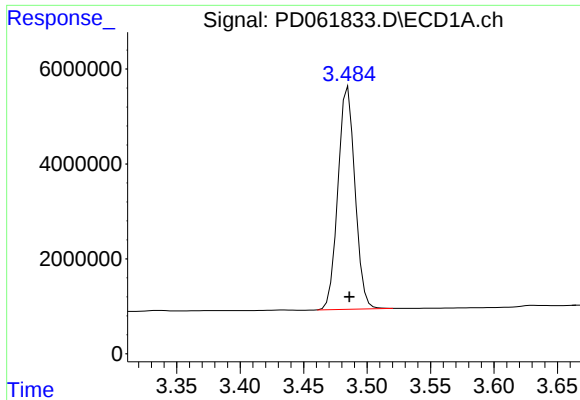

#1 Tetrachloro-m-xylene


R.T.: 3.485 min
Delta R.T.: 0.000 min
Response: 43881432
Conc: 52.41 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD032921

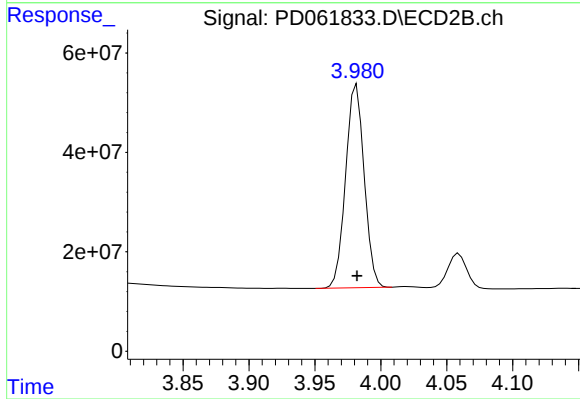


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 399976648
Conc: 46.03 ng/ml

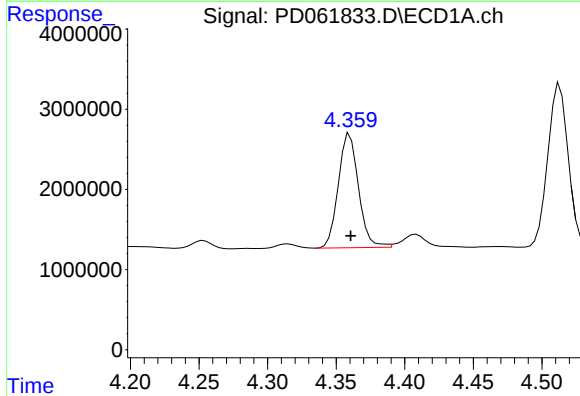


#23 Chlordane-1

R.T.: 4.360 min
Delta R.T.: 0.000 min
Response: 14611990
Conc: 459.85 ng/ml

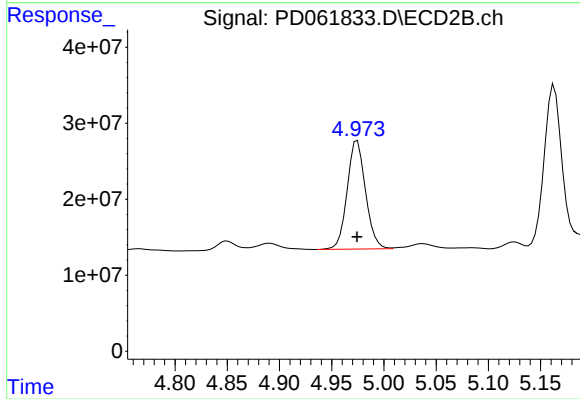

#23 Chlordane-1


R.T.: 4.975 min
Delta R.T.: 0.000 min
Response: 174243427
Conc: 449.14 ng/ml

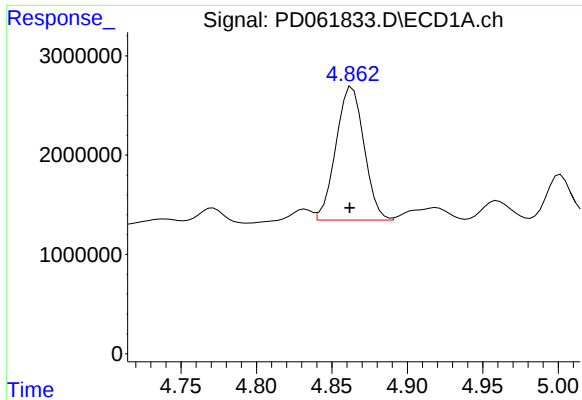

#24 Chlordane-2


R.T.: 4.863 min
Delta R.T.: 0.002 min
Response: 17420427
Conc: 446.55 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD032921

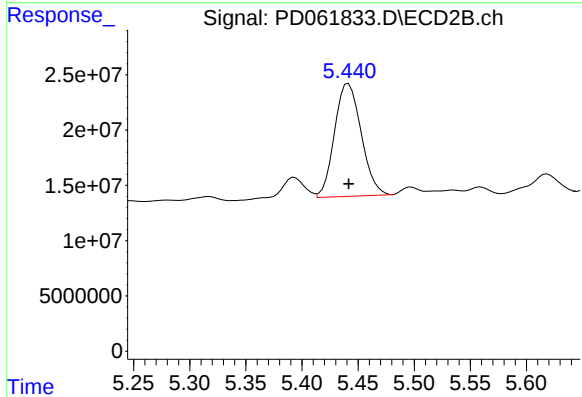


#24 Chlordane-2

R.T.: 5.441 min
Delta R.T.: 0.000 min
Response: 168550309
Conc: 439.26 ng/ml

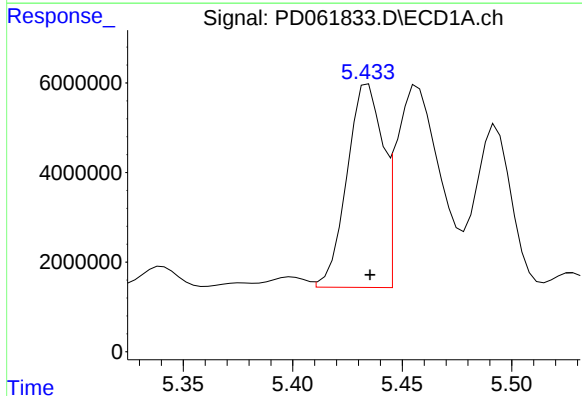


#25 Chlordane-3

R.T.: 5.435 min
Delta R.T.: 0.000 min
Response: 51180913
Conc: 441.17 ng/ml

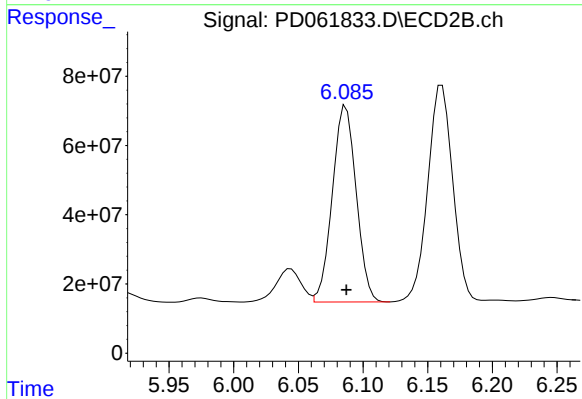

#25 Chlordane-3


R.T.: 6.087 min
Delta R.T.: 0.000 min
Response: 726728622
Conc: 438.39 ng/ml

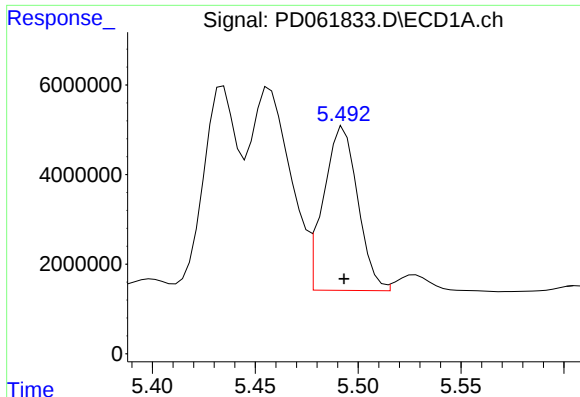

#26 Chlordane-4


R.T.: 5.493 min
Delta R.T.: 0.000 min
Response: 42193092
Conc: 438.56 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD032921

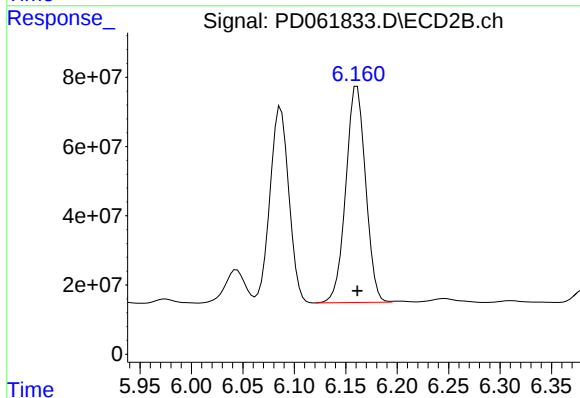


#26 Chlordane-4

R.T.: 6.161 min
Delta R.T.: 0.000 min
Response: 837279004
Conc: 436.32 ng/ml

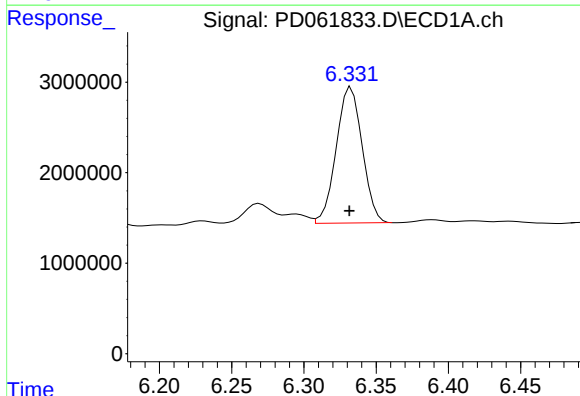


#27 Chlordane-5

R.T.: 6.333 min
Delta R.T.: 0.001 min
Response: 18787009
Conc: 426.65 ng/ml

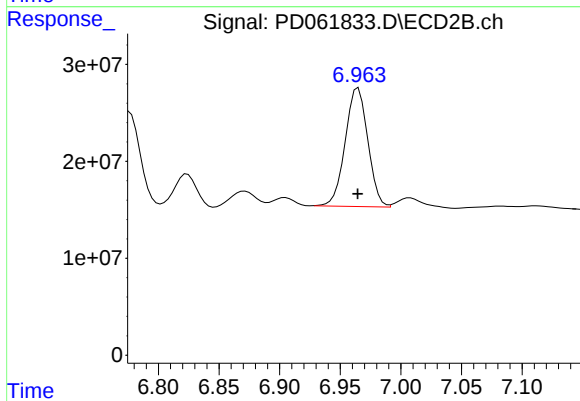

#27 Chlordane-5


R.T.: 6.965 min
Delta R.T.: 0.000 min
Response: 158899967
Conc: 440.90 ng/ml

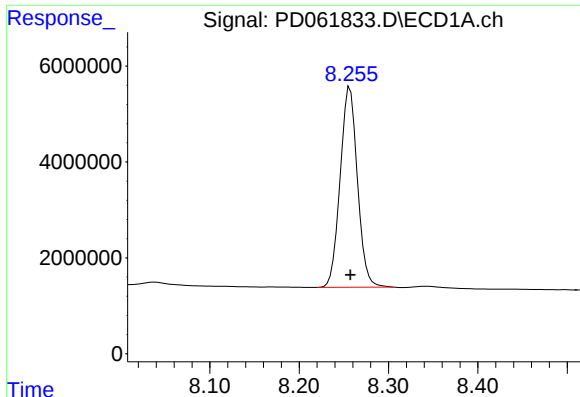

#28 Decachlorobiphenyl

R.T.: 8.257 min
Delta R.T.: 0.000 min
Response: 56079160
Conc: 45.58 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD032921

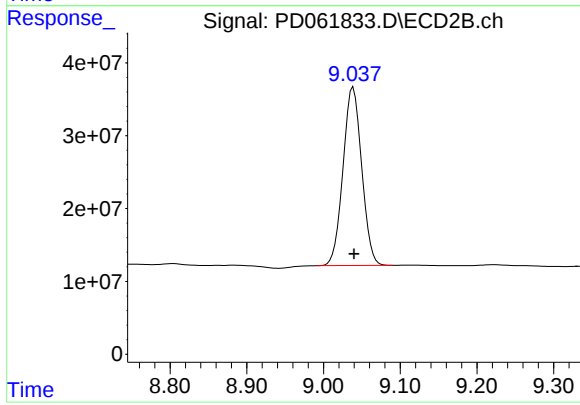

#28 Decachlorobiphenyl

R.T.: 9.039 min
Delta R.T.: -0.001 min
Response: 416104096
Conc: 44.08 ng/ml