

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032922\
 Data File : PD068814.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Mar 2022 08:44
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 30 00:57:43 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 03:30:32 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	0.000	4.204f	0	1088537	N.D.	0.114 #
Target Compounds						
3) MA gamma-BHC...	0.000	4.868	0	120550	N.D.	0.010 #
4) MA Heptachlor	0.000	5.392	0	130139	N.D.	0.011 #
6) B beta-BHC	0.000	5.030	0	349948	N.D.	0.064 #
9) A Endosulfan I	0.000	6.450	0	2173724	N.D.	0.232 #
10) B gamma-Chl...	5.397	0.000	87945	0	0.058	N.D. #
11) B alpha-Chl...	0.000	6.395	0	13187708	N.D.	1.325 #
12) B 4,4'-DDE	0.000	6.572f	0	277320	N.D.	0.030 #
14) MA Endrin	6.020f	0.000	464859	0	0.353	N.D. #
20) A Methoxychlor	0.000	7.800	0	595961	N.D.	0.163 #
24) Chlordane-2	0.000	5.648f	0	170881	N.D.	0.447 #
25) Chlordane-3	5.397	0.000	87945	0	0.631	N.D. #
26) Chlordane-4	0.000	6.395	0	13187708	N.D.	8.483 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032922\
Data File : PD068814.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Mar 2022 08:44
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 30 00:57:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 03:30:32 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

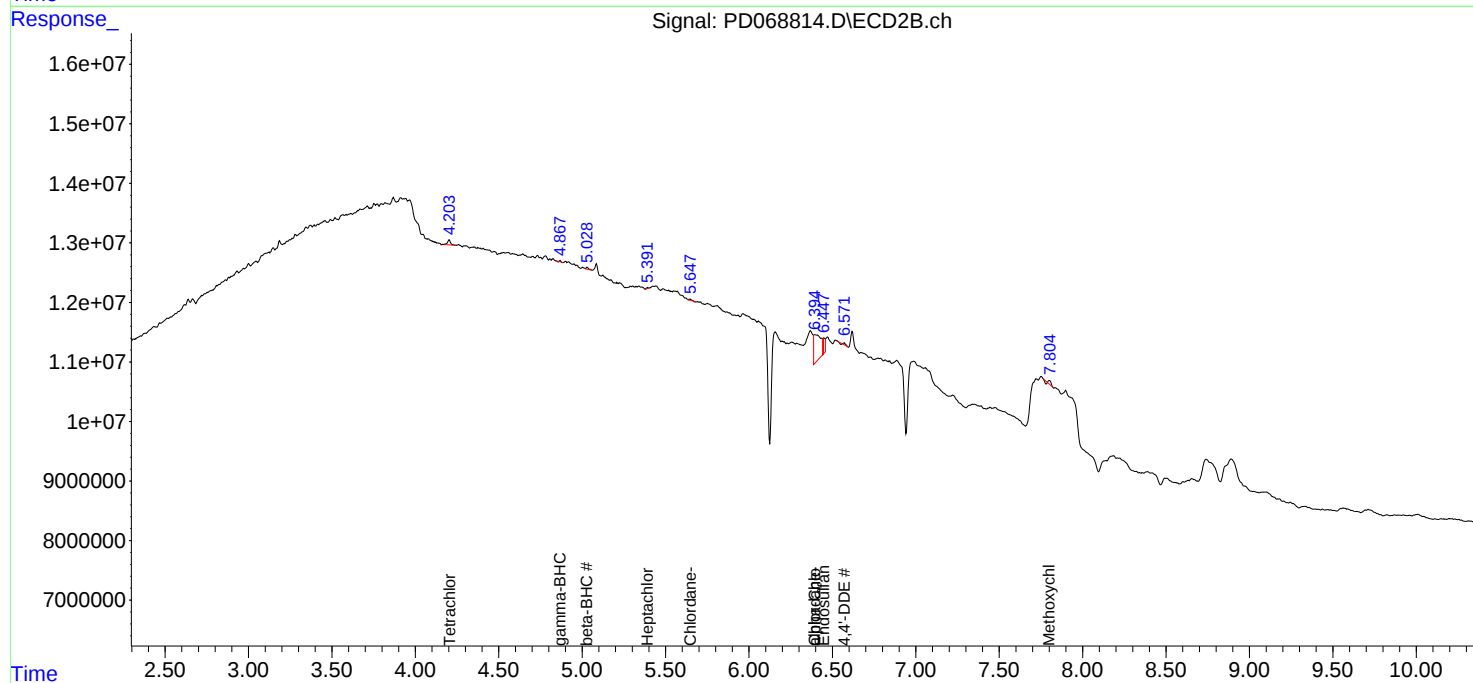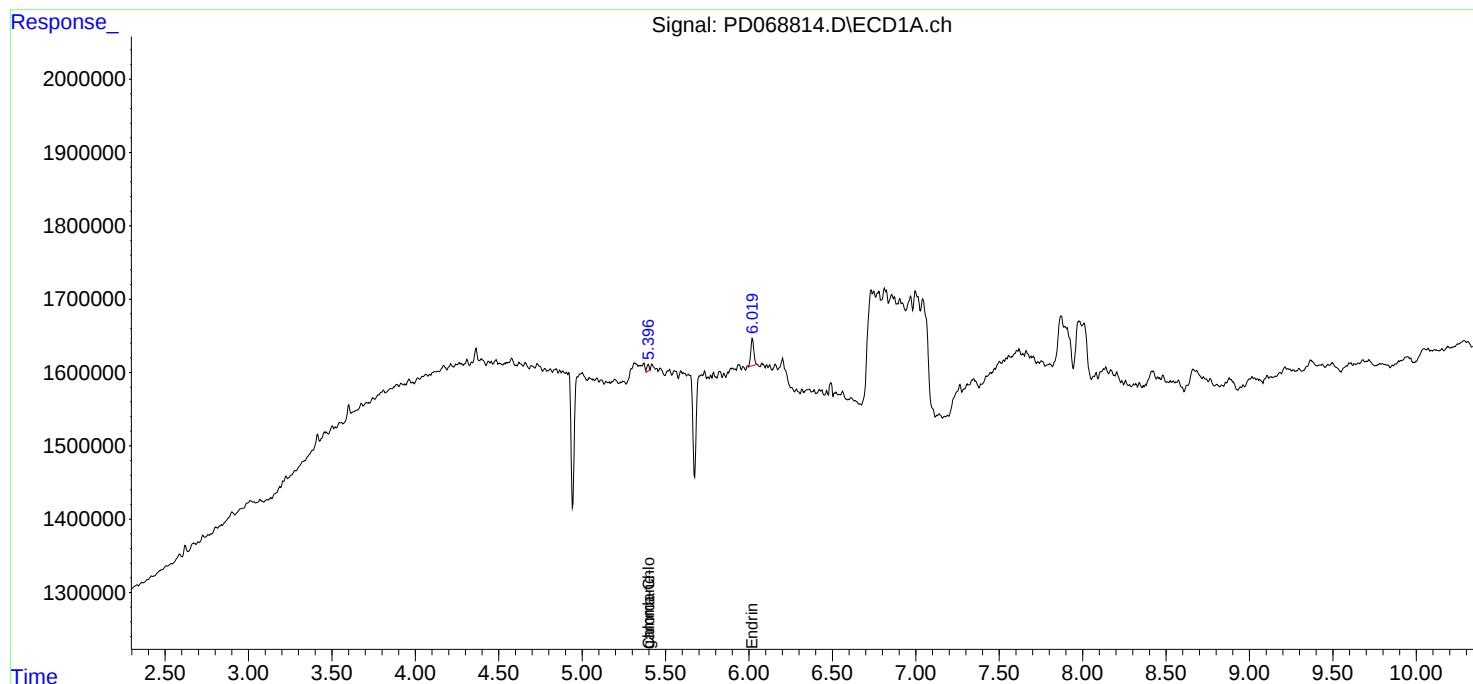


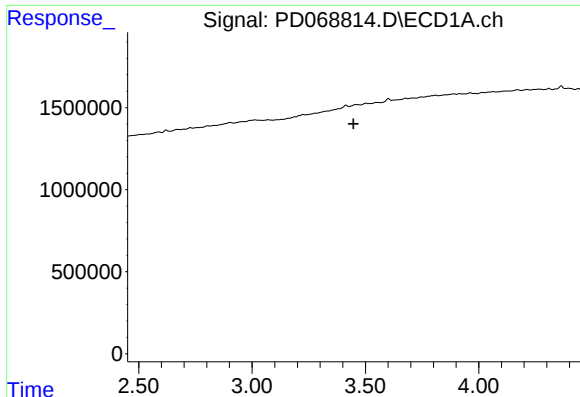

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.448 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

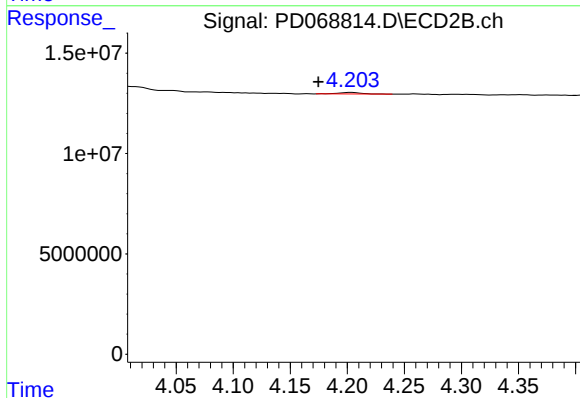


#1 Tetrachloro-m-xylene

R.T.: 4.204 min
Delta R.T.: 0.029 min
Response: 1088537
Conc: 0.11 ng/ml

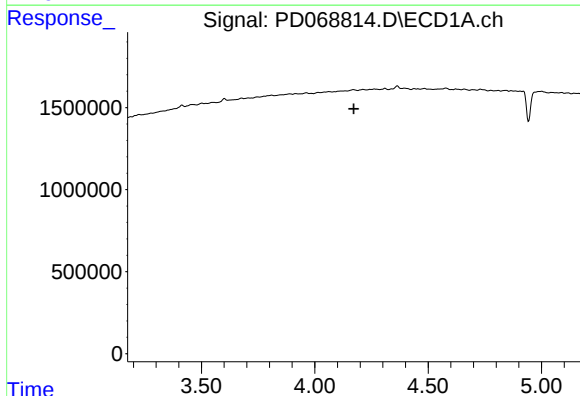


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T.: 4.172 min
Response: 0
Conc: N.D.

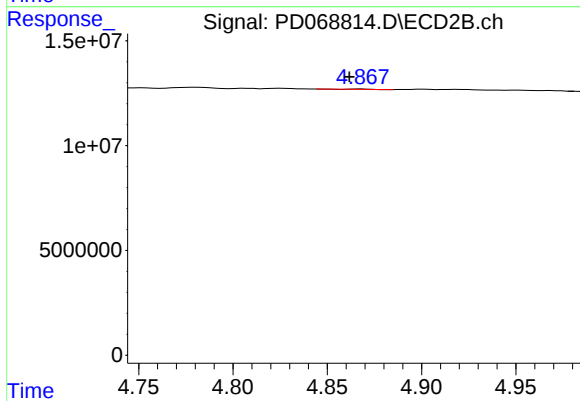

#3 gamma-BHC (Lindane)


R.T.: 4.868 min
Delta R.T.: 0.007 min
Response: 120550
Conc: 0.01 ng/ml

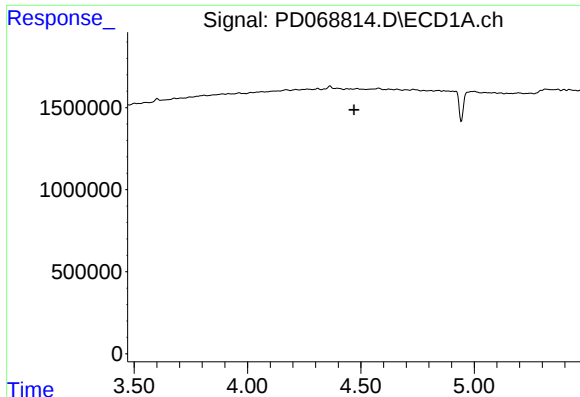

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.470 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

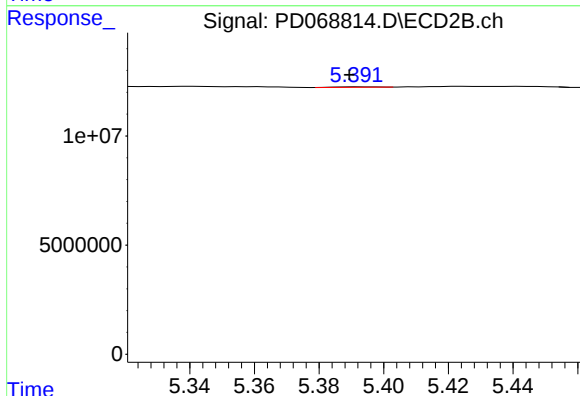


#4 Heptachlor

R.T.: 5.392 min
Delta R.T.: 0.003 min
Response: 130139
Conc: 0.01 ng/ml

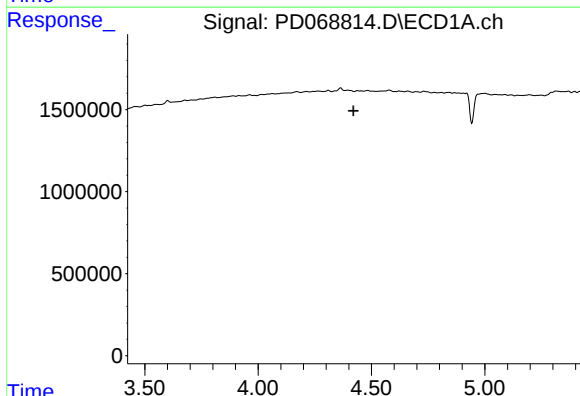


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.421 min
Response: 0
Conc: N.D.

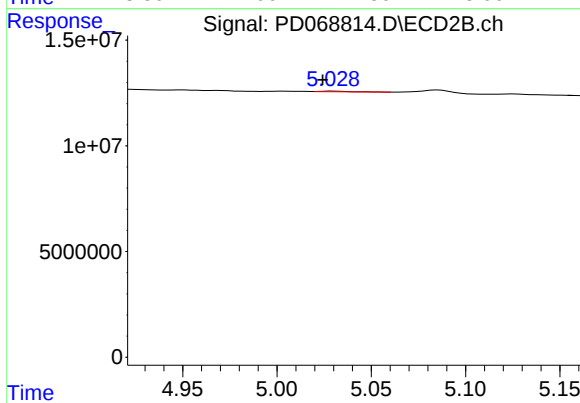

#6 beta-BHC


R.T.: 5.030 min
Delta R.T.: 0.006 min
Response: 349948
Conc: 0.06 ng/ml

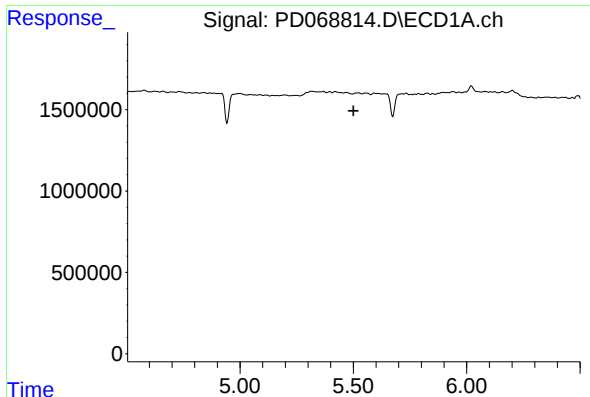

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.501 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

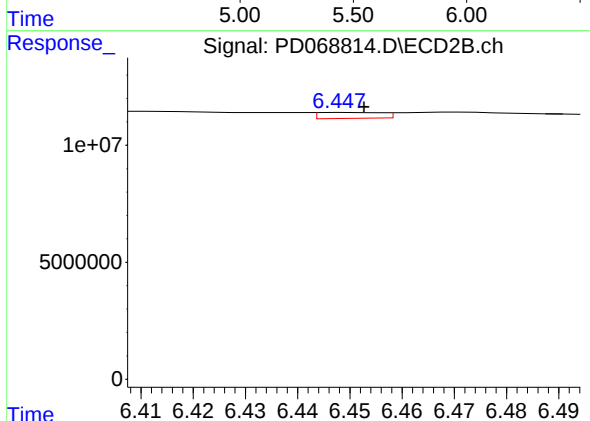


#9 Endosulfan I

R.T.: 6.450 min
Delta R.T.: -0.003 min
Response: 2173724
Conc: 0.23 ng/ml

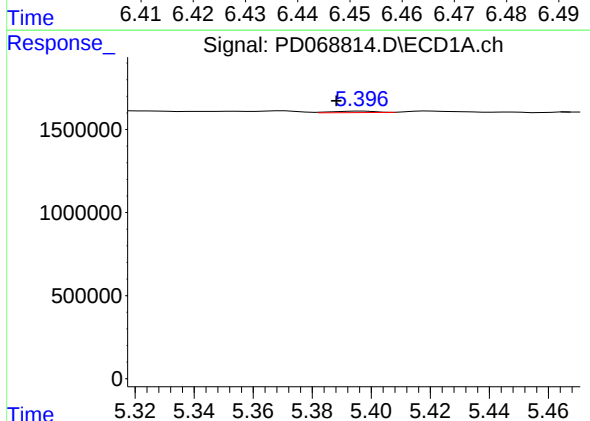


#10 gamma-Chlordane

R.T.: 5.397 min
Delta R.T.: 0.009 min
Response: 87945
Conc: 0.06 ng/ml

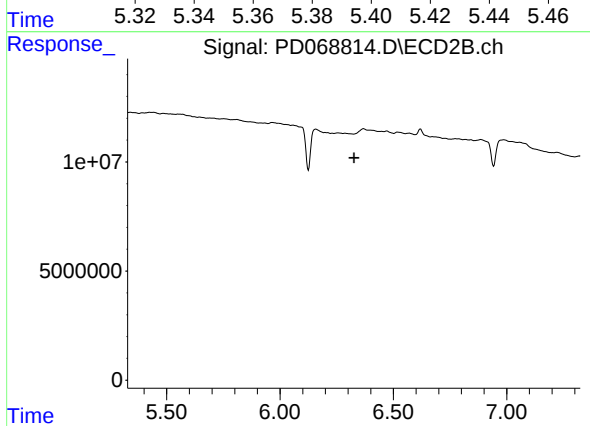

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.327 min
Response: 0
Conc: N.D.

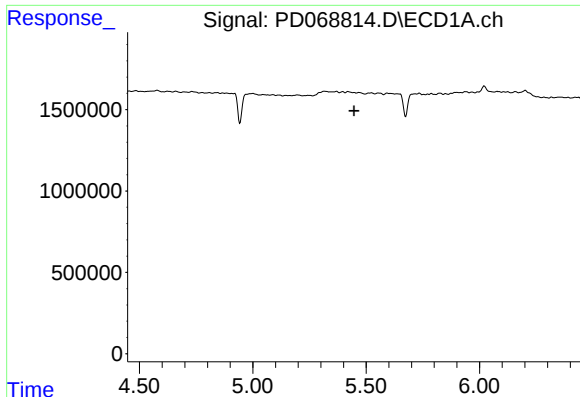

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.447 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

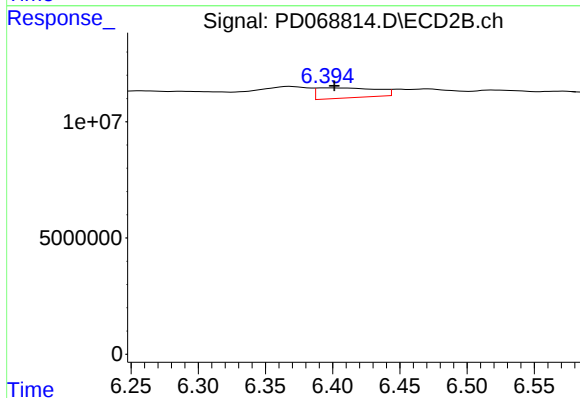


#11 alpha-Chlordane

R.T.: 6.395 min
Delta R.T.: -0.006 min
Response: 13187708
Conc: 1.32 ng/ml

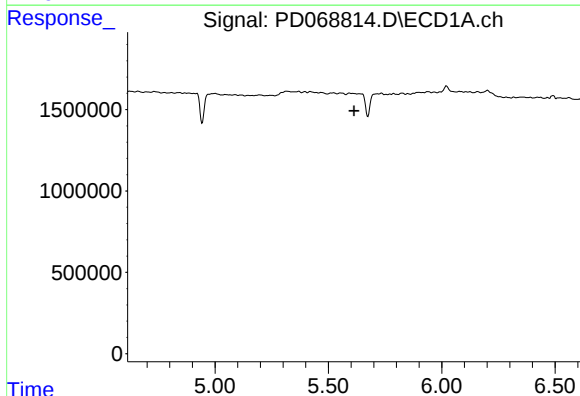


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 5.614 min
Response: 0
Conc: N.D.

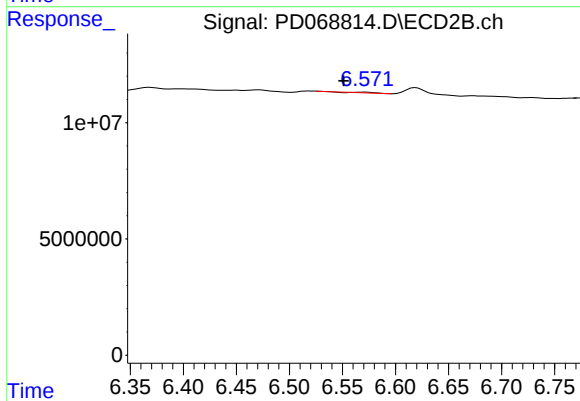

#12 4,4'-DDE


R.T.: 6.572 min
Delta R.T.: 0.020 min
Response: 277320
Conc: 0.03 ng/ml

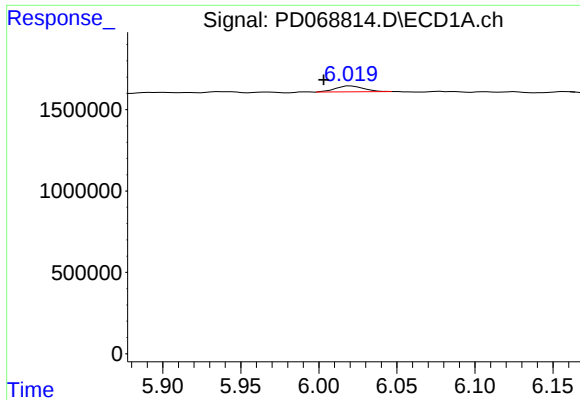

#14 Endrin


R.T.: 6.020 min
Delta R.T.: 0.017 min
Response: 464859
Conc: 0.35 ng/ml

Instrument :
ECD_D
ClientSampleId :

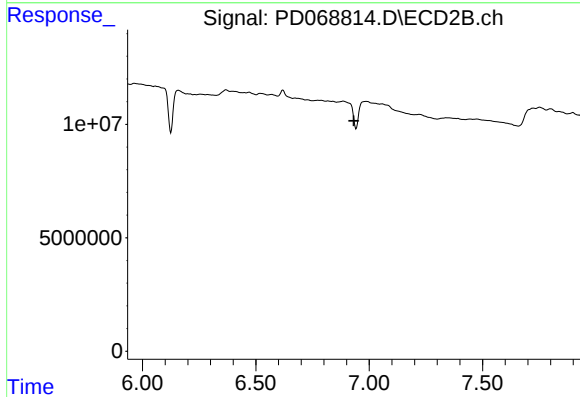


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.932 min
Response: 0
Conc: N.D.

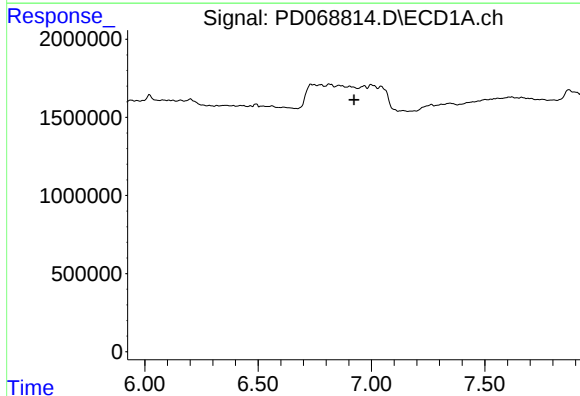


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.924 min
Response: 0
Conc: N.D.

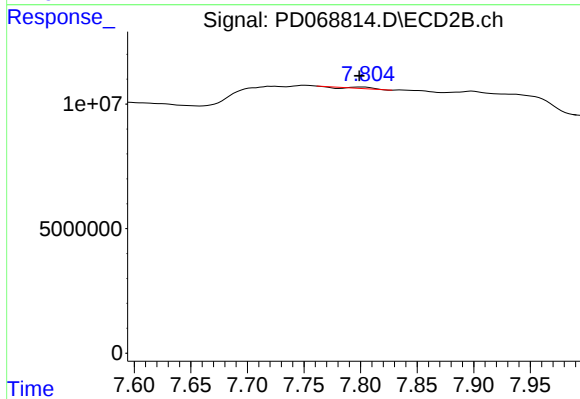

#20 Methoxychlor


R.T.: 7.800 min
Delta R.T.: 0.001 min
Response: 595961
Conc: 0.16 ng/ml

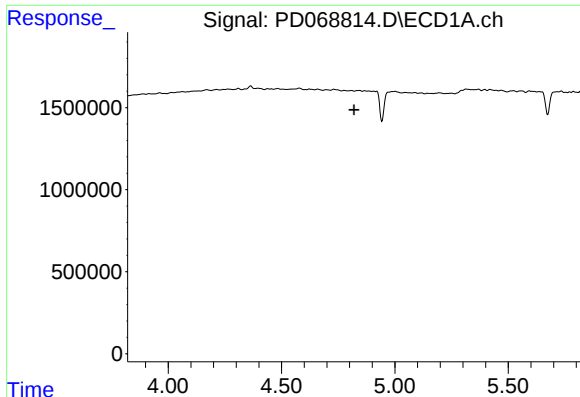

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.820 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

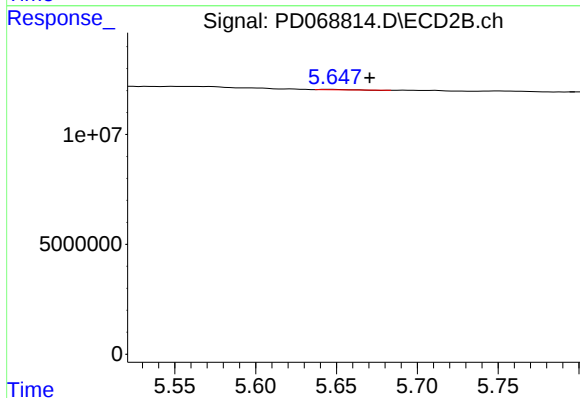


#24 Chlordane-2

R.T.: 5.648 min
Delta R.T.: -0.023 min
Response: 170881
Conc: 0.45 ng/ml

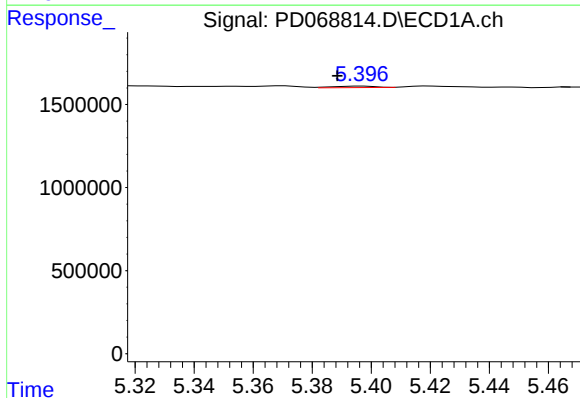


#25 Chlordane-3

R.T.: 5.397 min
Delta R.T.: 0.008 min
Response: 87945
Conc: 0.63 ng/ml

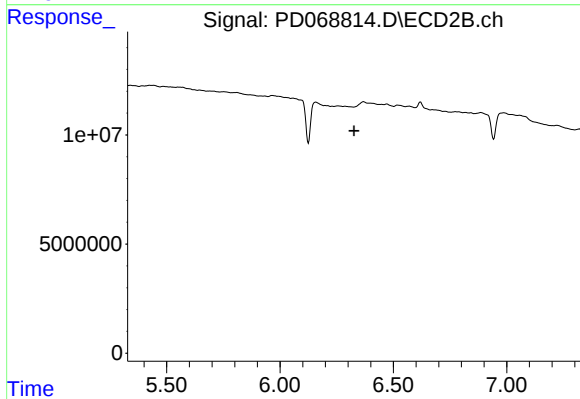

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 6.327 min
Response: 0
Conc: N.D.

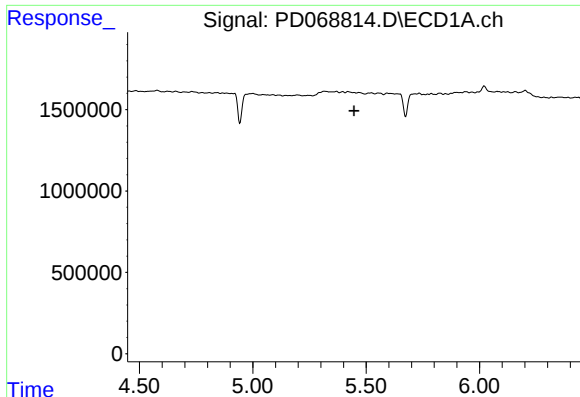

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.447 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

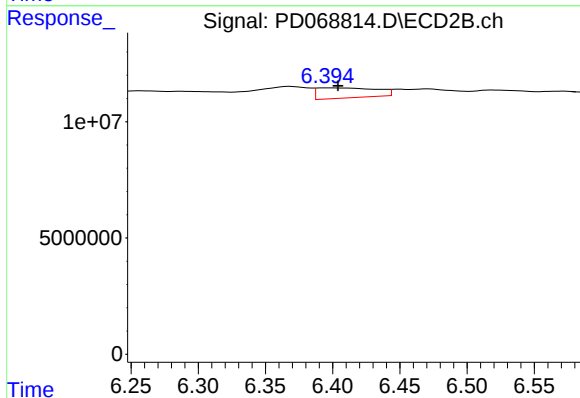


#26 Chlordane-4

R.T.: 6.395 min
Delta R.T.: -0.009 min
Response: 13187708
Conc: 8.48 ng/ml

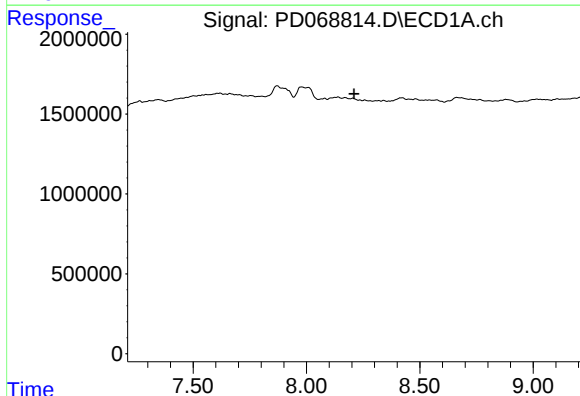

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 8.210 min
Response: 0
Conc: N.D.

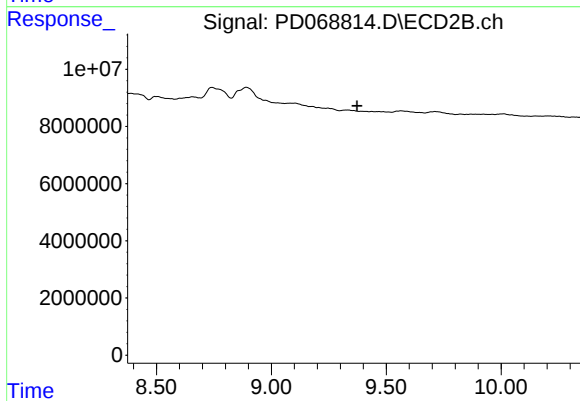

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 9.373 min
Response: 0
Conc: N.D.