

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033019\
 Data File : PD052357.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Mar 2019 22:21
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 03:41:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 29 13:06:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.221	4.043	29976560	699.5E6	21.482	24.134
28)	SA Decachlor...	7.819	9.158	31437070	388.1E6	23.588	24.957
Target Compounds							
2)	A alpha-BHC	3.660f	0.000	595873	0	0.262	N.D. #
3)	MA gamma-BHC...	3.928f	0.000	2509778	0	1.148	N.D. #
8)	B Heptachlo...	0.000	5.921	0	7205115	N.D.	0.223 #
10)	B gamma-Chl...	0.000	6.168	0	9445096	N.D.	0.295 #
22)	Mirex	0.000	8.265	0	3782803	N.D.	0.293 #
25)	Chlordane-3	0.000	6.168	0	9445096	N.D.	2.140 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033019\
Data File : PD052357.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Mar 2019 22:21
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 03:41:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
Quant Title : GC Extractables
QLast Update : Fri Mar 29 13:06:45 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

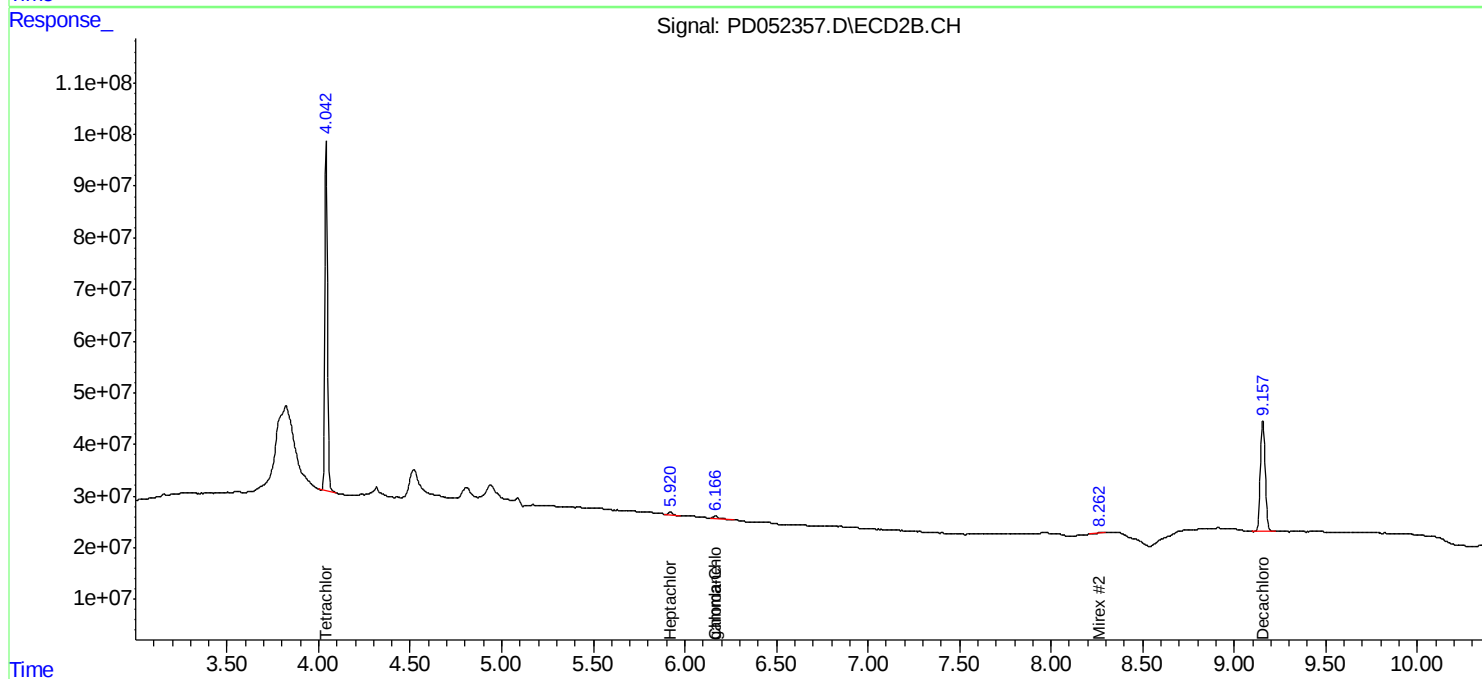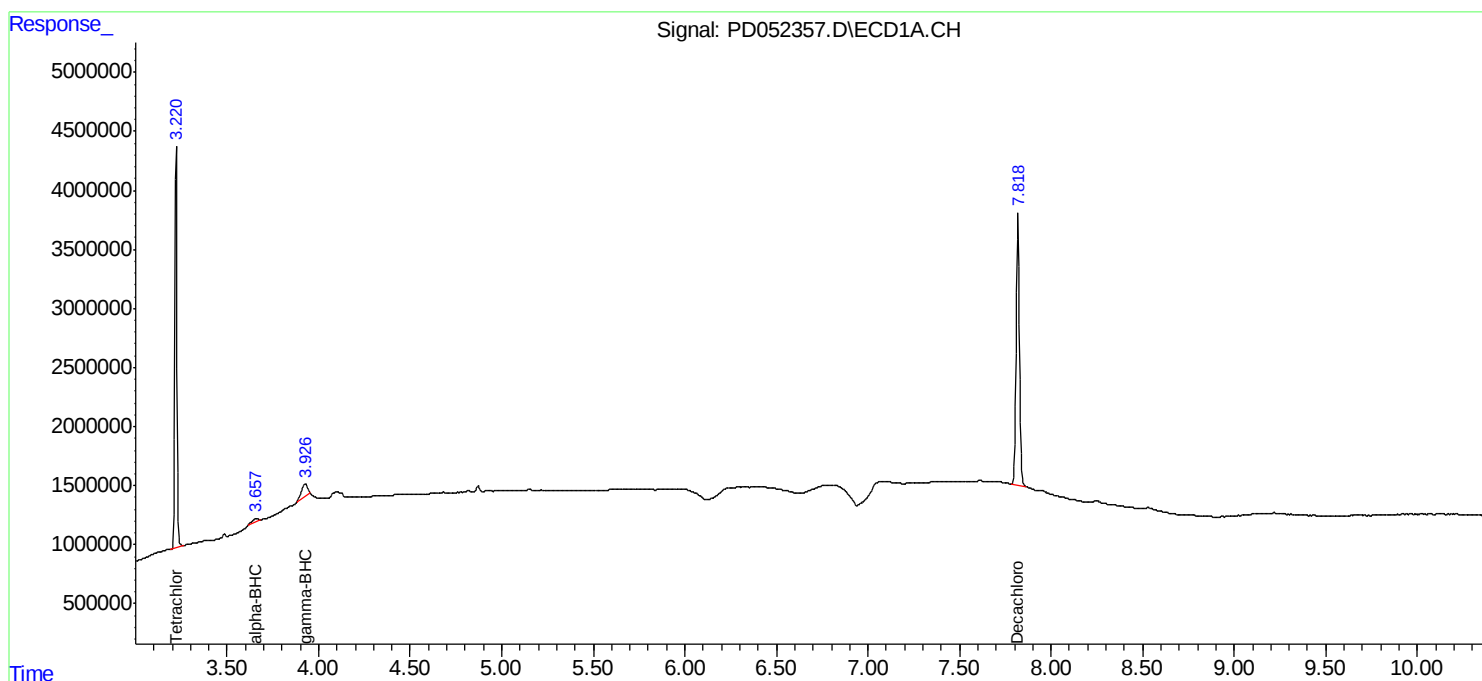


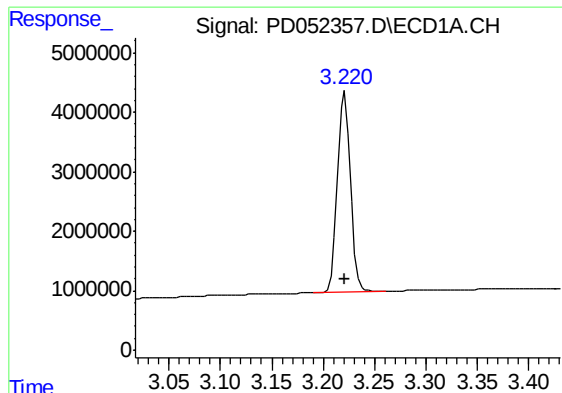

#1 Tetrachloro-m-xylene


R.T.: 3.221 min
Delta R.T.: 0.000 min
Response: 29976560
Conc: 21.48 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

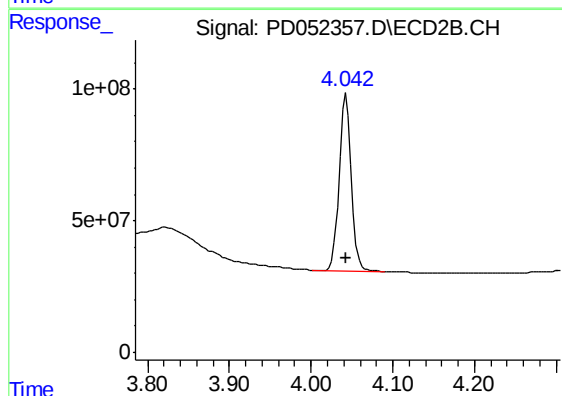


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 699498746
Conc: 24.13 ng/ml

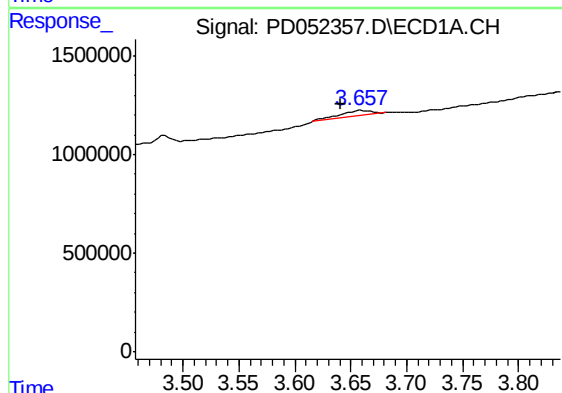


#2 alpha-BHC

R.T.: 3.660 min
Delta R.T.: 0.018 min
Response: 595873
Conc: 0.26 ng/ml

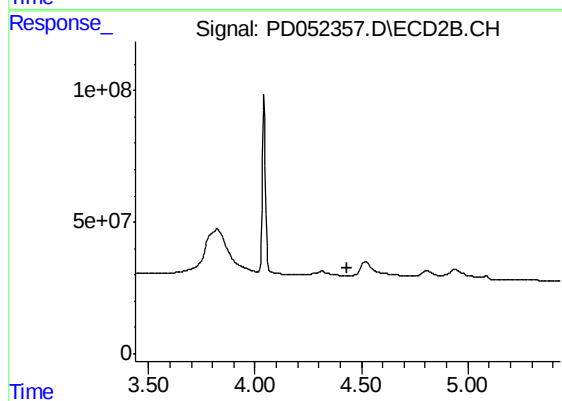

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.436 min
Response: 0
Conc: N.D.

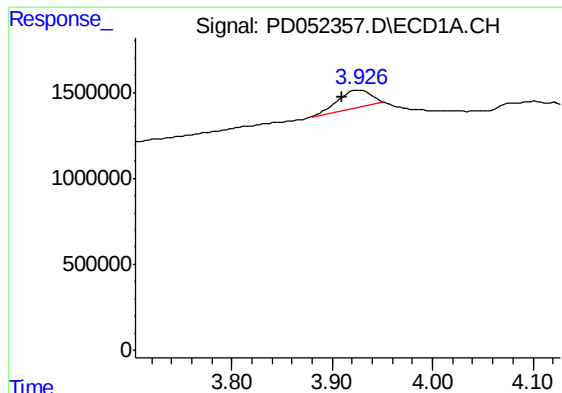

#3 gamma-BHC (Lindane)


R.T.: 3.928 min
Delta R.T.: 0.018 min
Response: 2509778
Conc: 1.15 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

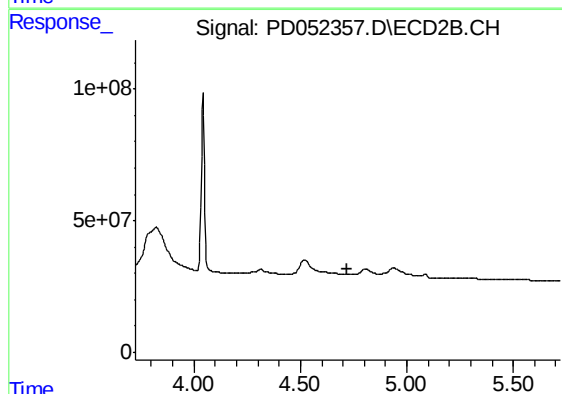


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.723 min
Response: 0
Conc: N.D.

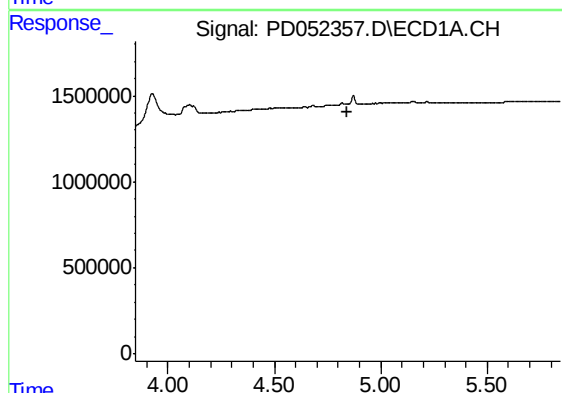


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.846 min
Response: 0
Conc: N.D.

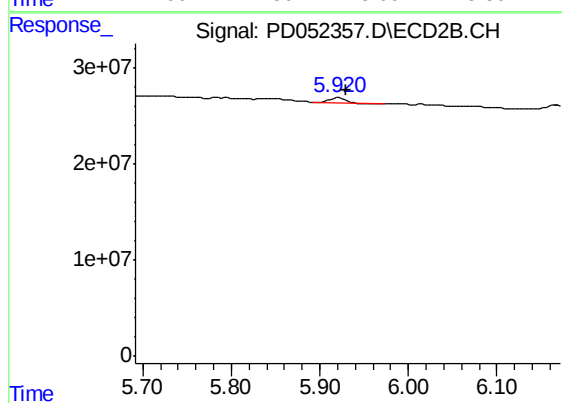

#8 Heptachlor epoxide


R.T.: 5.921 min
Delta R.T.: -0.009 min
Response: 7205115
Conc: 0.22 ng/ml

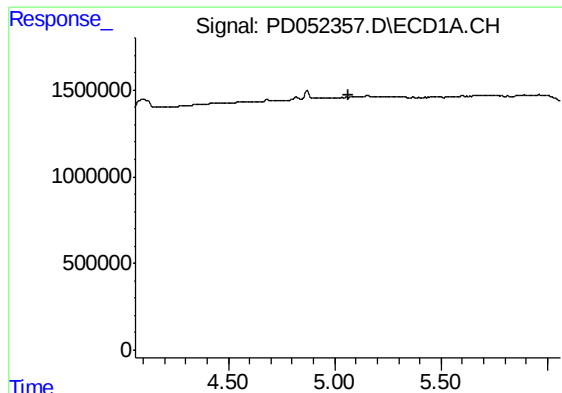

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.063 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

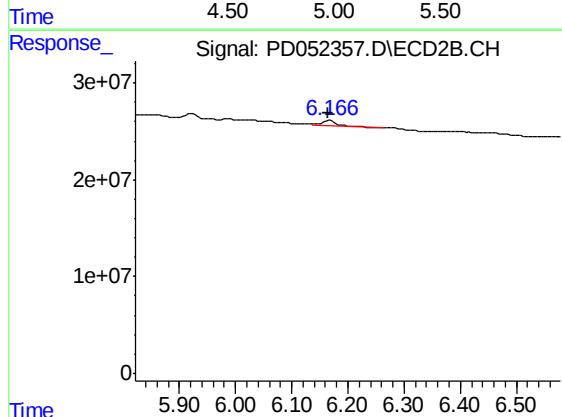


#10 gamma-Chlordane

R.T.: 6.168 min
Delta R.T.: 0.002 min
Response: 9445096
Conc: 0.30 ng/ml

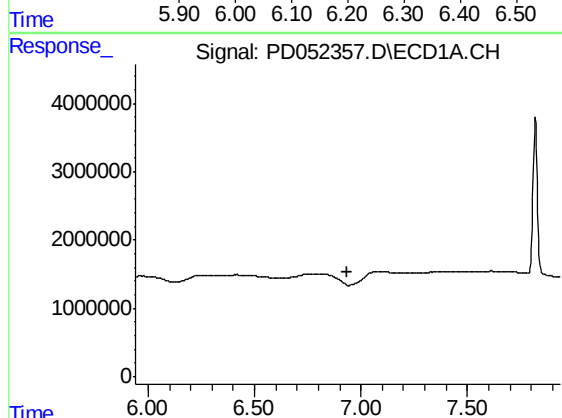


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 6.938 min
Response: 0
Conc: N.D.

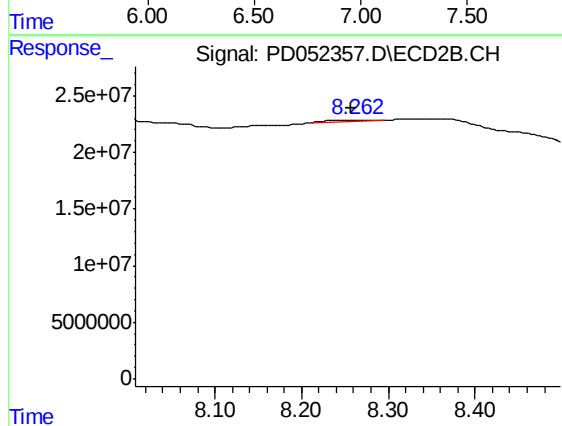

#22 Mirex


R.T.: 8.265 min
Delta R.T.: 0.008 min
Response: 3782803
Conc: 0.29 ng/ml

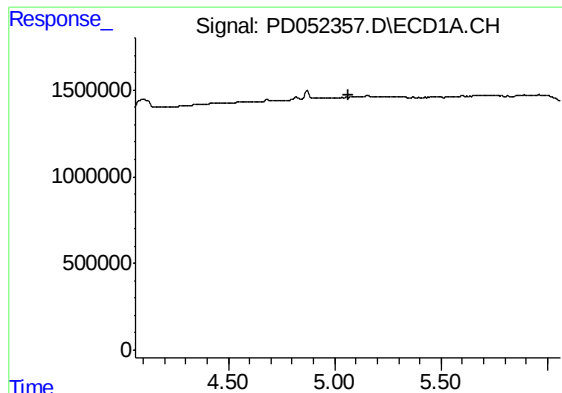

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.064 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

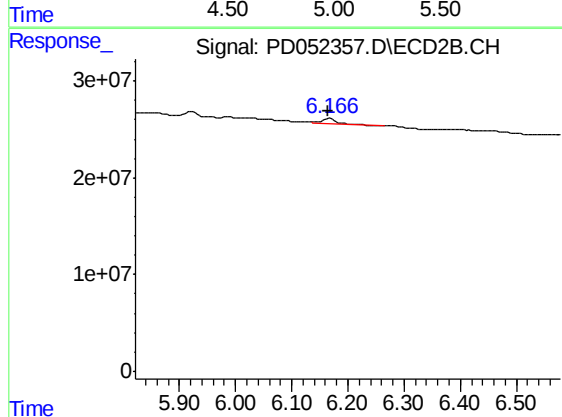


#25 Chlordane-3

R.T.: 6.168 min
Delta R.T.: 0.002 min
Response: 9445096
Conc: 2.14 ng/ml

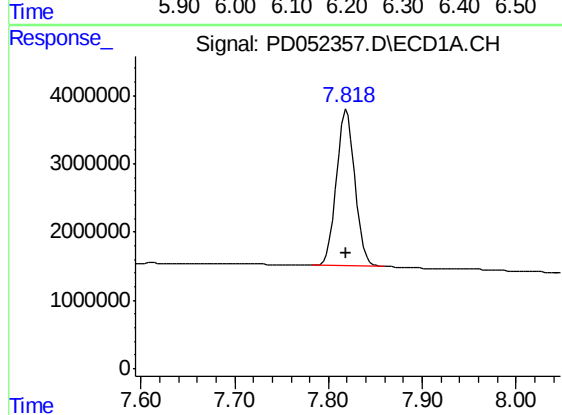

#28 Decachlorobiphenyl

R.T.: 7.819 min
Delta R.T.: 0.000 min
Response: 31437070
Conc: 23.59 ng/ml

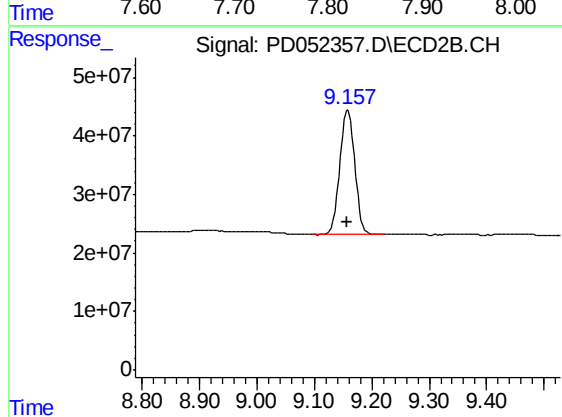

#28 Decachlorobiphenyl

R.T.: 9.158 min
Delta R.T.: 0.001 min
Response: 388110171
Conc: 24.96 ng/ml