

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033019\
 Data File : PD052381.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Mar 2019 23:05
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 03:45:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 29 13:06:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.221	4.043	29899660	702.5E6	21.427	24.238
28)	SA Decachlor...	7.819	9.159	31951882	424.4E6	23.974	27.290
Target Compounds							
3)	MA gamma-BHC...	3.924	0.000	3081682	0	1.409	N.D. #
8)	B Heptachlo...	4.871f	5.925	641676	192.5E6	0.338	5.962 #
9)	A Endosulfan I	0.000	6.282	0	74855932	N.D.	2.562 #
10)	B gamma-Chl...	0.000	6.167	0	195.7E6	N.D.	6.116 #
25)	Chlordane-3	0.000	6.167	0	195.7E6	N.D.	44.341 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033019\
Data File : PD052381.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Mar 2019 23:05
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 03:45:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
Quant Title : GC Extractables
QLast Update : Fri Mar 29 13:06:45 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

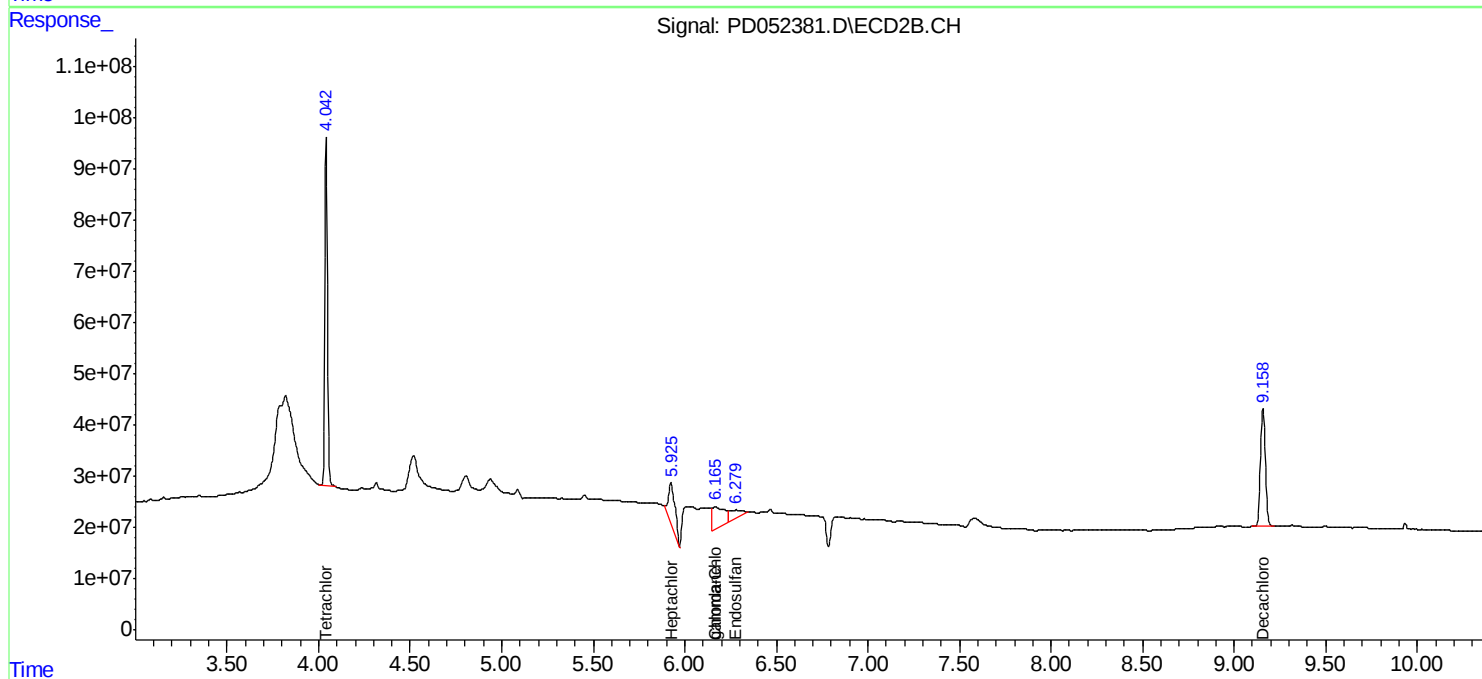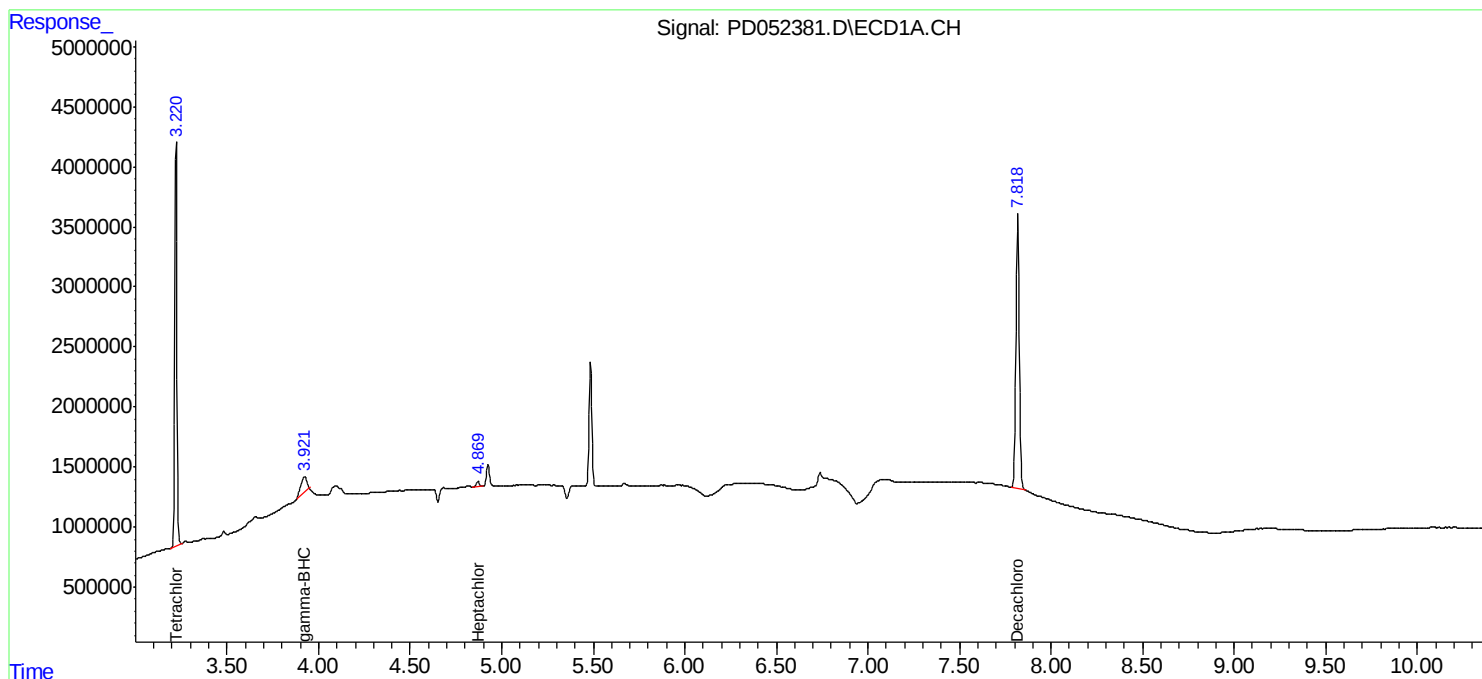


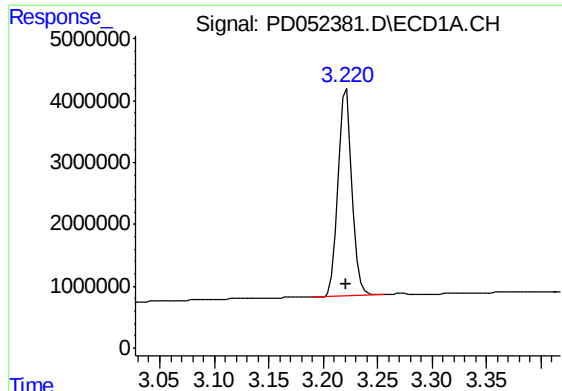

#1 Tetrachloro-m-xylene


R.T.: 3.221 min
Delta R.T.: 0.000 min
Response: 29899660
Conc: 21.43 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

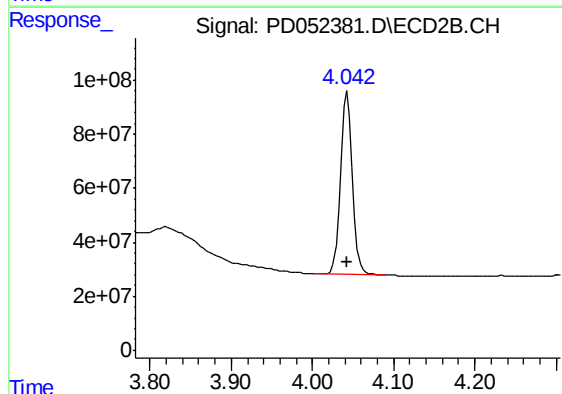


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 702510663
Conc: 24.24 ng/ml

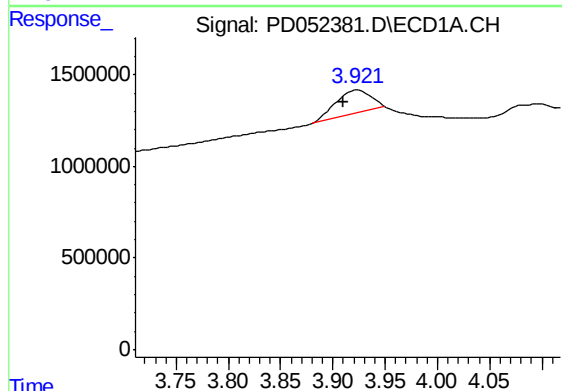


#3 gamma-BHC (Lindane)

R.T.: 3.924 min
Delta R.T.: 0.014 min
Response: 3081682
Conc: 1.41 ng/ml

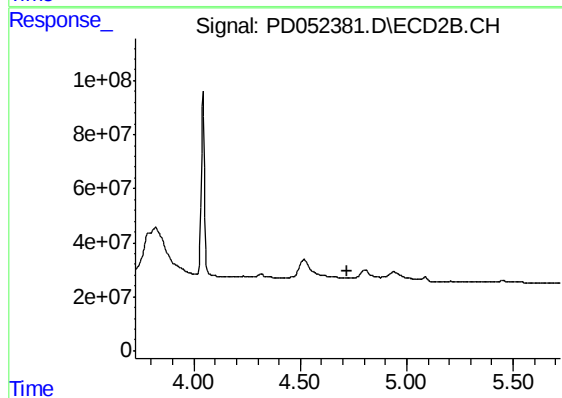

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.723 min
Response: 0
Conc: N.D.

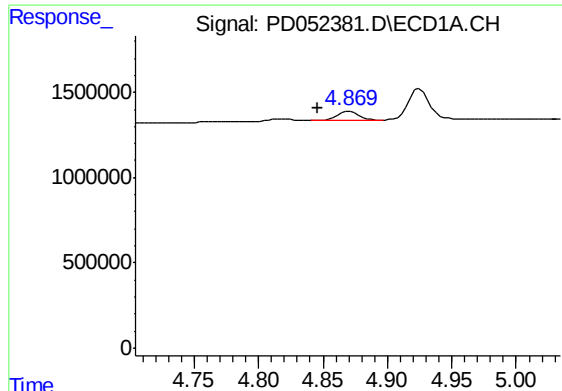

#8 Heptachlor epoxide


R.T.: 4.871 min
Delta R.T.: 0.025 min
Response: 641676
Conc: 0.34 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

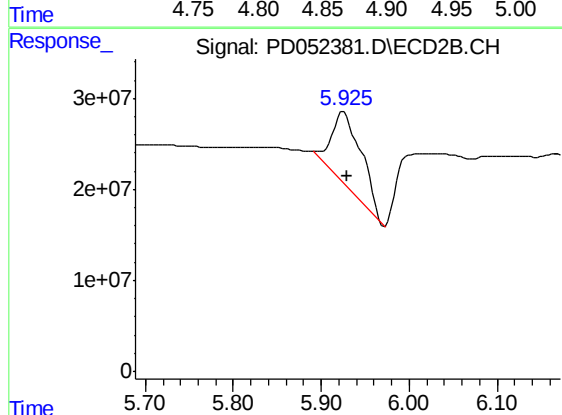


#8 Heptachlor epoxide

R.T.: 5.925 min
Delta R.T.: -0.005 min
Response: 192460334
Conc: 5.96 ng/ml

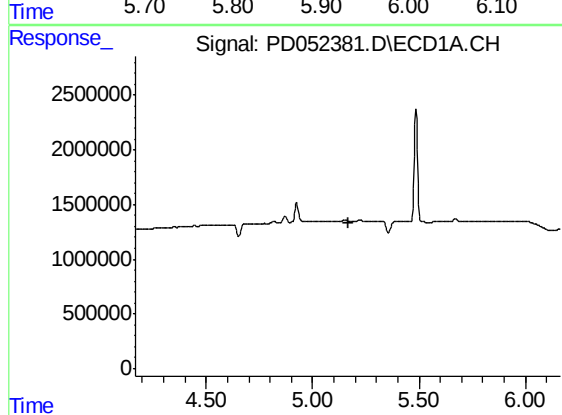


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.167 min
Response: 0
Conc: N.D.

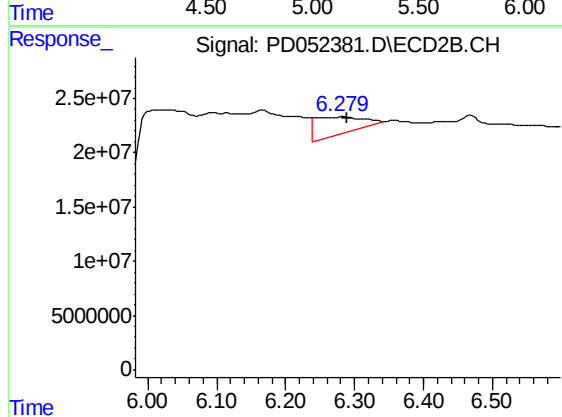

#9 Endosulfan I


R.T.: 6.282 min
Delta R.T.: -0.008 min
Response: 74855932
Conc: 2.56 ng/ml

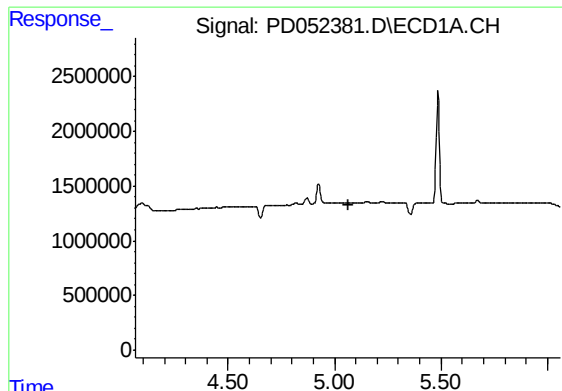

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.063 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

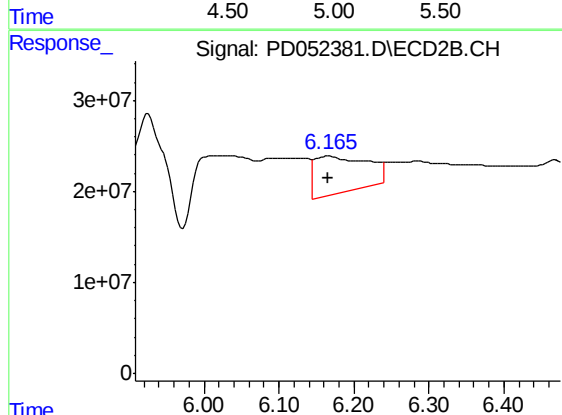


#10 gamma-Chlordane

R.T.: 6.167 min
Delta R.T.: 0.002 min
Response: 195666632
Conc: 6.12 ng/ml

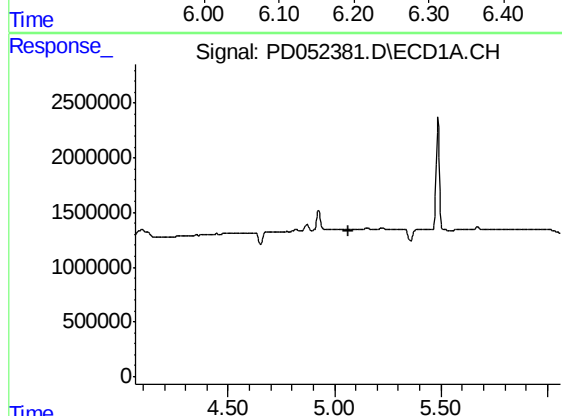


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.064 min
Response: 0
Conc: N.D.

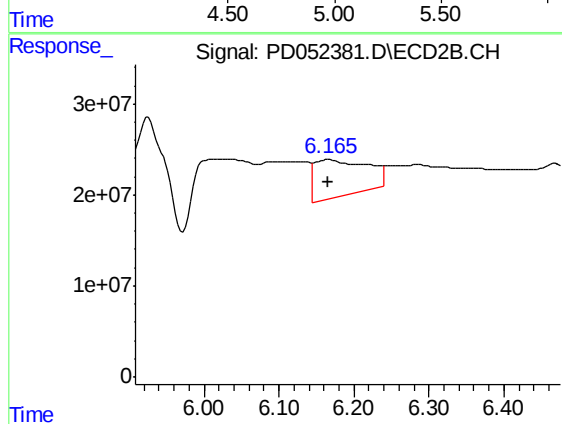

#25 Chlordane-3


R.T.: 6.167 min
Delta R.T.: 0.001 min
Response: 195666632
Conc: 44.34 ng/ml

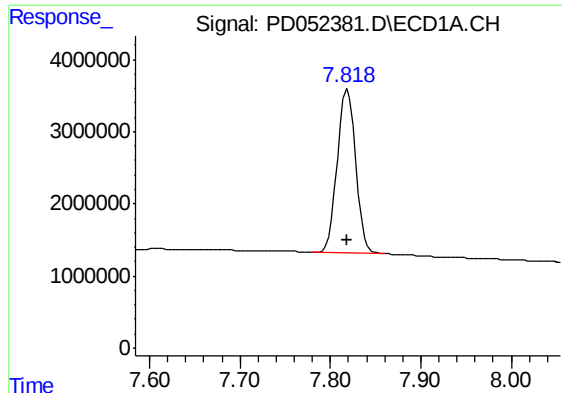

#28 Decachlorobiphenyl

R.T.: 7.819 min
Delta R.T.: 0.000 min
Response: 31951882
Conc: 23.97 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

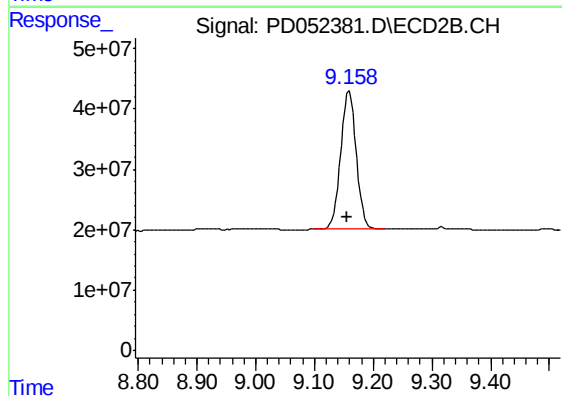

#28 Decachlorobiphenyl

R.T.: 9.159 min
Delta R.T.: 0.003 min
Response: 424394896
Conc: 27.29 ng/ml