

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033019\
 Data File : PD052393.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Apr 2019 2:50
 Operator : AJ\SJ
 Sample : MDL-BL-CHL-W-06
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MDL-BL-CHL-W-06

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 03:48:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 29 13:06:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.221	4.043	30229466	686.5E6	21.663	23.685
28) SA Decachlor...	7.819	9.159	31252716	430.2E6	23.450	27.665
Target Compounds						
3) MA gamma-BHC...	3.922	0.000	2064438	0	0.944	N.D. #
4) MA Heptachlor	0.000	5.246	0	193652	N.D.	0.005 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033019\
Data File : PD052393.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Apr 2019 2:50
Operator : AJ\SJ
Sample : MDL-BL-CHL-W-06
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
MDL-BL-CHL-W-06

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 03:48:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
Quant Title : GC Extractables
QLast Update : Fri Mar 29 13:06:45 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

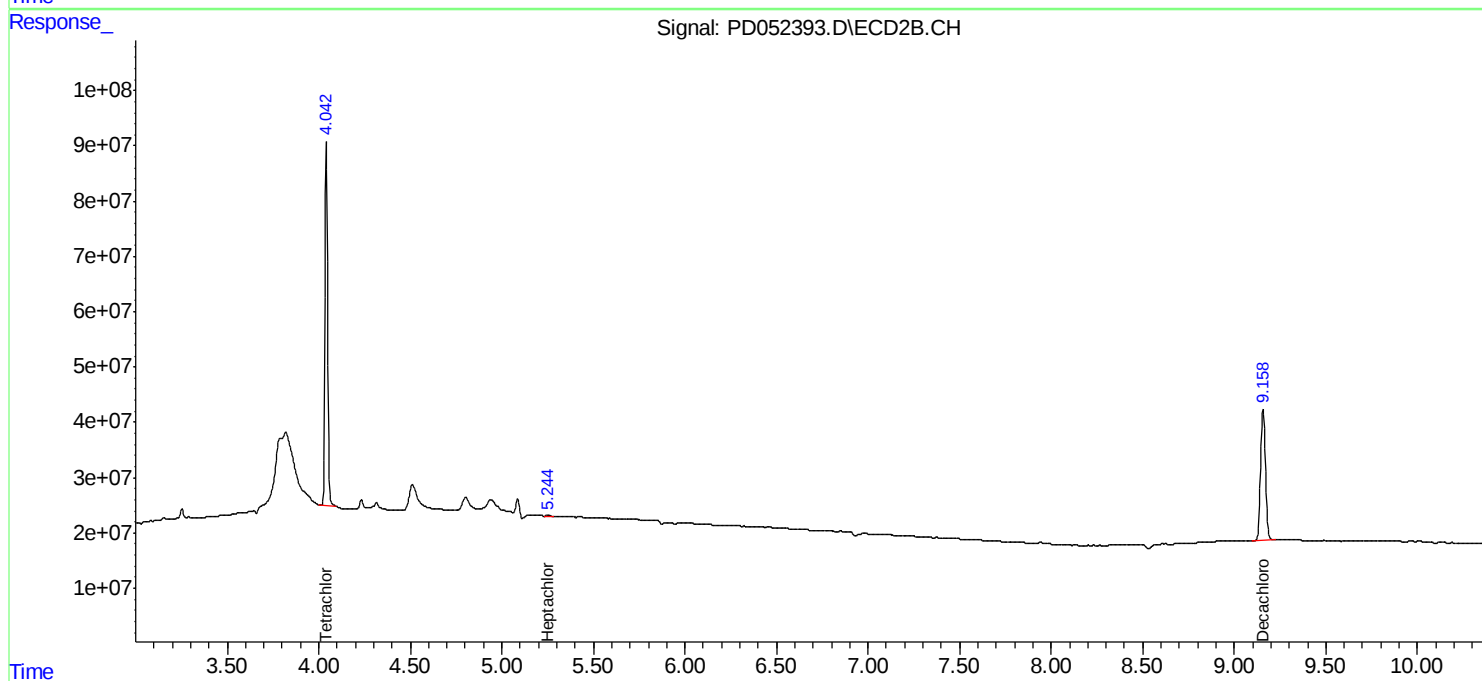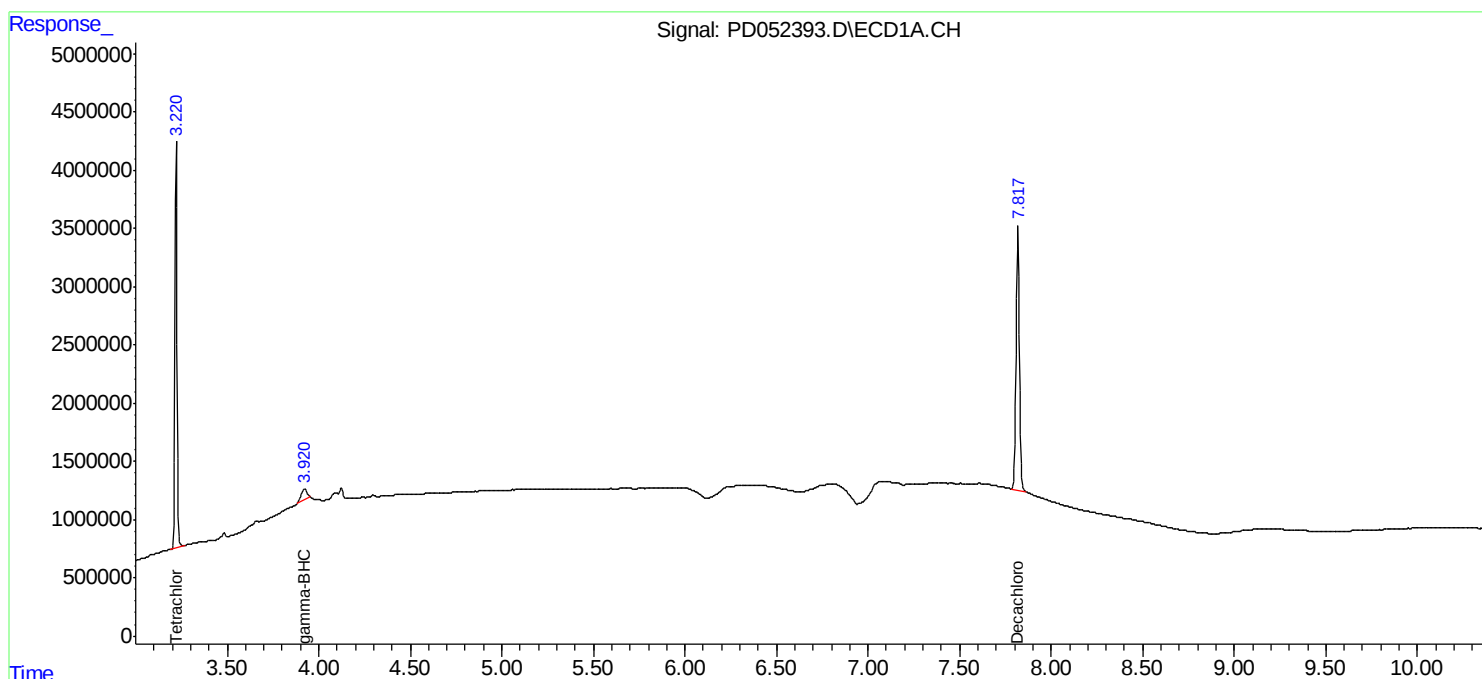


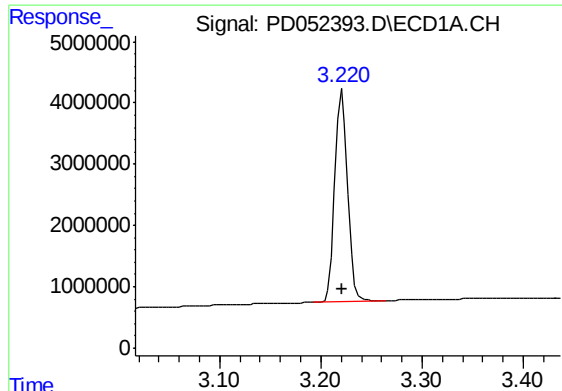

#1 Tetrachloro-m-xylene


R.T.: 3.221 min
Delta R.T.: 0.000 min
Response: 30229466
Conc: 21.66 ng/ml

Instrument :
ECD_D
ClientSampleId :
MDL-BL-CHL-W-06

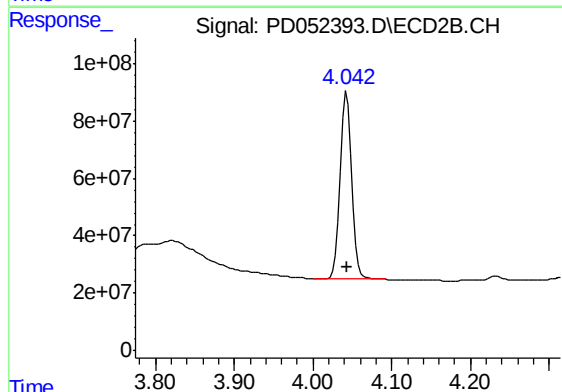


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 686472873
Conc: 23.68 ng/ml

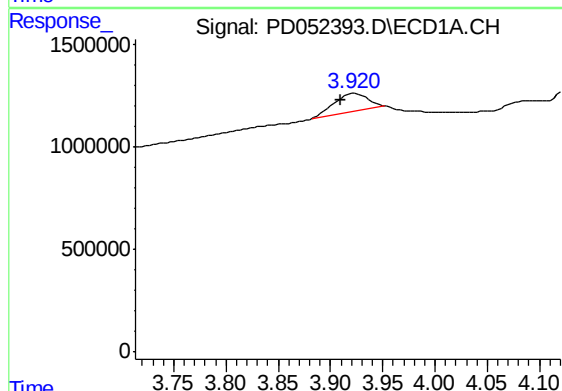


#3 gamma-BHC (Lindane)

R.T.: 3.922 min
Delta R.T.: 0.013 min
Response: 2064438
Conc: 0.94 ng/ml

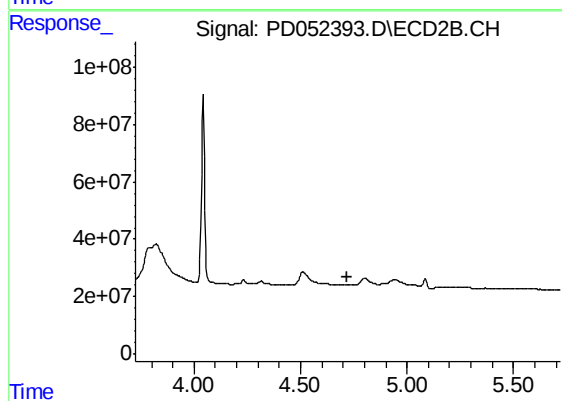

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.723 min
Response: 0
Conc: N.D.

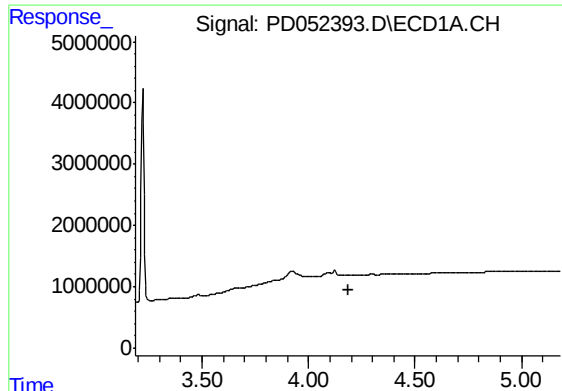

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.187 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
MDL-BL-CHL-W-06

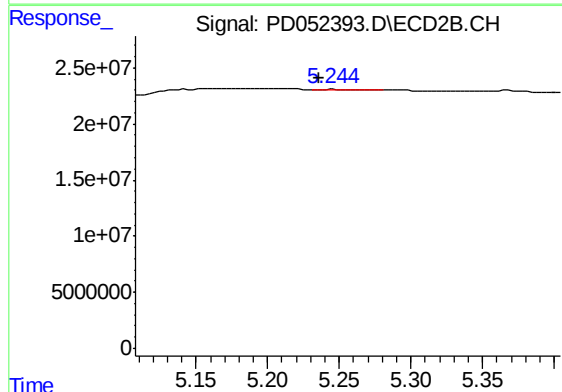


#4 Heptachlor

R.T.: 5.246 min
Delta R.T.: 0.010 min
Response: 193652
Conc: 0.00 ng/ml

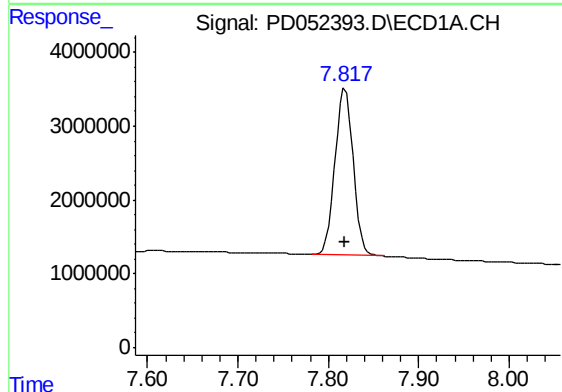

#28 Decachlorobiphenyl

R.T.: 7.819 min
Delta R.T.: 0.000 min
Response: 31252716
Conc: 23.45 ng/ml

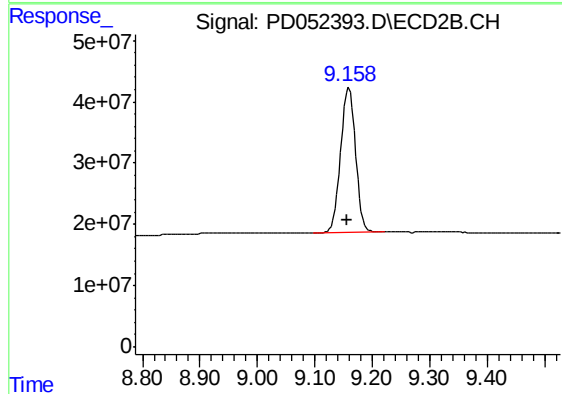

#28 Decachlorobiphenyl

R.T.: 9.159 min
Delta R.T.: 0.002 min
Response: 430229221
Conc: 27.67 ng/ml